

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041693.D
 Acq On : 07 Sep 2023 13:52
 Operator : MA/JU
 Sample : 04166-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH9G3

Quant Time: Sep 08 02:53:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 06 02:20:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	4869	0.400	ng/ul	0.00
4) Naphthalene-d8	10.818	136	11561	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.643	164	5145	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	9318	0.400	ng/ul	0.00
17) Chrysene-d12	21.565	240	3699	0.400	ng/ul	0.00
23) Perylene-d12	23.994	264	4751	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	34026	4.573	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	5131	0.345	ng/ul	-0.01
18) Fluoranthene-d10	19.413	212	7045	0.393	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	812	0.105	ng/ul#	67
20) Pyrene	19.780	202	2329	0.054	ng/ul#	1
26) Benzo(a)pyrene	23.839	252	4139	0.120	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041693.D
Acq On : 07 Sep 2023 13:52
Operator : MA/JU
Sample : 04166-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH9G3

Quant Time: Sep 08 02:53:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 06 02:20:07 2023
Response via : Initial Calibration




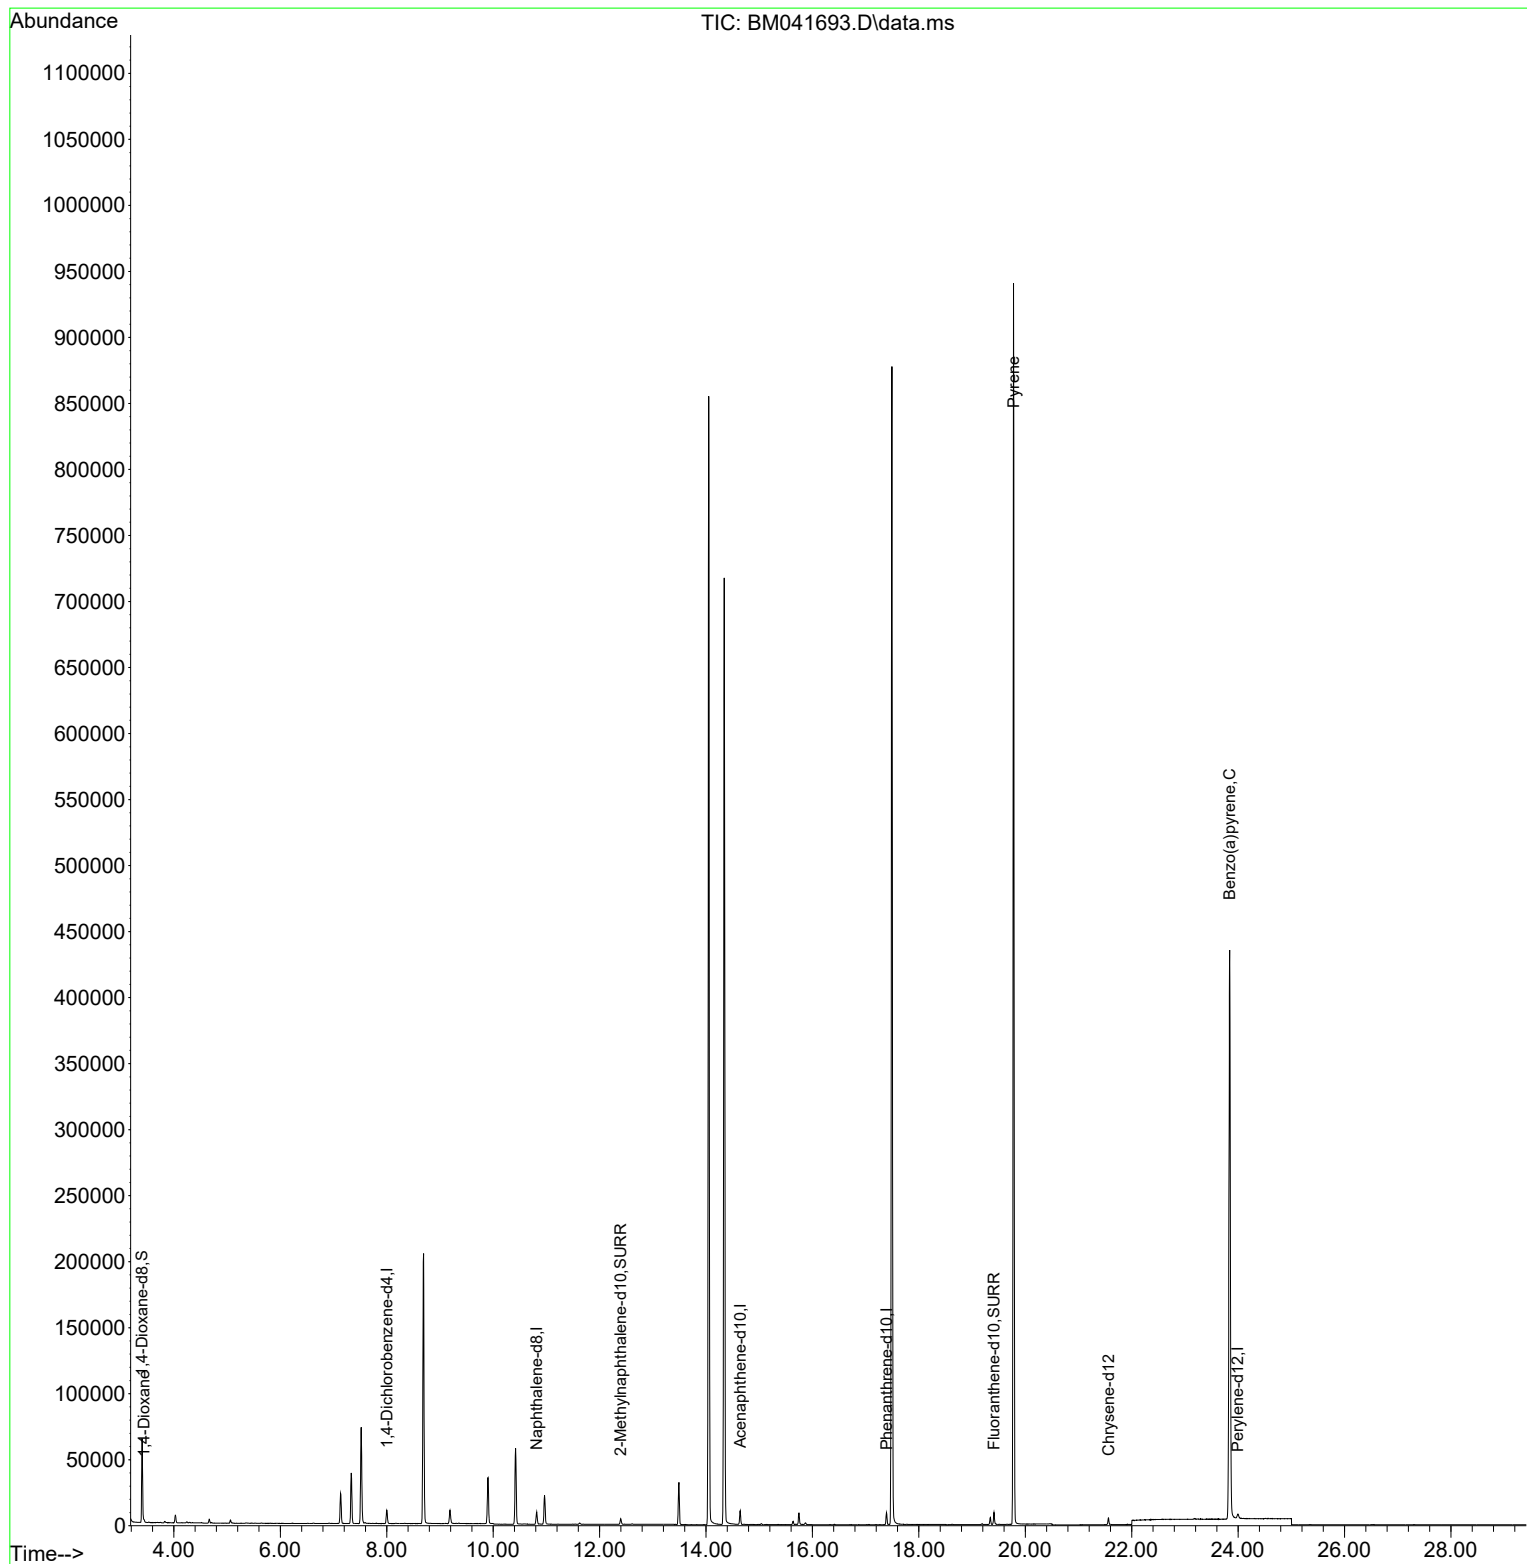


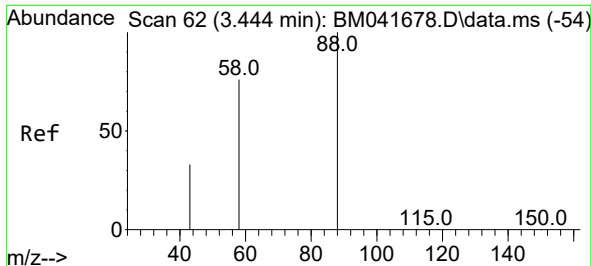

#2
1,4-Dioxane
Concen: 0.105 ng/ul
RT: 3.440 min Scan# 61
Delta R.T. -0.004 min
Lab File: BM041693.D
Acq: 07 Sep 2023 13:52




Instrument :
BNA_M
ClientSampleId :
BH9G3


Tgt Ion: 88 Resp: 812
Ion Ratio Lower Upper
88 100
43 84.1 33.8 50.6#
58 58.0 54.2 81.2

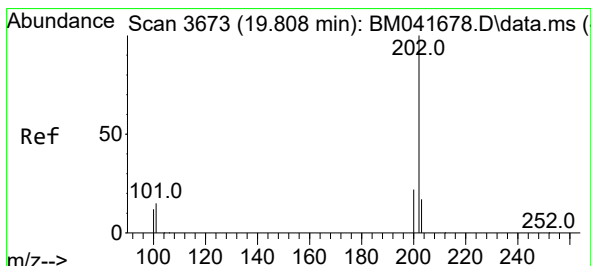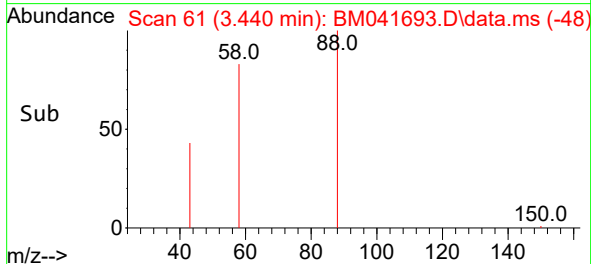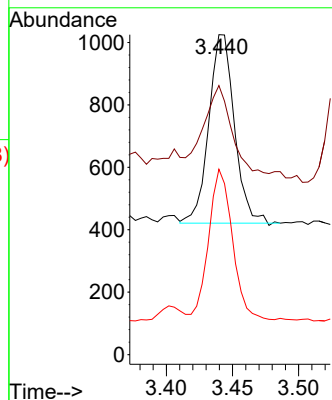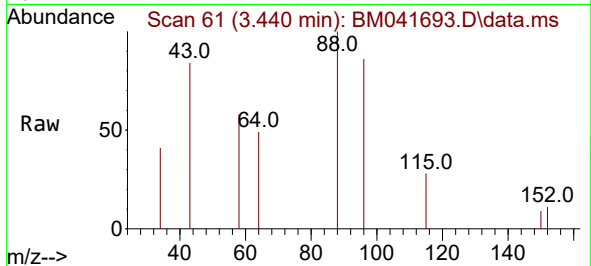

#20
Pyrene
Concen: 0.054 ng/ul
RT: 19.780 min Scan# 3667
Delta R.T. -0.037 min
Lab File: BM041693.D
Acq: 07 Sep 2023 13:52


Tgt Ion: 202 Resp: 2329
Ion Ratio Lower Upper
202 100
101 166.6 11.8 17.8#
100 1243.2 9.8 14.6#

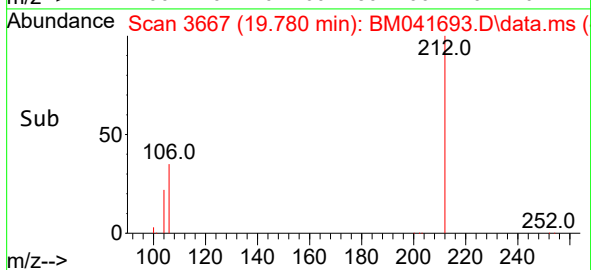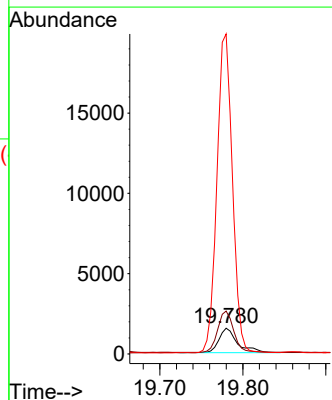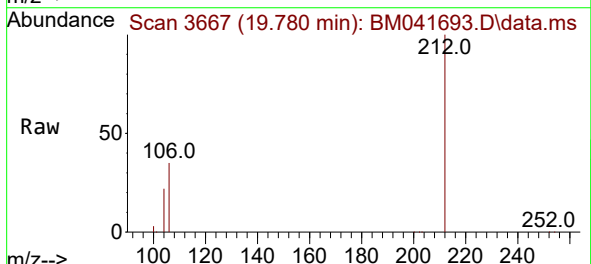

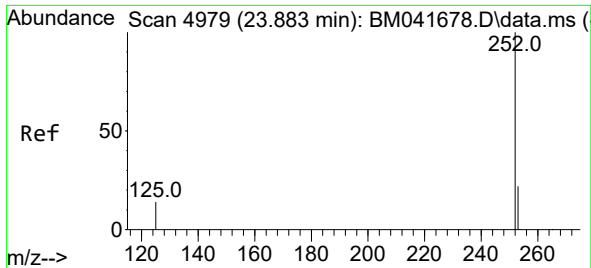

#26
Benzo(a)pyrene
Concen: 0.120 ng/ul
RT: 23.839 min Scan# 4964
Delta R.T. -0.058 min
Lab File: BM041693.D
Acq: 07 Sep 2023 13:52

Instrument :
BNA_M
ClientSampleId :
BH9G3

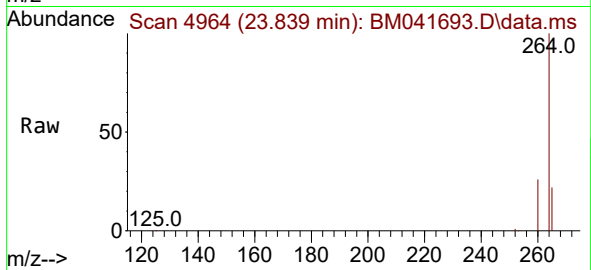

Tgt Ion:252 Resp: 4139
Ion Ratio Lower Upper
252 100
253 49.0 22.4 33.6#
125 53.9 21.0 31.4#

