

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041695.D
 Acq On : 07 Sep 2023 15:08
 Operator : MA/JU
 Sample : 04166-05
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJJ4

Quant Time: Sep 08 02:53:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 06 02:20:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	5612	0.400	ng/ul	0.00
4) Naphthalene-d8	10.818	136	13249	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.643	164	5774	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	10324	0.400	ng/ul	0.00
17) Chrysene-d12	21.568	240	3934	0.400	ng/ul	0.00
23) Perylene-d12	24.000	264	5066	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	35596	4.150	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	4935	0.289	ng/ul	-0.01
18) Fluoranthene-d10	19.413	212	6683	0.350	ng/ul	0.00
Target Compounds				Qvalue		
2) 1,4-Dioxane	3.440	88	1089	0.122	ng/ul#	77
20) Pyrene	19.785	202	2397	0.052	ng/ul#	1
26) Benzo(a)pyrene	23.845	252	3898	0.106	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041695.D
Acq On : 07 Sep 2023 15:08
Operator : MA/JU
Sample : 04166-05
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJJ4

Quant Time: Sep 08 02:53:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 06 02:20:07 2023
Response via : Initial Calibration




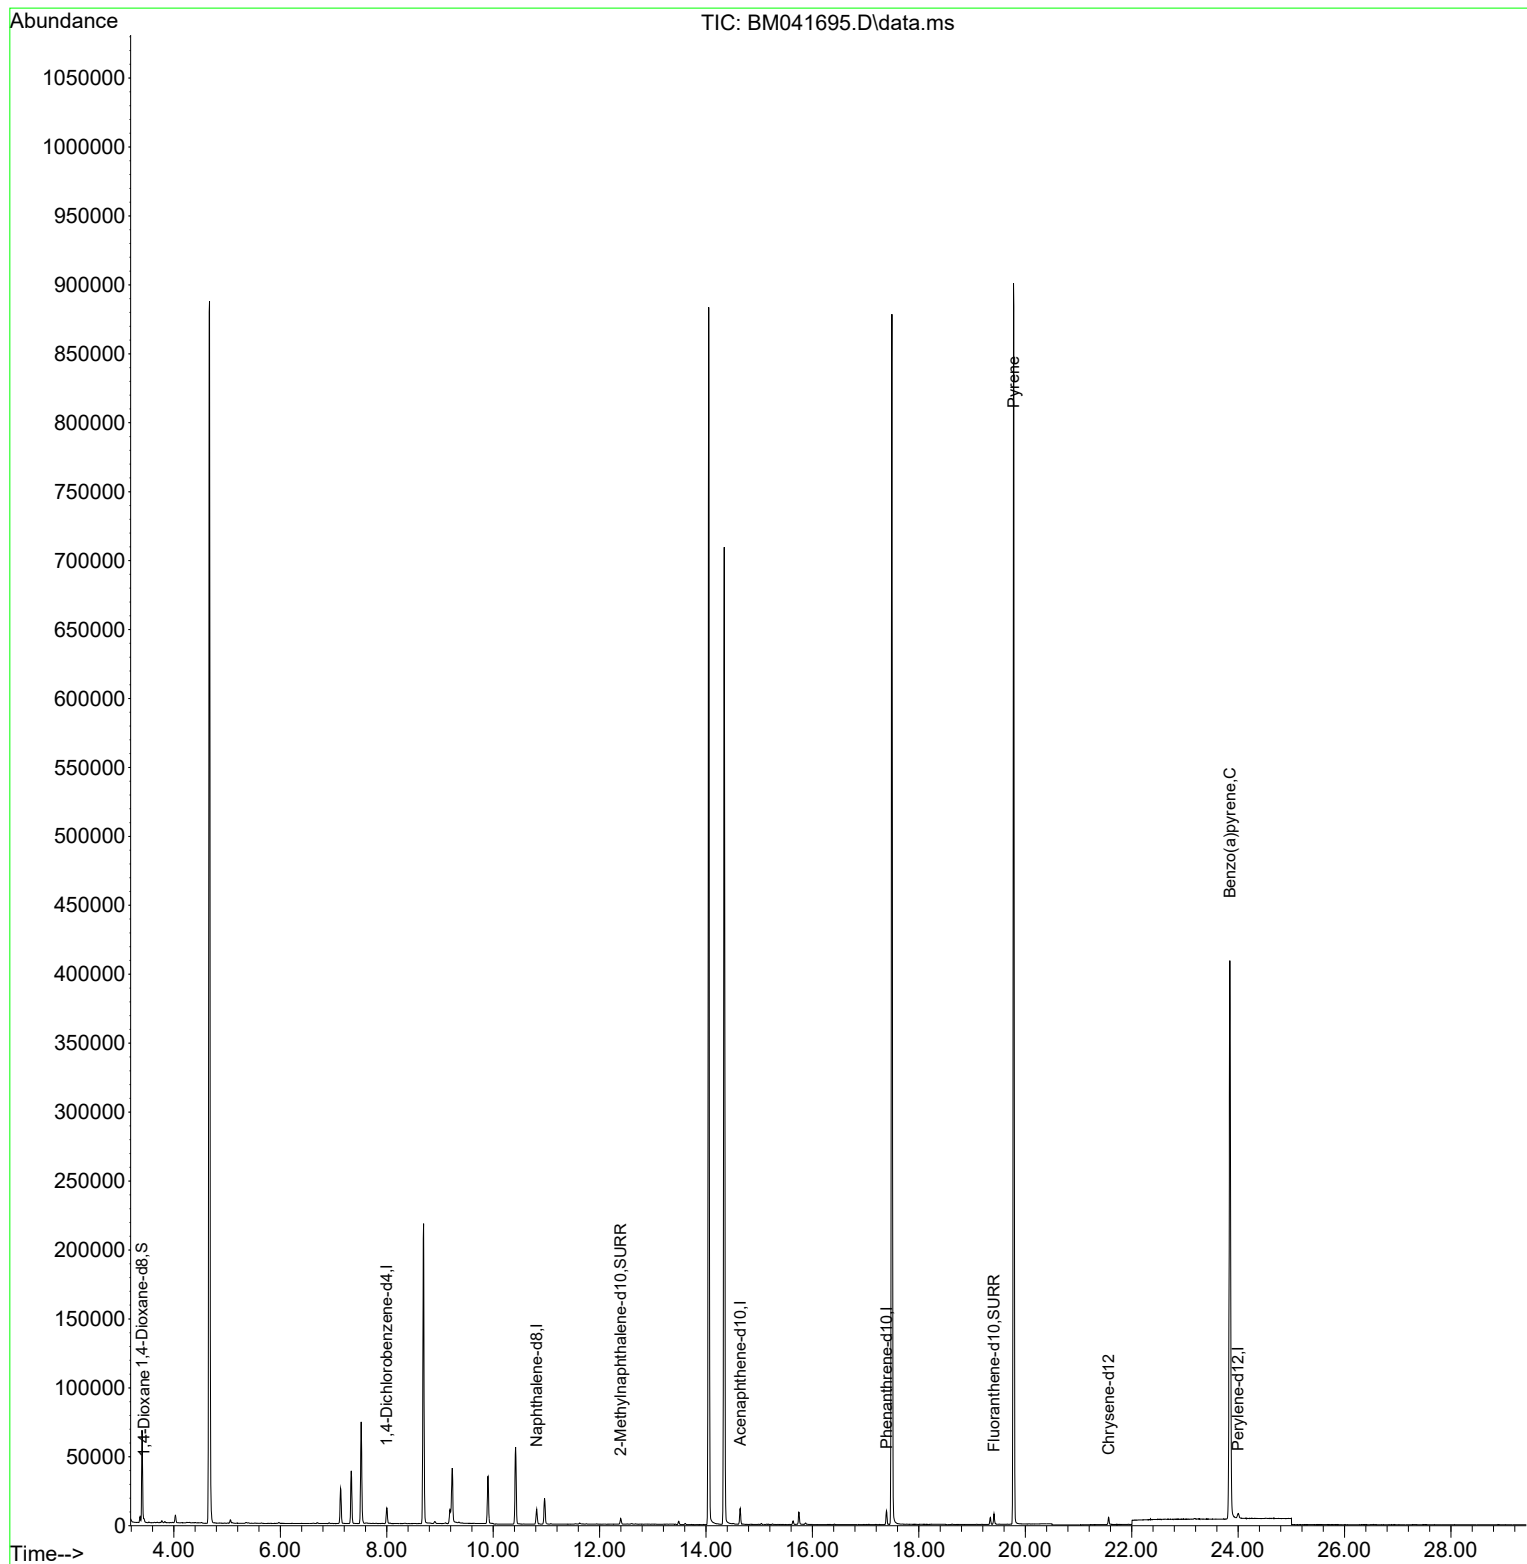


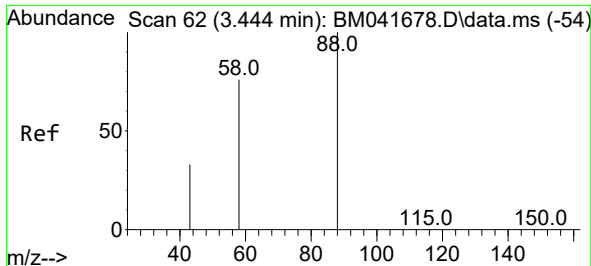

#2
1,4-Dioxane
Concen: 0.122 ng/ul
RT: 3.440 min Scan# 61
Delta R.T. -0.004 min
Lab File: BM041695.D
Acq: 07 Sep 2023 15:08




Instrument :
BNA_M
ClientSampleId :
BBJJ4


Tgt Ion: 88 Resp: 1089
Ion Ratio Lower Upper
88 100
43 74.1 33.8 50.6#
58 62.5 54.2 81.2

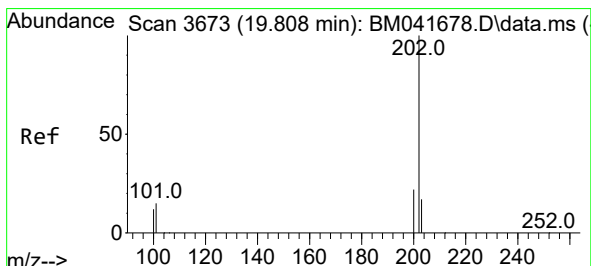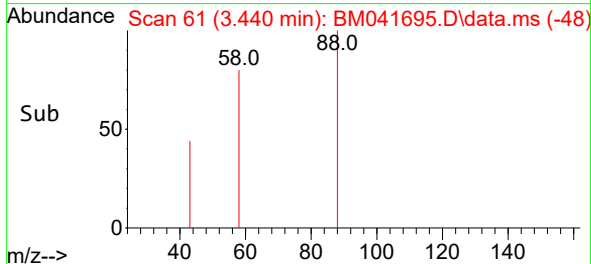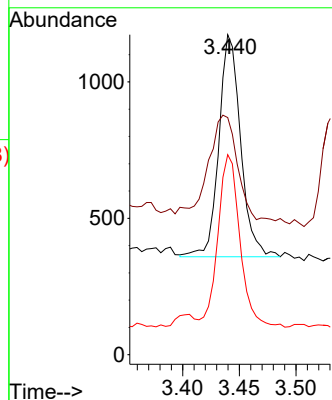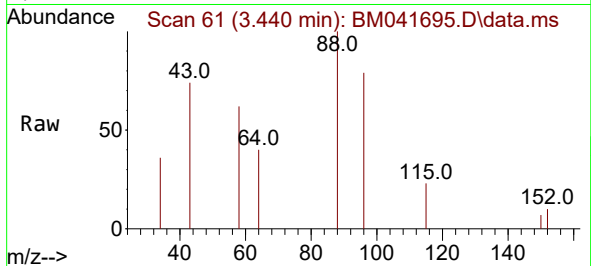

#20
Pyrene
Concen: 0.052 ng/ul
RT: 19.785 min Scan# 3668
Delta R.T. -0.032 min
Lab File: BM041695.D
Acq: 07 Sep 2023 15:08


Tgt Ion: 202 Resp: 2397
Ion Ratio Lower Upper
202 100
101 156.6 11.8 17.8#
100 1103.5 9.8 14.6#

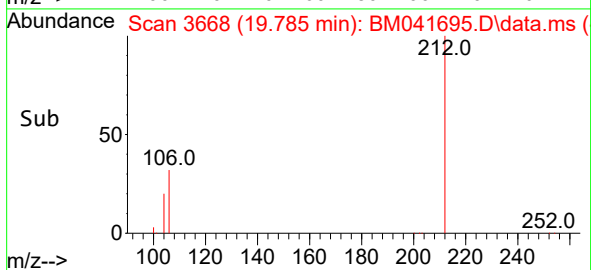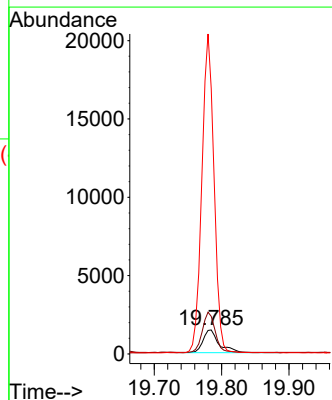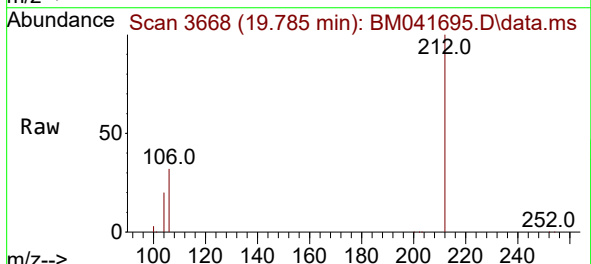

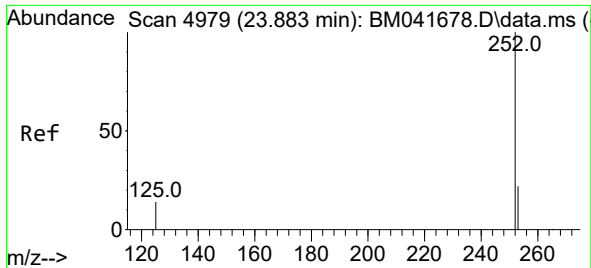

#26
Benzo(a)pyrene
Concen: 0.106 ng/ul
RT: 23.845 min Scan# 49
Delta R.T. -0.053 min
Lab File: BM041695.D
Acq: 07 Sep 2023 15:08

Instrument :
BNA_M
ClientSampleId :
BBJJ4

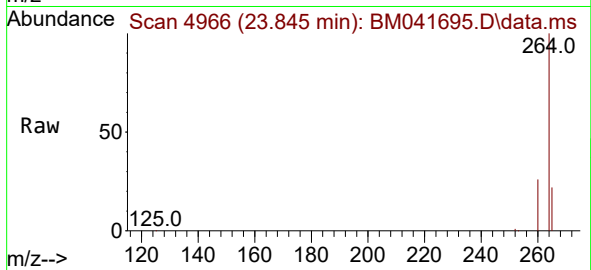

Tgt Ion:252 Resp: 3898
Ion Ratio Lower Upper
252 100
253 50.6 22.4 33.6#
125 54.6 21.0 31.4#

