

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041701.D
 Acq On : 07 Sep 2023 18:57
 Operator : MA/JU
 Sample : PB155166BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK166

Quant Time: Sep 08 02:54:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 06 02:20:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	5858	0.400	ng/ul	0.00
4) Naphthalene-d8	10.818	136	14217	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.643	164	6363	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	11539	0.400	ng/ul	0.00
17) Chrysene-d12	21.562	240	4633	0.400	ng/ul	0.00
23) Perylene-d12	23.991	264	6204	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	55152	6.160	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	5818	0.318	ng/ul	-0.01
18) Fluoranthene-d10	19.413	212	7338	0.327	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.780	202	2285	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.836	252	4629	0.103	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041701.D
Acq On : 07 Sep 2023 18:57
Operator : MA/JU
Sample : PB155166BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK166

Quant Time: Sep 08 02:54:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 06 02:20:07 2023
Response via : Initial Calibration

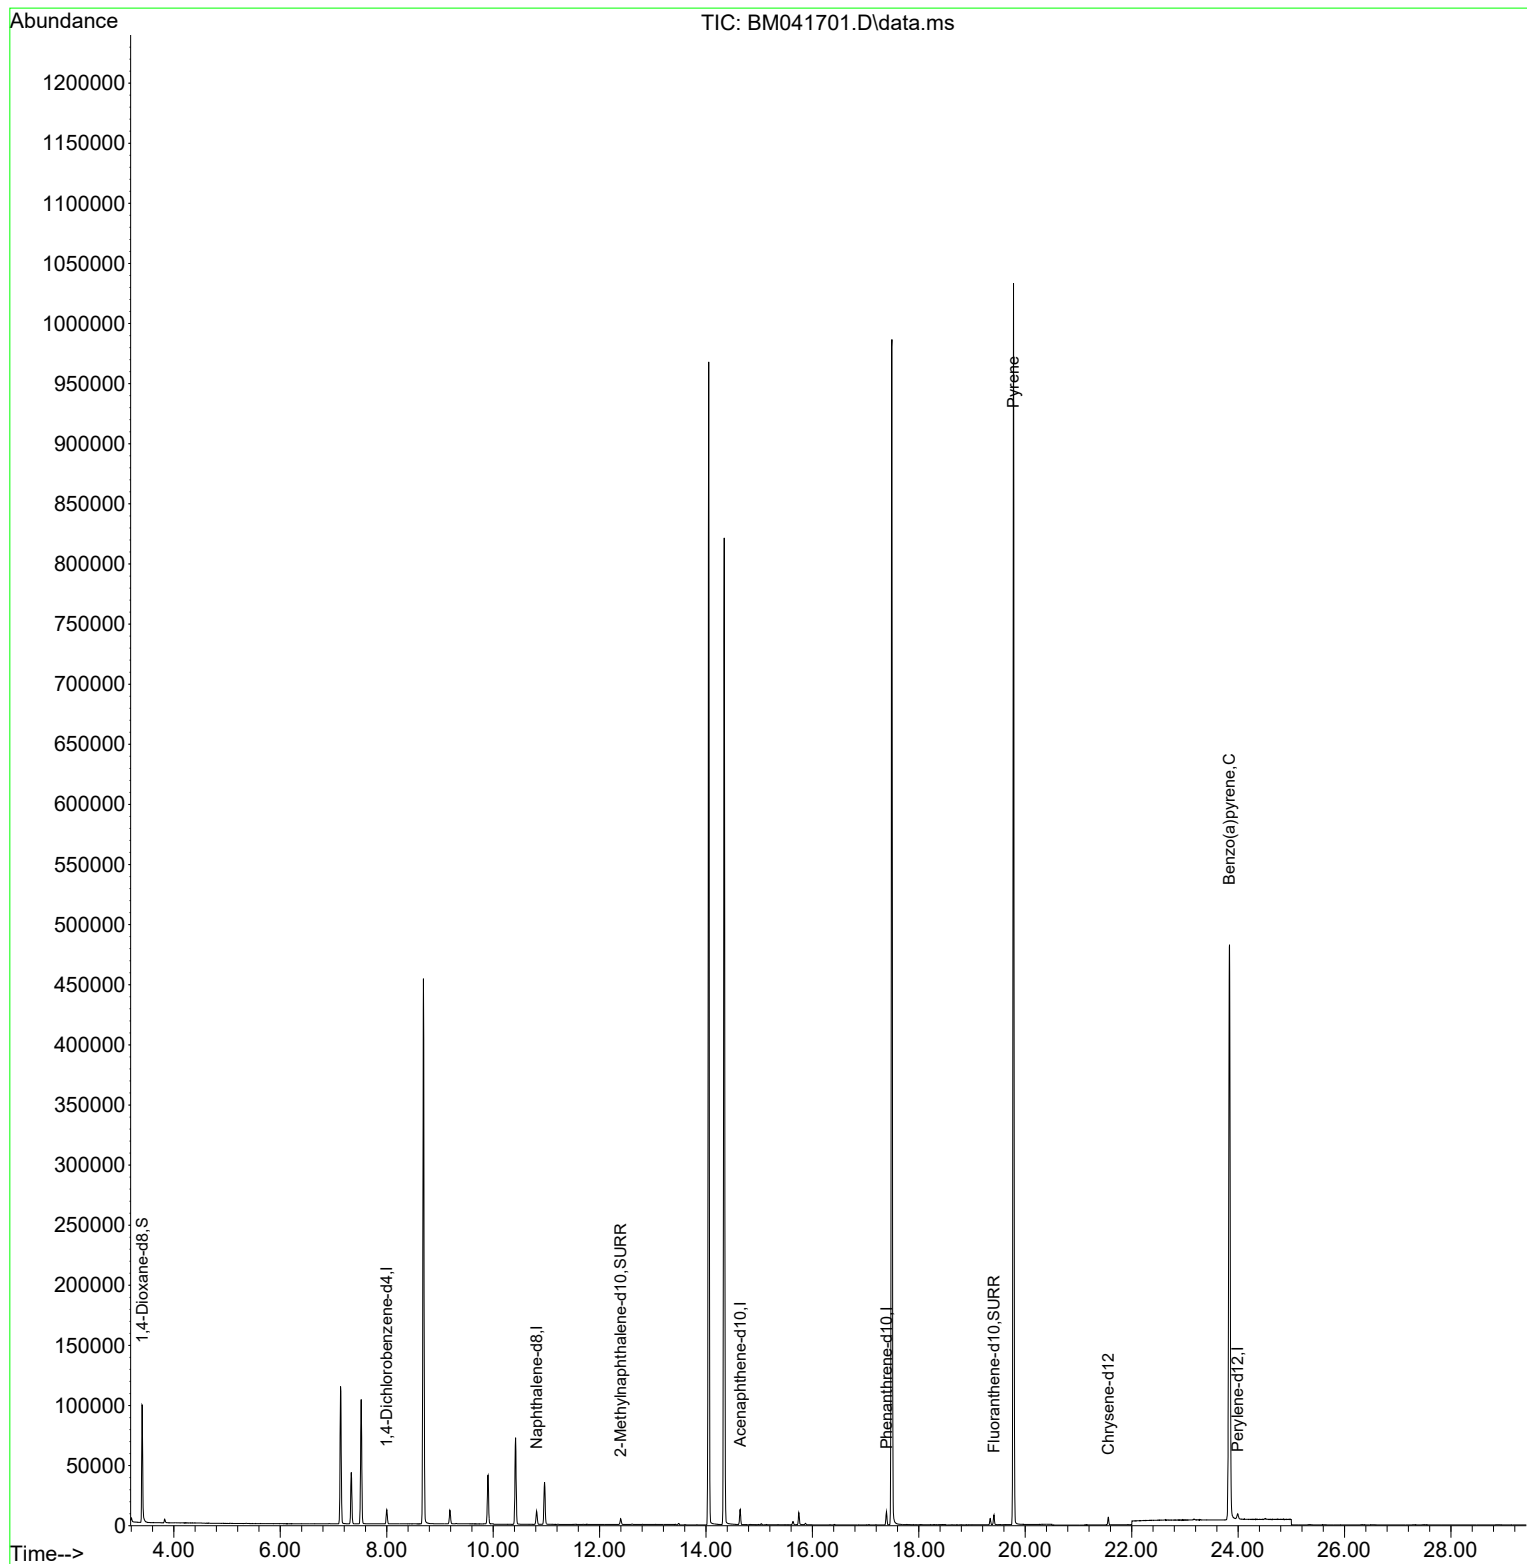

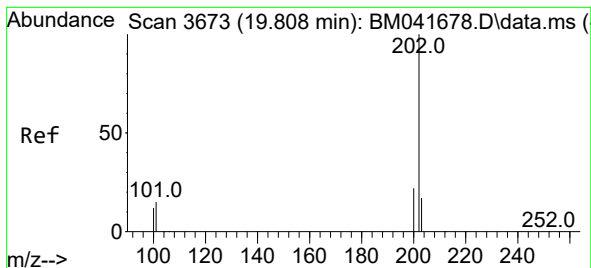

#20

Pyrene

Concen: 0.042 ng/ul

RT: 19.780 min Scan# 3

Delta R.T. -0.037 min

Lab File: BM041701.D

Acq: 07 Sep 2023 18:57

Instrument :

BNA_M

ClientSampleId :

SBLK166





Tgt Ion:202 Resp: 2285

Ion Ratio Lower Upper

202 100

101 171.1 11.8 17.8#

100 1244.8 9.8 14.6#

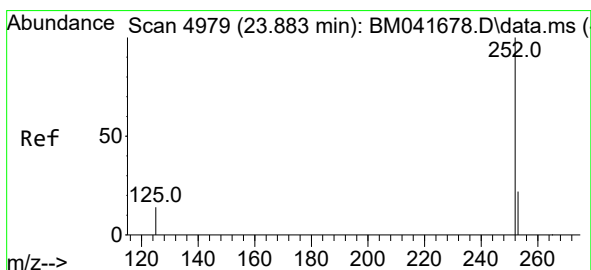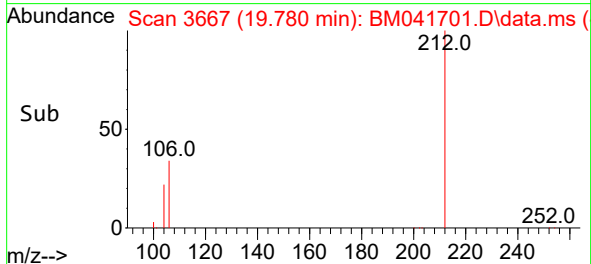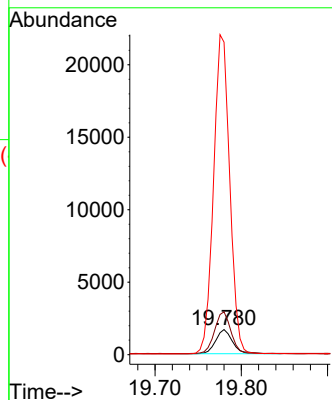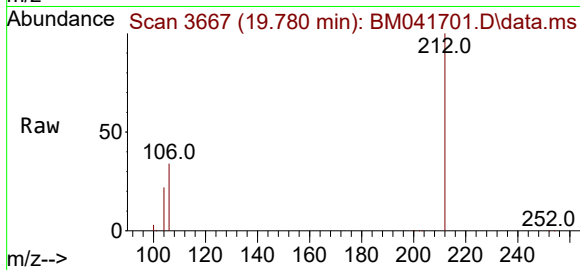

#26

Benzo(a)pyrene

Concen: 0.103 ng/ul

RT: 23.836 min Scan# 4963

Delta R.T. -0.061 min

Lab File: BM041701.D

Acq: 07 Sep 2023 18:57

Tgt Ion:252 Resp: 4629

Ion Ratio Lower Upper

252 100

253 46.7 22.4 33.6#

125 51.3 21.0 31.4#

