

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041725.D
 Acq On : 08 Sep 2023 10:28
 Operator : MA/JU
 Sample : 04153-06
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 08 22:54:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	8902	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	23605	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	10847	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.388	188	22370	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	7501	0.400	ng/ul	0.00
23) Perylene-d12	23.982	264	7960	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	1352388	99.406	ng/ul	-0.04
6) 2-Methylnaphthalene-d10	12.390	152	7493	0.247	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	11447	0.315	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.440	88	1890	0.134	ng/ul#	79
20) Pyrene	19.775	202	3820	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.830	252	5647	0.098	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041725.D
Acq On : 08 Sep 2023 10:28
Operator : MA/JU
Sample : 04153-06
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Sep 08 22:54:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

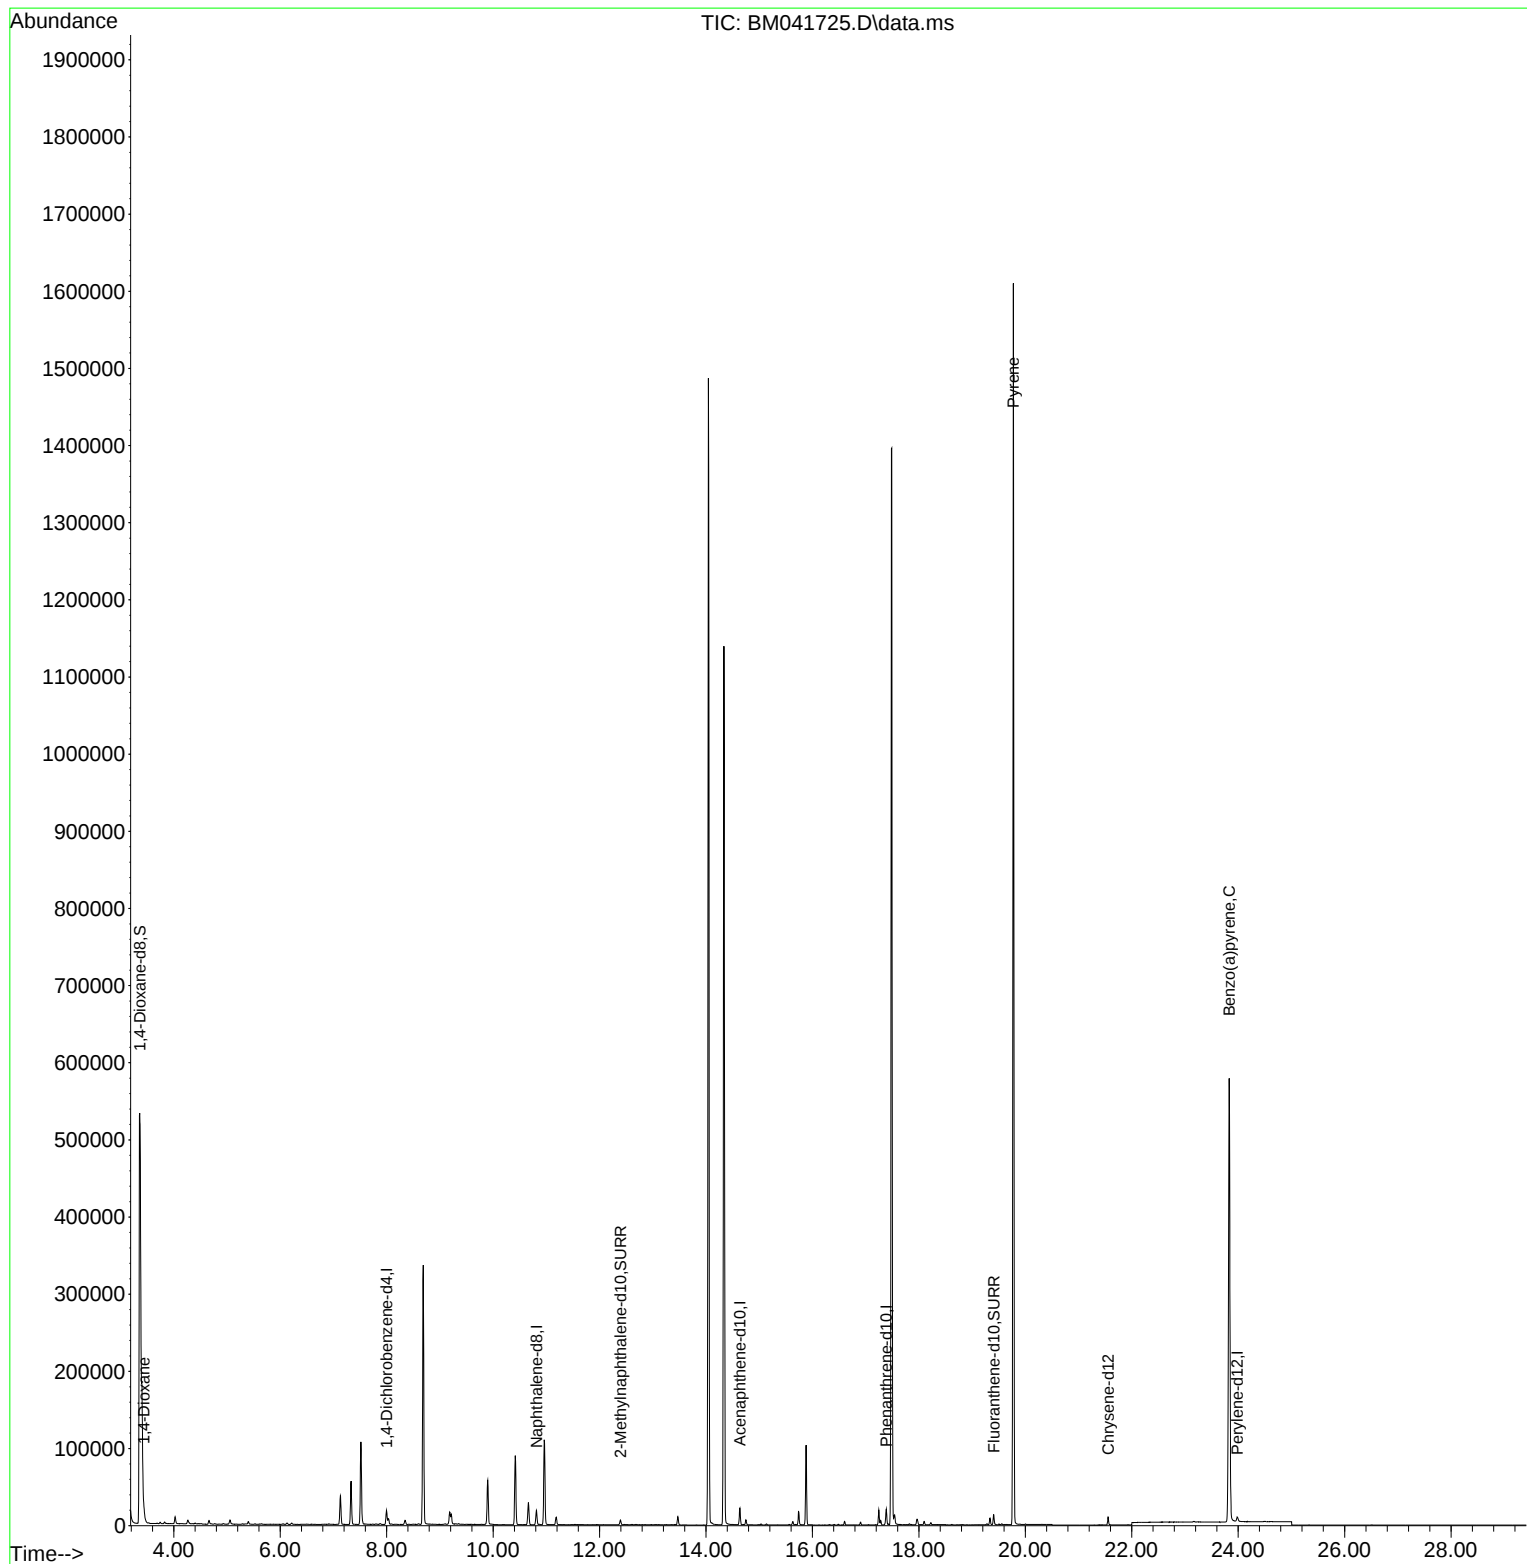



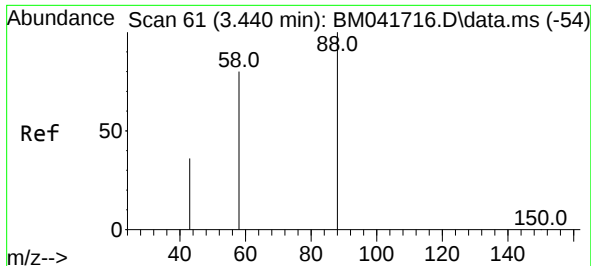


#2
1,4-Dioxane
Concen: 0.134 ng/ul
RT: 3.440 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM041725.D
Acq: 08 Sep 2023 10:28

Instrument :
BNA_M
ClientSampleId :



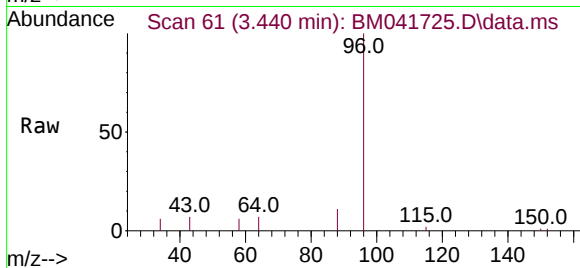



Tgt Ion: 88 Resp: 1890
Ion Ratio Lower Upper
88 100
43 64.2 33.8 50.6#
58 57.3 54.2 81.2

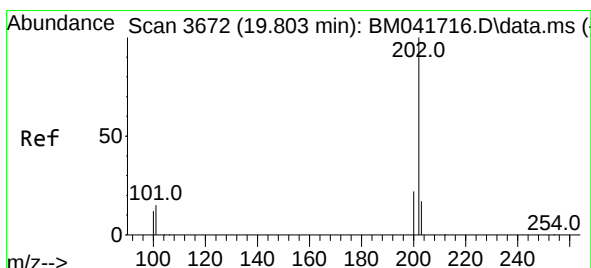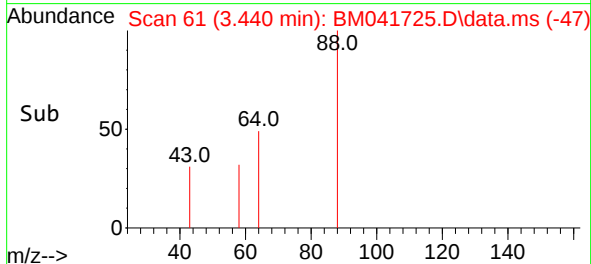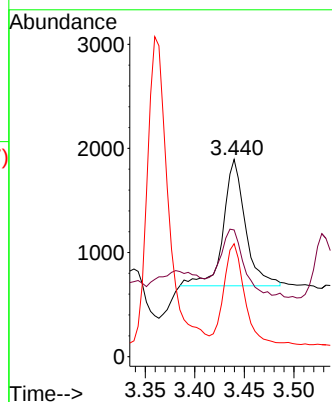

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.775 min Scan# 3666
Delta R.T. -0.028 min
Lab File: BM041725.D
Acq: 08 Sep 2023 10:28

Tgt Ion: 202 Resp: 3820
Ion Ratio Lower Upper
202 100
101 183.8 11.8 17.8#
100 1399.2 9.8 14.6#

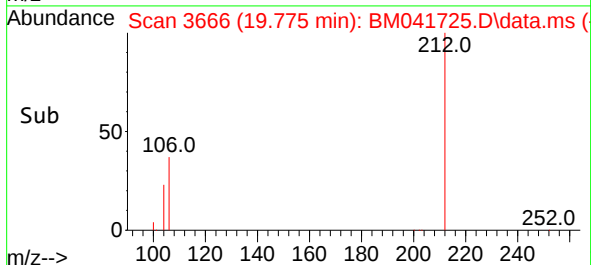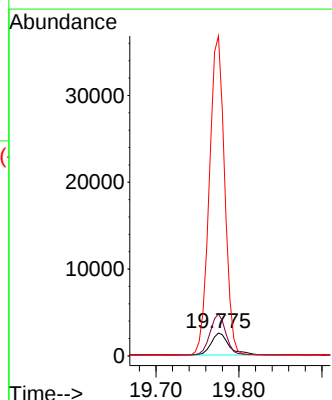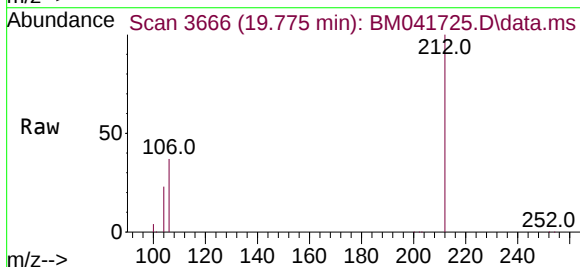

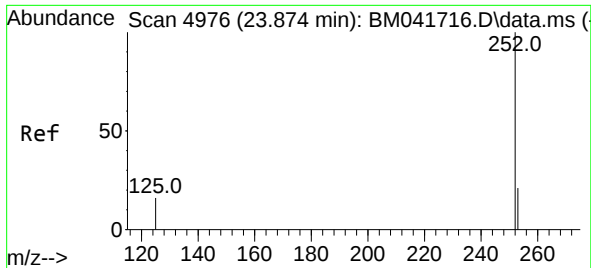

#26

Benzo(a)pyrene

Concen: 0.098 ng/ul

RT: 23.830 min Scan# 49

Delta R.T. -0.044 min


Lab File: BM041725.D

Acq: 08 Sep 2023 10:28

Instrument :

BNA_M

ClientSampleId :

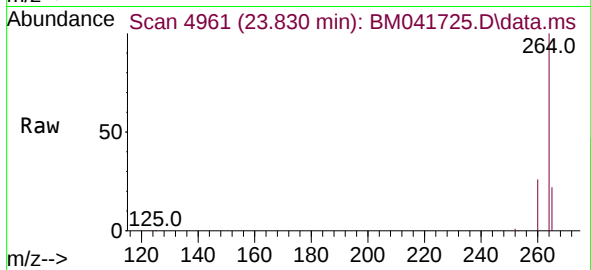

Tgt Ion:252 Resp: 5647

Ion Ratio Lower Upper

252 100

253 46.2 22.4 33.6#

125 46.5 21.0 31.4#

