

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041726.D
 Acq On : 08 Sep 2023 11:05
 Operator : MA/JU
 Sample : 04153-07
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 08 22:54:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	7865	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	20580	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	9750	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.388	188	17934	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	6336	0.400	ng/ul	0.00
23) Perylene-d12	23.983	264	6897	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	52262	4.348	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152	9687	0.366	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	13059	0.425	ng/ul	0.00
Target Compounds						
						Qvalue
20) Pyrene	19.775	202	4287	0.058	ng/ul#	1
26) Benzo(a)pyrene	23.830	252	6694	0.133	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041726.D
Acq On : 08 Sep 2023 11:05
Operator : MA/JU
Sample : 04153-07
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 08 22:54:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

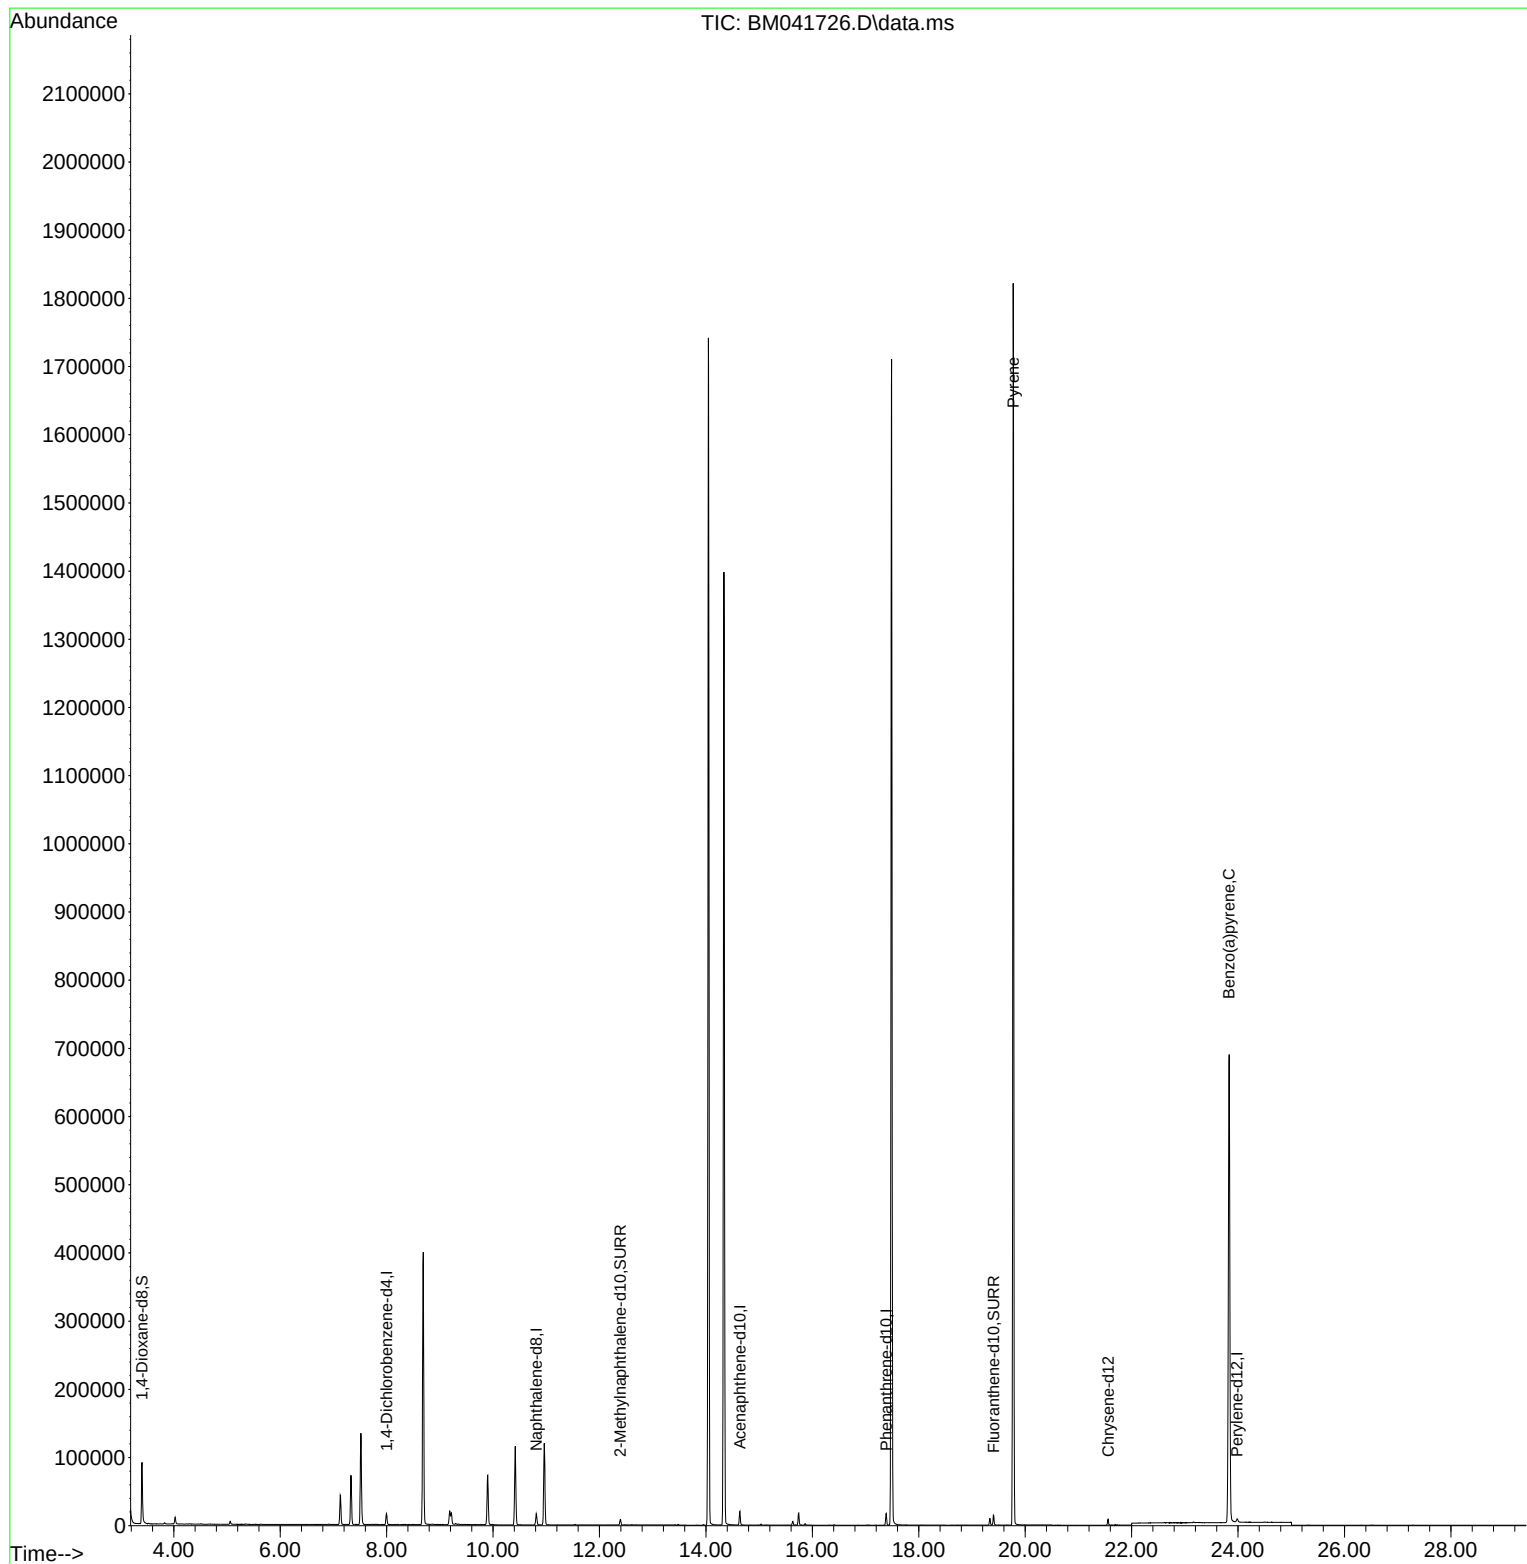

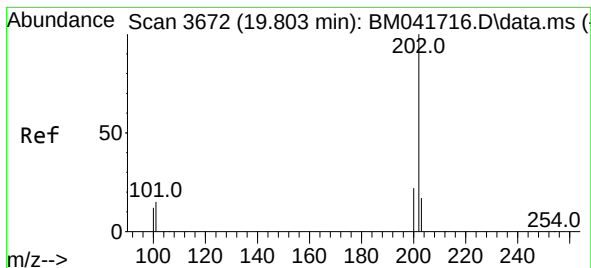

#20

Pyrene

Concen: 0.058 ng/ul

RT: 19.775 min Scan# 3666

Delta R.T. -0.028 min

Lab File: BM041726.D

Acq: 08 Sep 2023 11:05

Instrument :

BNA_M

ClientSampleId :





Tgt Ion:202 Resp: 4287

Ion Ratio Lower Upper

202 100

101 183.0 11.8 17.8#

100 1415.8 9.8 14.6#

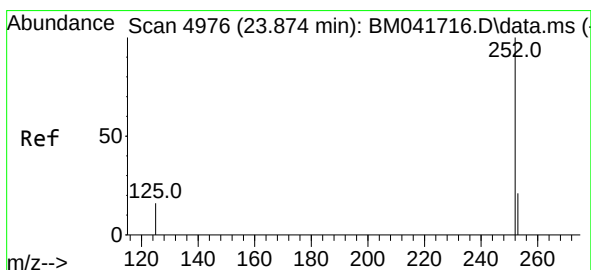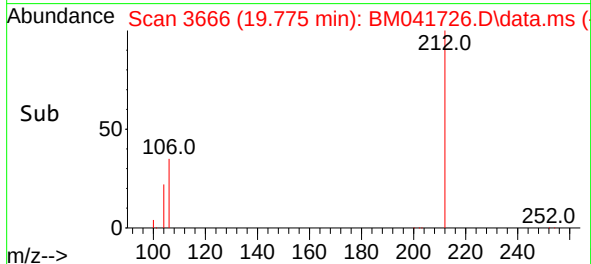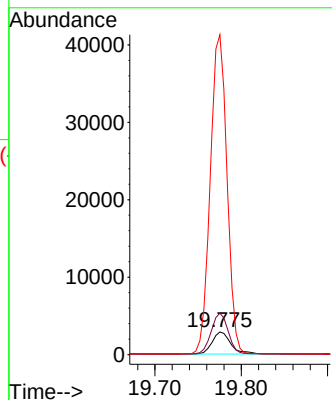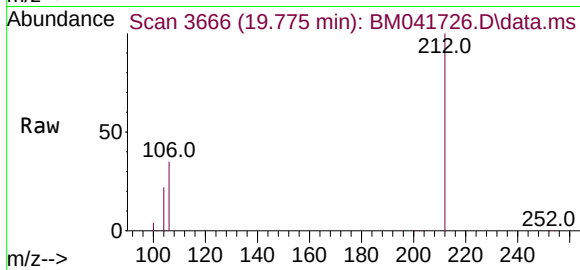

#26

Benzo(a)pyrene

Concen: 0.133 ng/ul

RT: 23.830 min Scan# 4961

Delta R.T. -0.044 min

Lab File: BM041726.D

Acq: 08 Sep 2023 11:05

Tgt Ion:252 Resp: 6694

Ion Ratio Lower Upper

252 100

253 40.9 22.4 33.6#

125 43.9 21.0 31.4#

