




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041721.D
Acq On : 08 Sep 2023 08:00
Operator : MA/JU
Sample : 04166-18
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJY0

Manual IntegrationsAPPROVED

Quant Time: Sep 08 08:30:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/09/2023
Supervised By :mohammad ahmed 09/09/2023

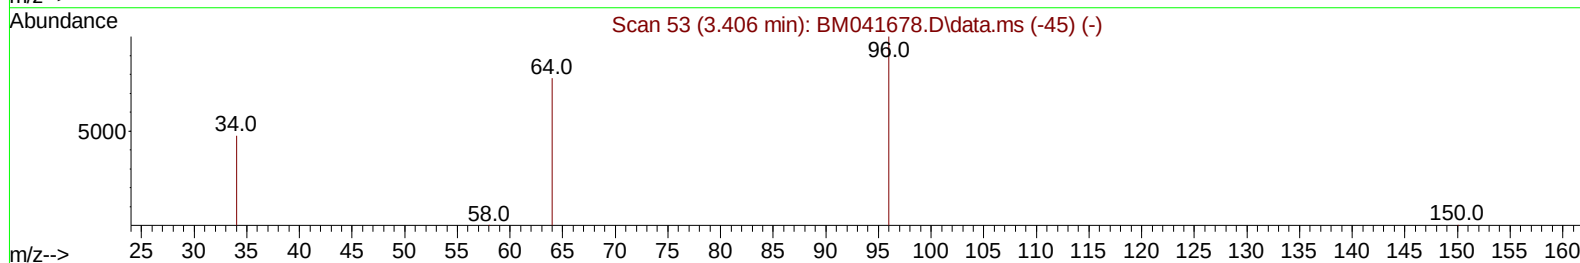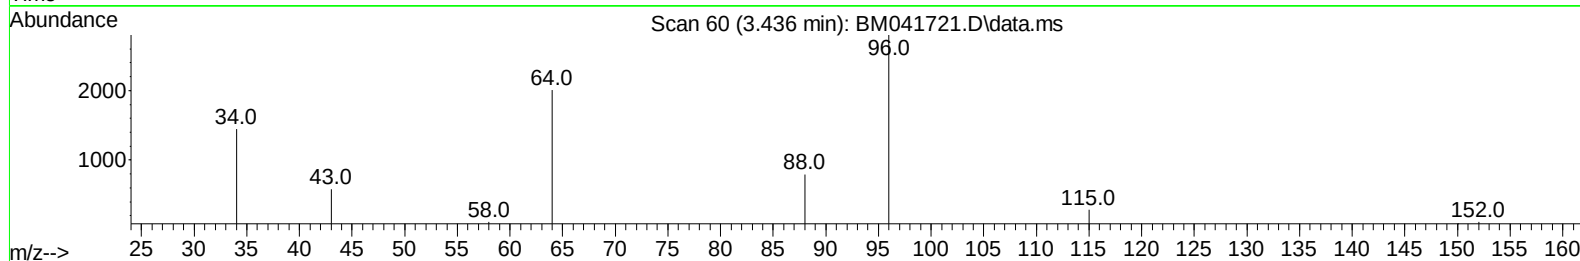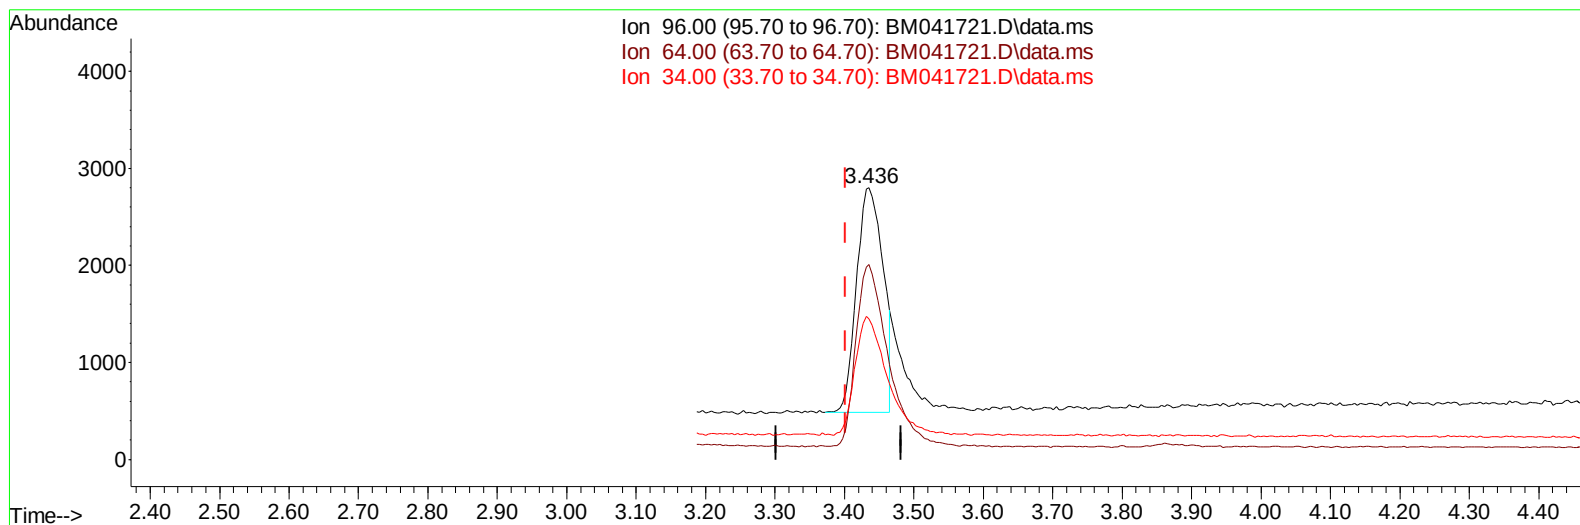

TIC: BM041721.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.436min (+ 0.034) 3.44 ng/u1

response 6137

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.30	71.88
34.00	53.80	51.80
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041721.D
Acq On : 08 Sep 2023 08:00
Operator : MA/JU
Sample : 04166-18
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJY0

Manual IntegrationsAPPROVED

Quant Time: Sep 08 08:30:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/09/2023
Supervised By :mohammad ahmed 09/09/2023

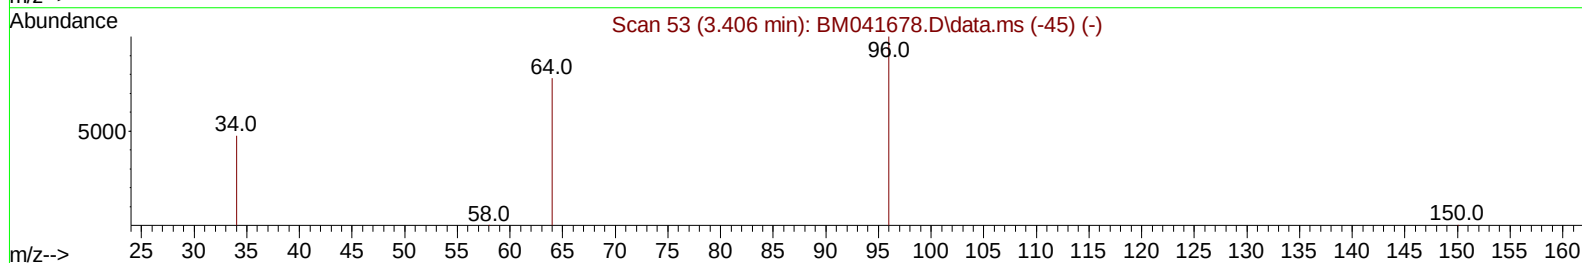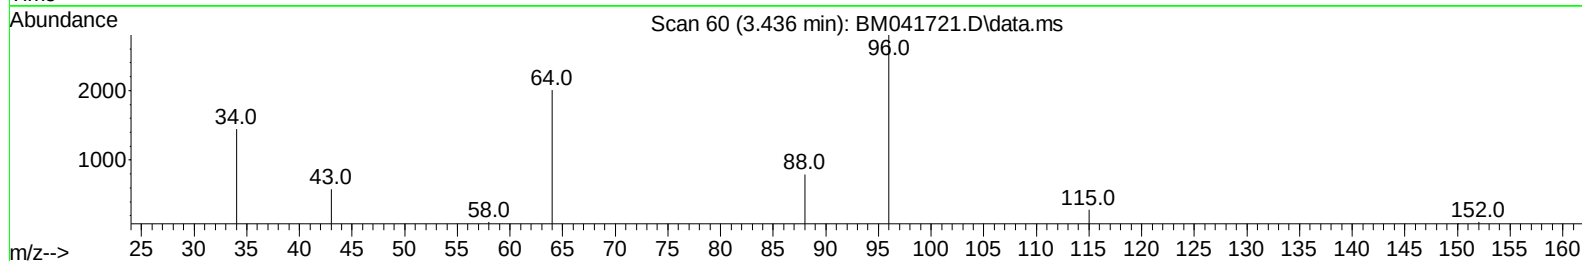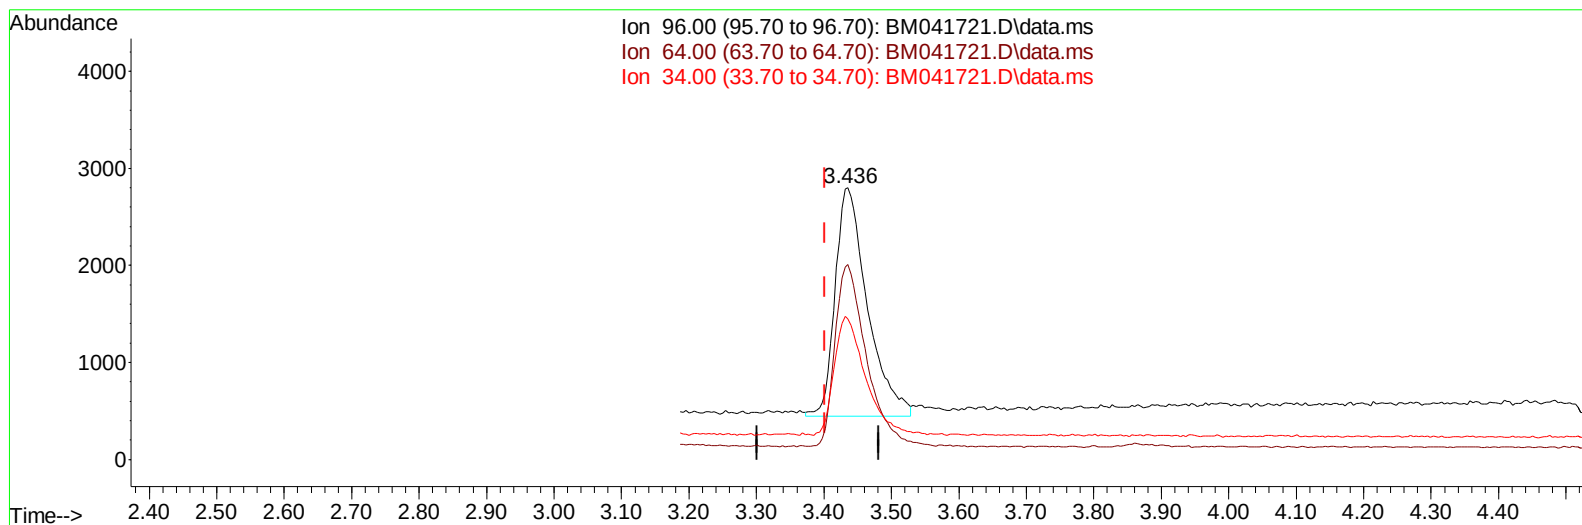

TIC: BM041721.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.436min (+ 0.034) 4.38 ng/ul m

response 7818

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.30	71.88
34.00	53.80	51.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041721.D
 Acq On : 08 Sep 2023 08:00
 Operator : MA/JU
 Sample : 04166-18
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJY0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/09/2023
 Supervised By :mohammad ahmed 09/09/2023

Quant Time: Sep 08 08:30:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.005	152		1167	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.812	136		2550	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.638	164		931	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.388	188		1467	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.556	240		466	0.400	ng/ul	# 0.00
23) Perylene-d12	23.983	264		559	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.436	96		7818m	4.384	ng/ul	0.03
6) 2-Methylnaphthalene-d10	12.396	152		1059	0.323	ng/ul	0.00
18) Fluoranthene-d10	19.408	212		912	0.404	ng/ul	0.00
Target Compounds						Qvalue	
19) Fluoranthene	19.436	202		186	0.034	ng/ul#	21

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041721.D
Acq On : 08 Sep 2023 08:00
Operator : MA/JU
Sample : 04166-18
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJY0

Manual IntegrationsAPPROVED

Quant Time: Sep 08 08:30:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/09/2023
Supervised By :mohammad ahmed 09/09/2023

