




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041725.D
Acq On : 08 Sep 2023 10:28
Operator : MA/JU
Sample : 04153-06
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH464

Manual IntegrationsAPPROVED

Quant Time: Sep 08 23:52:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/09/2023
Supervised By :mohammad ahmed 09/09/2023

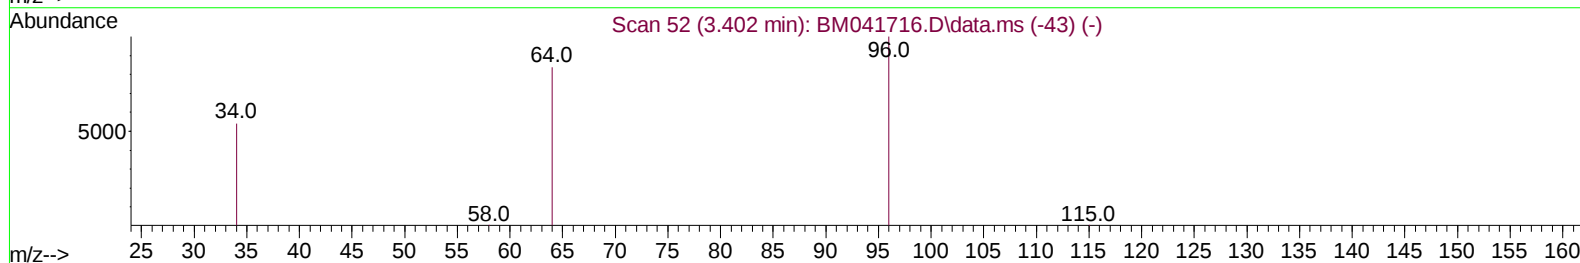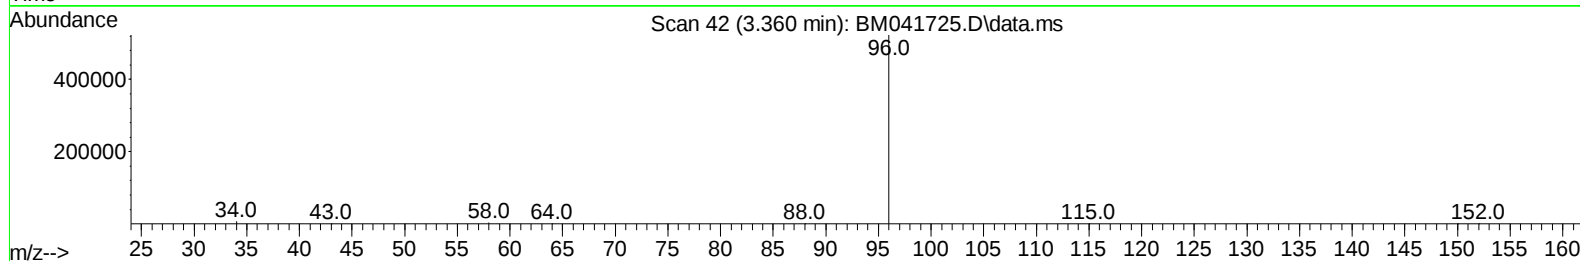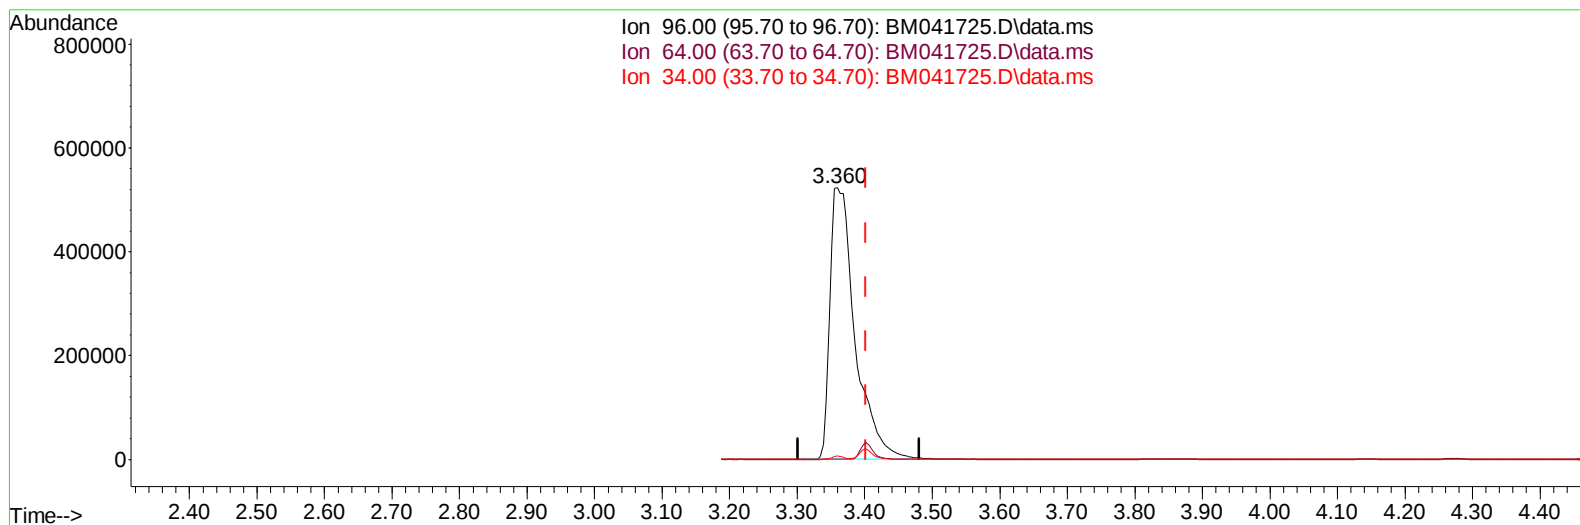

TIC: BM041725.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.360min (-0.042) 99.41 ng/u1

response 1352388

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.30	0.12#
34.00	53.80	1.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041725.D
 Acq On : 08 Sep 2023 10:28
 Operator : MA/JU
 Sample : 04153-06
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH464

Manual IntegrationsAPPROVED

Quant Time: Sep 08 23:52:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/09/2023
 Supervised By :mohammad ahmed 09/09/2023

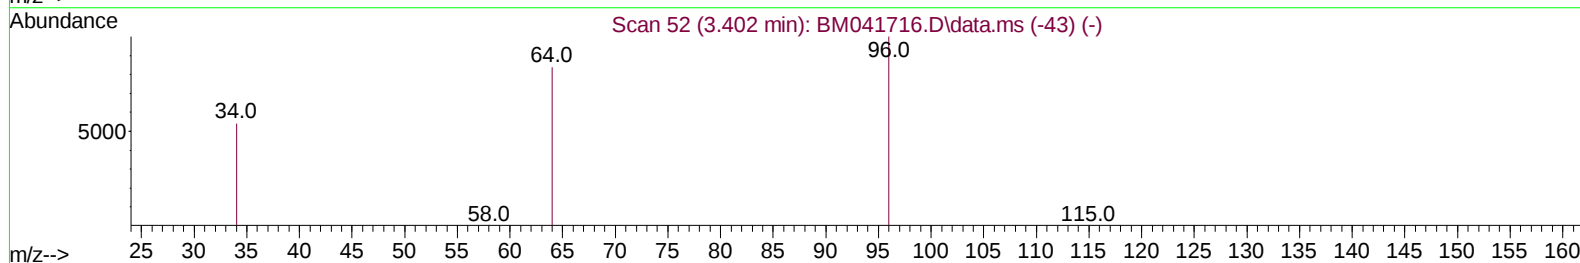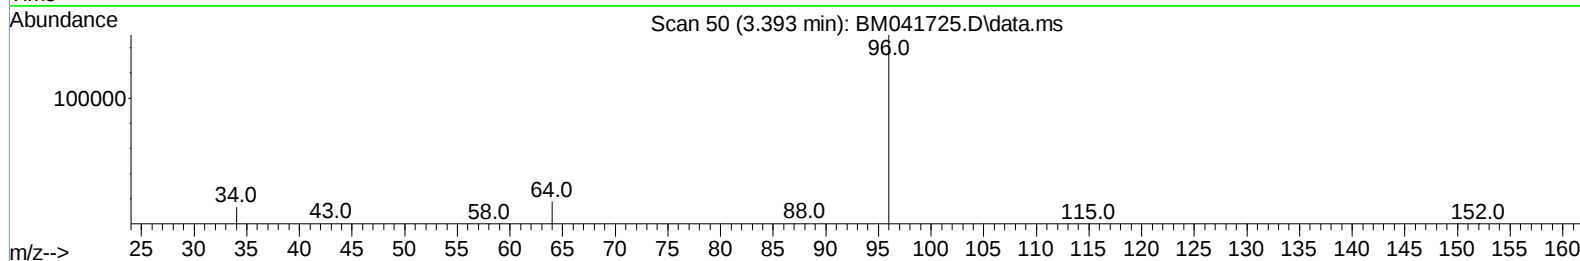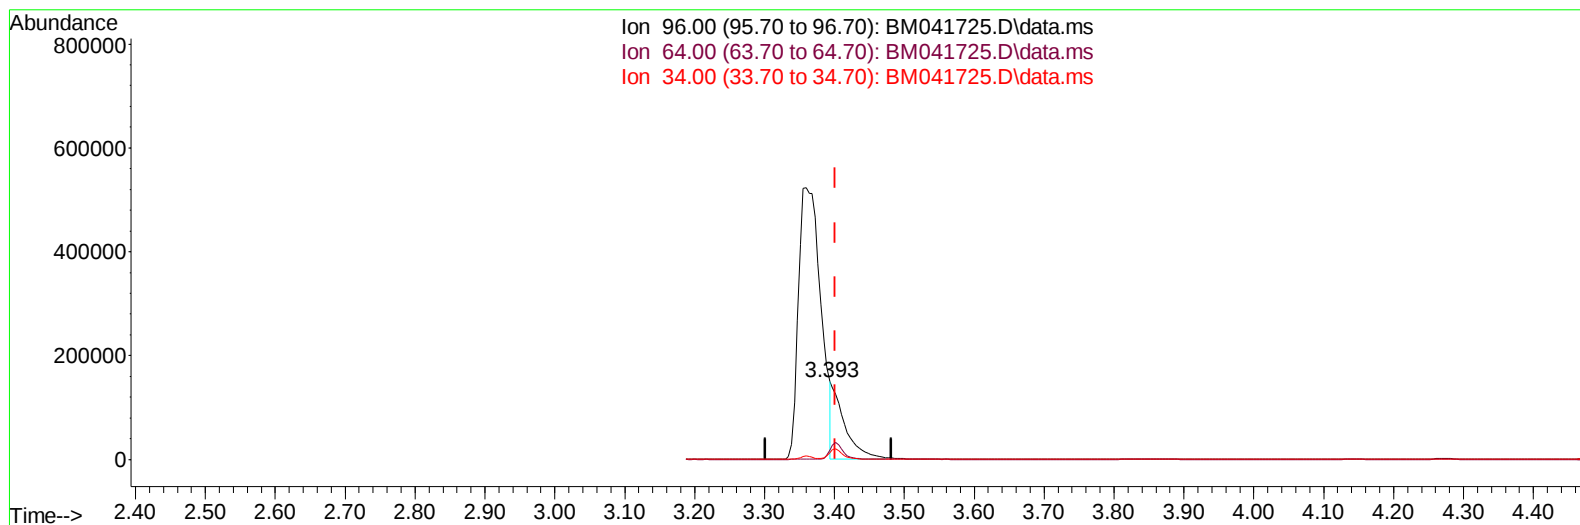

TIC: BM041725.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.393min (-0.008) 14.38 ng/ul m

response 195673

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.30	11.79#
34.00	53.80	9.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041725.D
 Acq On : 08 Sep 2023 10:28
 Operator : MA/JU
 Sample : 04153-06
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH464

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/09/2023
 Supervised By :mohammad ahmed 09/09/2023

Quant Time: Sep 08 23:52:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.996	152		8902	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136		23605	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164		10847	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.388	188		22370	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240		7501	0.400	ng/ul	0.00
23) Perylene-d12	23.982	264		7960	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.393	96		195673m	14.383	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152		7493	0.247	ng/ul	0.00
18) Fluoranthene-d10	19.408	212		11447	0.315	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.440	88		1890	0.134	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041725.D
Acq On : 08 Sep 2023 10:28
Operator : MA/JU
Sample : 04153-06
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH464

Manual IntegrationsAPPROVED

Quant Time: Sep 08 23:52:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/09/2023
Supervised By :mohammad ahmed 09/09/2023

