

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041677.D
 Acq On : 07 Sep 2023 02:41
 Operator : MA/JU
 Sample : 04209-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH468

Quant Time: Sep 07 03:22:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 06 02:20:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	7208	0.400	ng/ul	0.00
4) Naphthalene-d8	10.823	136	18491	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.643	164	9634	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.396	188	17865	0.400	ng/ul	0.00
17) Chrysene-d12	21.562	240	8841	0.400	ng/ul #	0.00
23) Perylene-d12	23.994	264	10794	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	47277	4.292	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.401	152	9918	0.417	ng/ul	0.00
18) Fluoranthene-d10	19.413	212	15742	0.367	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.444	88	385	0.034	ng/ul#	27

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041677.D
Acq On : 07 Sep 2023 02:41
Operator : MA/JU
Sample : 04209-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH468

Quant Time: Sep 07 03:22:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 06 02:20:07 2023
Response via : Initial Calibration

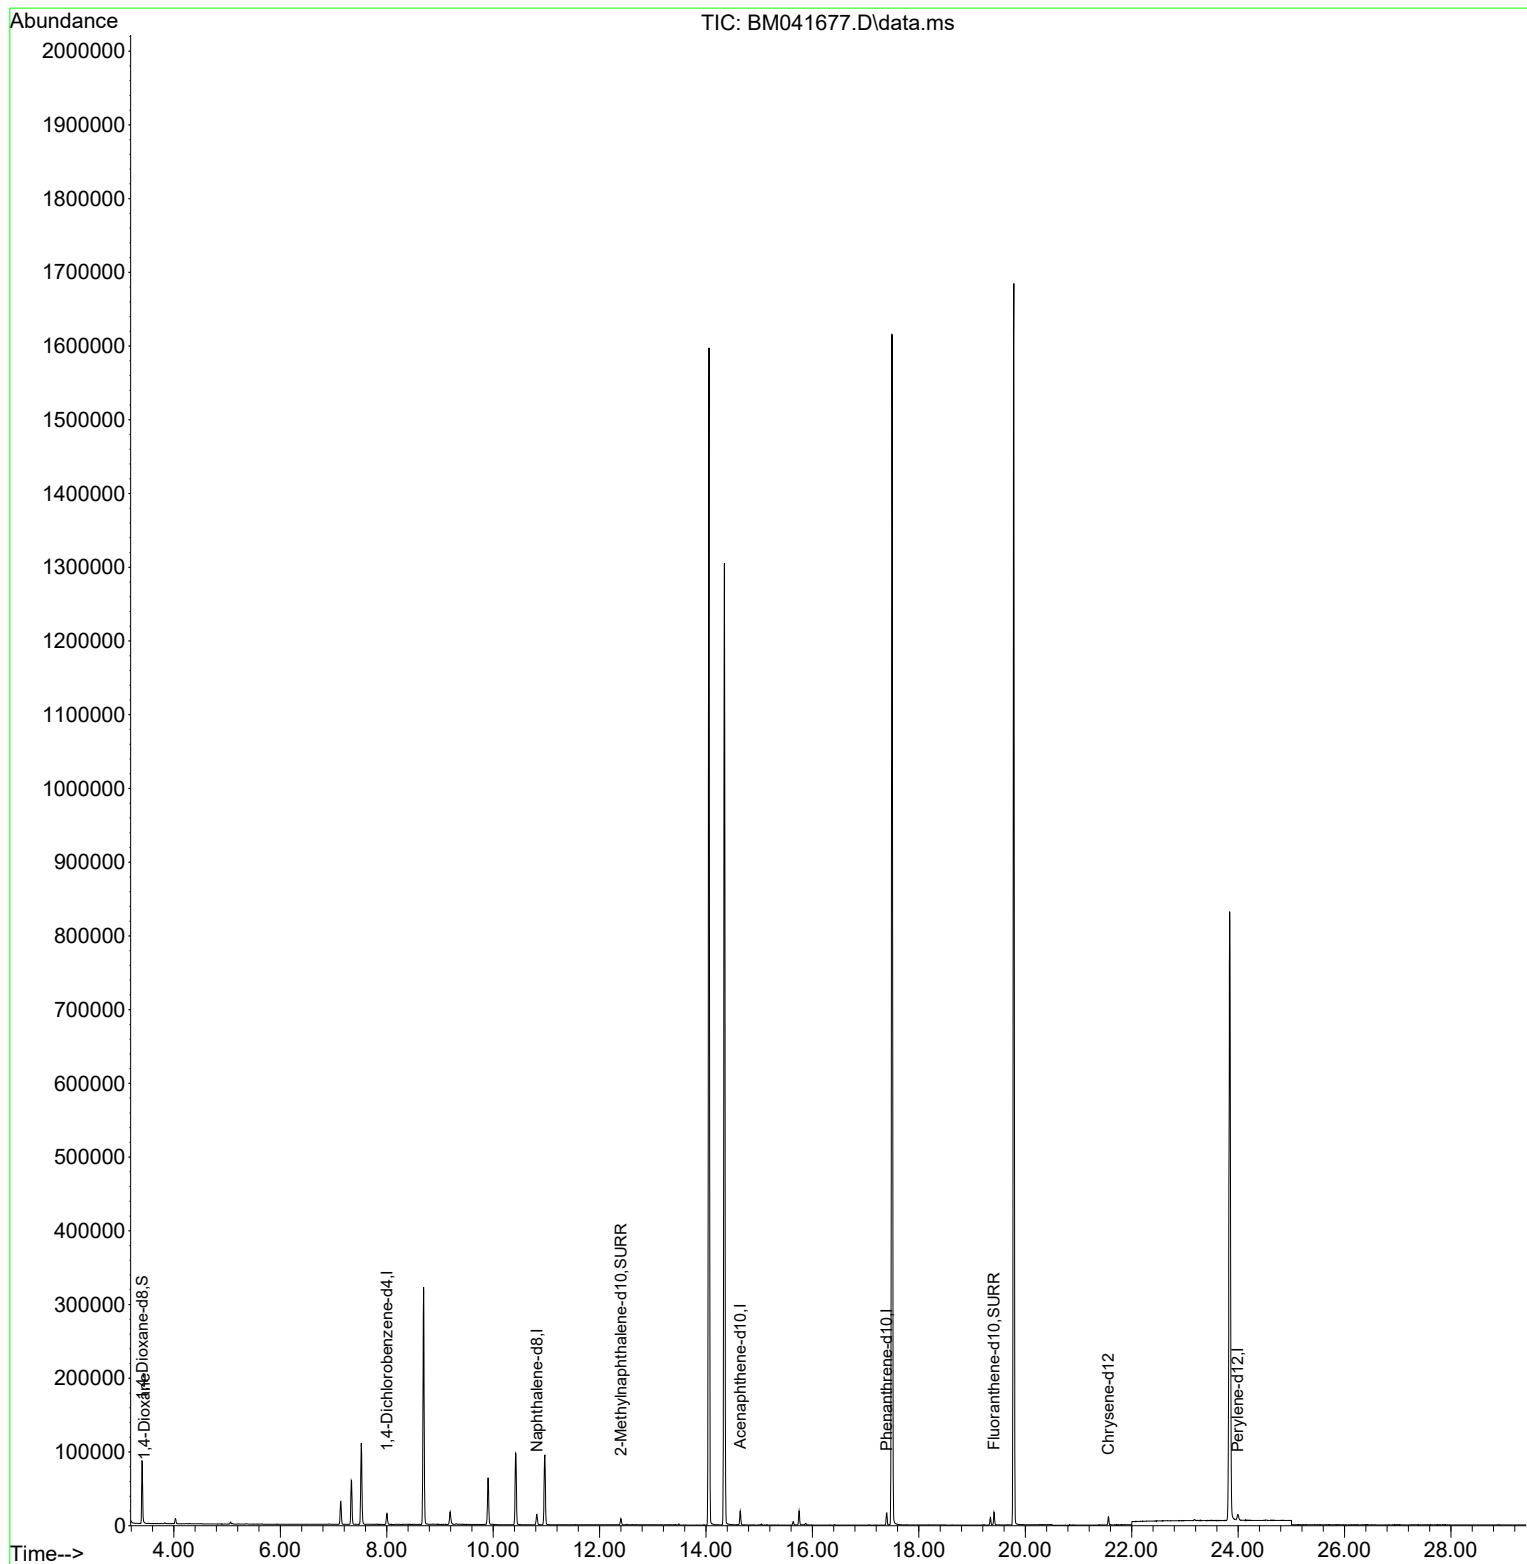

Abundance Scan 62 (3.444 min): BM041663.D\data.ms (-53)

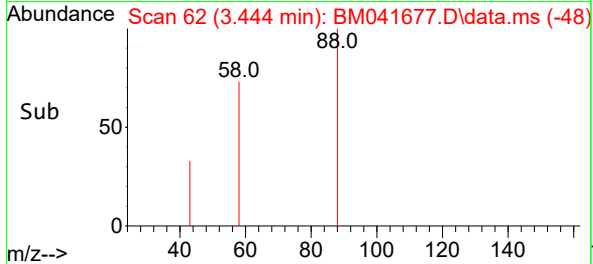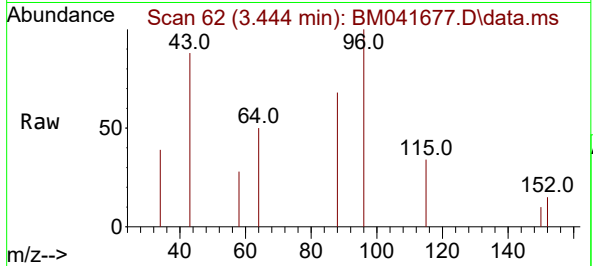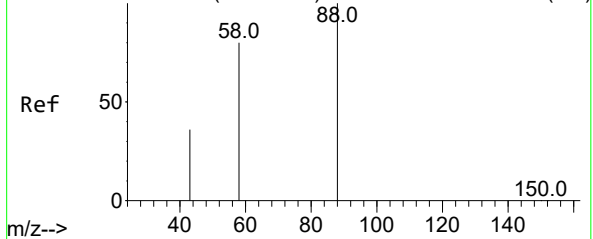

#2
1,4-Dioxane
Concen: 0.034 ng/ul
RT: 3.444 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM041677.D
Acq: 07 Sep 2023 02:41

Instrument :
BNA_M
ClientSampleId :
BH468

Tgt Ion:	88	Resp:	385
Ion	Ratio	Lower	Upper
88	100		
43	129.0	33.8	50.6#
58	41.2	54.2	81.2#

