

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041683.D
 Acq On : 07 Sep 2023 07:01
 Operator : MA/JU
 Sample : 04209-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH471

Quant Time: Sep 08 02:52:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 06 02:20:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	6732	0.400	ng/ul	0.00
4) Naphthalene-d8	10.817	136	15781	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.643	164	7763	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	15210	0.400	ng/ul	0.00
17) Chrysene-d12	21.562	240	7773	0.400	ng/ul	# 0.00
23) Perylene-d12	23.994	264	10264	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	40291	3.916	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.401	152	6615	0.326	ng/ul	0.00
18) Fluoranthene-d10	19.413	212	12526	0.332	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.444	88	1573	0.147	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041683.D
Acq On : 07 Sep 2023 07:01
Operator : MA/JU
Sample : 04209-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH471

Quant Time: Sep 08 02:52:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 06 02:20:07 2023
Response via : Initial Calibration

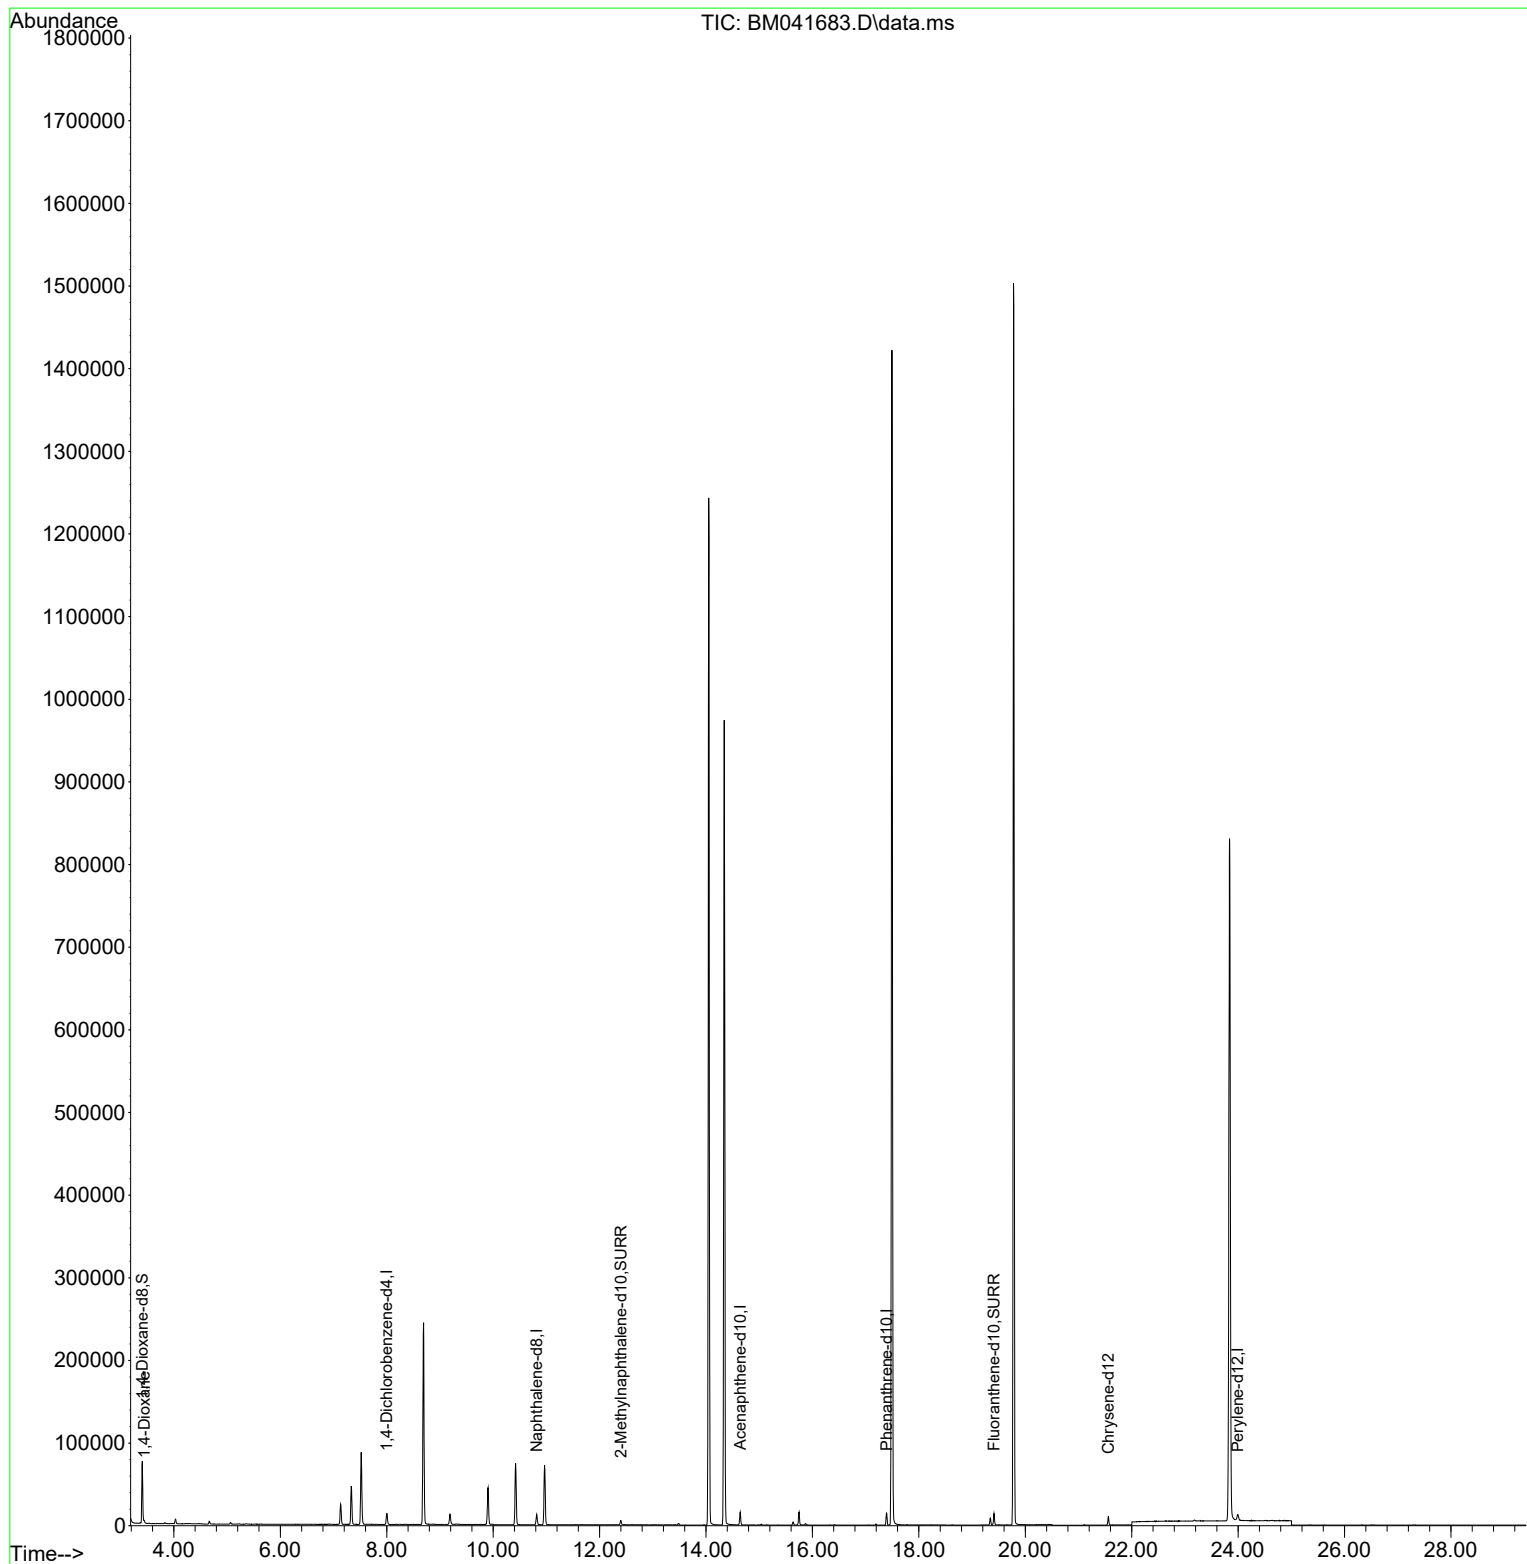

Abundance Scan 62 (3.444 min): BM041678.D\data.ms (-54)

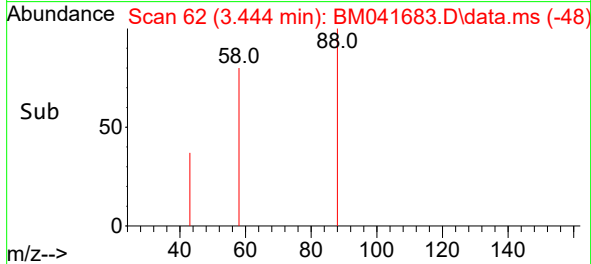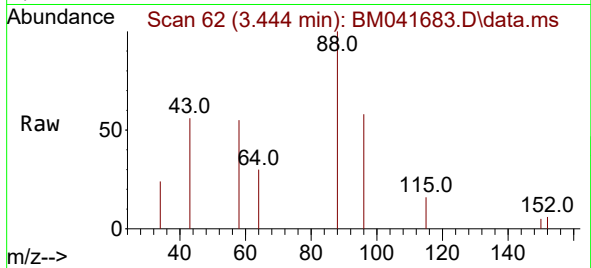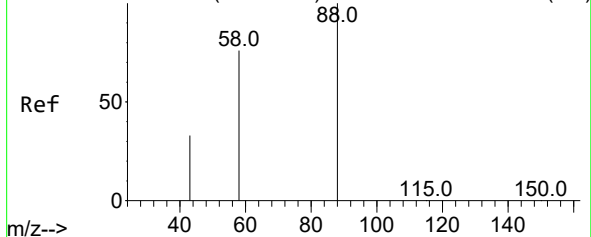

#2
1,4-Dioxane
Concen: 0.147 ng/ul
RT: 3.444 min Scan# 61
Delta R.T. -0.000 min
Lab File: BM041683.D
Acq: 07 Sep 2023 07:01

Instrument :
BNA_M
ClientSampleId :
BH471

Tgt Ion: 88 Resp: 1573
Ion Ratio Lower Upper
88 100
43 55.7 33.8 50.6#
58 55.2 54.2 81.2

