

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041692.D
 Acq On : 07 Sep 2023 13:14
 Operator : MA/JU
 Sample : 04148-19
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBKE8

Quant Time: Sep 08 02:53:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 06 02:20:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	5802	0.400	ng/ul	0.00
4) Naphthalene-d8	10.818	136	13932	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.643	164	6425	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	12267	0.400	ng/ul	0.00
17) Chrysene-d12	21.565	240	5268	0.400	ng/ul	0.00
23) Perylene-d12	24.000	264	6801	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	33498	3.778	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	5617	0.313	ng/ul	-0.01
18) Fluoranthene-d10	19.413	212	9059	0.355	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.444	88	1714	0.186	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041692.D
Acq On : 07 Sep 2023 13:14
Operator : MA/JU
Sample : 04148-19
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBKE8


Quant Time: Sep 08 02:53:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 06 02:20:07 2023
Response via : Initial Calibration

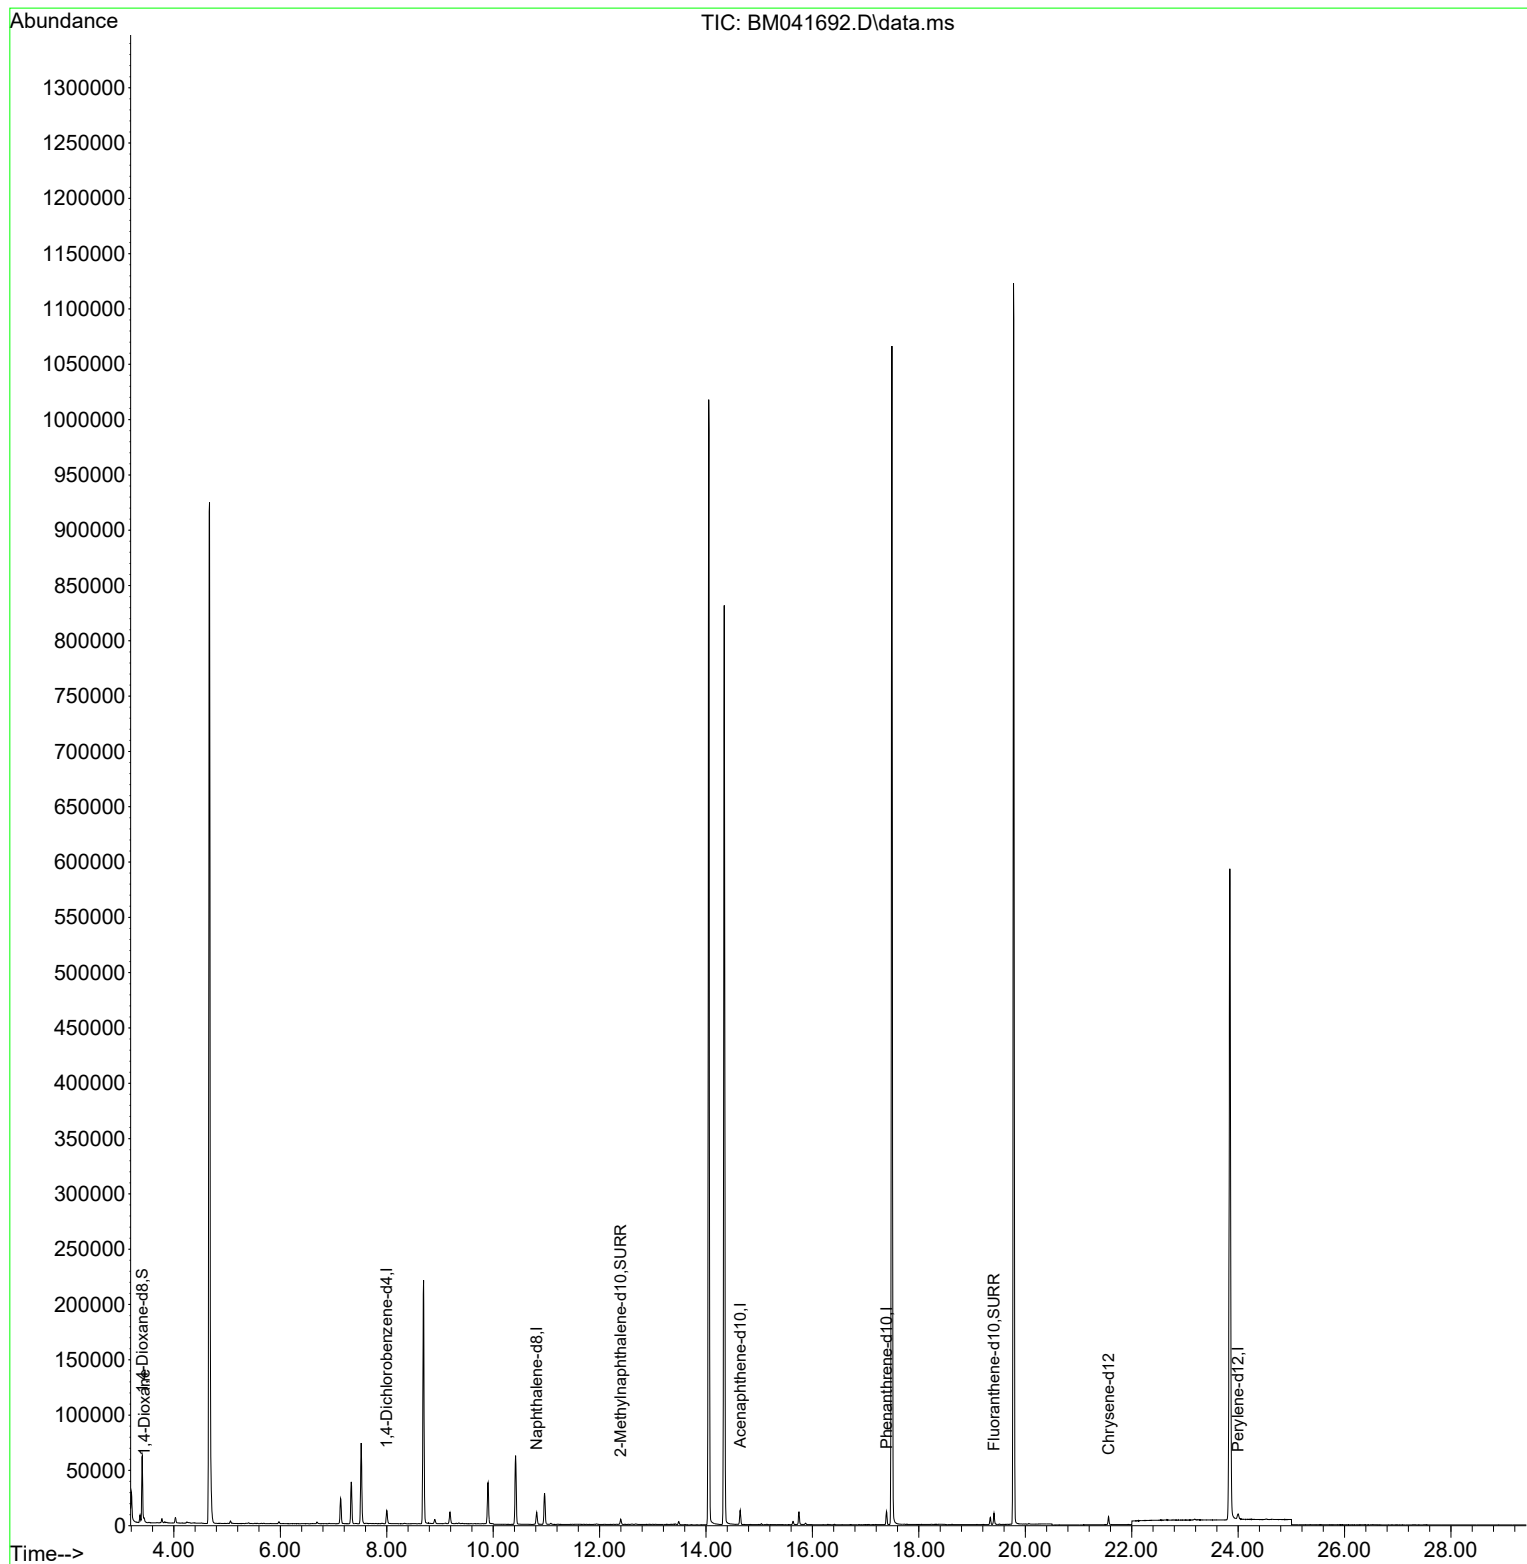


Abundance Scan 61 (3.440 min): BM041688.D\data.ms (-55)

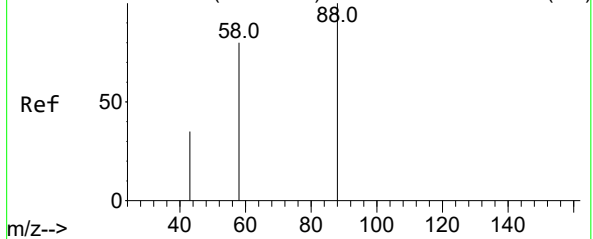

Abundance Scan 62 (3.444 min): BM041692.D\data.ms

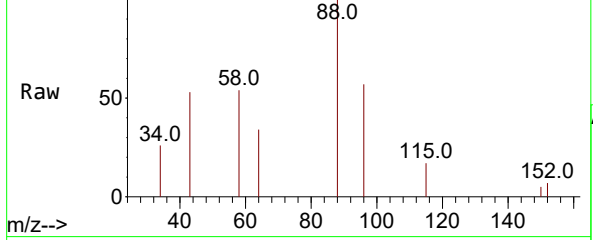

Abundance Scan 62 (3.444 min): BM041692.D\data.ms (-48)

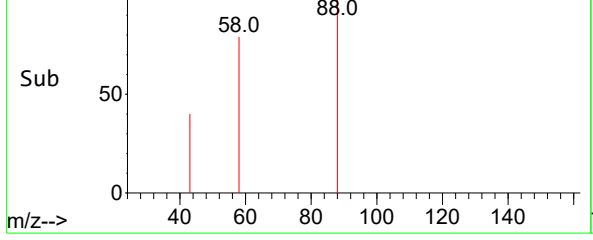

#2
1,4-Dioxane
Concen: 0.186 ng/ul
RT: 3.444 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM041692.D
Acq: 07 Sep 2023 13:14

Instrument :
BNA_M
ClientSampleId :
BBKE8

Tgt Ion: 88	Resp: 1714
Ion Ratio	Lower Upper
88	100
43	53.4 33.8 50.6#
58	53.8 54.2 81.2#

