

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041693.D
 Acq On : 07 Sep 2023 13:52
 Operator : MA/JU
 Sample : 04166-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH9G3

Quant Time: Sep 08 02:53:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 06 02:20:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	4869	0.400	ng/ul	0.00
4) Naphthalene-d8	10.818	136	11561	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.643	164	5145	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	9318	0.400	ng/ul	0.00
17) Chrysene-d12	21.565	240	3699	0.400	ng/ul	0.00
23) Perylene-d12	23.994	264	4751	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	34026	4.573	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	5131	0.345	ng/ul	-0.01
18) Fluoranthene-d10	19.413	212	7045	0.393	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	812	0.105	ng/ul#	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041693.D
Acq On : 07 Sep 2023 13:52
Operator : MA/JU
Sample : 04166-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH9G3


Quant Time: Sep 08 02:53:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 06 02:20:07 2023
Response via : Initial Calibration

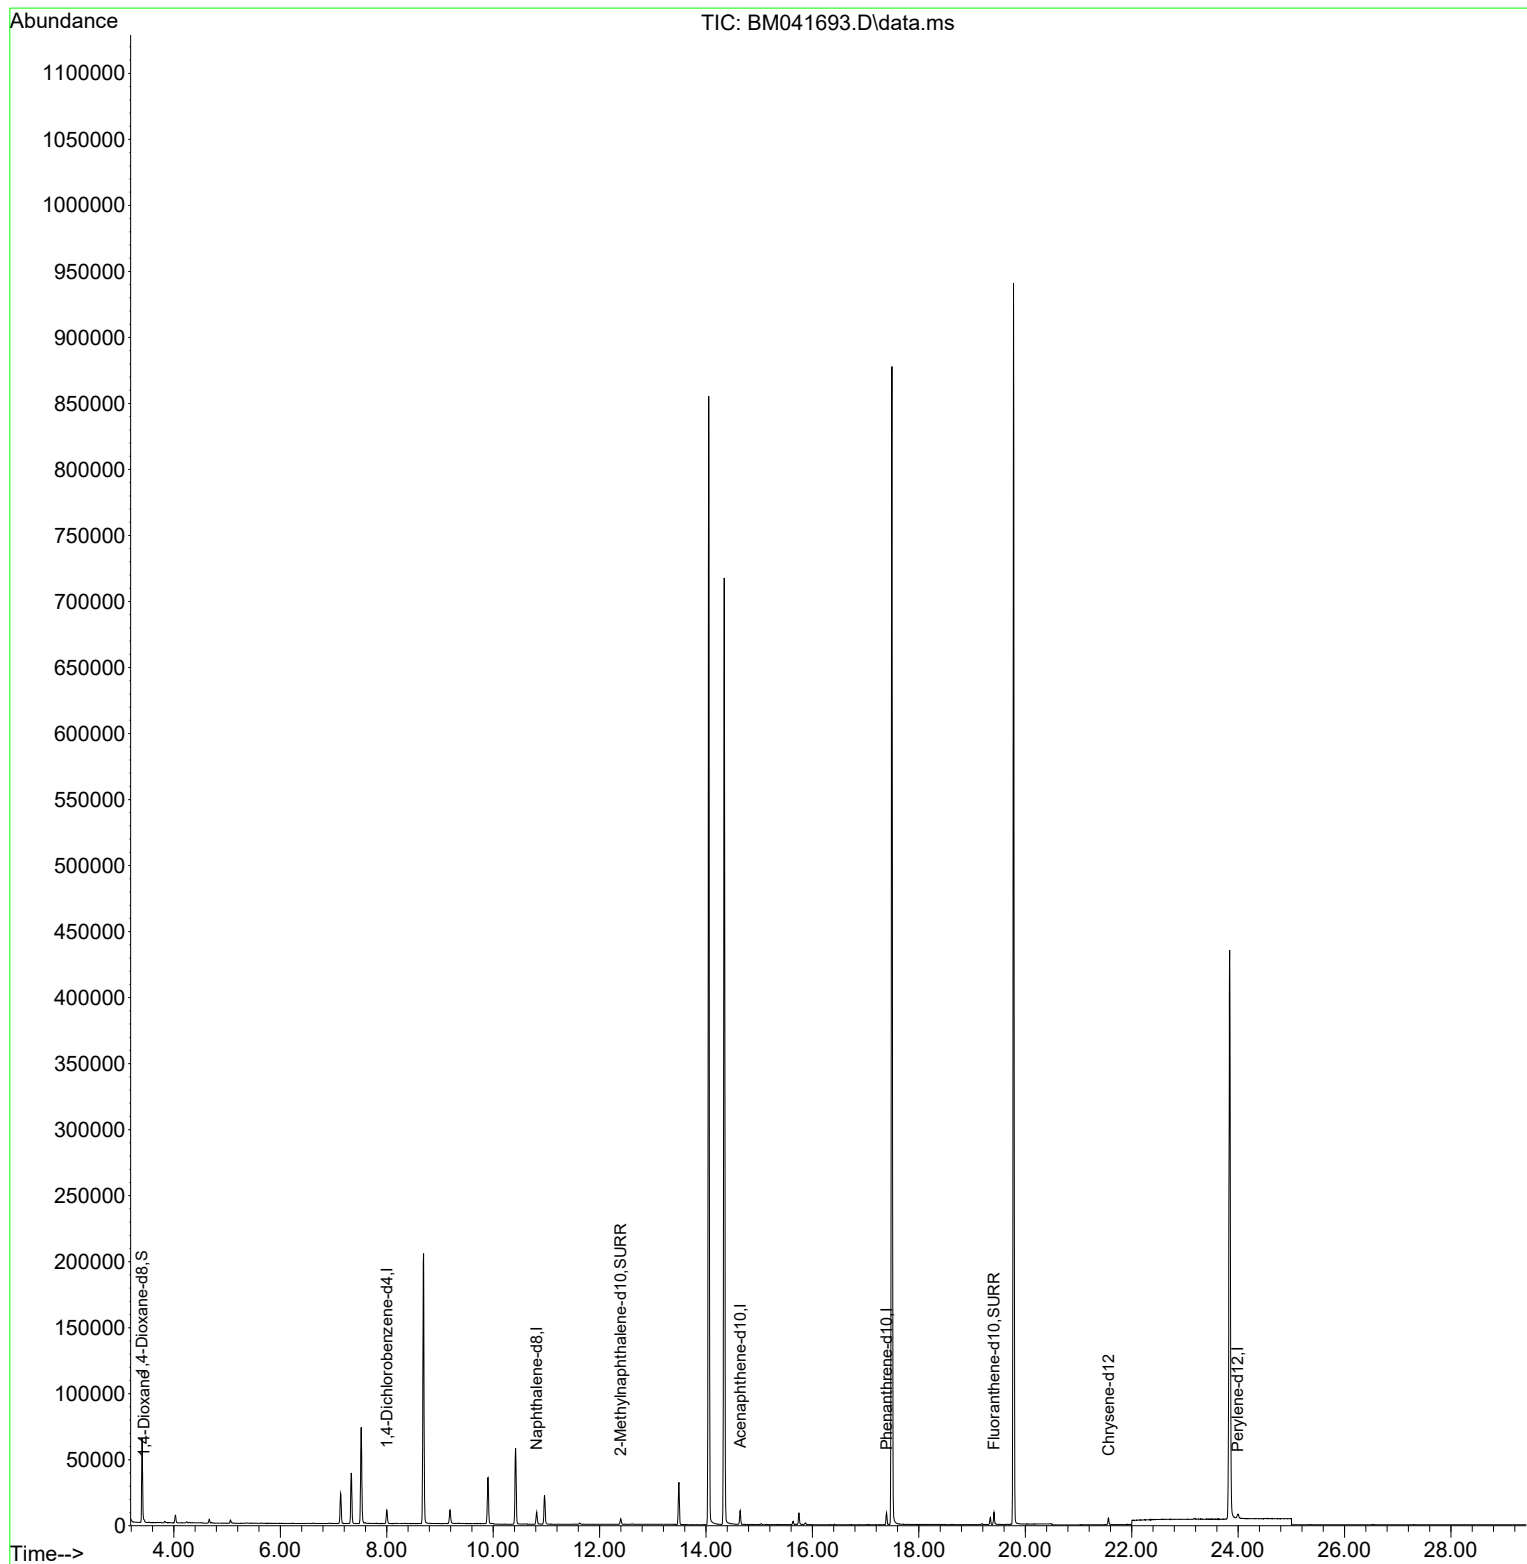


Abundance Scan 61 (3.440 min): BM041688.D\data.ms (-55)

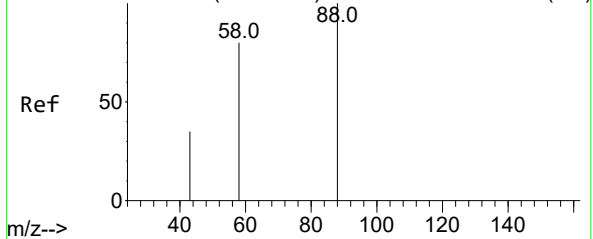

Abundance Scan 61 (3.440 min): BM041693.D\data.ms

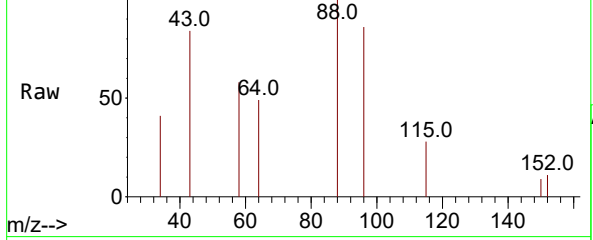

Abundance Scan 61 (3.440 min): BM041693.D\data.ms (-48)

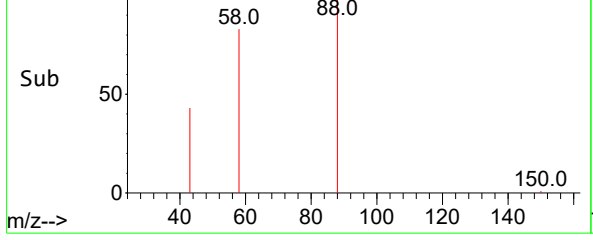

#2
1,4-Dioxane
Concen: 0.105 ng/ul
RT: 3.440 min Scan# 61
Delta R.T. -0.004 min
Lab File: BM041693.D
Acq: 07 Sep 2023 13:52

Instrument :
BNA_M
ClientSampleId :
BH9G3

Tgt Ion:	88	Resp:	812
Ion	Ratio	Lower	Upper
88	100		
43	84.1	33.8	50.6#
58	58.0	54.2	81.2

