

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041706.D
 Acq On : 07 Sep 2023 22:06
 Operator : MA/JU
 Sample : 04148-14
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBKJ8

Quant Time: Sep 08 02:55:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 06 02:20:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	7689	0.400	ng/ul	0.00
4) Naphthalene-d8	10.818	136	19595	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.638	164	9108	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	16306	0.400	ng/ul	0.00
17) Chrysene-d12	21.559	240	5376	0.400	ng/ul	-0.01
23) Perylene-d12	23.988	264	6253	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	40073	3.410	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	7522	0.298	ng/ul	-0.01
18) Fluoranthene-d10	19.408	212	10942	0.420	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	1577	0.129	ng/ul#	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041706.D
Acq On : 07 Sep 2023 22:06
Operator : MA/JU
Sample : 04148-14
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBKJ8


Quant Time: Sep 08 02:55:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 06 02:20:07 2023
Response via : Initial Calibration

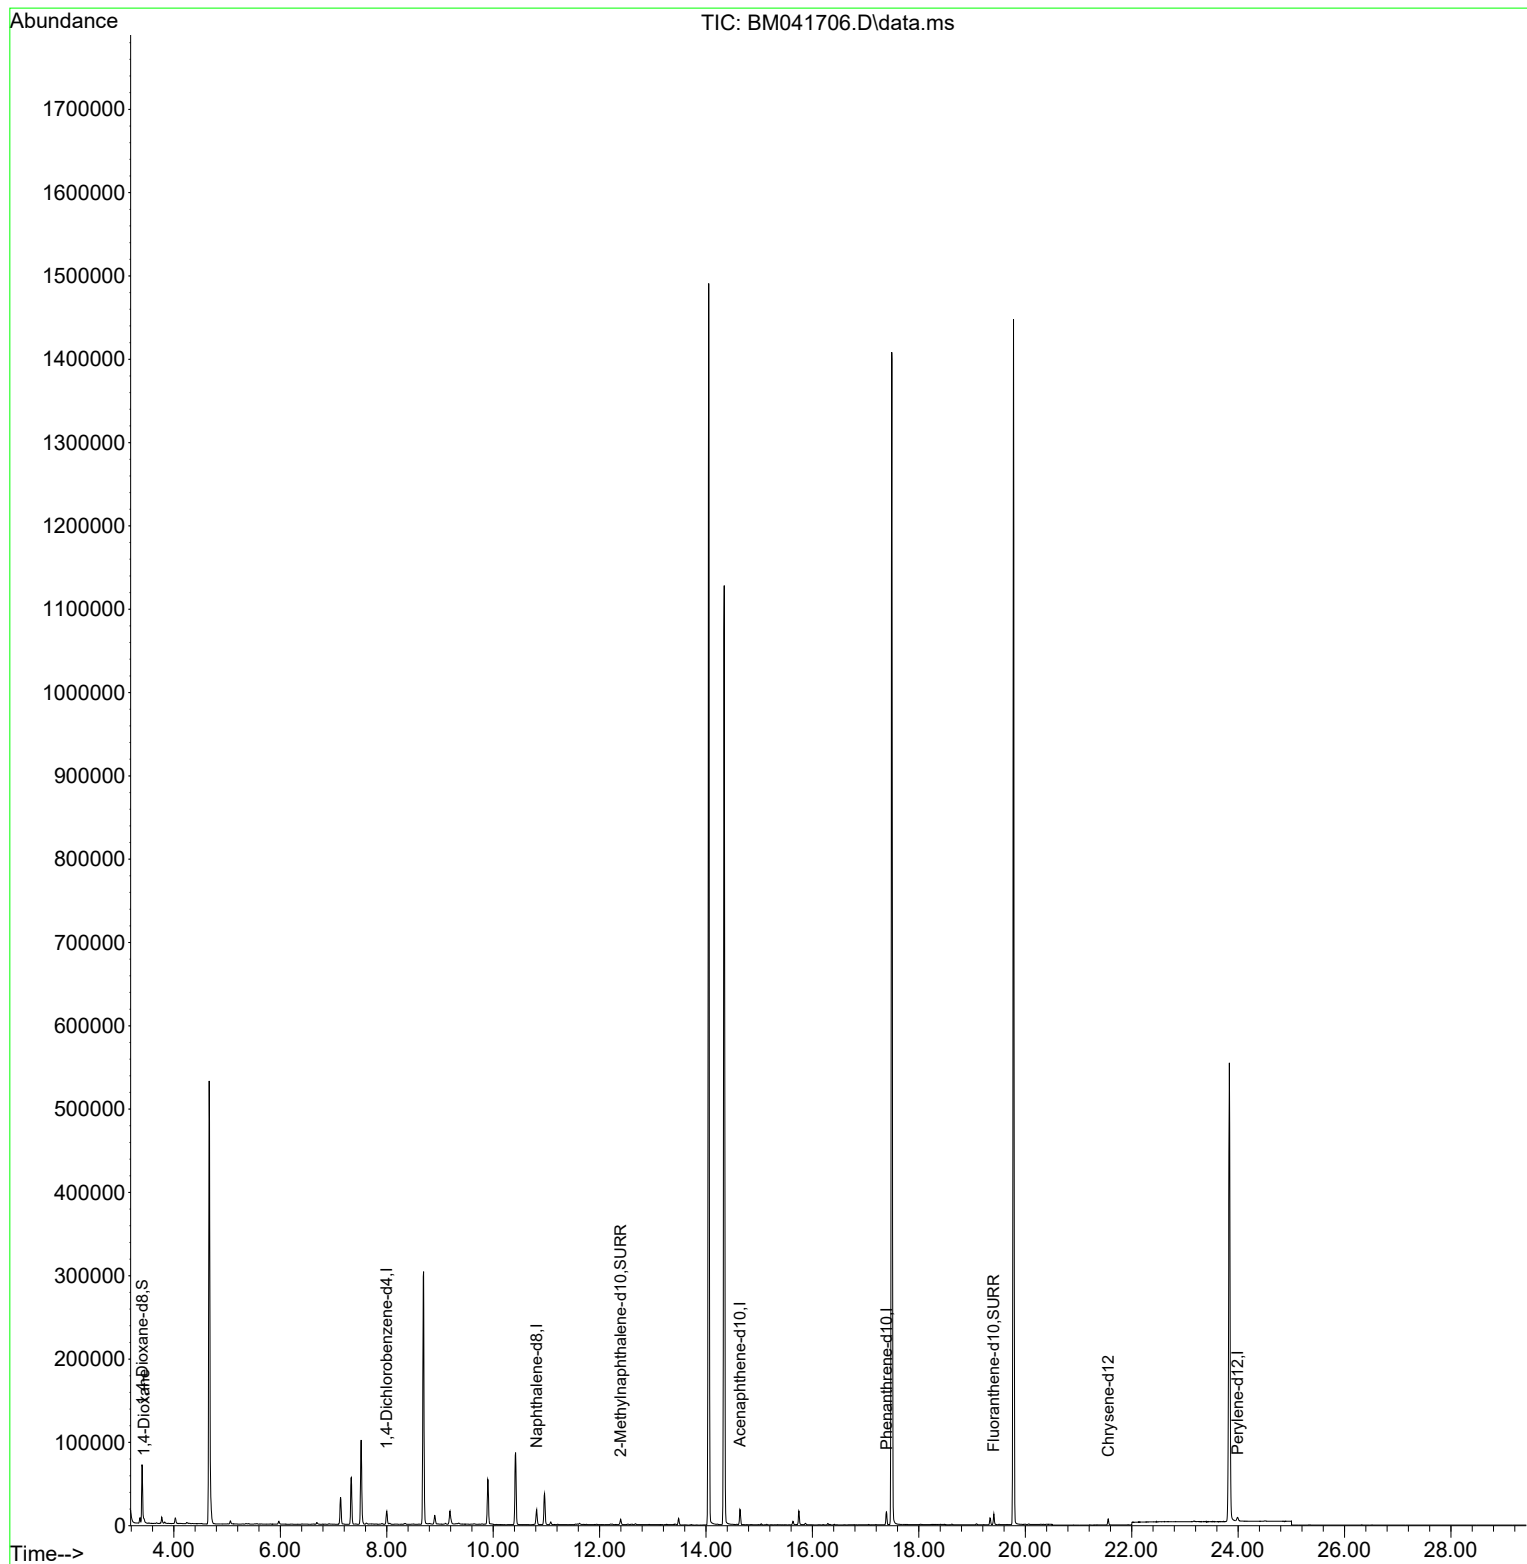


Abundance Scan 61 (3.439 min): BM041699.D\data.ms (-52)

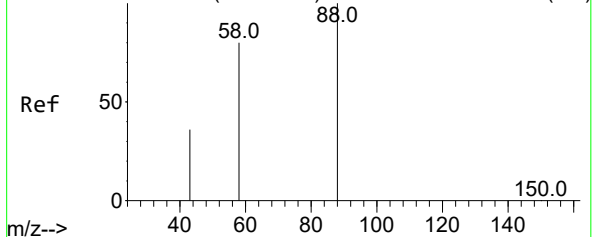

Abundance Scan 61 (3.440 min): BM041706.D\data.ms

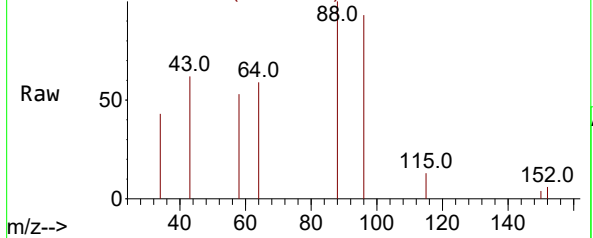

Abundance Scan 61 (3.440 min): BM041706.D\data.ms (-48)

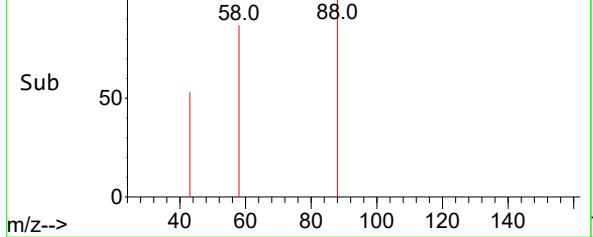

#2
1,4-Dioxane
Concen: 0.129 ng/ul
RT: 3.440 min Scan# 61
Delta R.T. -0.004 min
Lab File: BM041706.D
Acq: 07 Sep 2023 22:06

Instrument :
BNA_M
ClientSampleId :
BBKJ8

Tgt Ion:	88	Resp:	1577
Ion	Ratio	Lower	Upper
88	100		
43	61.6	33.8	50.6#
58	53.3	54.2	81.2#

