

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041719.D
 Acq On : 08 Sep 2023 06:47
 Operator : MA/JU
 Sample : 04166-16
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJP0

Quant Time: Sep 08 07:17:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	9049	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	23523	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	11231	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.388	188	20599	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	7205	0.400	ng/ul	0.00
23) Perylene-d12	23.982	264	7587	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	60926	4.406	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152	8722	0.288	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	13277	0.380	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	1718	0.120	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041719.D
Acq On : 08 Sep 2023 06:47
Operator : MA/JU
Sample : 04166-16
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJP0


Quant Time: Sep 08 07:17:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

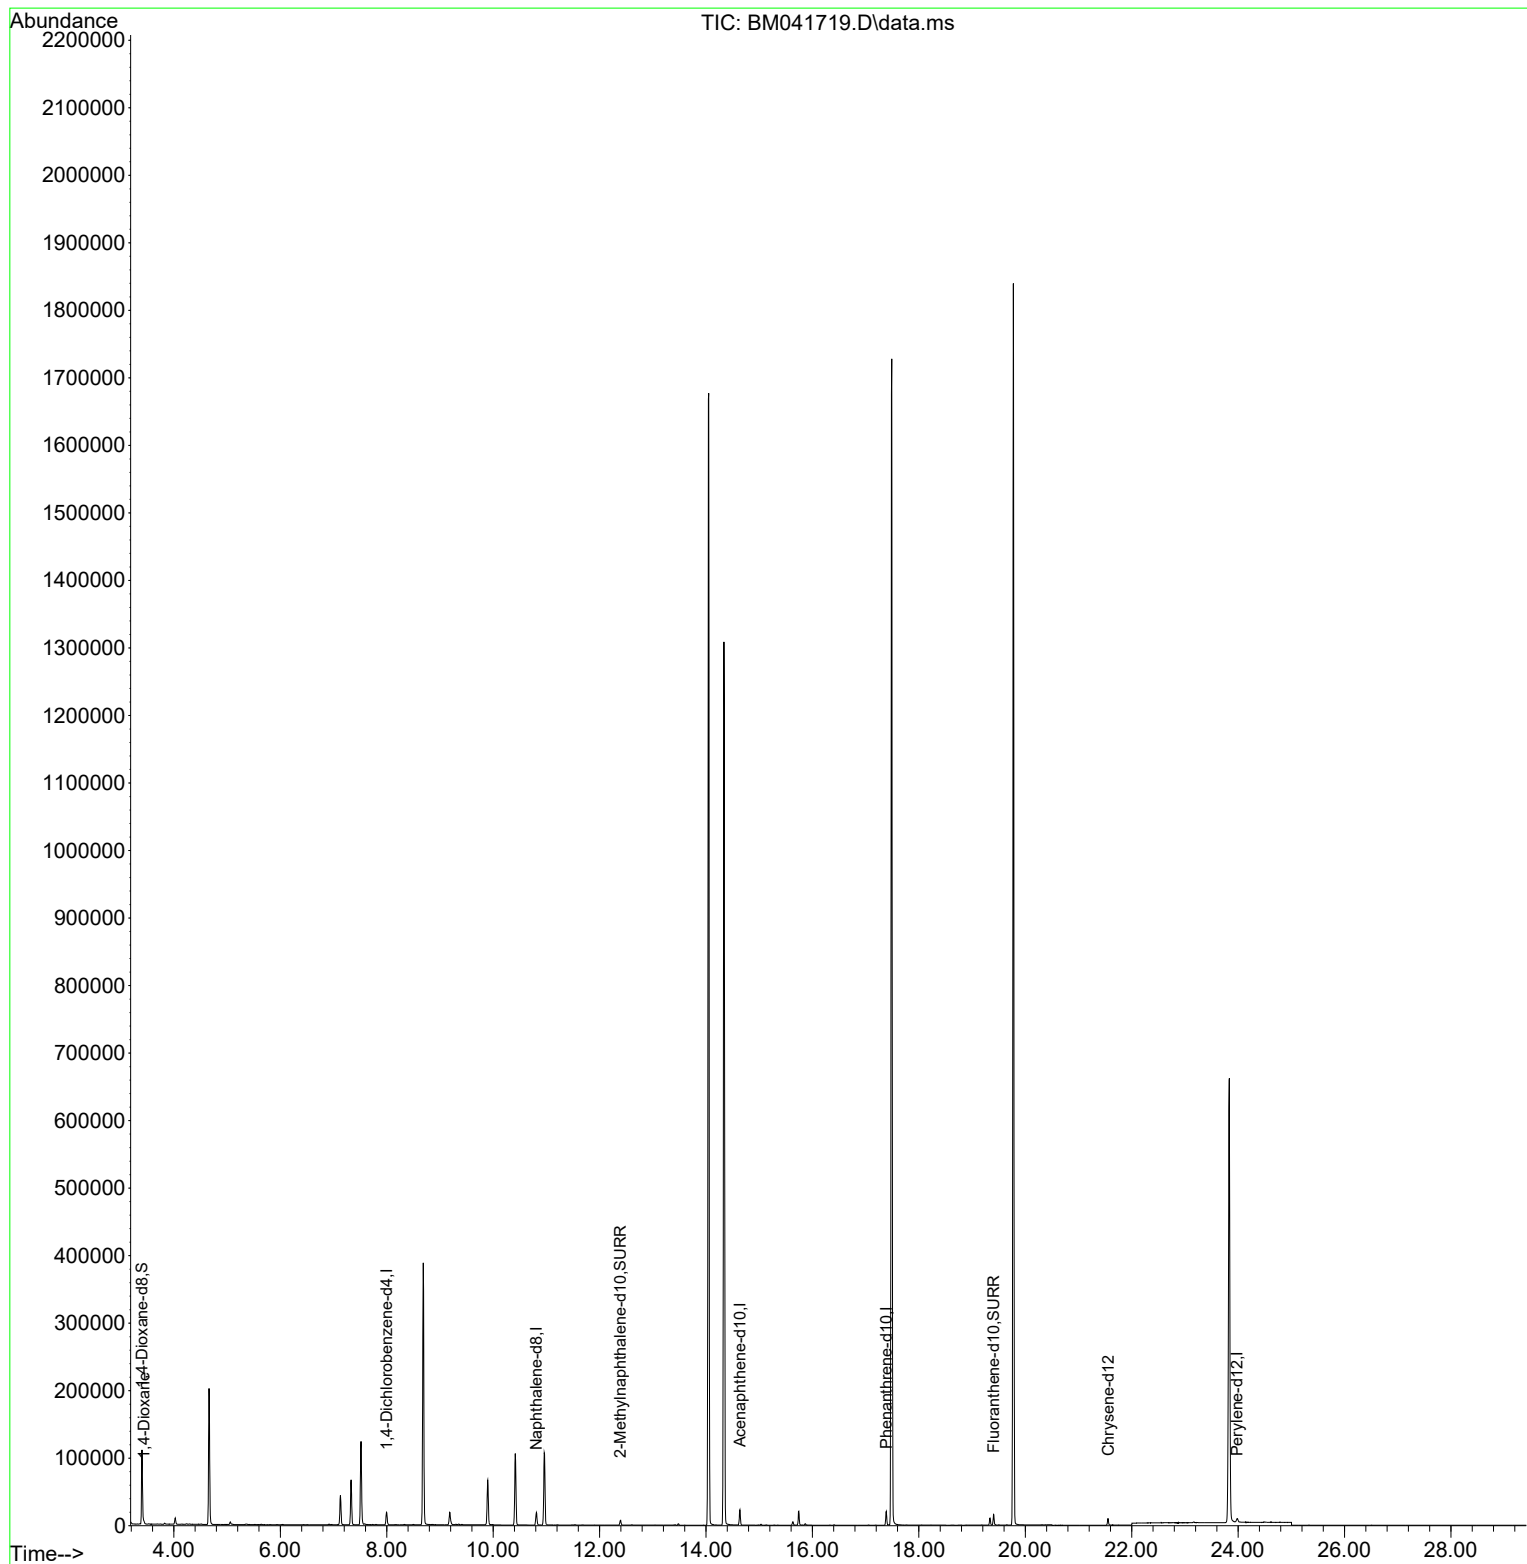


Abundance Scan 61 (3.440 min): BM041716.D\data.ms (-54)

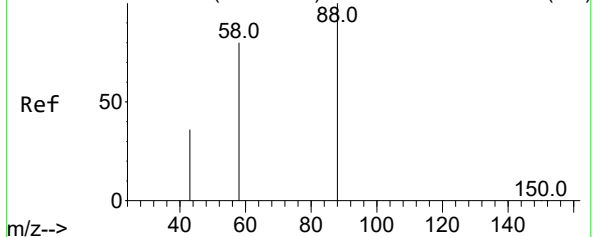

Abundance Scan 61 (3.440 min): BM041719.D\data.ms

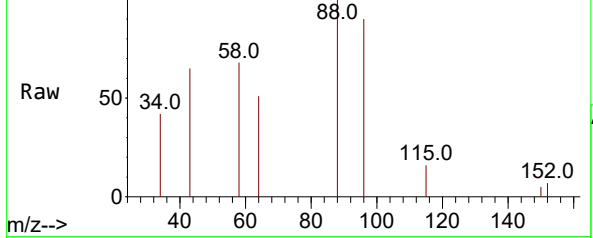

Abundance Scan 61 (3.440 min): BM041719.D\data.ms (-47)

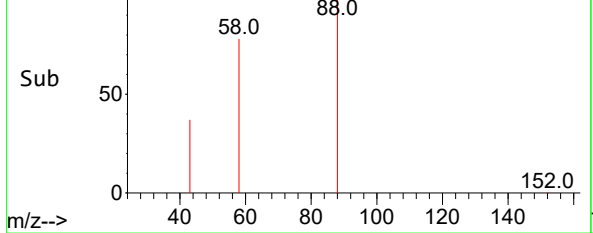

#2
1,4-Dioxane
Concen: 0.120 ng/ul
RT: 3.440 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM041719.D
Acq: 08 Sep 2023 06:47

Instrument :
BNA_M
ClientSampleId :
BBJP0

Tgt Ion: 88 Resp: 1718
Ion Ratio Lower Upper
88 100
43 64.7 33.8 50.6#
58 68.4 54.2 81.2

