

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041725.D
 Acq On : 08 Sep 2023 10:28
 Operator : MA/JU
 Sample : 04153-06
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH464

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/09/2023
 Supervised By :mohammad ahmed 09/09/2023

Quant Time: Sep 08 23:52:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	8902	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	23605	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	10847	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.388	188	22370	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	7501	0.400	ng/ul	0.00
23) Perylene-d12	23.982	264	7960	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	195673m	14.383	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152	7493	0.247	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	11447	0.315	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	1890	0.134	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041725.D
Acq On : 08 Sep 2023 10:28
Operator : MA/JU
Sample : 04153-06
Misc :
ALS Vial : 66 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BH464

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/09/2023
Supervised By :mohammad ahmed 09/09/2023


Quant Time: Sep 08 23:52:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

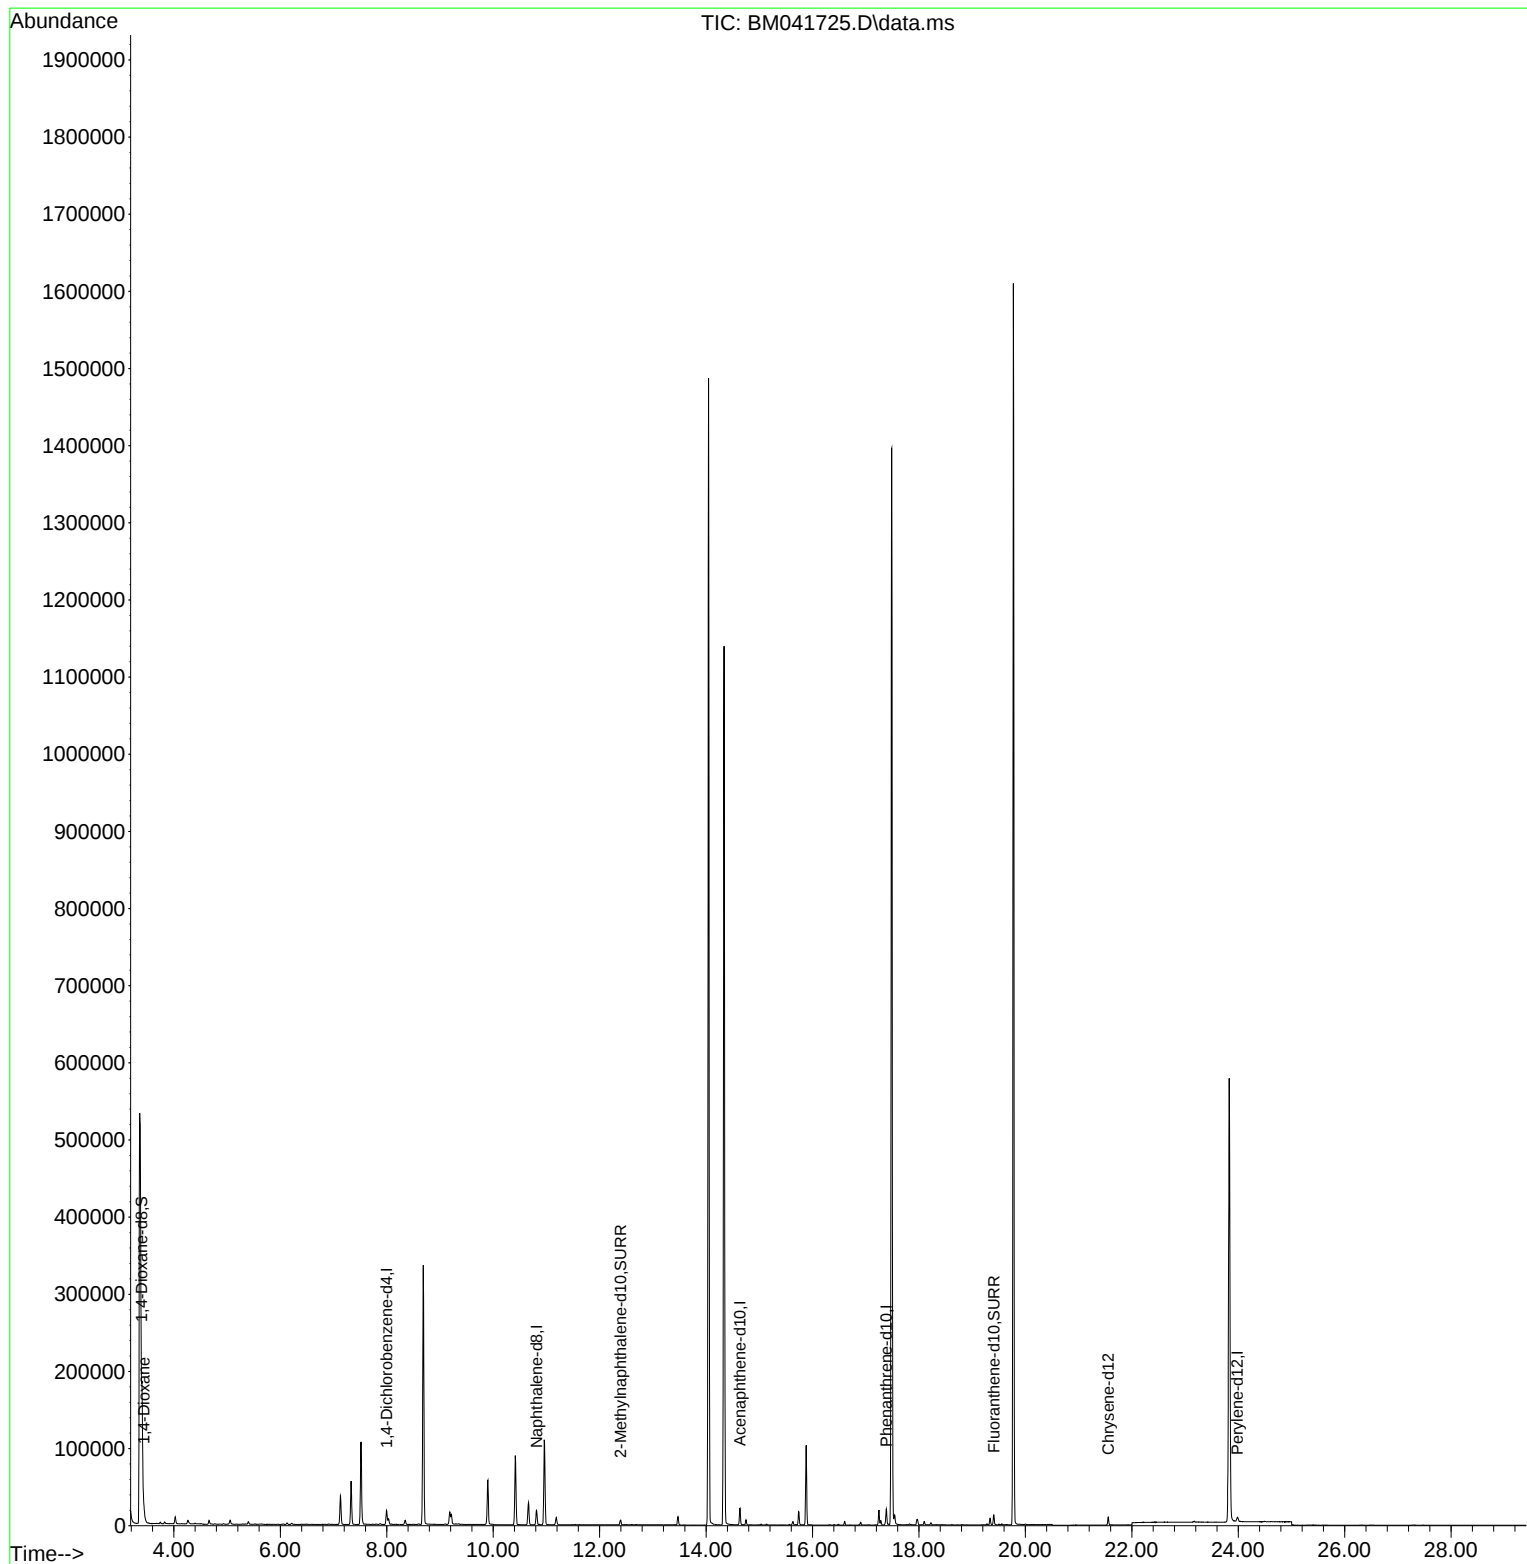

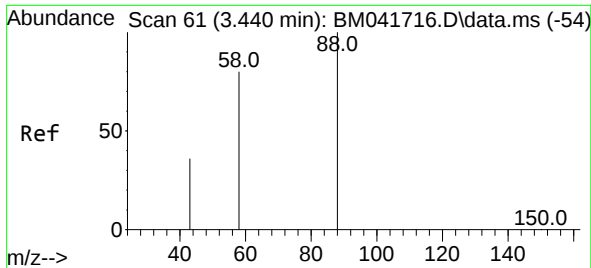

#2
 1,4-Dioxane
 Concen: 0.134 ng/ul
 RT: 3.440 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BM041725.D
 Acq: 08 Sep 2023 10:28

Instrument :
 BNA_M
 ClientSampleId :
 BH464

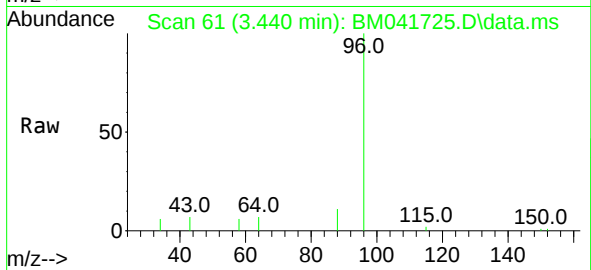

Tgt Ion: 88 Resp: 1890

Ion	Ratio	Lower	Upper
88	100		
43	64.2	33.8	50.6
58	57.3	54.2	81.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/09/2023
 Supervised By :mohammad ahmed 09/09/2023

