

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041727.D
 Acq On : 08 Sep 2023 11:43
 Operator : MA/JU
 Sample : 04153-08
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH476

Quant Time: Sep 08 22:54:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	8350	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	22060	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	10643	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.388	188	21266	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	6720	0.400	ng/ul	0.00
23) Perylene-d12	23.982	264	7050	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	51371	4.026	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152	8745	0.308	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	13221	0.406	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	1657	0.125	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041727.D
Acq On : 08 Sep 2023 11:43
Operator : MA/JU
Sample : 04153-08
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH476


Quant Time: Sep 08 22:54:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

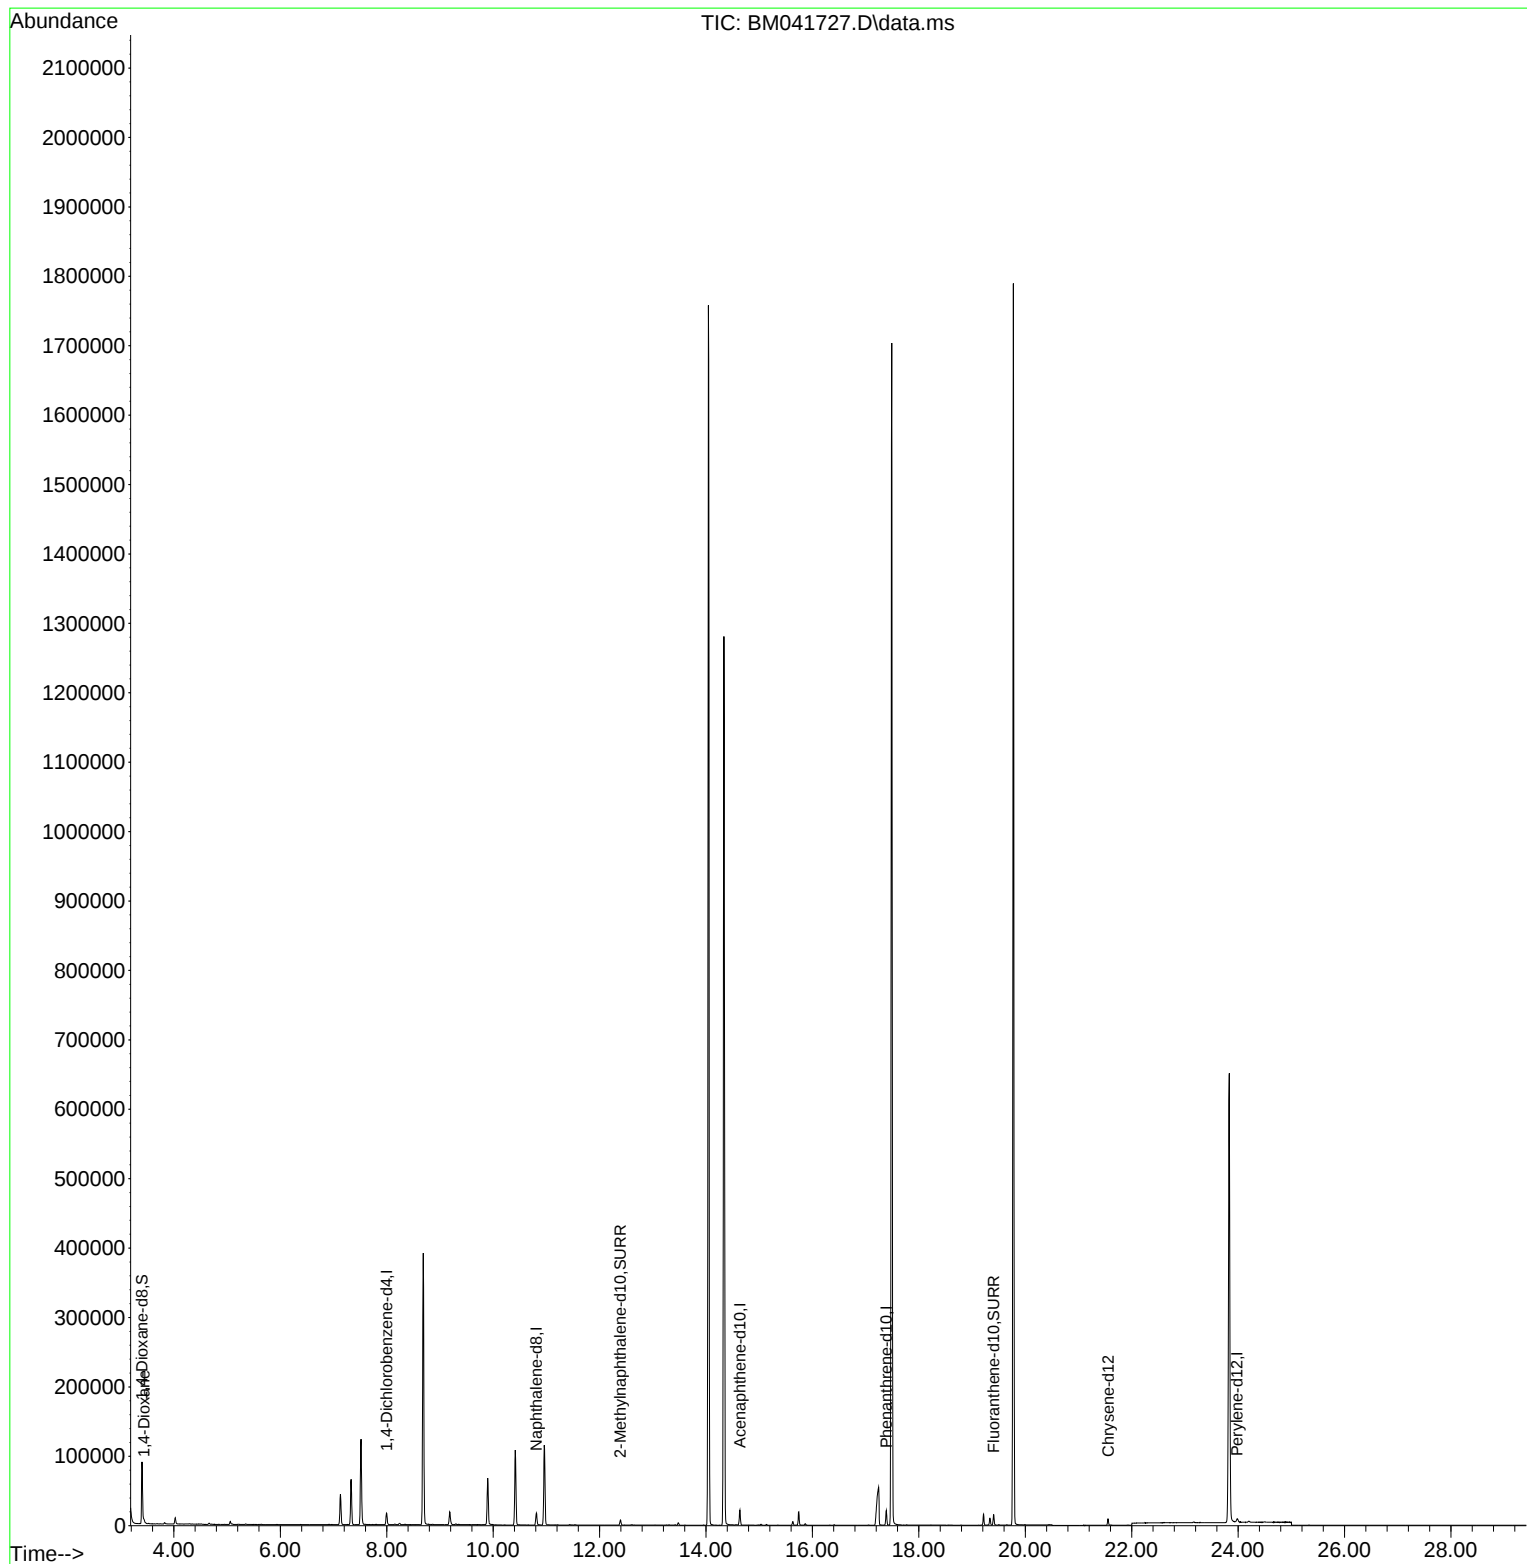

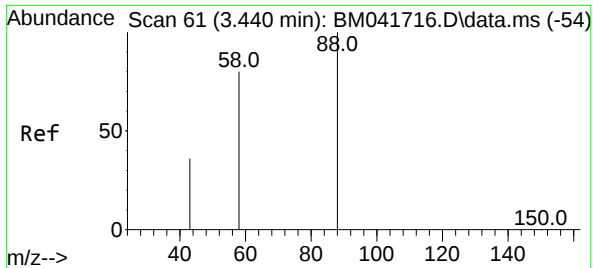

#2
 1,4-Dioxane
 Concen: 0.125 ng/ul
 RT: 3.440 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BM041727.D
 Acq: 08 Sep 2023 11:43

Instrument :
 BNA_M
 ClientSampleId :
 BH476

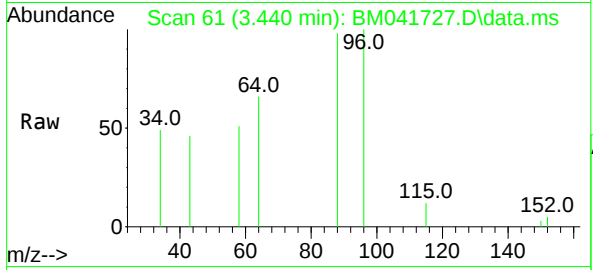

Tgt Ion:	88	Resp:	1657
Ion	Ratio	Lower	Upper
88	100		
43	46.8	33.8	50.6
58	52.3	54.2	81.2#

