
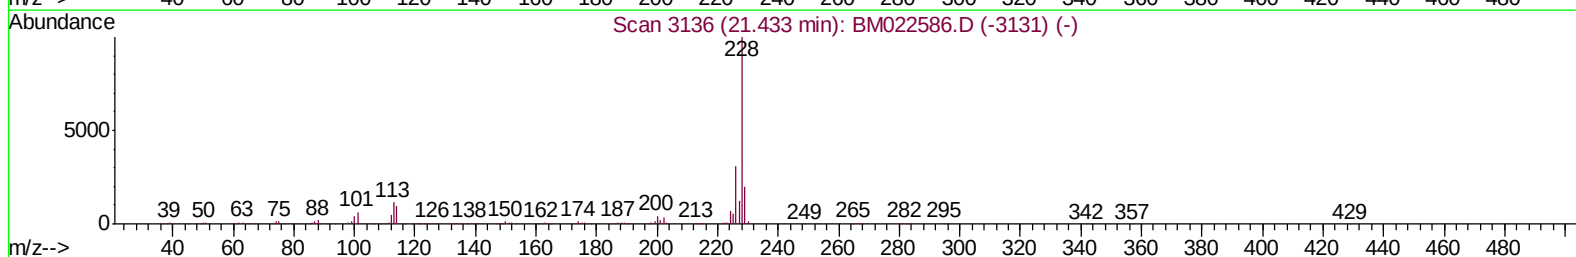
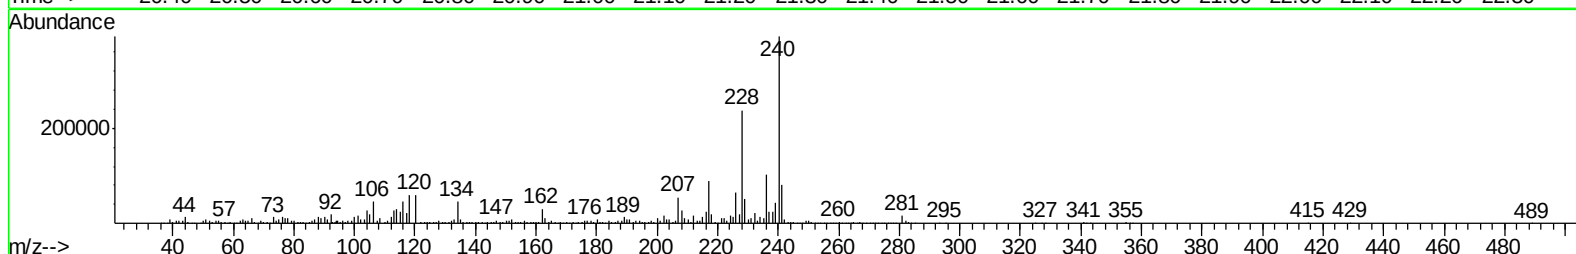


Data File : BM022592.D
Acq On : 09 Sep 2019 07:33
Operator : HP/JU
Sample : K4706-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Sep 09 08:18:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 09 07:45:00 2019
Response via : Initial Calibration

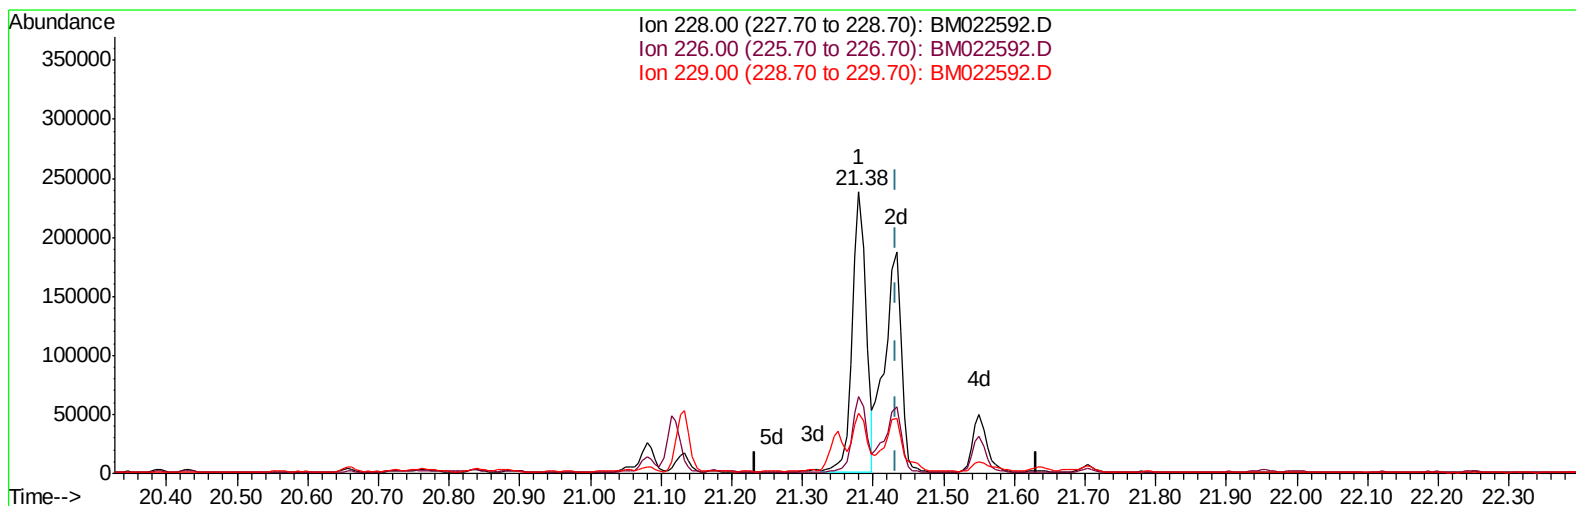

TIC: BM022592.D

(85) Chrysene

21.380min (-0.053) 1.67ng/ul

response 323573

Ion	Exp%	Act%
228.00	100	100
226.00	30.30	27.27
229.00	19.70	21.43
0.00	0.00	0.00