

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090819\
 Data File : BM022575.D
 Acq On : 08 Sep 2019 20:32
 Operator : HP/JU
 Sample : K4707-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CJ4

Quant Time: Sep 09 01:46:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 09 01:43:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	317160	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	1421761	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.49	164	903496	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.22	188	1859540	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	1882655	20.00	ng/ul	0.00
86) Perylene-d12	23.69	264	2173251	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.30	96	32690	4.29	ng/uL	0.00
5) Phenol-d5	7.01	99	133333	4.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.19	67	376219	22.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.39	132	396713	17.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	255324	10.73	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	240335	23.43	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	219390	23.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.26	165	445771	18.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	56423	1.78	ng/ul	0.00
44) Dimethylphthalate-d6	13.90	166	1793909	24.50	ng/ul	0.00
47) Acenaphthylene-d8	14.18	160	1994489	22.75	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	45205	3.62	ng/ul	0.00
58) Fluorene-d10	15.48	176	1513123	24.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	165818	19.62	ng/ul	0.00
71) Anthracene-d10	17.32	188	2556101	26.83	ng/ul	0.00
79) Pyrene-d10	19.61	212	2874510	27.52	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.54	264	3228474	27.64	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.94	163	131589	1.771	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090819\
Data File : BM022575.D
Acq On : 08 Sep 2019 20:32
Operator : HP/JU
Sample : K4707-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CJ4

Quant Time: Sep 09 01:46:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 09 01:43:30 2019
Response via : Initial Calibration

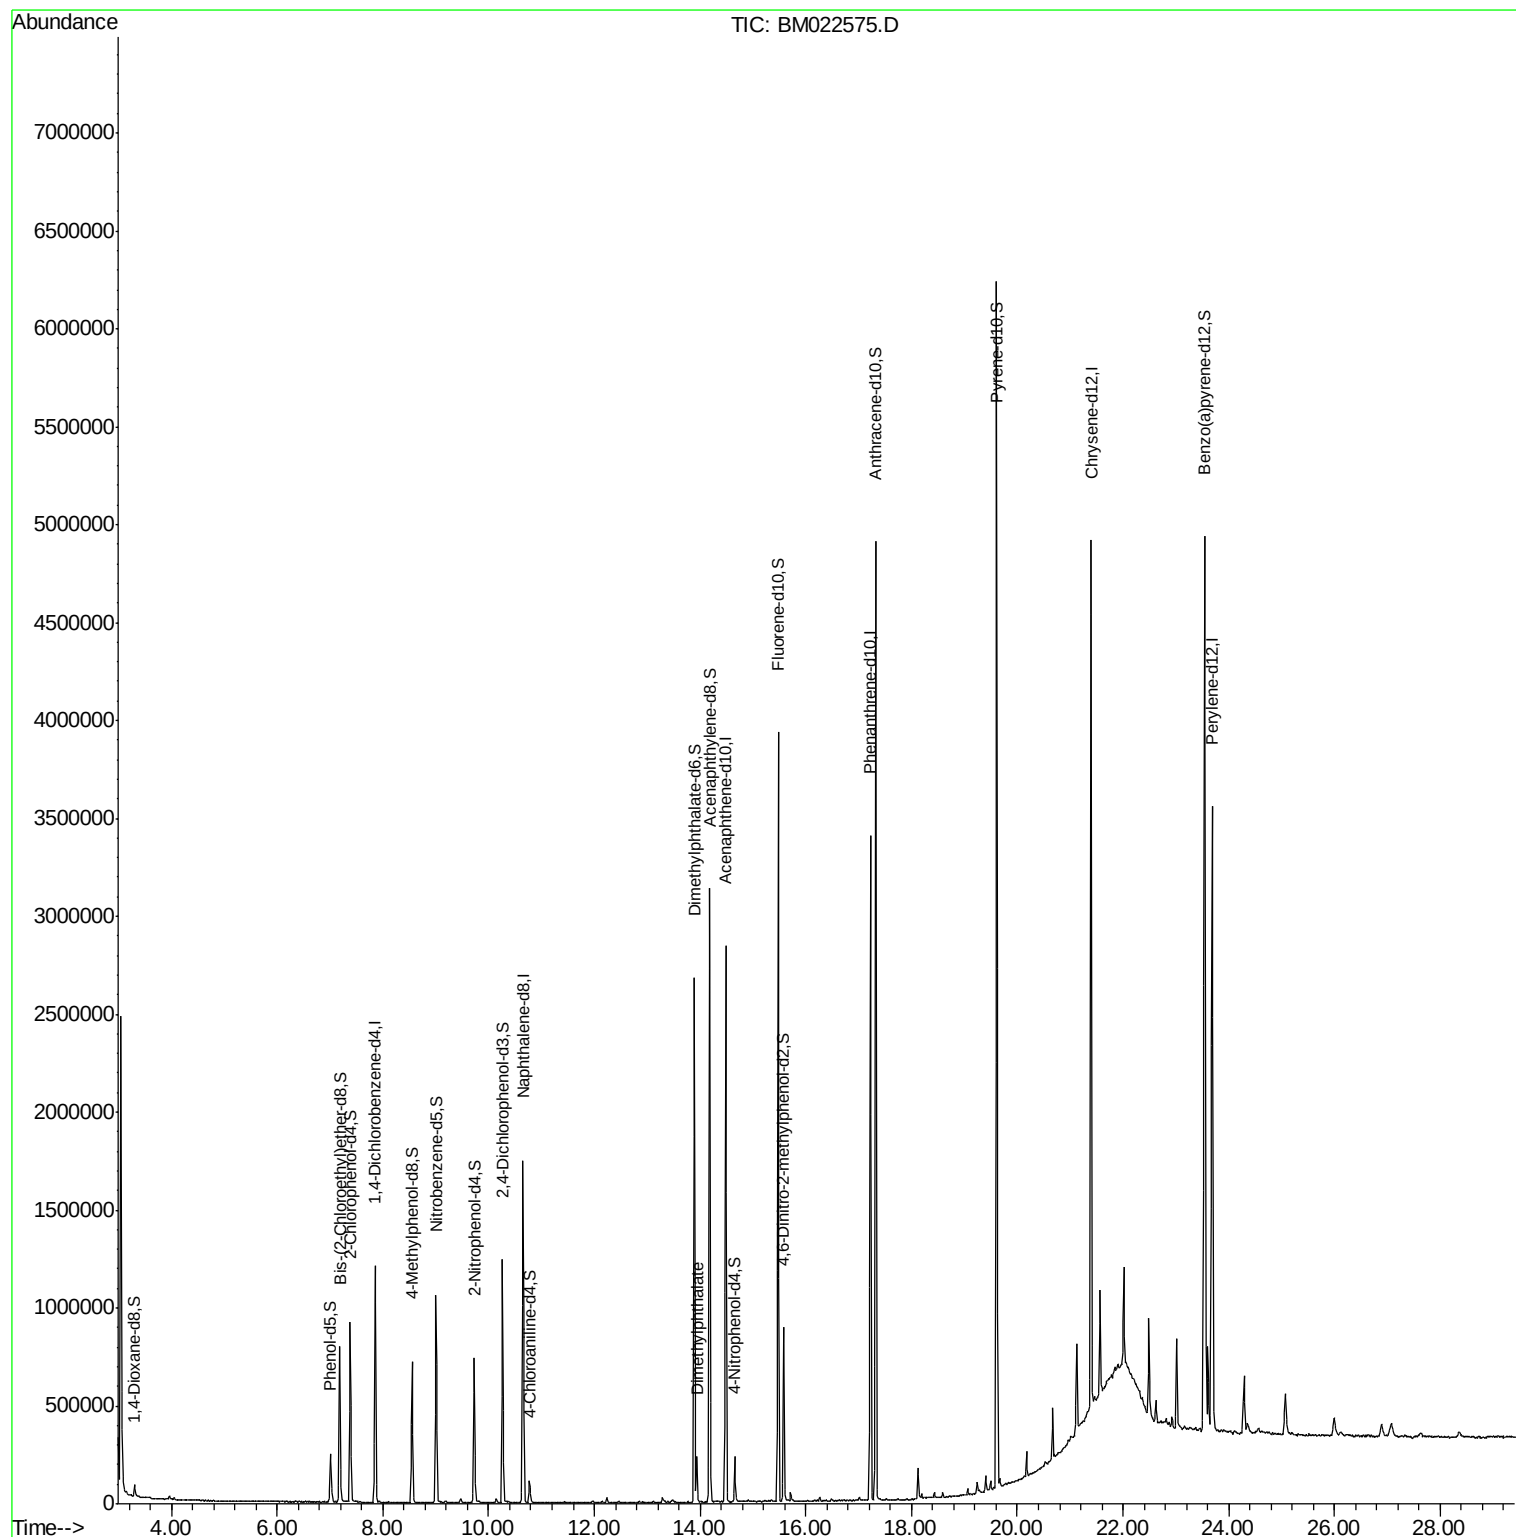

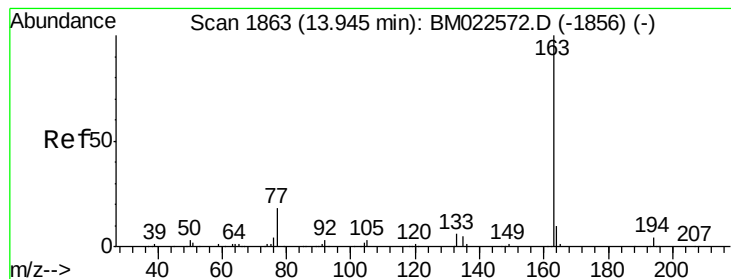

#45

Dimethylphthalate

Concen: 1.771 ng/ul

RT: 13.94 min Scan# 1862

Delta R.T. -0.01 min

Lab File: BM022575.D

Acq: 08 Sep 2019 20:32

Instrument :

BNA_M

ClientSampleId :

C0CJ4


Tot Ion:163 Resp: 131589

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 10.4 7.8 11.8

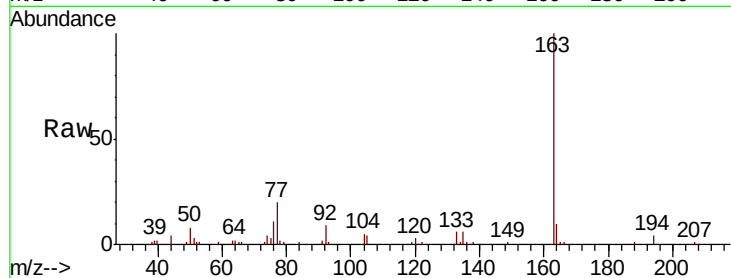

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

