

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090822\
 Data File : BM036518.D
 Acq On : 07 Sep 2022 20:37
 Operator : CG/JU
 Sample : N4483-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW351

Quant Time: Sep 08 00:54:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 02 01:33:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	197073	20.000	ng/ul	0.00
20) Naphthalene-d8	10.522	136	925535	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.374	164	592513	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.115	188	1200234	20.000	ng/ul	0.00
79) Chrysene-d12	21.309	240	990309	20.000	ng/ul	# 0.00
88) Perylene-d12	23.597	264	812366	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.128	96	19248	3.722	ng/uL	0.00
4) Pyridine-d5	3.563	84	85396	5.988	ng/ul	0.00
7) Phenol-d5	6.904	99	418025	24.850	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	268084	25.318	ng/ul	0.00
11) 2-Chlorophenol-d4	7.251	132	342237	25.894	ng/ul	0.00
15) 4-Methylphenol-d8	8.445	113	312714	24.897	ng/ul	0.00
21) Nitrobenzene-d5	8.892	128	182146	25.957	ng/ul	0.00
24) 2-Nitrophenol-d4	9.610	143	197733	27.780	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.151	165	341190	26.827	ng/ul	0.00
31) 4-Chloroaniline-d4	10.669	131	350214	17.762	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	1077412	28.742	ng/ul	0.00
49) Acenaphthylene-d8	14.068	160	1274779	27.266	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	160488	22.595	ng/ul	0.00
60) Fluorene-d10	15.368	176	966979	28.548	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.504	200	108551	17.592	ng/ul	0.00
73) Anthracene-d10	17.215	188	1455205	27.267	ng/ul	0.00
81) Pyrene-d10	19.515	212	1651064	32.140	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.450	264	1156540	29.037	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.928	94	22691	1.297	ng/ul#	86
16) Acetophenone	8.557	105	29695	1.470	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090822\
Data File : BM036518.D
Acq On : 07 Sep 2022 20:37
Operator : CG/JU
Sample : N4483-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW351

Quant Time: Sep 08 00:54:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 02 01:33:23 2022
Response via : Initial Calibration




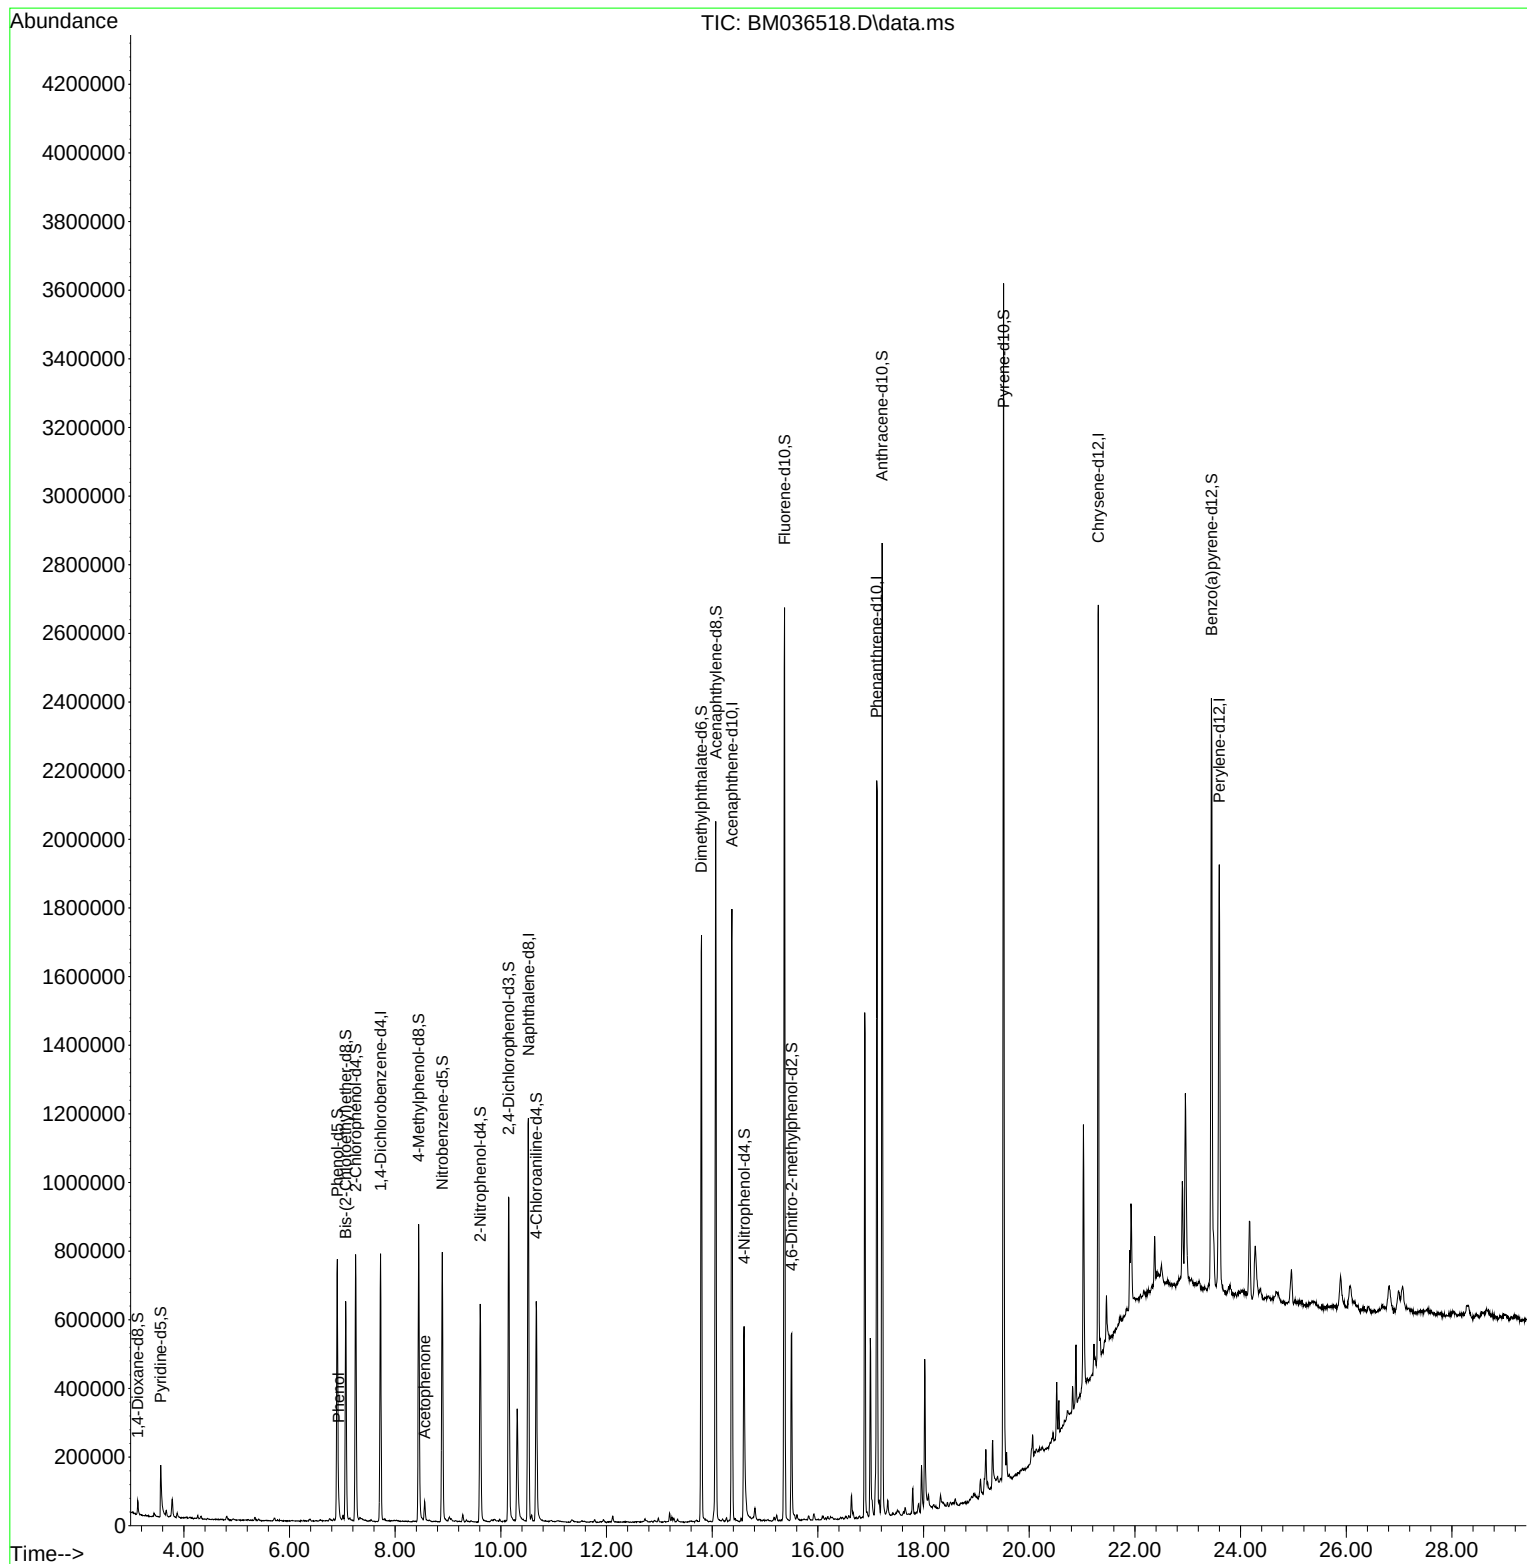


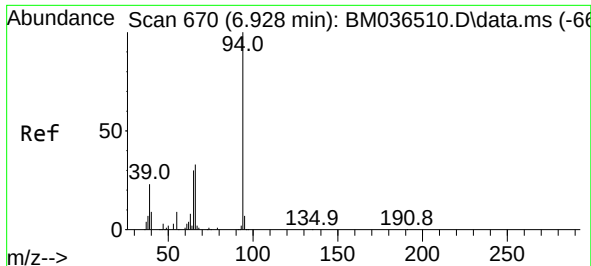

#8
Phenol
Concen: 1.297 ng/ul
RT: 6.928 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM036518.D
Acq: 07 Sep 2022 20:37

Instrument :
BNA_M
ClientSampleId :
EW351

Tgt Ion: 94 Resp: 22691
Ion Ratio Lower Upper
94 100
65 32.9 21.3 31.9#
66 43.5 27.4 41.0#

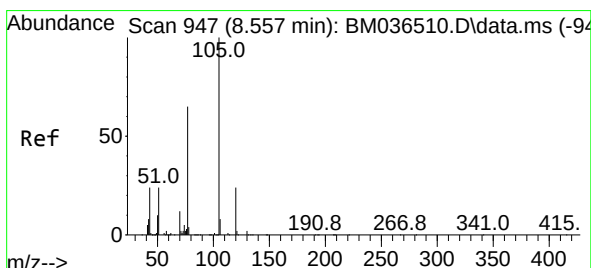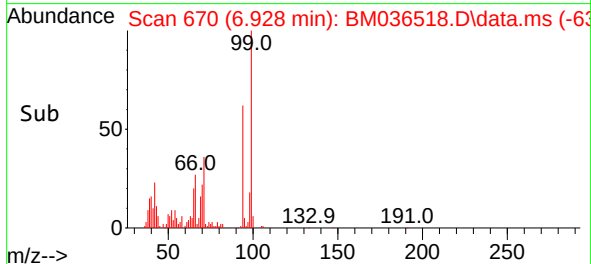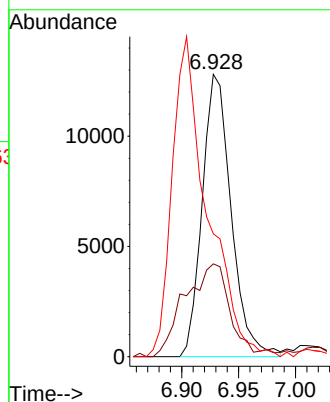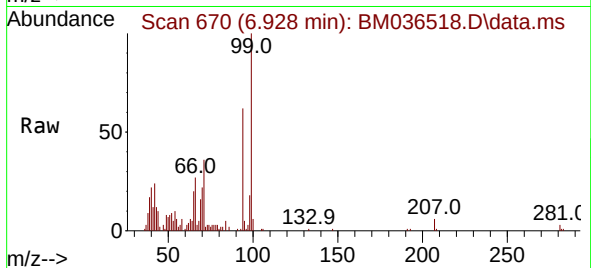

#16
Acetophenone
Concen: 1.470 ng/ul
RT: 8.557 min Scan# 947
Delta R.T. -0.000 min
Lab File: BM036518.D
Acq: 07 Sep 2022 20:37

Tgt Ion:105 Resp: 29695
Ion Ratio Lower Upper
105 100
77 79.7 59.8 89.6
51 31.8 22.1 33.1

