

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090822\
 Data File : BM036515.D
 Acq On : 07 Sep 2022 18:49
 Operator : CG/JU
 Sample : N4483-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW363

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/08/2022
 Supervised By :mohammad ahmed 09/19/2022

Quant Time: Sep 08 00:53:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 02 01:33:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	233910	20.000	ng/u1	0.00
20) Naphthalene-d8	10.522	136	1092999	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.374	164	683939	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.121	188	1394208	20.000	ng/u1	0.00
79) Chrysene-d12	21.309	240	1167489	20.000	ng/u1	0.00
88) Perylene-d12	23.597	264	996777	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	17740	2.890	ng/uL	0.00
4) Pyridine-d5	3.581	84	22037m	1.302	ng/u1	0.02
7) Phenol-d5	6.904	99	378587	18.961	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	250110	19.901	ng/u1	0.00
11) 2-Chlorophenol-d4	7.251	132	323588	20.627	ng/u1	0.00
15) 4-Methylphenol-d8	8.445	113	314288	21.082	ng/u1	0.00
21) Nitrobenzene-d5	8.892	128	170331	20.554	ng/u1	0.00
24) 2-Nitrophenol-d4	9.610	143	175652	20.897	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.151	165	308628	20.548	ng/u1	0.00
31) 4-Chloroaniline-d4	10.675	131	437400	18.785	ng/u1	0.00
46) Dimethylphthalate-d6	13.798	166	1011365	23.374	ng/u1	0.00
49) Acenaphthylene-d8	14.069	160	1229014	22.773	ng/u1	0.00
54) 4-Nitrophenol-d4	14.604	143	142595	17.392	ng/u1	0.00
60) Fluorene-d10	15.368	176	912230	23.331	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.504	200	79712	11.121	ng/u1	0.00
73) Anthracene-d10	17.215	188	1408780	22.725	ng/u1	0.00
81) Pyrene-d10	19.515	212	1650580	27.254	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.450	264	1194658	24.445	ng/u1	0.00
Target Compounds					Qvalue	
72) Phenanthrene	17.162	178	138934	1.896	ng/u1	98
80) Fluoranthene	19.180	202	359719	4.915	ng/u1	97
82) Pyrene	19.545	202	301775	3.951	ng/u1	96
85) Benzo(a)anthracene	21.292	228	109978	1.568	ng/u1	97
87) Chrysene	21.345	228	121541	1.763	ng/u1	96
90) Benzo(b)fluoranthene	22.903	252	151123	2.487	ng/u1#	94
93) Benzo(a)pyrene	23.497	252	103205	1.726	ng/u1	93
94) Indeno(1,2,3-cd)pyrene	25.956	276	70508	1.003	ng/u1	92
96) Benzo(g,h,i)perylene	26.685	276	67800	1.128	ng/u1	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090822\
Data File : BM036515.D
Acq On : 07 Sep 2022 18:49
Operator : CG/JU
Sample : N4483-14
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EW363

Quant Time: Sep 08 00:53:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 02 01:33:23 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/08/2022
Supervised By :mohammad ahmed 09/19/2022

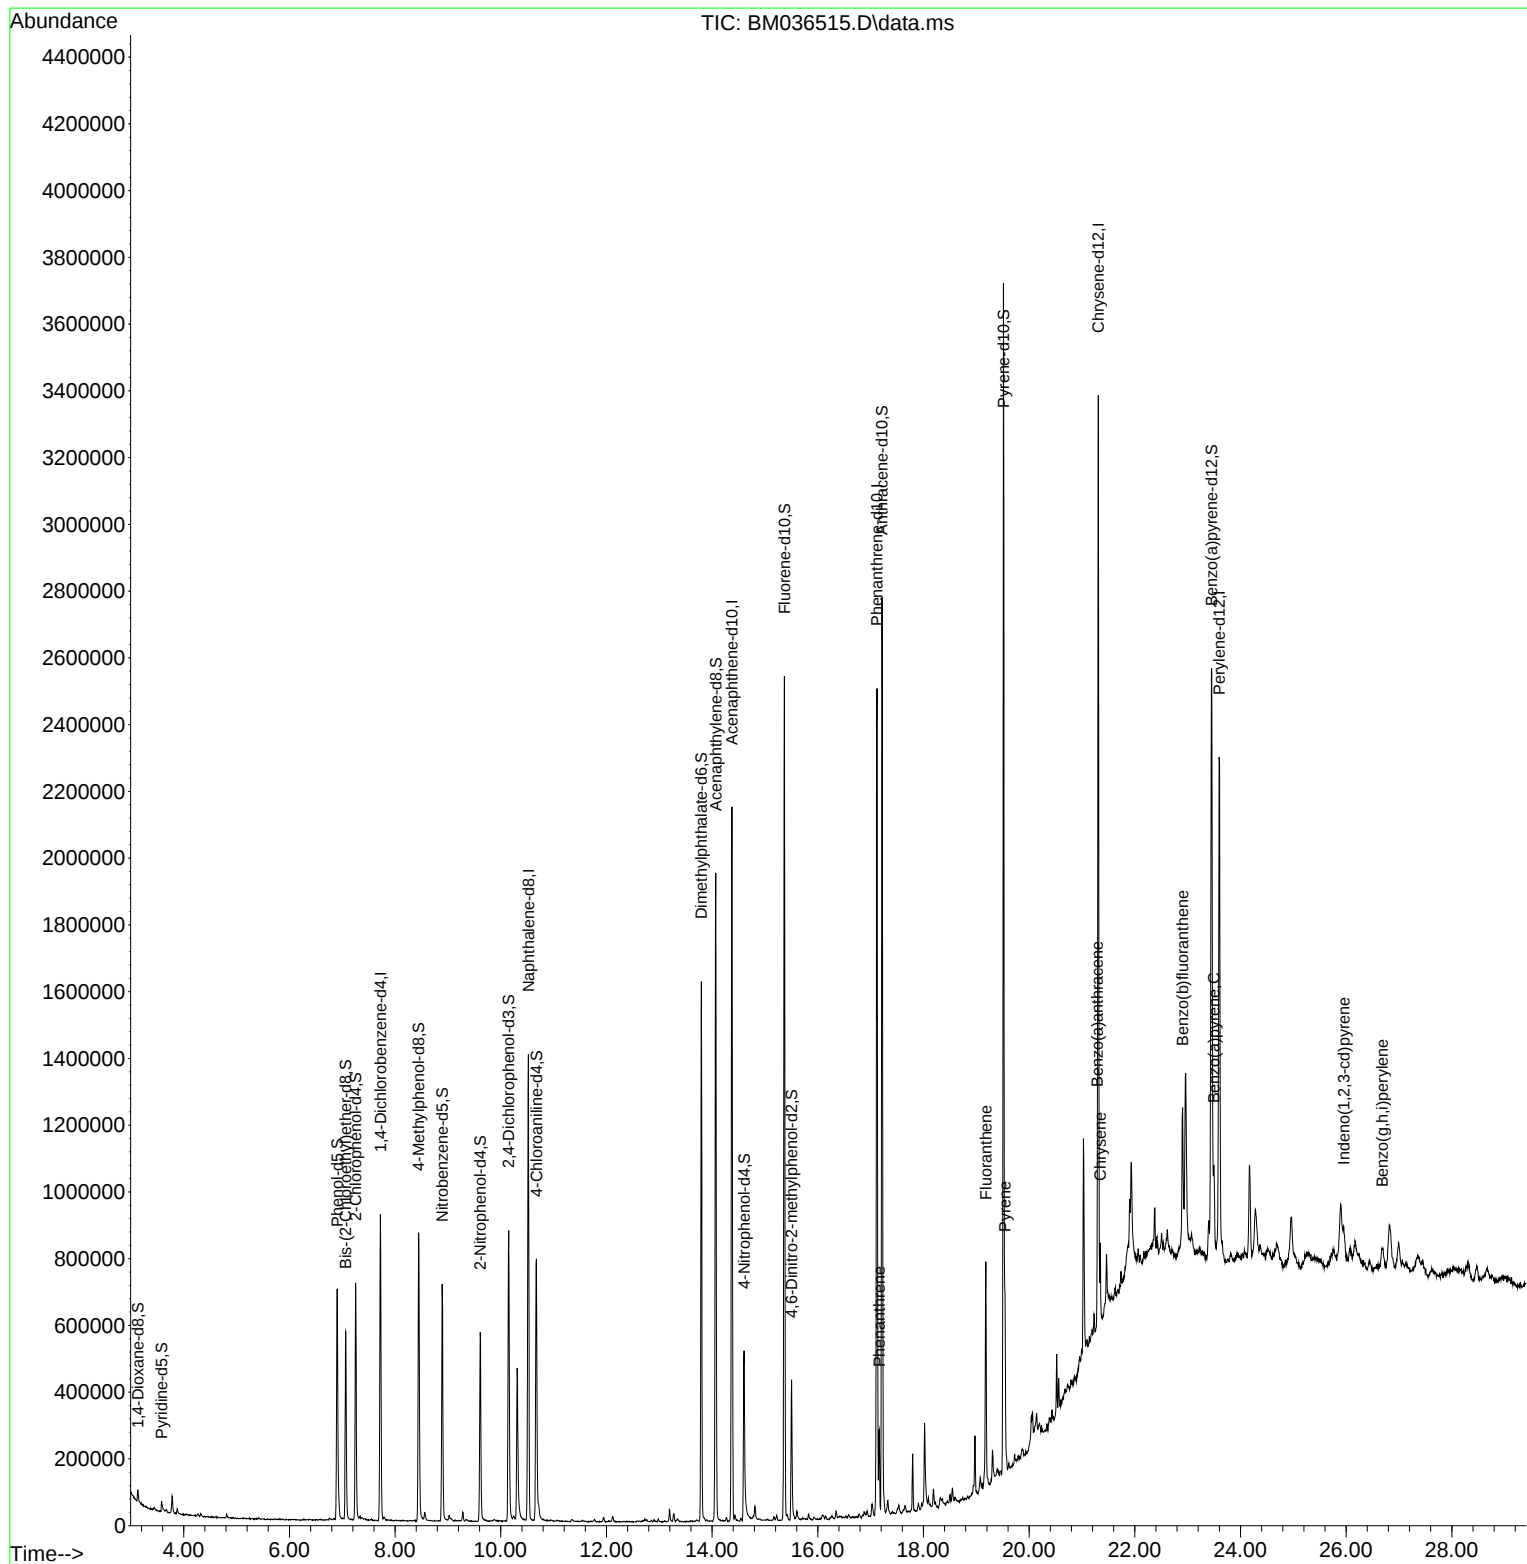

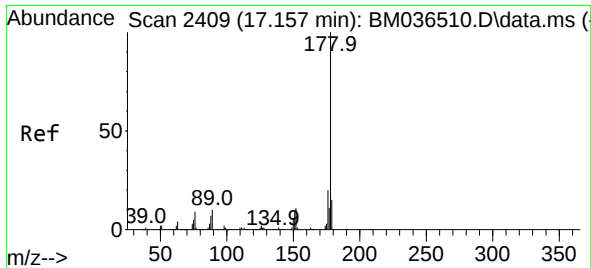

#72
Phenanthrene
Concen: 1.896 ng/ul
RT: 17.162 min Scan# 2409
Delta R.T. -0.000 min
Lab File: BM036515.D
Acq: 07 Sep 2022 18:49




Instrument :
BNA_M
ClientSampleId :
EW363

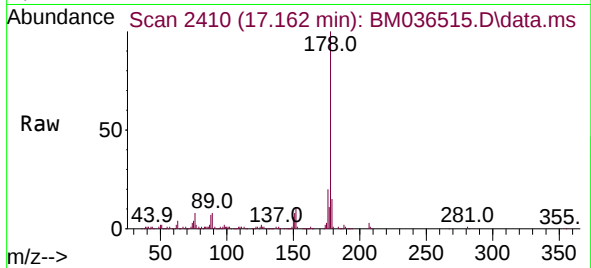


Tgt Ion:178 Resp: 138934
Ion Ratio Lower Upper
178 100
179 15.3 12.2 18.2
176 19.8 14.9 22.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 09/08/2022
Supervised By :mohammad ahmed 09/19/2022

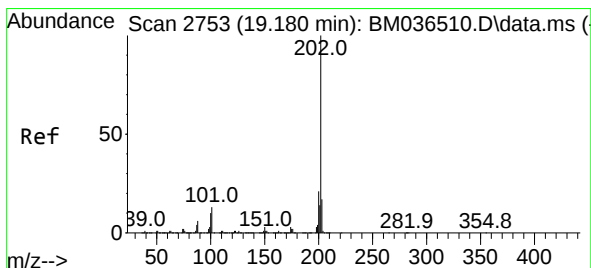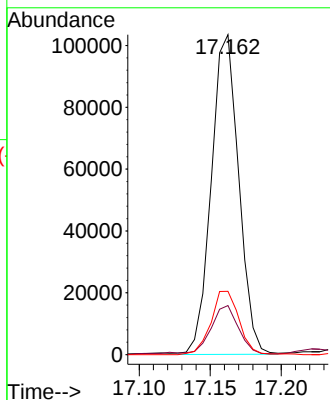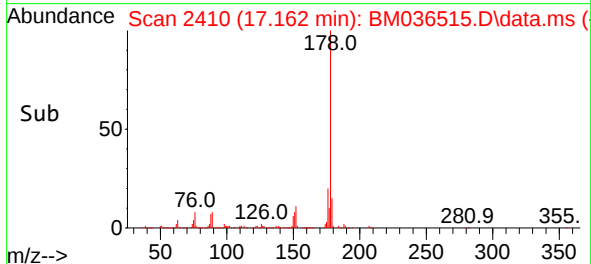


#80
Fluoranthene
Concen: 4.915 ng/ul
RT: 19.180 min Scan# 2753
Delta R.T. -0.006 min
Lab File: BM036515.D
Acq: 07 Sep 2022 18:49

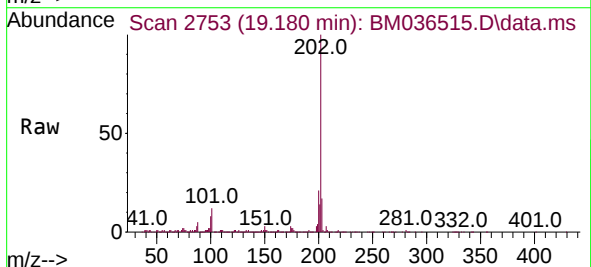

Tgt Ion:202 Resp: 359719
Ion Ratio Lower Upper
202 100
101 11.5 10.1 15.1
100 8.3 7.8 11.6

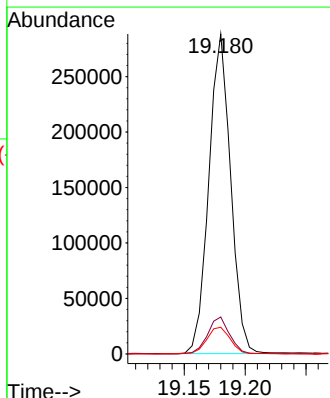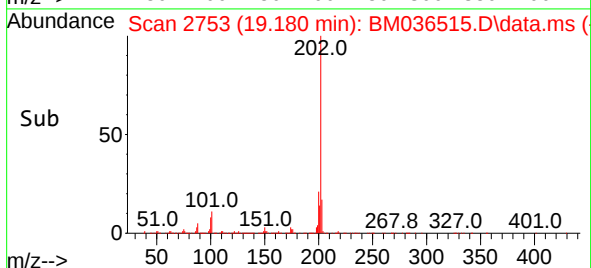

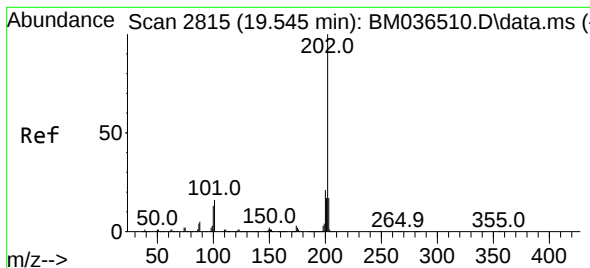

#82

Pyrene

Concen: 3.951 ng/ul

RT: 19.545 min Scan# 2815

Delta R.T. -0.000 min

Lab File: BM036515.D

Acq: 07 Sep 2022 18:49

Instrument :

BNA_M

ClientSampleId :





EW363

Tgt Ion:	202	Resp:	301775
Ion Ratio	Lower	Upper	
202	100		
101	13.5	11.9	17.9
100	10.8	10.2	15.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/08/2022
Supervised By :mohammad ahmed 09/19/2022

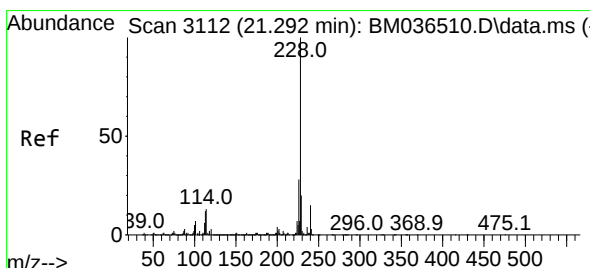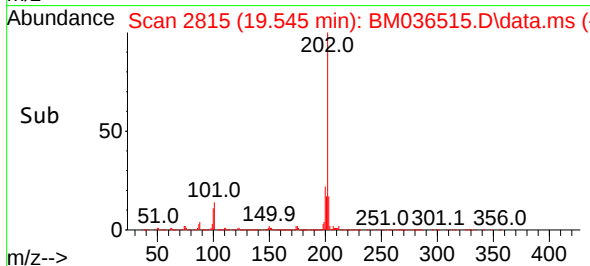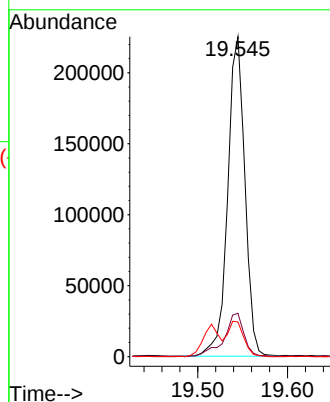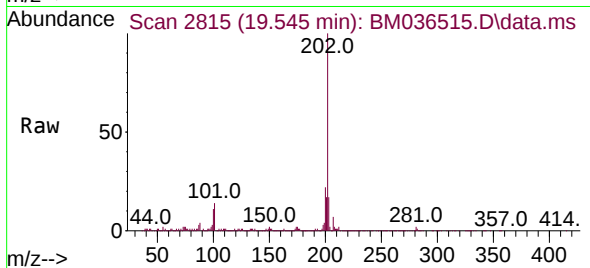

#85

Benzo(a)anthracene

Concen: 1.568 ng/ul




RT: 21.292 min Scan# 3112


Delta R.T. -0.006 min

Lab File: BM036515.D

Acq: 07 Sep 2022 18:49

Tgt Ion:	228	Resp:	109978
Ion Ratio	Lower	Upper	
228	100		
229	21.8	15.6	23.4
226	27.9	21.7	32.5

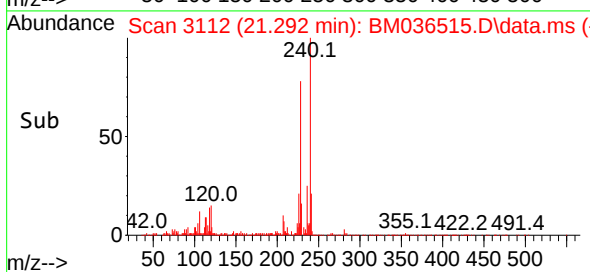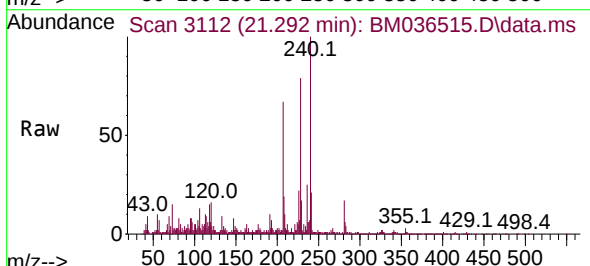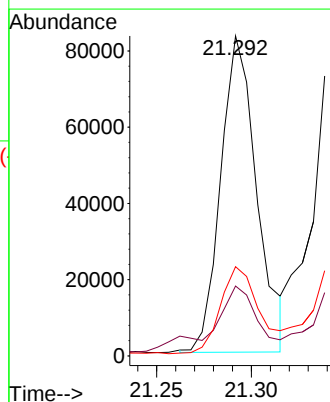

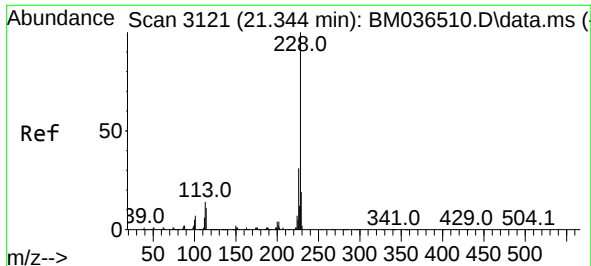





#87
Chrysene
Concen: 1.763 ng/ul
RT: 21.345 min Scan# 3121
Delta R.T. -0.000 min
Lab File: BM036515.D
Acq: 07 Sep 2022 18:49

Instrument :
BNA_M
ClientSampleId :
EW363

Tgt Ion:228 Resp: 12154
Ion Ratio Lower Upper
228 100
226 31.1 23.7 35.5
229 22.7 15.5 23.3




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/08/2022
Supervised By :mohammad ahmed 09/19/2022

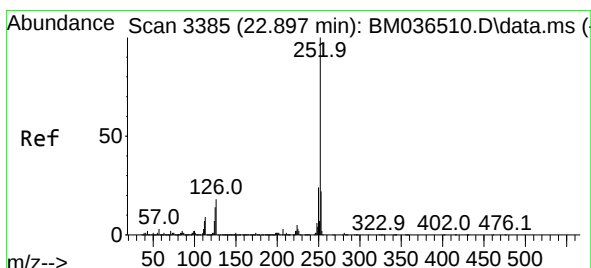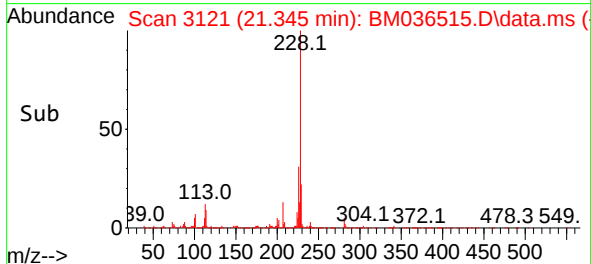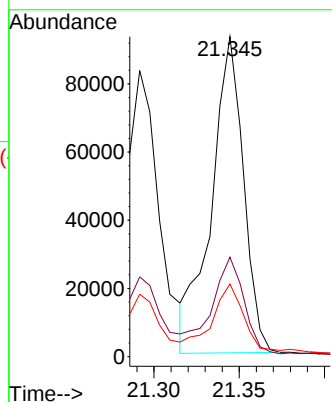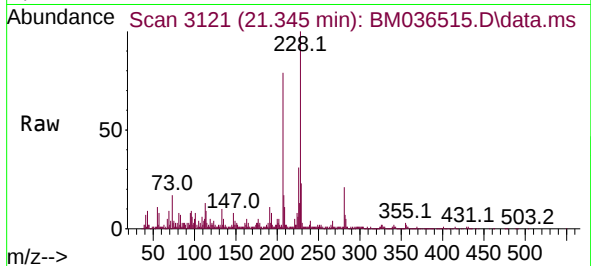

#90
Benzo(b)fluoranthene
Concen: 2.487 ng/ul
RT: 22.903 min Scan# 3386
Delta R.T. -0.006 min
Lab File: BM036515.D
Acq: 07 Sep 2022 18:49

Tgt Ion:252 Resp: 151123
Ion Ratio Lower Upper
252 100
253 24.1 17.5 26.3
125 16.6 10.7 16.1#

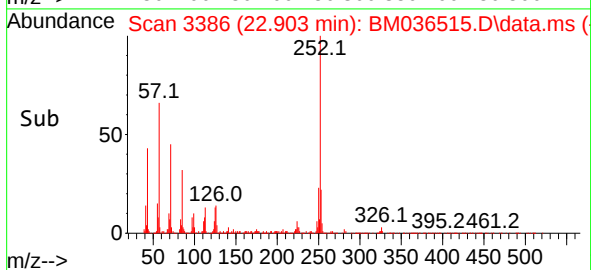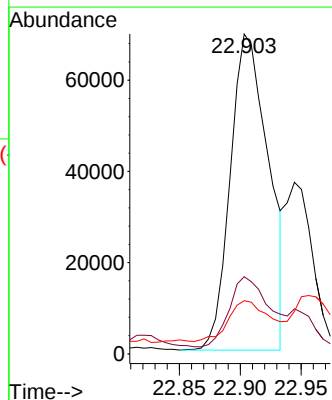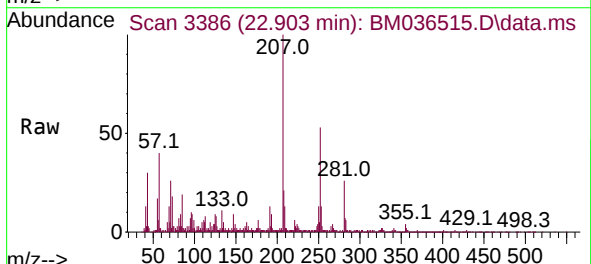

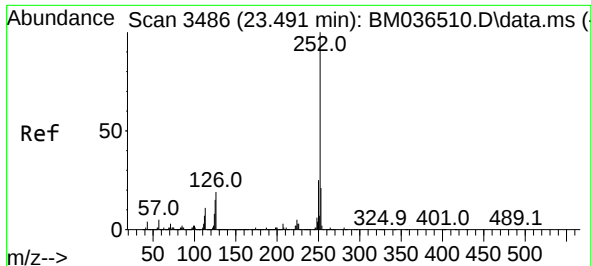





#93
Benzo(a)pyrene
Concen: 1.726 ng/ul
RT: 23.497 min Scan# 3487
Delta R.T. -0.006 min
Lab File: BM036515.D
Acq: 07 Sep 2022 18:49

Instrument : BNA_M
ClientSampleId : EW363

Tgt Ion:252 Resp: 103205
Ion Ratio Lower Upper
252 100
253 24.6 17.3 25.9
125 17.7 11.8 17.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/08/2022
Supervised By :mohammad ahmed 09/19/2022

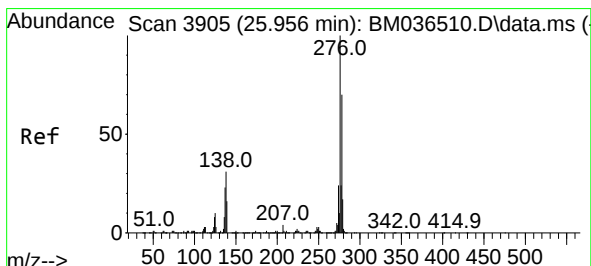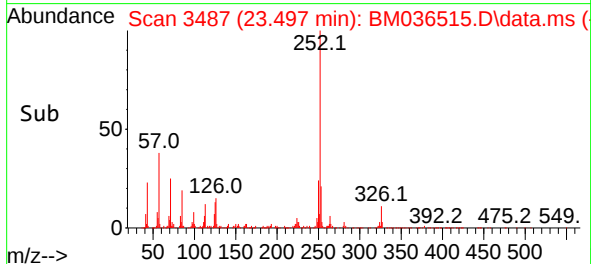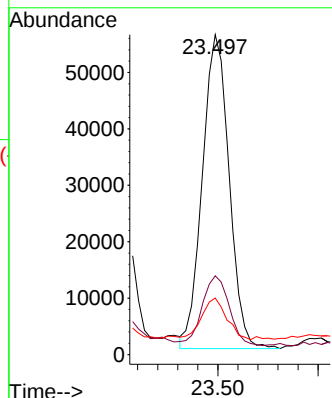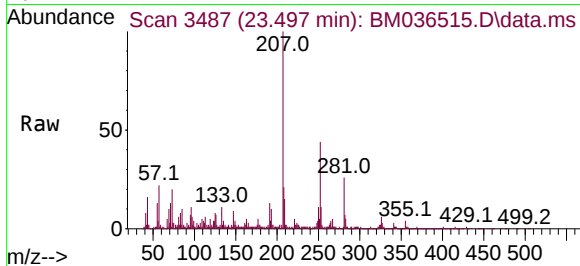

#94
Indeno(1,2,3-cd)pyrene
Concen: 1.003 ng/ul
RT: 25.956 min Scan# 3905
Delta R.T. -0.012 min
Lab File: BM036515.D
Acq: 07 Sep 2022 18:49

Tgt Ion:276 Resp: 70508
Ion Ratio Lower Upper
276 100
138 26.3 25.6 38.4
277 27.5 20.1 30.1

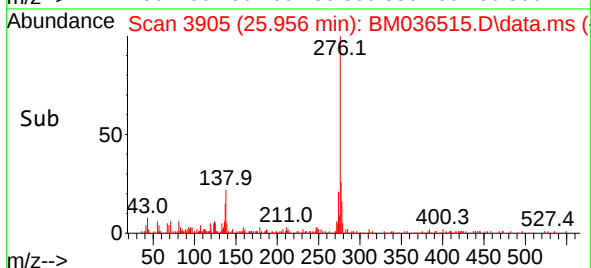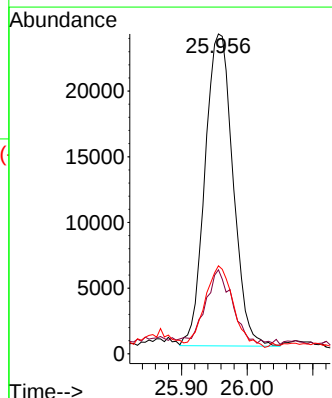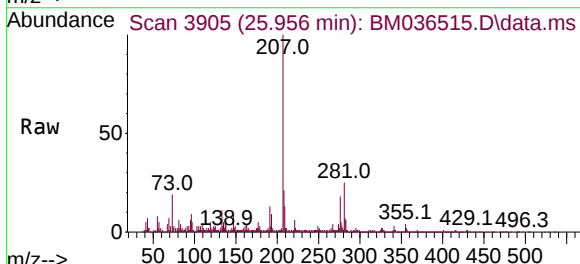

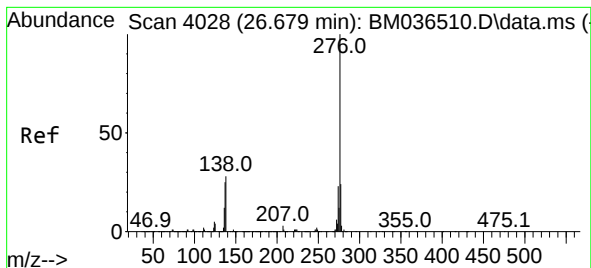

#96

Benzo(g,h,i)perylene

Concen: 1.128 ng/ul

RT: 26.685 min Scan# 40

Delta R.T. -0.012 min

Lab File: BM036515.D


Acq: 07 Sep 2022 18:49

Instrument :

BNA_M

ClientSampleId :

EW363

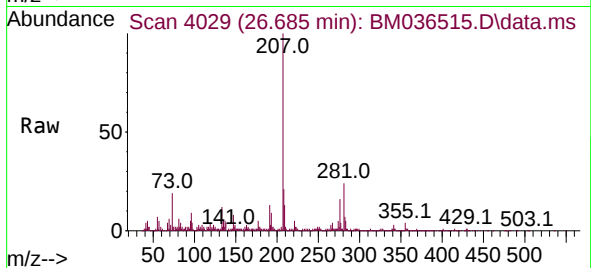

Tgt Ion:	276	Resp:	67800
Ion Ratio	Lower	Upper	
276	100		
138	24.6	21.3	31.9
277	27.2	18.6	28.0

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/08/2022
Supervised By :mohammad ahmed 09/19/2022

