

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090822\
 Data File : BM036516.D
 Acq On : 07 Sep 2022 19:25
 Operator : CG/JU
 Sample : N4483-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW358

Quant Time: Sep 08 00:53:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 02 01:33:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	206395	20.000	ng/u1	0.00
20) Naphthalene-d8	10.522	136	969327	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.374	164	604960	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.115	188	1234061	20.000	ng/u1	0.00
79) Chrysene-d12	21.309	240	987361	20.000	ng/u1	0.00
88) Perylene-d12	23.597	264	817563	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.128	96	19485	3.598	ng/uL	0.00
4) Pyridine-d5	3.558	84	142796	9.561	ng/u1	0.00
7) Phenol-d5	6.904	99	448424	25.453	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	278696	25.132	ng/u1	0.00
11) 2-Chlorophenol-d4	7.251	132	362429	26.183	ng/u1	0.00
15) 4-Methylphenol-d8	8.445	113	373321	28.380	ng/u1	0.00
21) Nitrobenzene-d5	8.892	128	189800	25.826	ng/u1	0.00
24) 2-Nitrophenol-d4	9.610	143	202963	27.226	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.151	165	365144	27.413	ng/u1	0.00
31) 4-Chloroaniline-d4	10.675	131	372297	18.029	ng/u1	0.00
46) Dimethylphthalate-d6	13.798	166	1142474	29.851	ng/u1	0.00
49) Acenaphthylene-d8	14.069	160	1359299	28.476	ng/u1	0.00
54) 4-Nitrophenol-d4	14.604	143	179197	24.710	ng/u1	0.00
60) Fluorene-d10	15.369	176	1036579	29.973	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.504	200	116238	18.321	ng/u1	0.00
73) Anthracene-d10	17.215	188	1568662	28.587	ng/u1	0.00
81) Pyrene-d10	19.515	212	1725174	33.683	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.450	264	1183766	29.532	ng/u1	0.00
Target Compounds						
					Qvalue	
80) Fluoranthene	19.180	202	70791	1.144	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090822\
Data File : BM036516.D
Acq On : 07 Sep 2022 19:25
Operator : CG/JU
Sample : N4483-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW358

Quant Time: Sep 08 00:53:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 02 01:33:23 2022
Response via : Initial Calibration

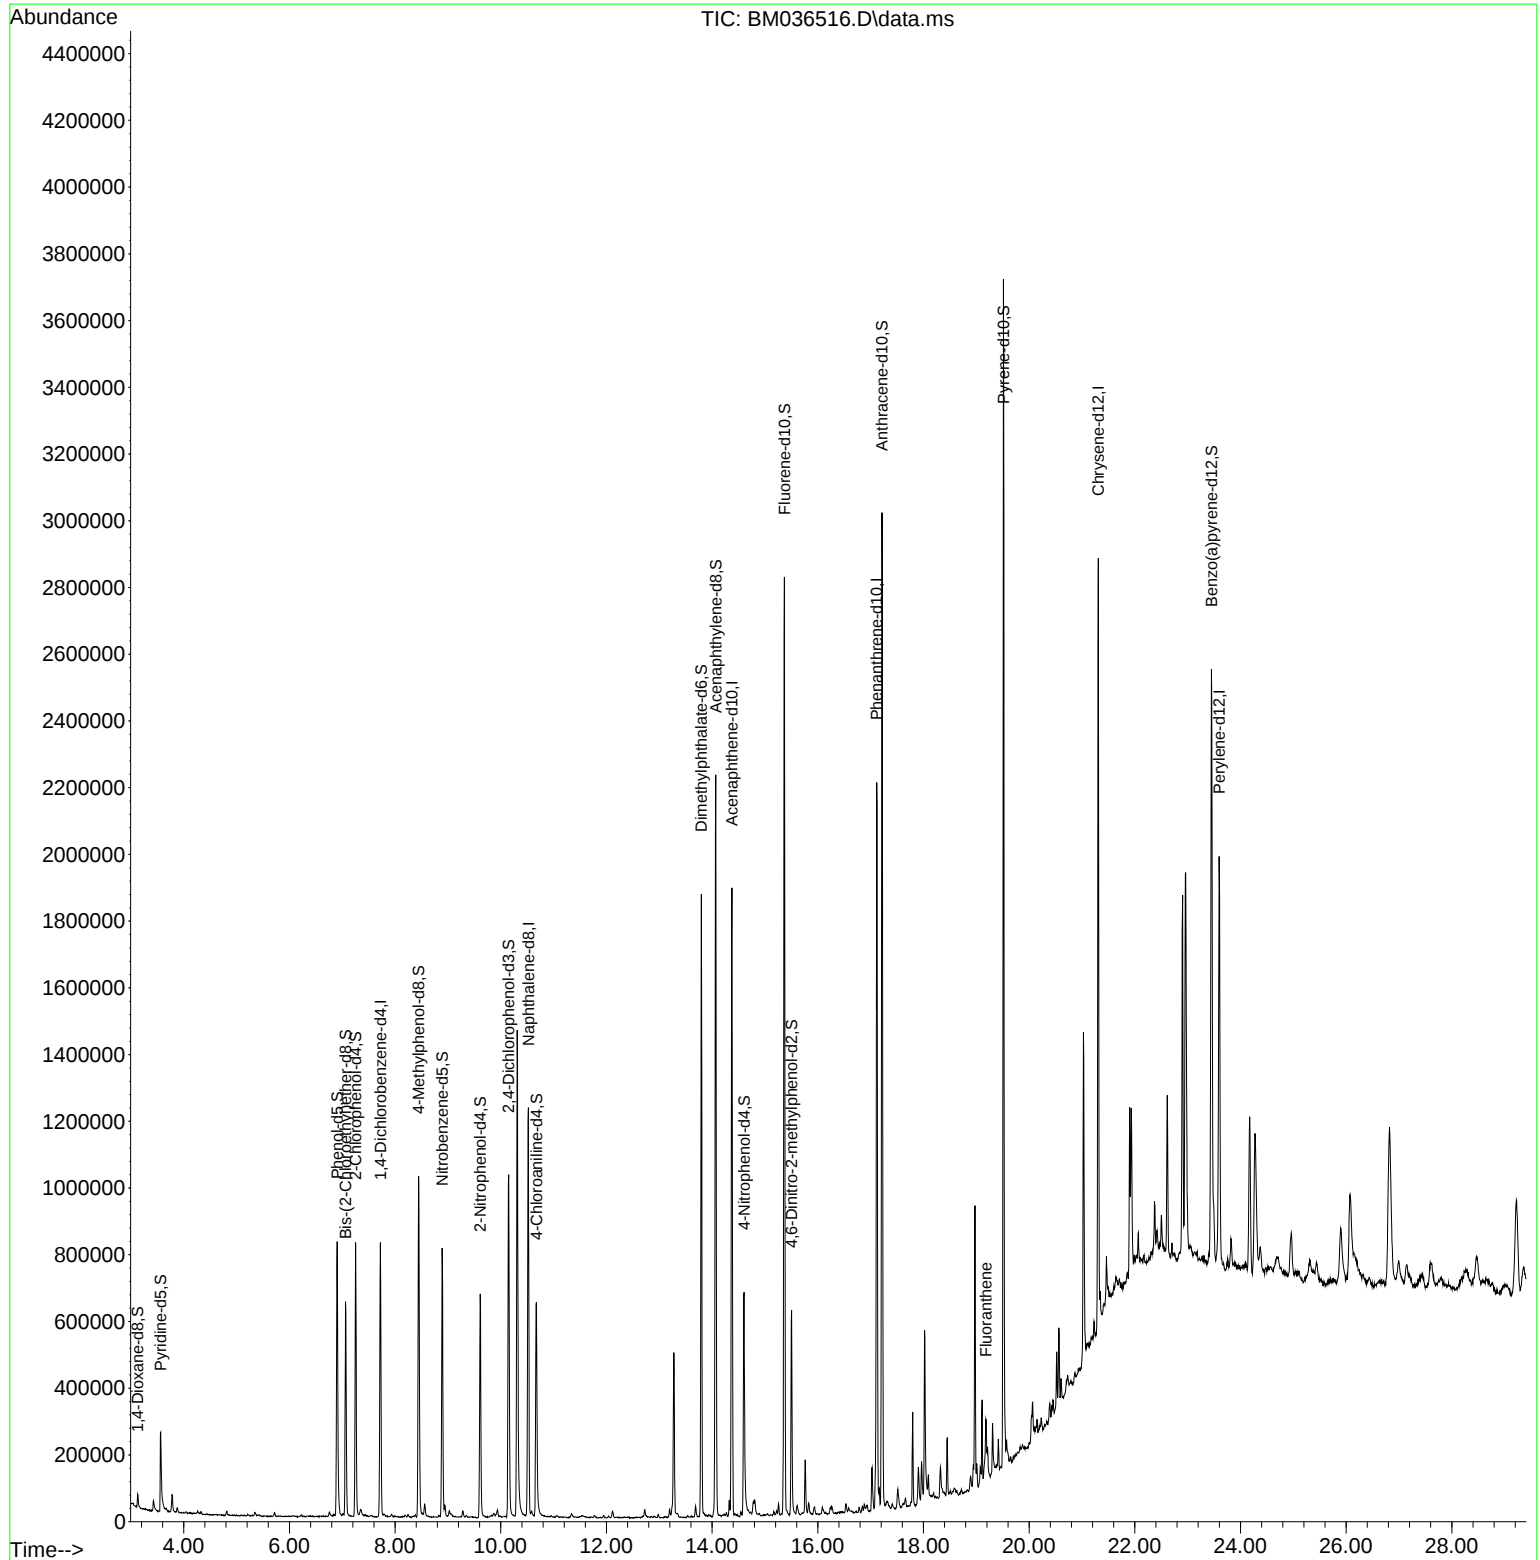

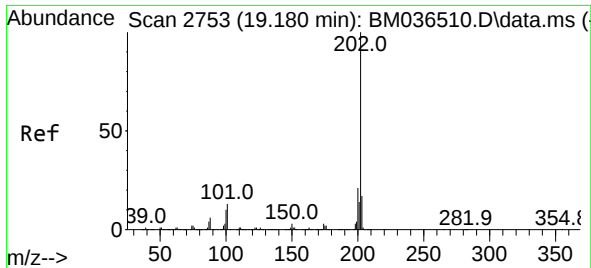

#80
 Fluoranthene
 Concen: 1.144 ng/ul
 RT: 19.180 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM036516.D
 Acq: 07 Sep 2022 19:25

Instrument :
 BNA_M
 ClientSampleId :
 EW358

Tgt Ion	Ratio	Lower	Upper
202	100		
101	11.3	10.1	15.1
100	9.7	7.8	11.6

