

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090822\
 Data File : BM036526.D
 Acq On : 08 Sep 2022 11:09
 Operator : CG/JU
 Sample : PB147480BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK480

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	21	24	29	rVB	62108	78654	1.41%	0.138%
2	3.552	94	96	116	rBV	785343	1322390	23.78%	2.319%
3	3.875	148	151	156	rVB2	14530	21579	0.39%	0.038%
4	6.898	659	665	683	rBV	903468	1426349	25.65%	2.501%
5	7.063	686	693	708	rVB	757418	1151481	20.71%	2.019%
6	7.251	717	725	742	rBV	931139	1474166	26.51%	2.585%
7	7.716	798	804	815	rBV	694398	1107132	19.91%	1.941%
8	8.445	920	928	949	rBV	1103431	1835168	33.00%	3.218%
9	8.892	996	1004	1015	rBV	898509	1488498	26.77%	2.610%
10	9.610	1119	1126	1138	rBV	758982	1260763	22.67%	2.211%
11	10.145	1209	1217	1234	rBV	1111299	1874845	33.72%	3.288%
12	10.516	1273	1280	1290	rBV	1090177	1739190	31.28%	3.050%
13	10.669	1298	1306	1330	rBV	1144476	1982065	35.64%	3.476%
14	12.122	1546	1553	1560	rBV	16430	30816	0.55%	0.054%
15	13.345	1758	1761	1766	rVB6	3594	5644	0.10%	0.010%
16	13.792	1830	1837	1848	rBV	2145392	2902470	52.20%	5.090%
17	14.063	1876	1883	1894	rBV	2592546	3624876	65.19%	6.356%
18	14.369	1929	1935	1943	rBV	1787210	2509506	45.13%	4.400%
19	14.598	1968	1974	1995	rBV	848631	1447262	26.03%	2.538%
20	15.363	2096	2104	2117	rBV	3412890	4688571	84.31%	8.221%
21	15.498	2122	2127	2140	rVV	982430	1364190	24.53%	2.392%
22	15.604	2142	2145	2150	rVB2	16247	22528	0.41%	0.040%
23	16.580	2307	2311	2317	rVB4	5376	6736	0.12%	0.012%
24	17.115	2396	2402	2410	rBV	2140468	2789214	50.16%	4.891%
25	17.215	2413	2419	2430	rVV	3642241	4827488	86.81%	8.465%
26	19.074	2731	2735	2742	rBV3	38132	54490	0.98%	0.096%
27	19.151	2743	2748	2754	rBV	38591	56950	1.02%	0.100%
28	19.515	2803	2810	2823	rBV	4166186	5560789	100.00%	9.751%
29	20.521	2977	2981	2987	rBV	121580	146005	2.63%	0.256%
30	21.303	3109	3114	3121	rBV	2523767	3089340	55.56%	5.417%
31	23.450	3472	3479	3494	rVB2	2384382	4611504	82.93%	8.086%
32	23.591	3497	3503	3513	rVB2	1320068	2527889	45.46%	4.433%




Sum of corrected areas: 57028548

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090822\
Data File : BM036526.D
Acq On : 08 Sep 2022 11:09
Operator : CG/JU
Sample : PB147480BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK480

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

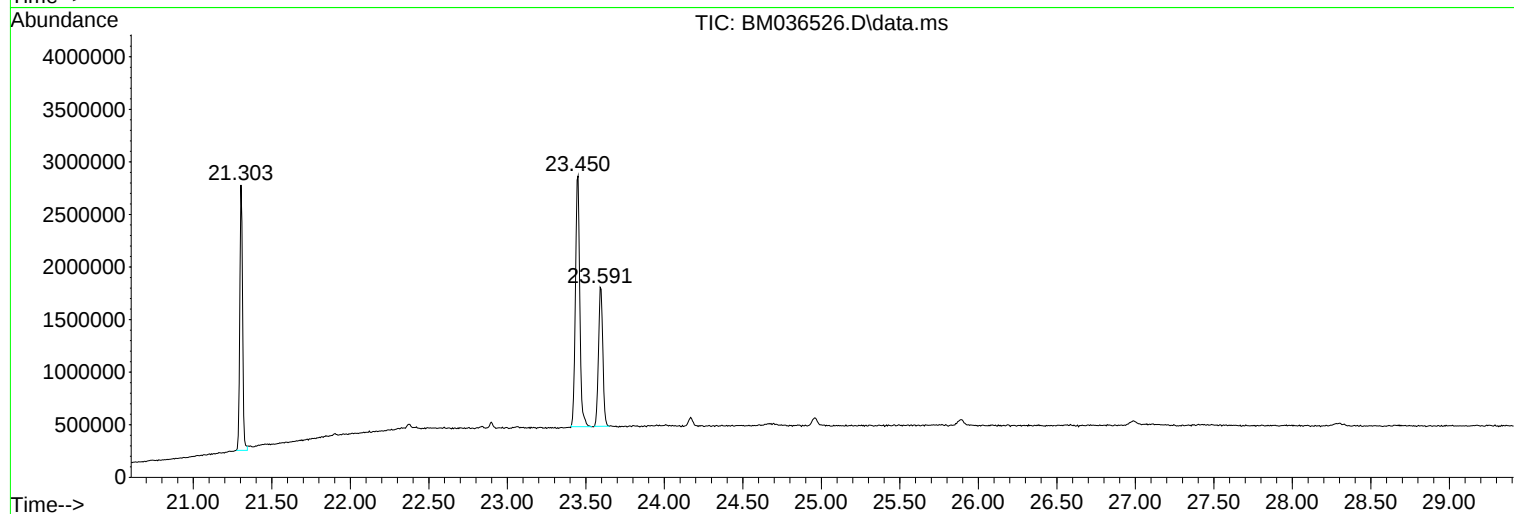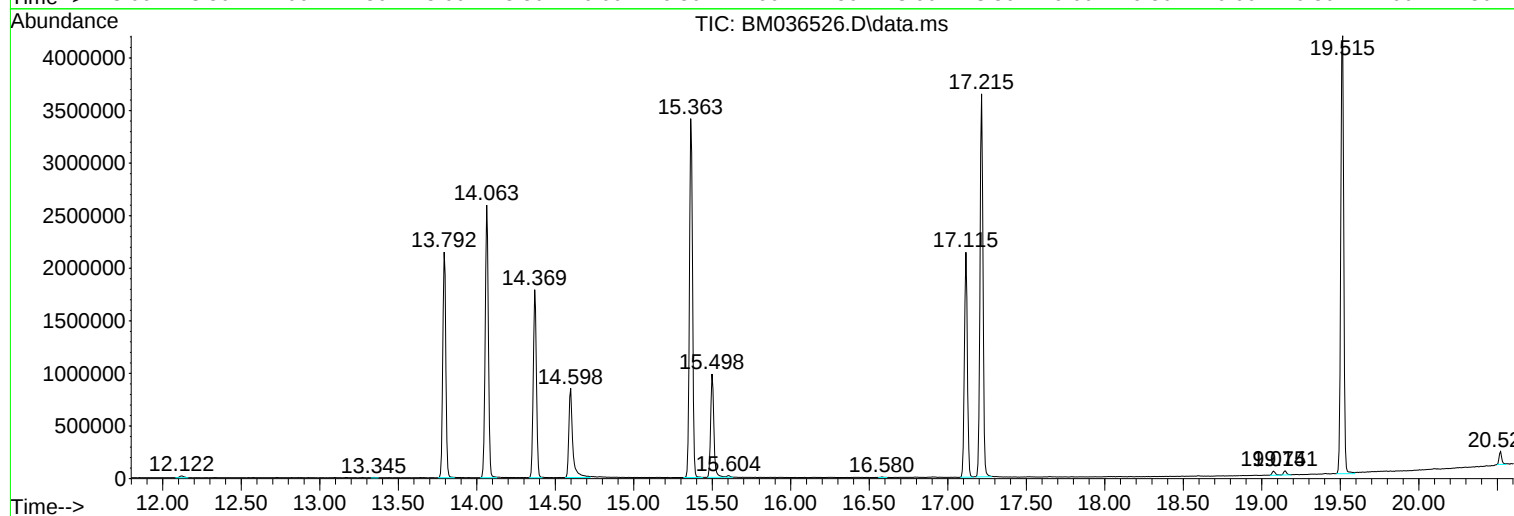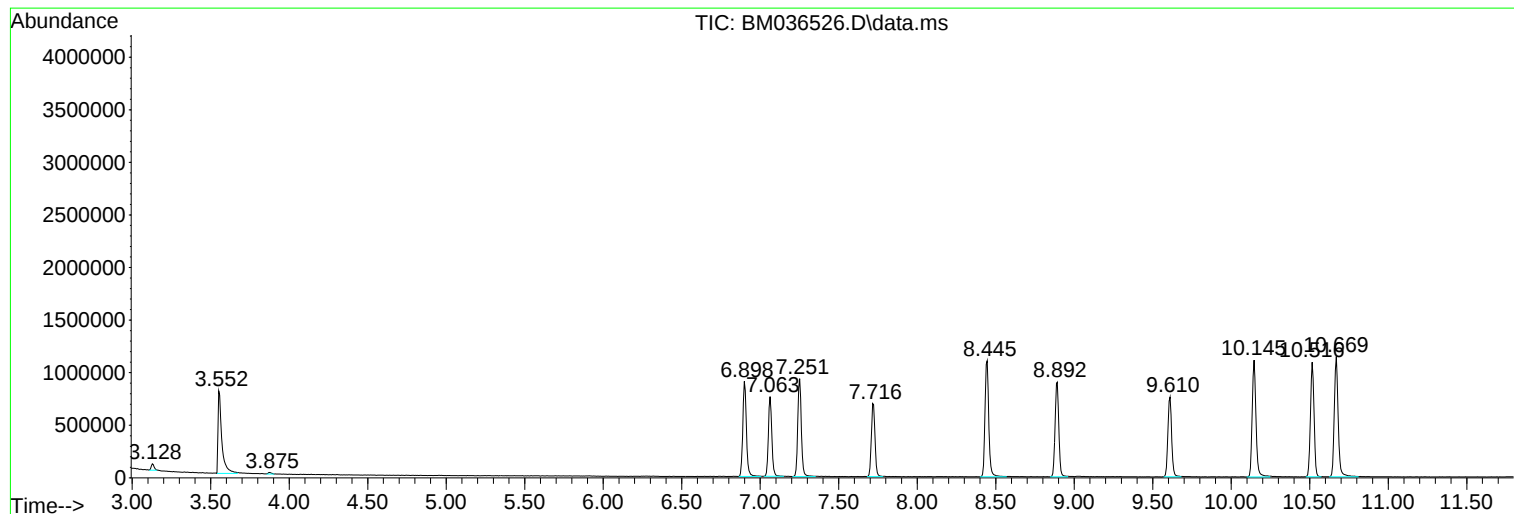

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090822\
Data File : BM036526.D
Acq On : 08 Sep 2022 11:09
Operator : CG/JU
Sample : PB147480BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK480

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090822\
Data File : BM036526.D
Acq On : 08 Sep 2022 11:09
Operator : CG/JU
Sample : PB147480BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK480

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc