

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
 Data File : BM041733.D
 Acq On : 08 Sep 2023 16:42
 Operator : MA/JU
 Sample : PB155206BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 09 00:26:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	5182	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	12443	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.634	164	5480	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.388	188	10057	0.400	ng/ul	0.00
17) Chrysene-d12	21.553	240	4024	0.400	ng/ul	0.00
23) Perylene-d12	23.979	264	4989	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	35938	4.538	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152	3910	0.244	ng/ul	0.00
18) Fluoranthene-d10	19.403	212	4929	0.253	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.628	166	1723	0.058	ng/ul#	16
20) Pyrene	19.775	202	1643	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.822	252	3027	0.083	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
Data File : BM041733.D
Acq On : 08 Sep 2023 16:42
Operator : MA/JU
Sample : PB155206BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 09 00:26:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration




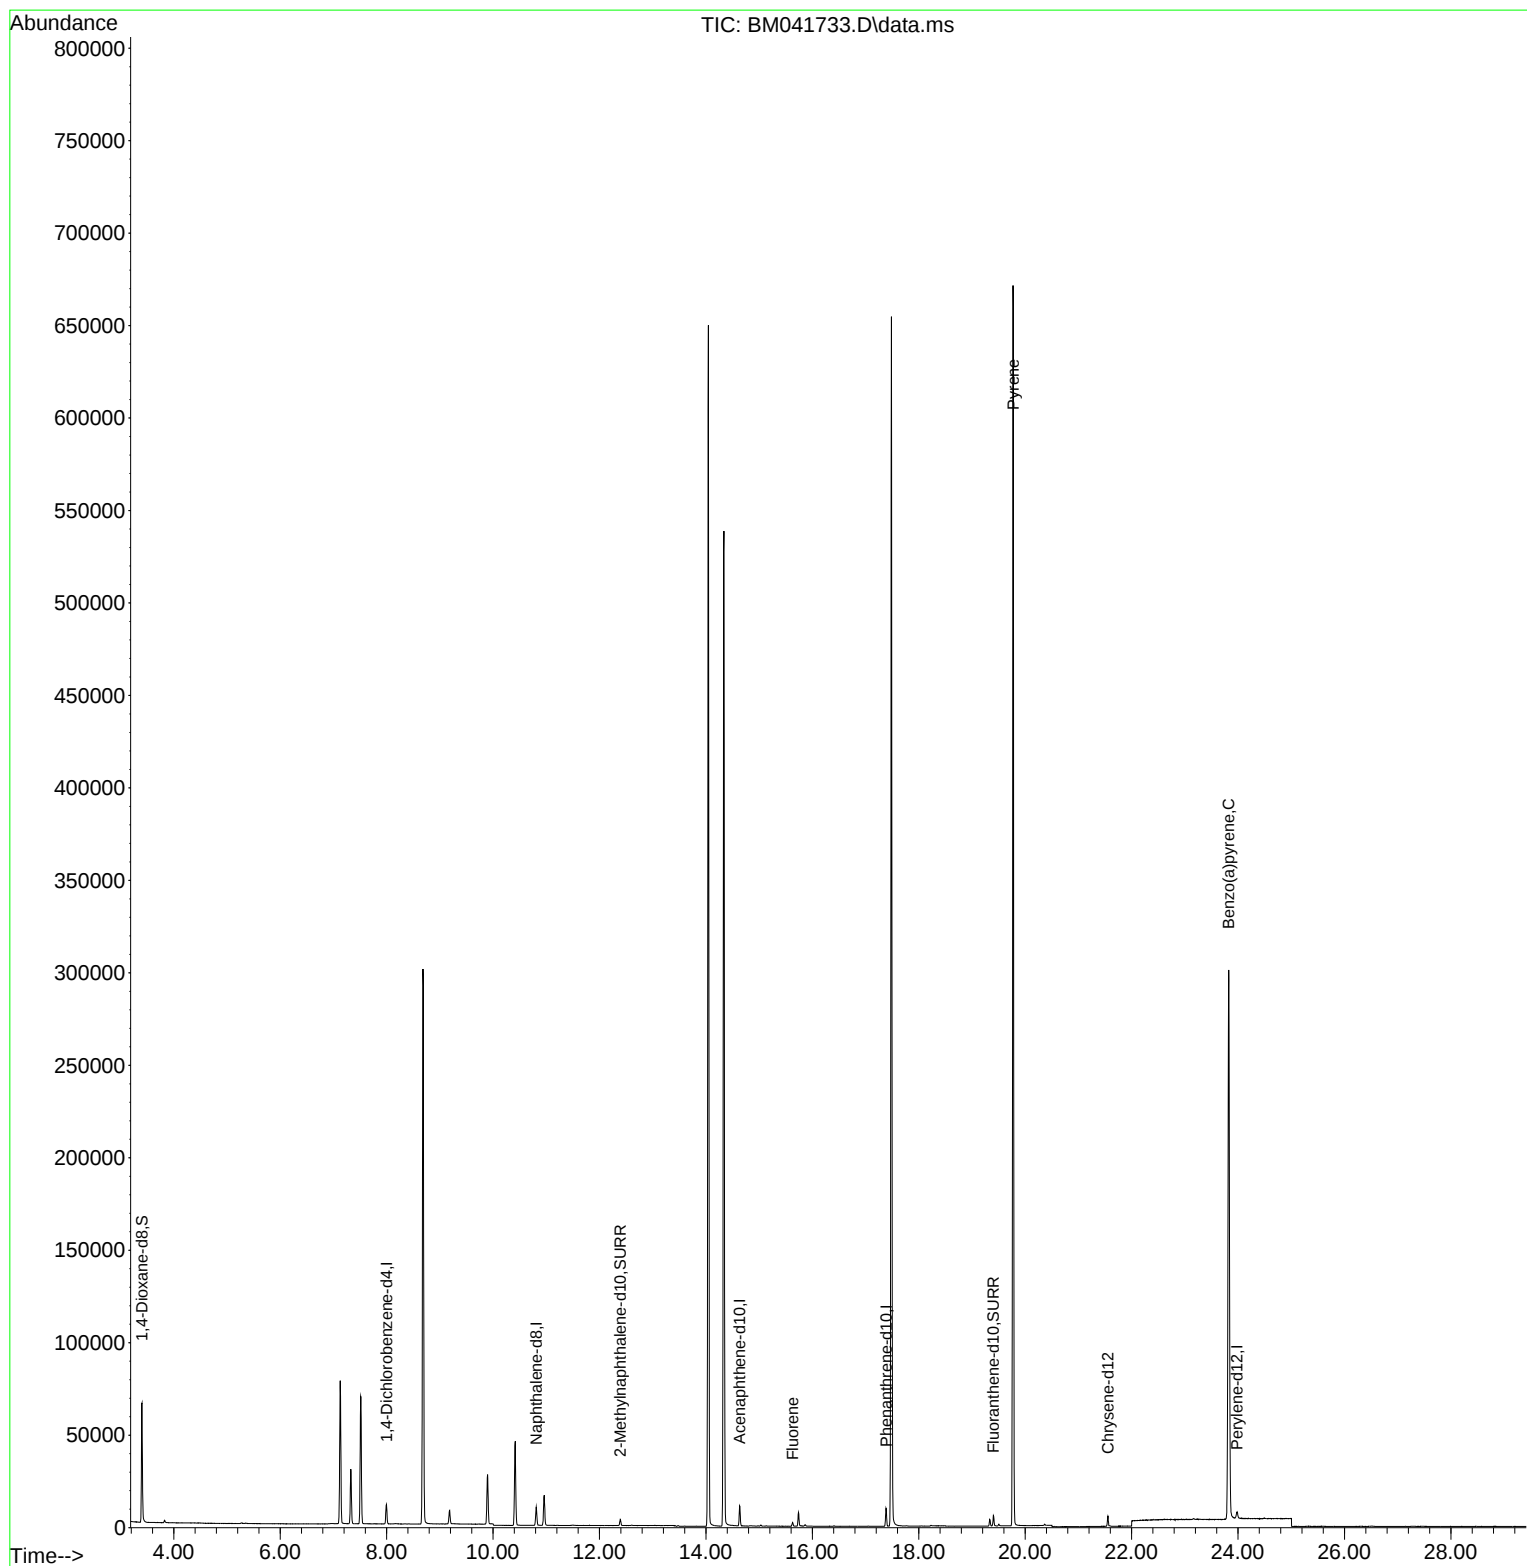


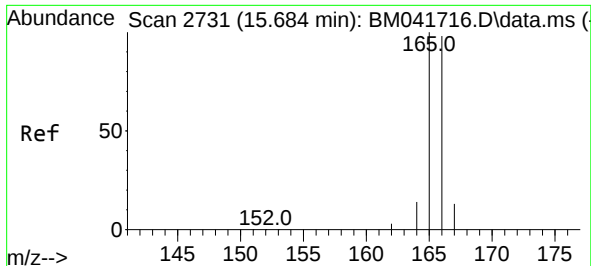

#12
Fluorene
Concen: 0.058 ng/ul
RT: 15.628 min Scan# 21
Delta R.T. -0.056 min
Lab File: BM041733.D
Acq: 08 Sep 2023 16:42




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:166 Resp: 1723
Ion Ratio Lower Upper
166 100
165 11.6 79.4 119.2#
167 36.3 11.3 16.9#

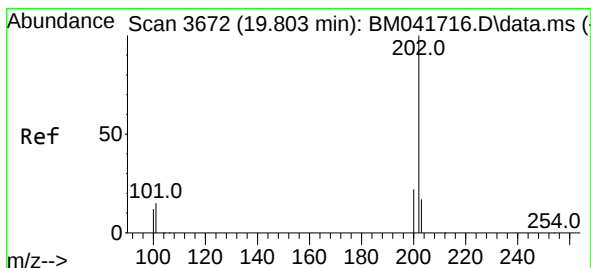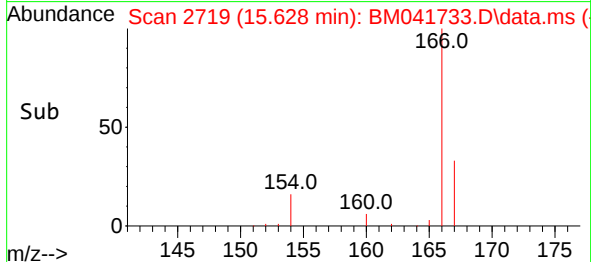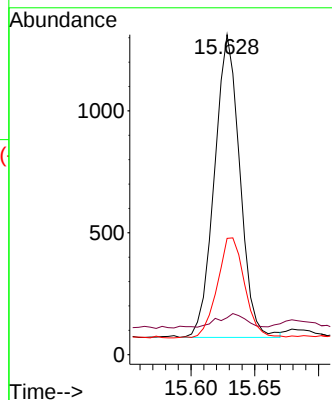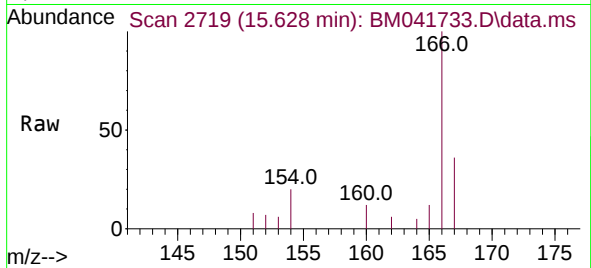

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.775 min Scan# 3666
Delta R.T. -0.028 min
Lab File: BM041733.D
Acq: 08 Sep 2023 16:42


Tgt Ion:202 Resp: 1643
Ion Ratio Lower Upper
202 100
101 169.6 11.8 17.8#
100 1160.0 9.8 14.6#

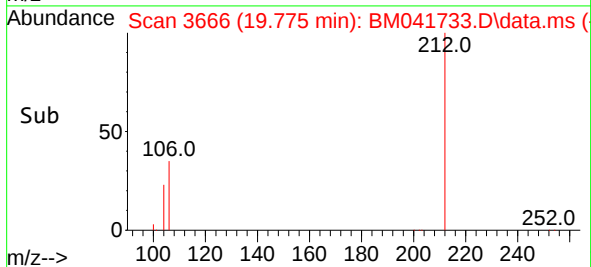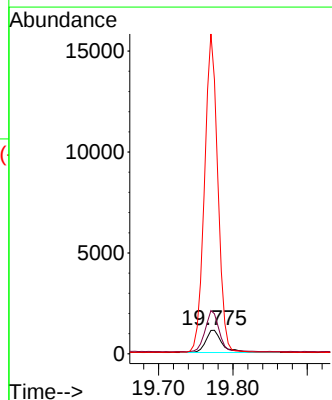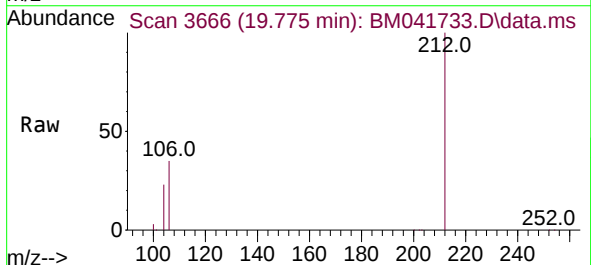

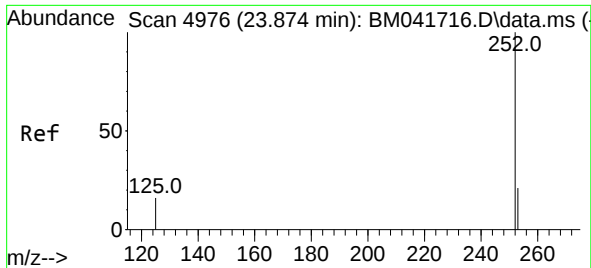

#26
Benzo(a)pyrene
Concen: 0.083 ng/ul
RT: 23.822 min Scan# 49
Delta R.T. -0.053 min
Lab File: BM041733.D
Acq: 08 Sep 2023 16:42

Instrument :
BNA_M
ClientSampleId :

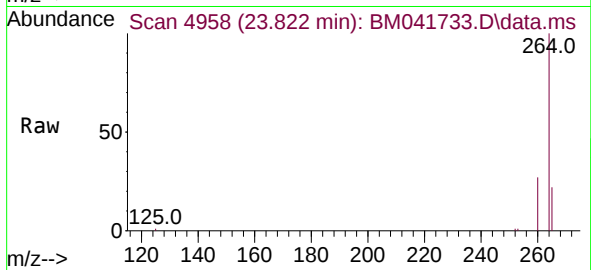

Tgt Ion:252 Resp: 3027
Ion Ratio Lower Upper
252 100
253 53.2 22.4 33.6#
125 58.8 21.0 31.4#

