

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
 Data File : BM041749.D
 Acq On : 09 Sep 2023 03:24
 Operator : MA/JU
 Sample : PB155276BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 09 05:08:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.992	152	4309	0.400	ng/ul	0.00
4) Naphthalene-d8	10.807	136	9998	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.634	164	4383	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.383	188	8003	0.400	ng/ul	0.00
17) Chrysene-d12	21.550	240	2960	0.400	ng/ul	0.00
23) Perylene-d12	23.974	264	3736	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	37041	5.625	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152	3518	0.273	ng/ul	0.00
18) Fluoranthene-d10	19.403	212	4246	0.296	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.628	166	1694	0.072	ng/ul#	16
20) Pyrene	19.770	202	1543	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.816	252	2960	0.109	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
Data File : BM041749.D
Acq On : 09 Sep 2023 03:24
Operator : MA/JU
Sample : PB155276BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 09 05:08:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

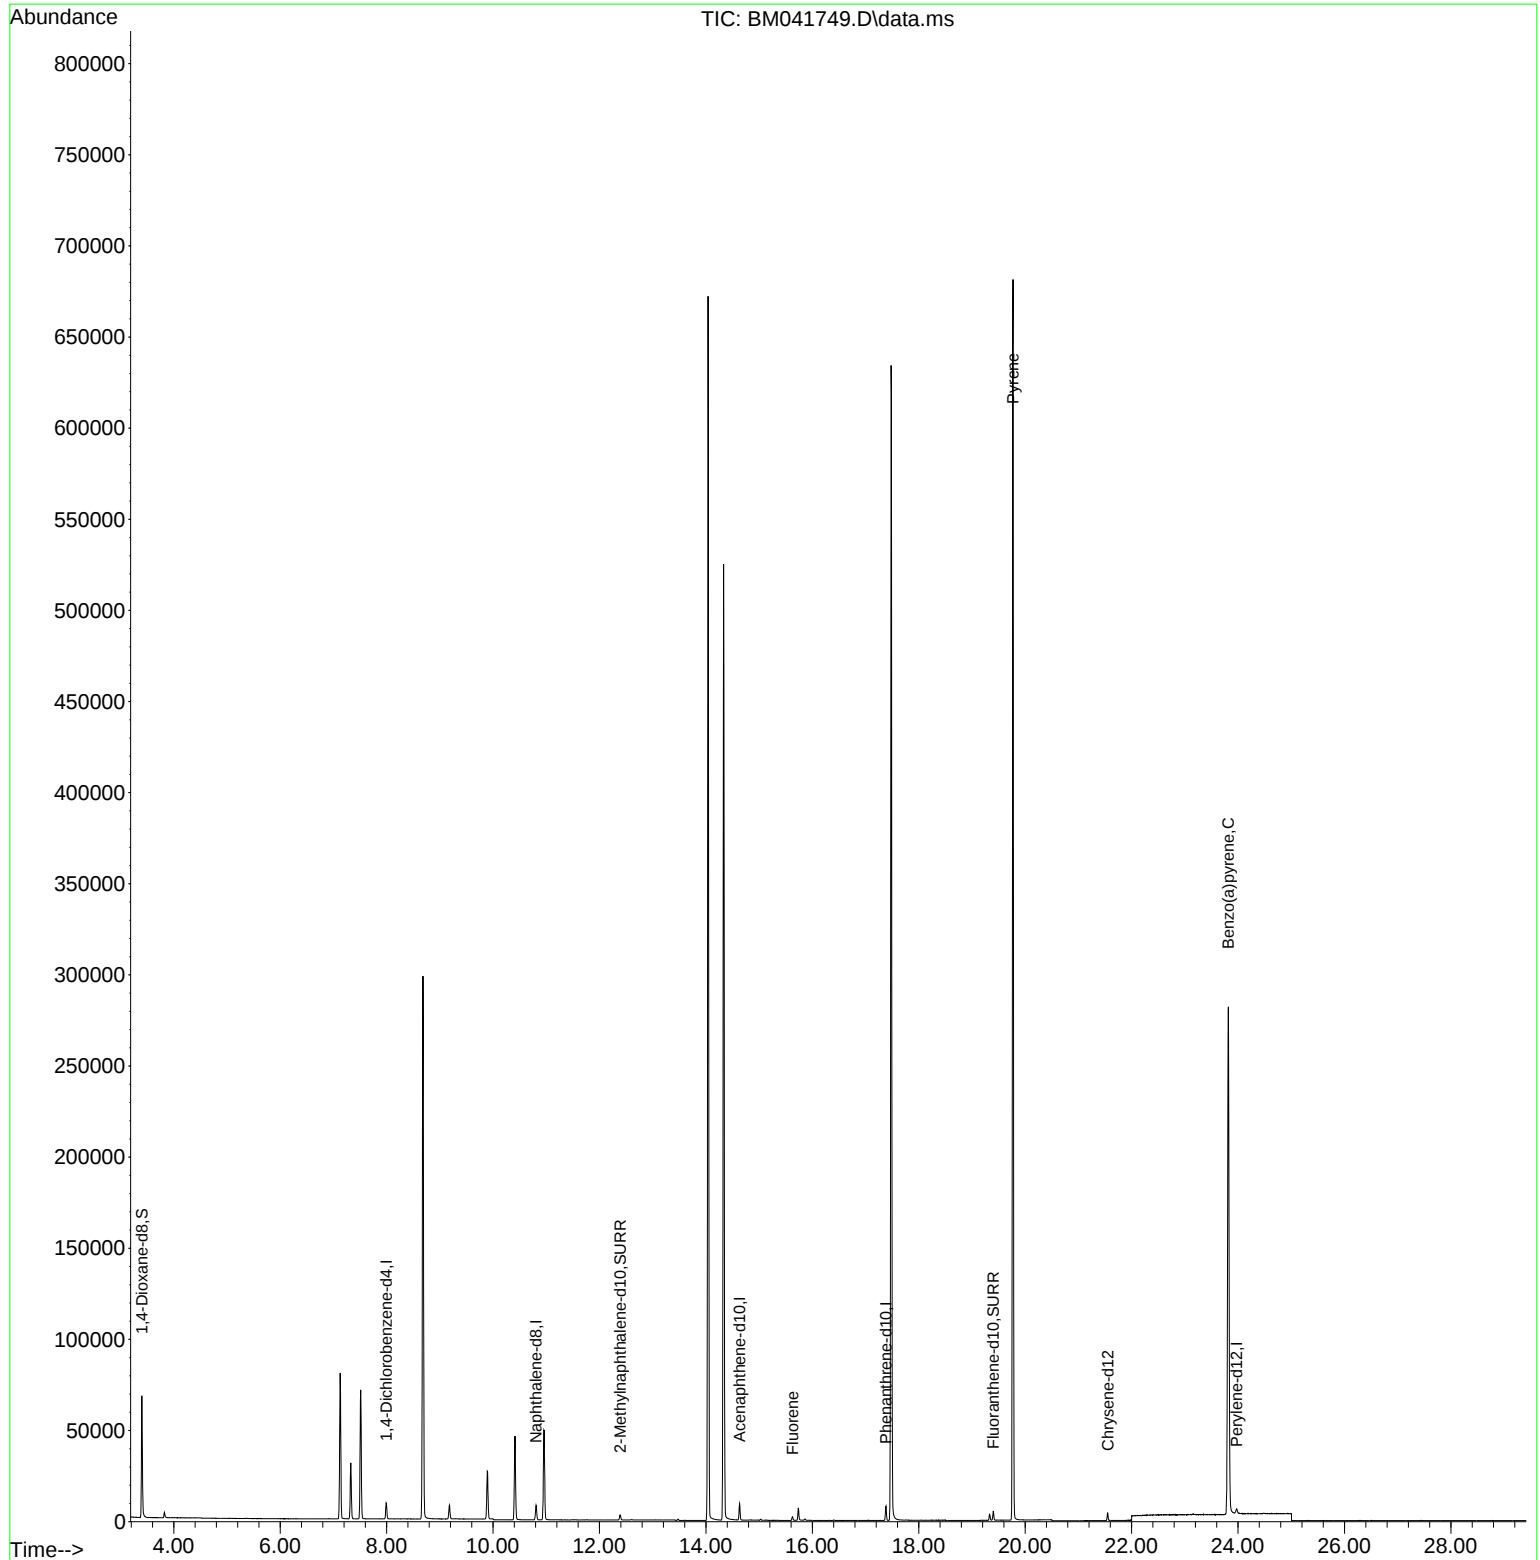

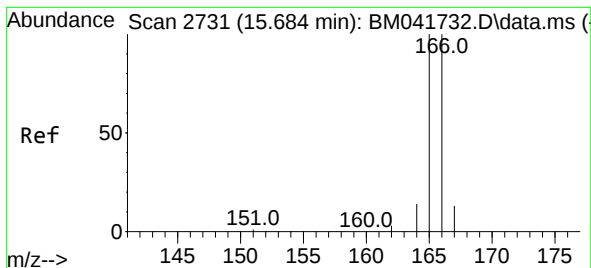

#12

Fluorene

Concen: 0.072 ng/ul

RT: 15.628 min Scan# 21

Delta R.T. -0.055 min

Lab File: BM041749.D





Acq: 09 Sep 2023 03:24

Instrument :

BNA_M

ClientSampleId :

Tgt Ion:166	Resp:	1694
Ion Ratio	Lower	Upper
166	100	
165	11.7	79.4 119.2#
167	36.6	11.3 16.9#

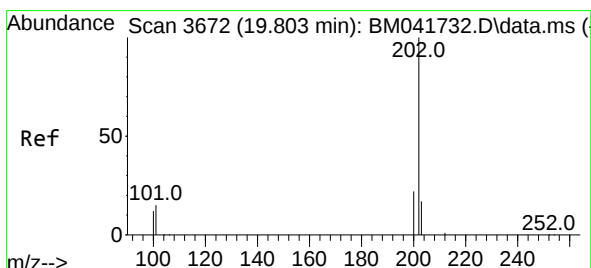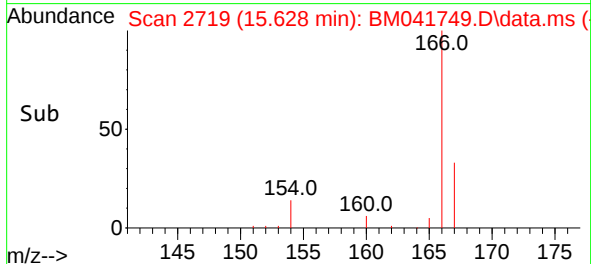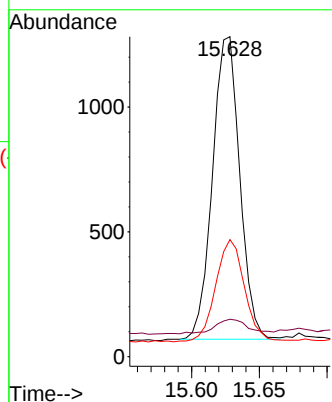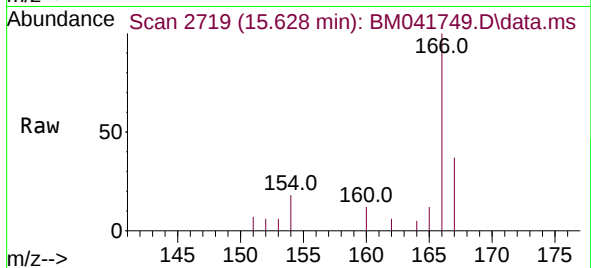

#20

Pyrene

Concen: 0.044 ng/ul




RT: 19.770 min Scan# 3665


Delta R.T. -0.033 min

Lab File: BM041749.D

Acq: 09 Sep 2023 03:24

Tgt Ion:202	Resp:	1543
Ion Ratio	Lower	Upper
202	100	
101	172.1	11.8 17.8#
100	1240.9	9.8 14.6#

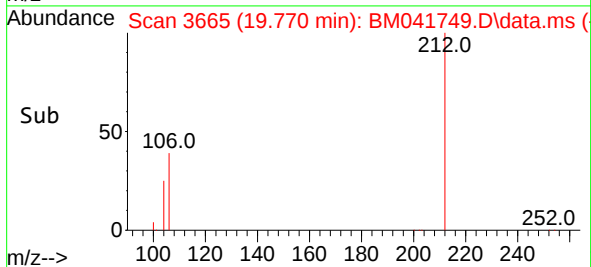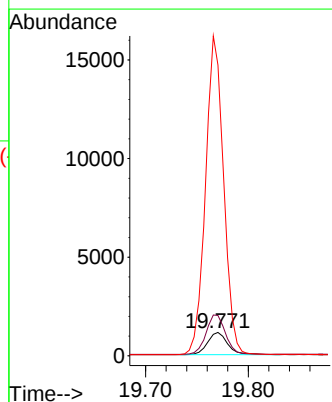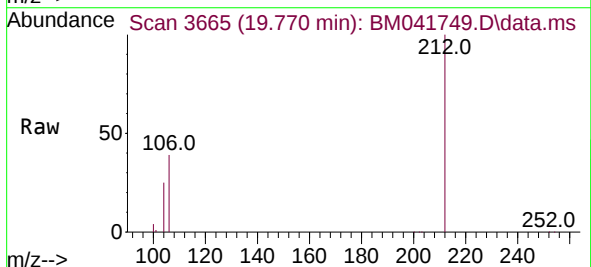

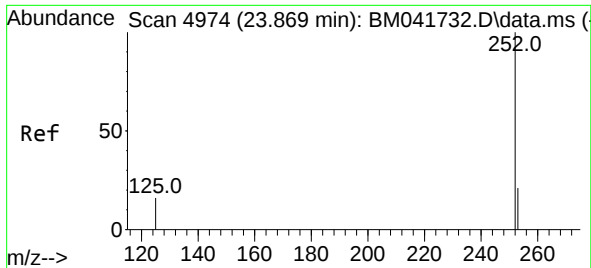

#26

Benzo(a)pyrene

Concen: 0.109 ng/ul

RT: 23.816 min Scan# 49

Delta R.T. -0.058 min


Lab File: BM041749.D

Acq: 09 Sep 2023 03:24

Instrument :

BNA_M

ClientSampleId :

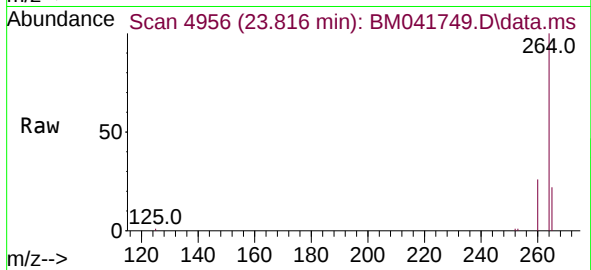

Tgt Ion:252 Resp: 2960

Ion Ratio Lower Upper

252 100

253 49.8 22.4 33.6#

125 57.8 21.0 31.4#

