




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
 Data File : BM041744.D
 Acq On : 08 Sep 2023 23:40
 Operator : MA/JU
 Sample : 04247-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBK14

Manual IntegrationsAPPROVED

Quant Time: Sep 09 00:28:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/09/2023
 Supervised By :mohammad ahmed 09/10/2023

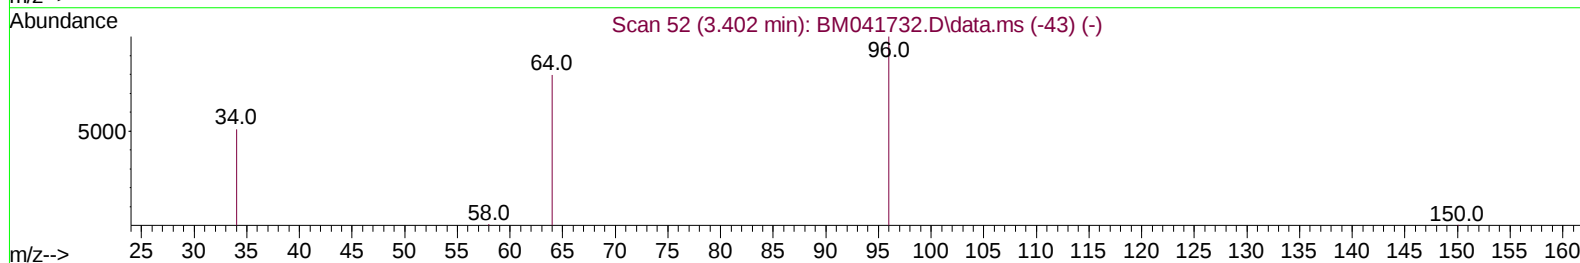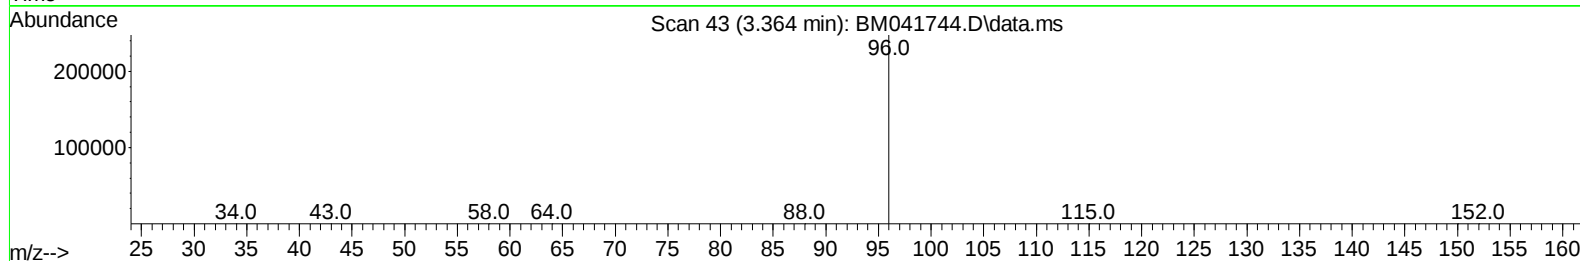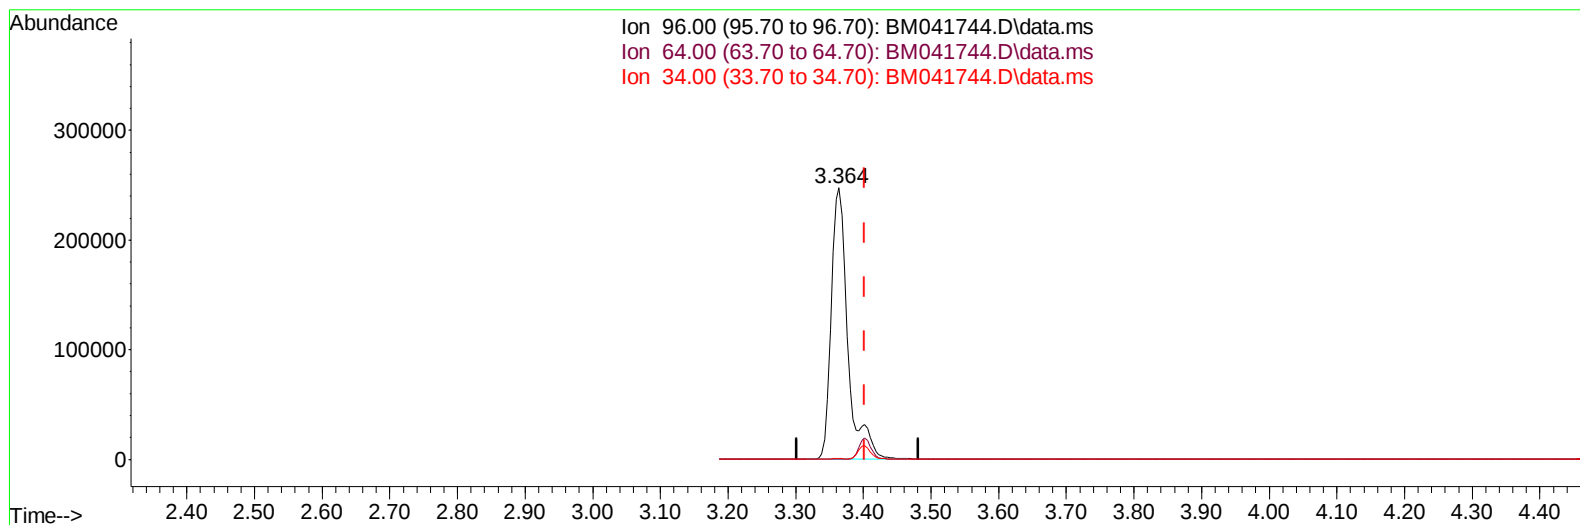

TIC: BM041744.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.364min (-0.038) 52.48 ng/u1

response 421701

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.30	0.12#
34.00	53.80	0.36#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
 Data File : BM041744.D
 Acq On : 08 Sep 2023 23:40
 Operator : MA/JU
 Sample : 04247-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBK14

Manual IntegrationsAPPROVED

Quant Time: Sep 09 00:28:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/09/2023
 Supervised By :mohammad ahmed 09/10/2023

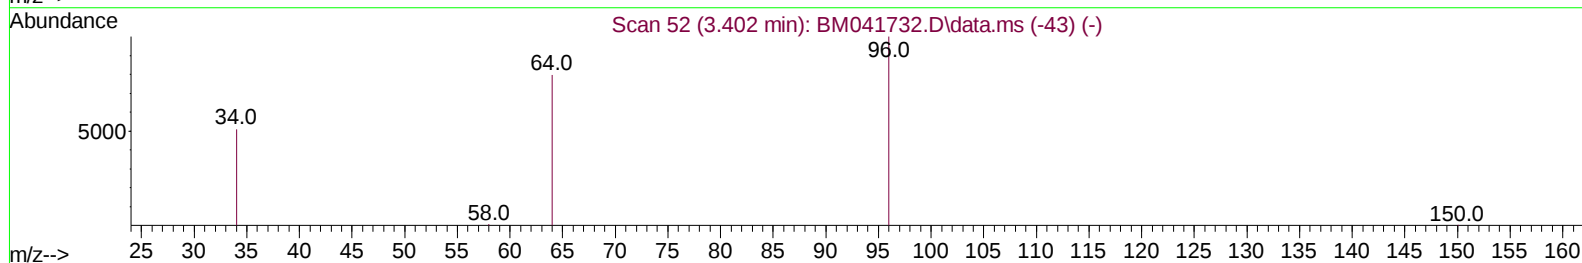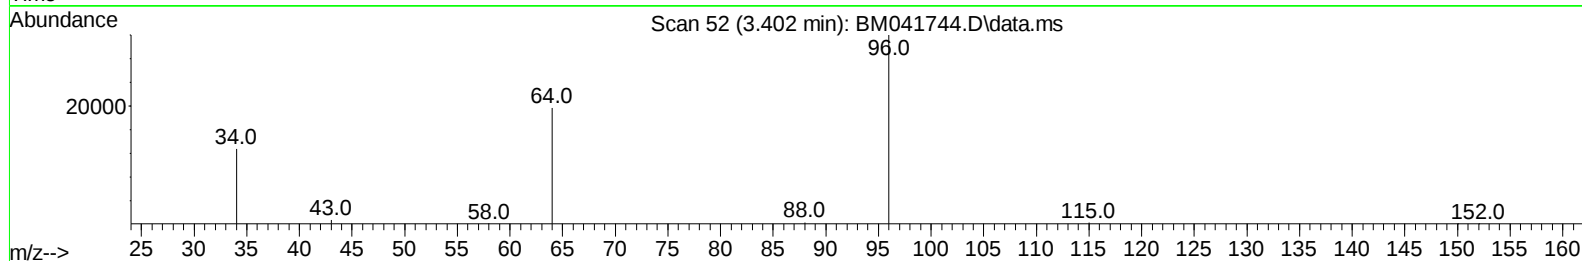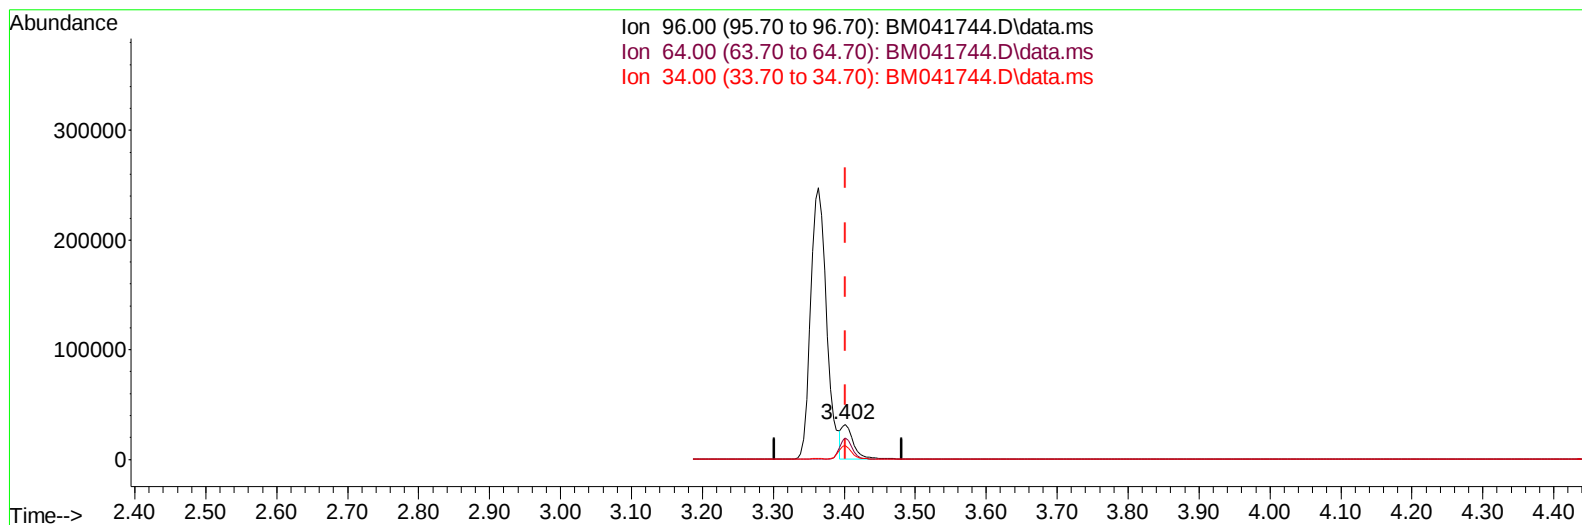

TIC: BM041744.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.402min (+ 0.000) 4.44 ng/ul m

response 35704

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.30	61.43
34.00	53.80	39.93#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
 Data File : BM041744.D
 Acq On : 08 Sep 2023 23:40
 Operator : MA/JU
 Sample : 04247-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBK14

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/09/2023
 Supervised By :mohammad ahmed 09/10/2023

Quant Time: Sep 09 00:28:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.996	152		5258	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136		12876	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.634	164		5919	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.384	188		11090	0.400	ng/ul	0.00
17) Chrysene-d12	21.550	240		4740	0.400	ng/ul	0.00
23) Perylene-d12	23.977	264		5720	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.402	96		35704m	4.443	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152		5238	0.316	ng/ul	0.00
18) Fluoranthene-d10	19.403	212		7614	0.331	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.440	88		11316	1.356	ng/ul	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
Data File : BM041744.D
Acq On : 08 Sep 2023 23:40
Operator : MA/JU
Sample : 04247-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBK14

Manual IntegrationsAPPROVED

Quant Time: Sep 09 00:28:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/09/2023
Supervised By :mohammad ahmed 09/10/2023

