

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
 Data File : BM041737.D
 Acq On : 08 Sep 2023 19:13
 Operator : MA/JU
 Sample : 04148-13
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJW9

Quant Time: Sep 09 00:27:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	4192	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	10261	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.634	164	4815	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.383	188	8815	0.400	ng/ul	0.00
17) Chrysene-d12	21.553	240	3870	0.400	ng/ul	0.00
23) Perylene-d12	23.977	264	5111	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	26544	4.143	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152	4205	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.403	212	7225	0.385	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.435	88	9049	1.360	ng/ul	91
14) Pentachlorophenol	17.012	266	82	0.023	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
Data File : BM041737.D
Acq On : 08 Sep 2023 19:13
Operator : MA/JU
Sample : 04148-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJW9

Quant Time: Sep 09 00:27:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

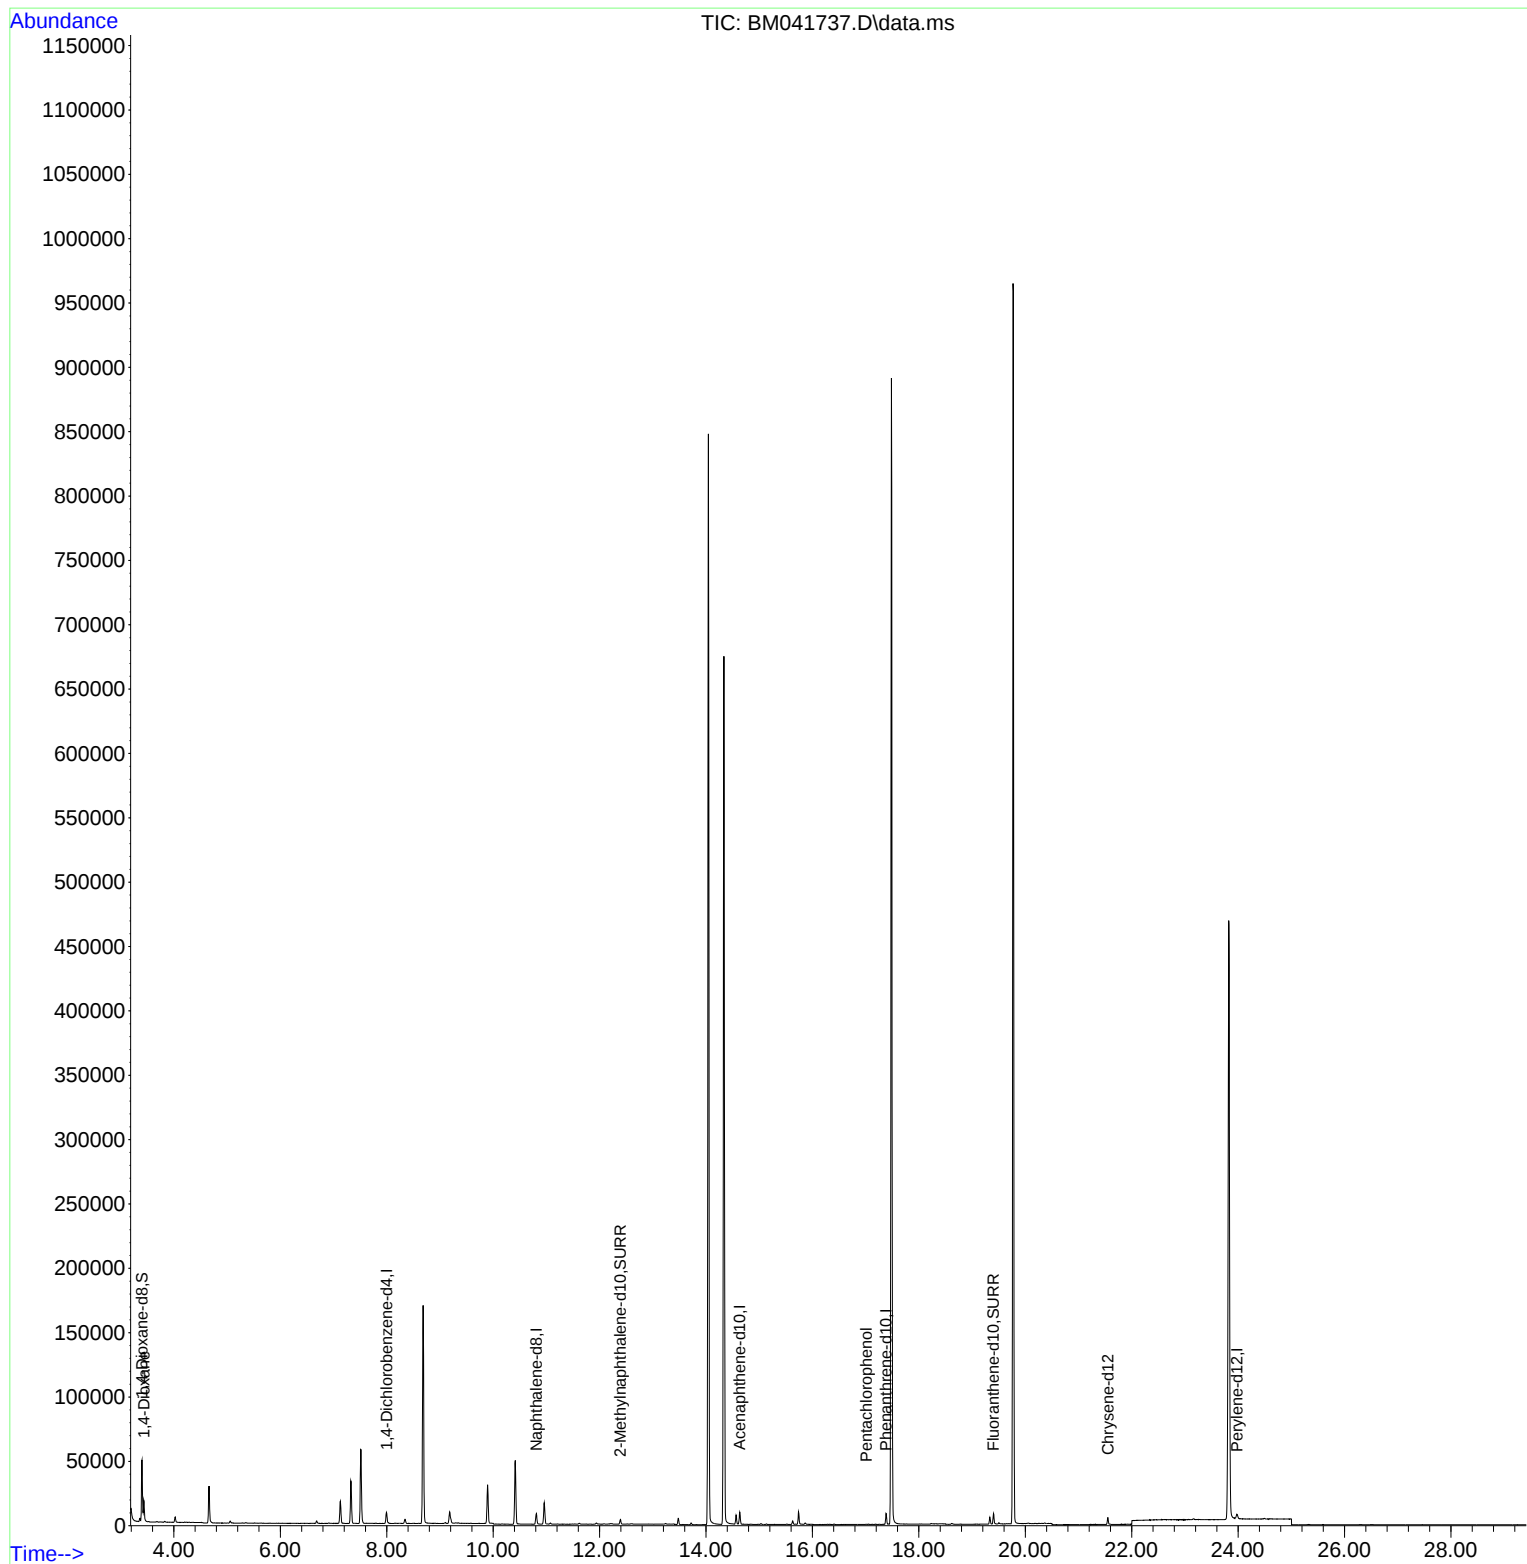

Abundance Scan 61 (3.440 min): BM041732.D\data.ms (-53)

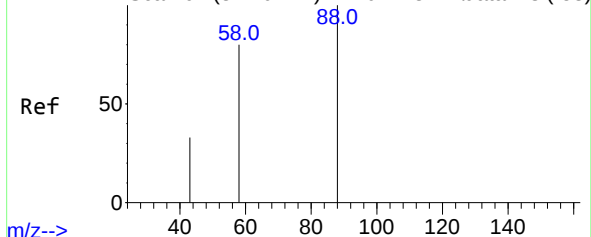

#2

1,4-Dioxane

Concen: 1.360 ng/ul

RT: 3.435 min Scan# 61

Delta R.T. -0.004 min

Lab File: BM041737.D

Acq: 08 Sep 2023 19:13

Instrument :

BNA_M

ClientSampleId :

BBJW9

Tgt Ion: 88 Resp: 9049


Ion Ratio Lower Upper

88 100


43 45.5 33.8 50.6

58 76.7 54.2 81.2


Abundance Scan 60 (3.435 min): BM041737.D\data.ms

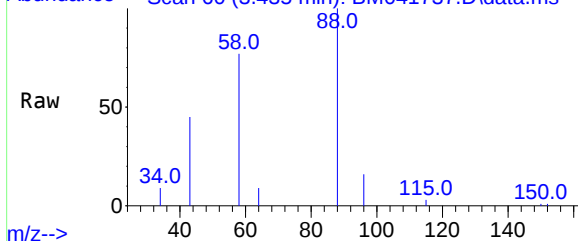


Abundance

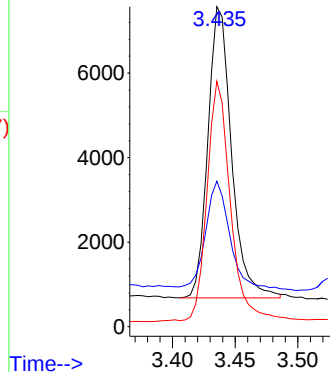

Abundance Scan 60 (3.435 min): BM041737.D\data.ms (-47)

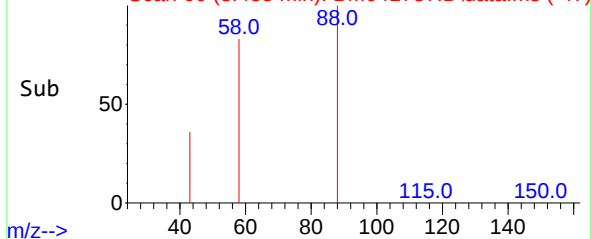

Abundance Scan 3039 (17.012 min): BM041732.D\data.ms (-)

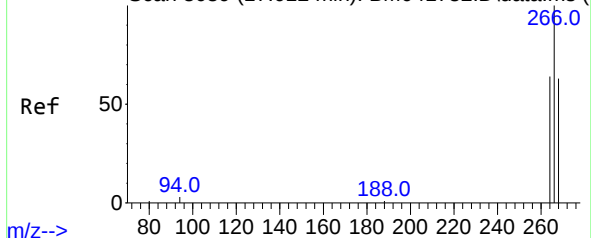

#14

Pentachlorophenol

Concen: 0.023 ng/ul

RT: 17.012 min Scan# 3039

Delta R.T. 0.000 min

Lab File: BM041737.D

Acq: 08 Sep 2023 19:13

Tgt Ion: 266 Resp: 82


Ion Ratio Lower Upper

266 100


264 70.7 50.0 75.0

268 78.0 50.8 76.2#

Abundance Scan 3039 (17.012 min): BM041737.D\data.ms

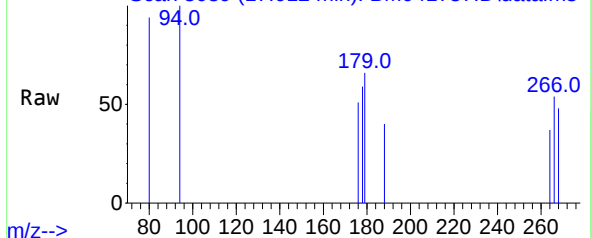

Abundance

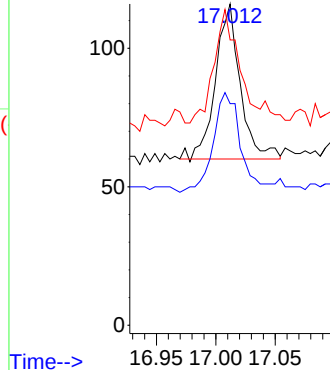

Abundance Scan 3039 (17.012 min): BM041737.D\data.ms (-)

