

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
 Data File : BM041738.D
 Acq On : 08 Sep 2023 19:54
 Operator : MA/JU
 Sample : 04166-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJX4

Quant Time: Sep 09 00:27:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	5180	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	12403	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.634	164	5635	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.383	188	10775	0.400	ng/ul	0.00
17) Chrysene-d12	21.550	240	4498	0.400	ng/ul	0.00
23) Perylene-d12	23.979	264	5452	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	34453	4.352	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152	5377	0.337	ng/ul	0.00
18) Fluoranthene-d10	19.403	212	7975	0.366	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	1508	0.183	ng/ul#	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
Data File : BM041738.D
Acq On : 08 Sep 2023 19:54
Operator : MA/JU
Sample : 04166-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJX4


Quant Time: Sep 09 00:27:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

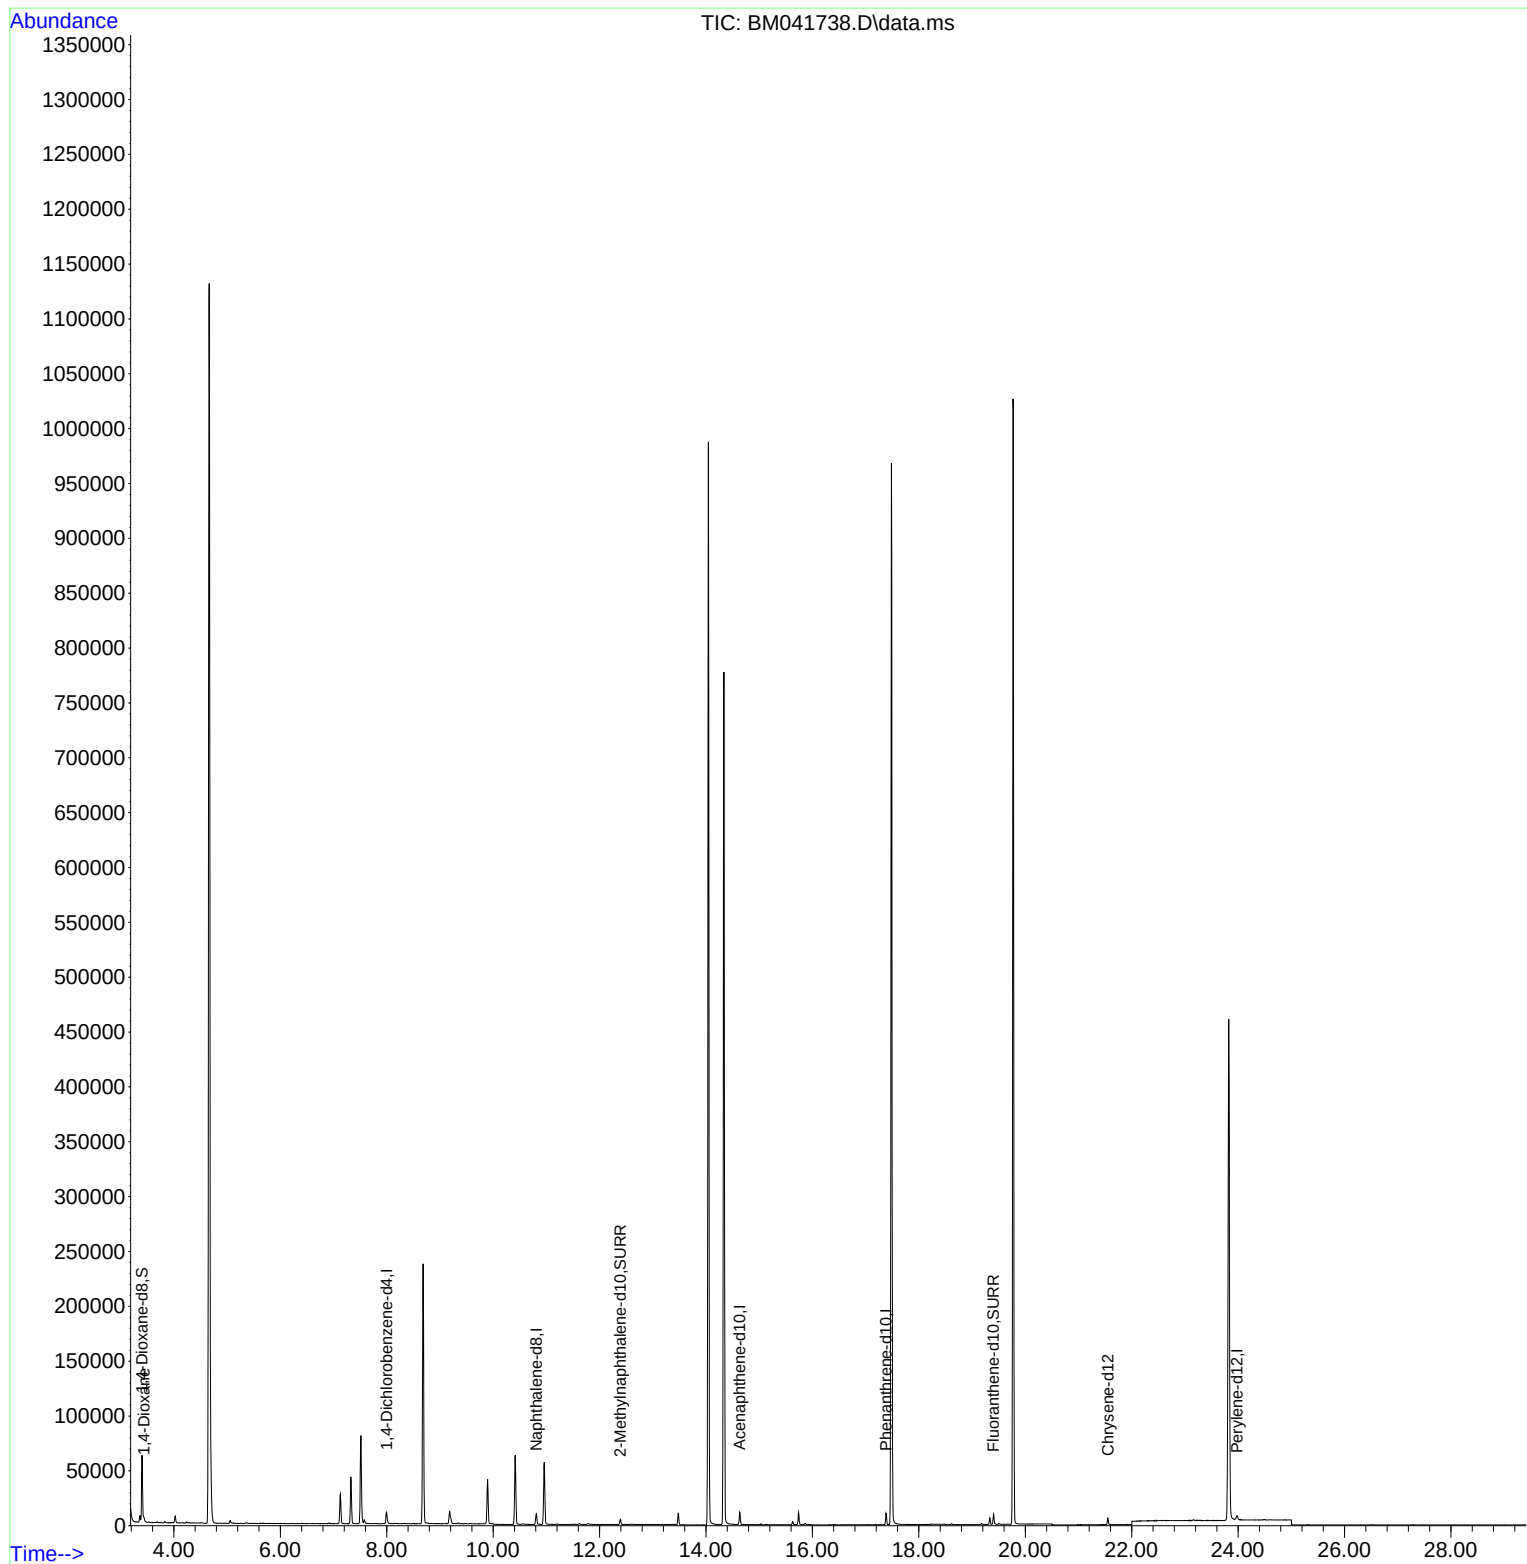


Abundance Scan 61 (3.440 min): BM041732.D\data.ms (-53)

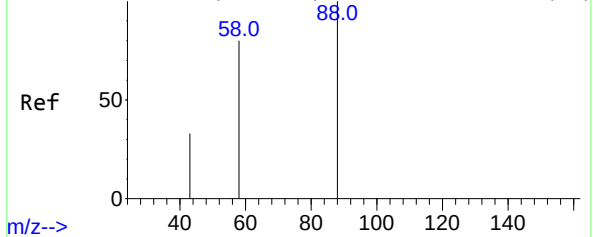

m/z-->

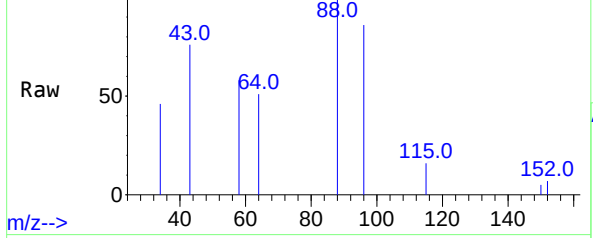

Abundance Scan 61 (3.440 min): BM041738.D\data.ms (-47)

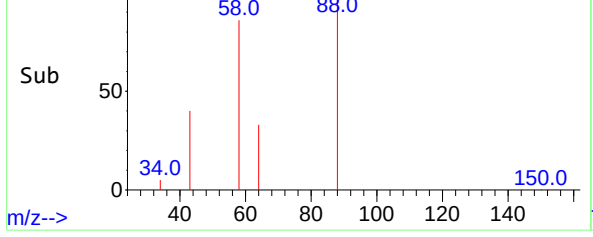

m/z-->

#2
1,4-Dioxane
Concen: 0.183 ng/ul
RT: 3.440 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM041738.D
Acq: 08 Sep 2023 19:54

Instrument :
BNA_M
ClientSampleId :
BBJX4

Tgt Ion:	88	Resp:	1508
Ion	Ratio	Lower	Upper
88	100		
43	75.6	33.8	50.6#
58	58.5	54.2	81.2

