

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
 Data File : BM041741.D
 Acq On : 08 Sep 2023 21:47
 Operator : MA/JU
 Sample : 04227-21
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJ90

Quant Time: Sep 09 00:28:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 06:08:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	5483	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	13354	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.634	164	6232	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.383	188	11557	0.400	ng/ul	0.00
17) Chrysene-d12	21.550	240	4824	0.400	ng/ul	0.00
23) Perylene-d12	23.974	264	6078	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	32028	3.822	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152	5536	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.403	212	8306	0.355	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	256	0.029	ng/ul#	29

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090823\
Data File : BM041741.D
Acq On : 08 Sep 2023 21:47
Operator : MA/JU
Sample : 04227-21
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJ90

Quant Time: Sep 09 00:28:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 06:08:11 2023
Response via : Initial Calibration

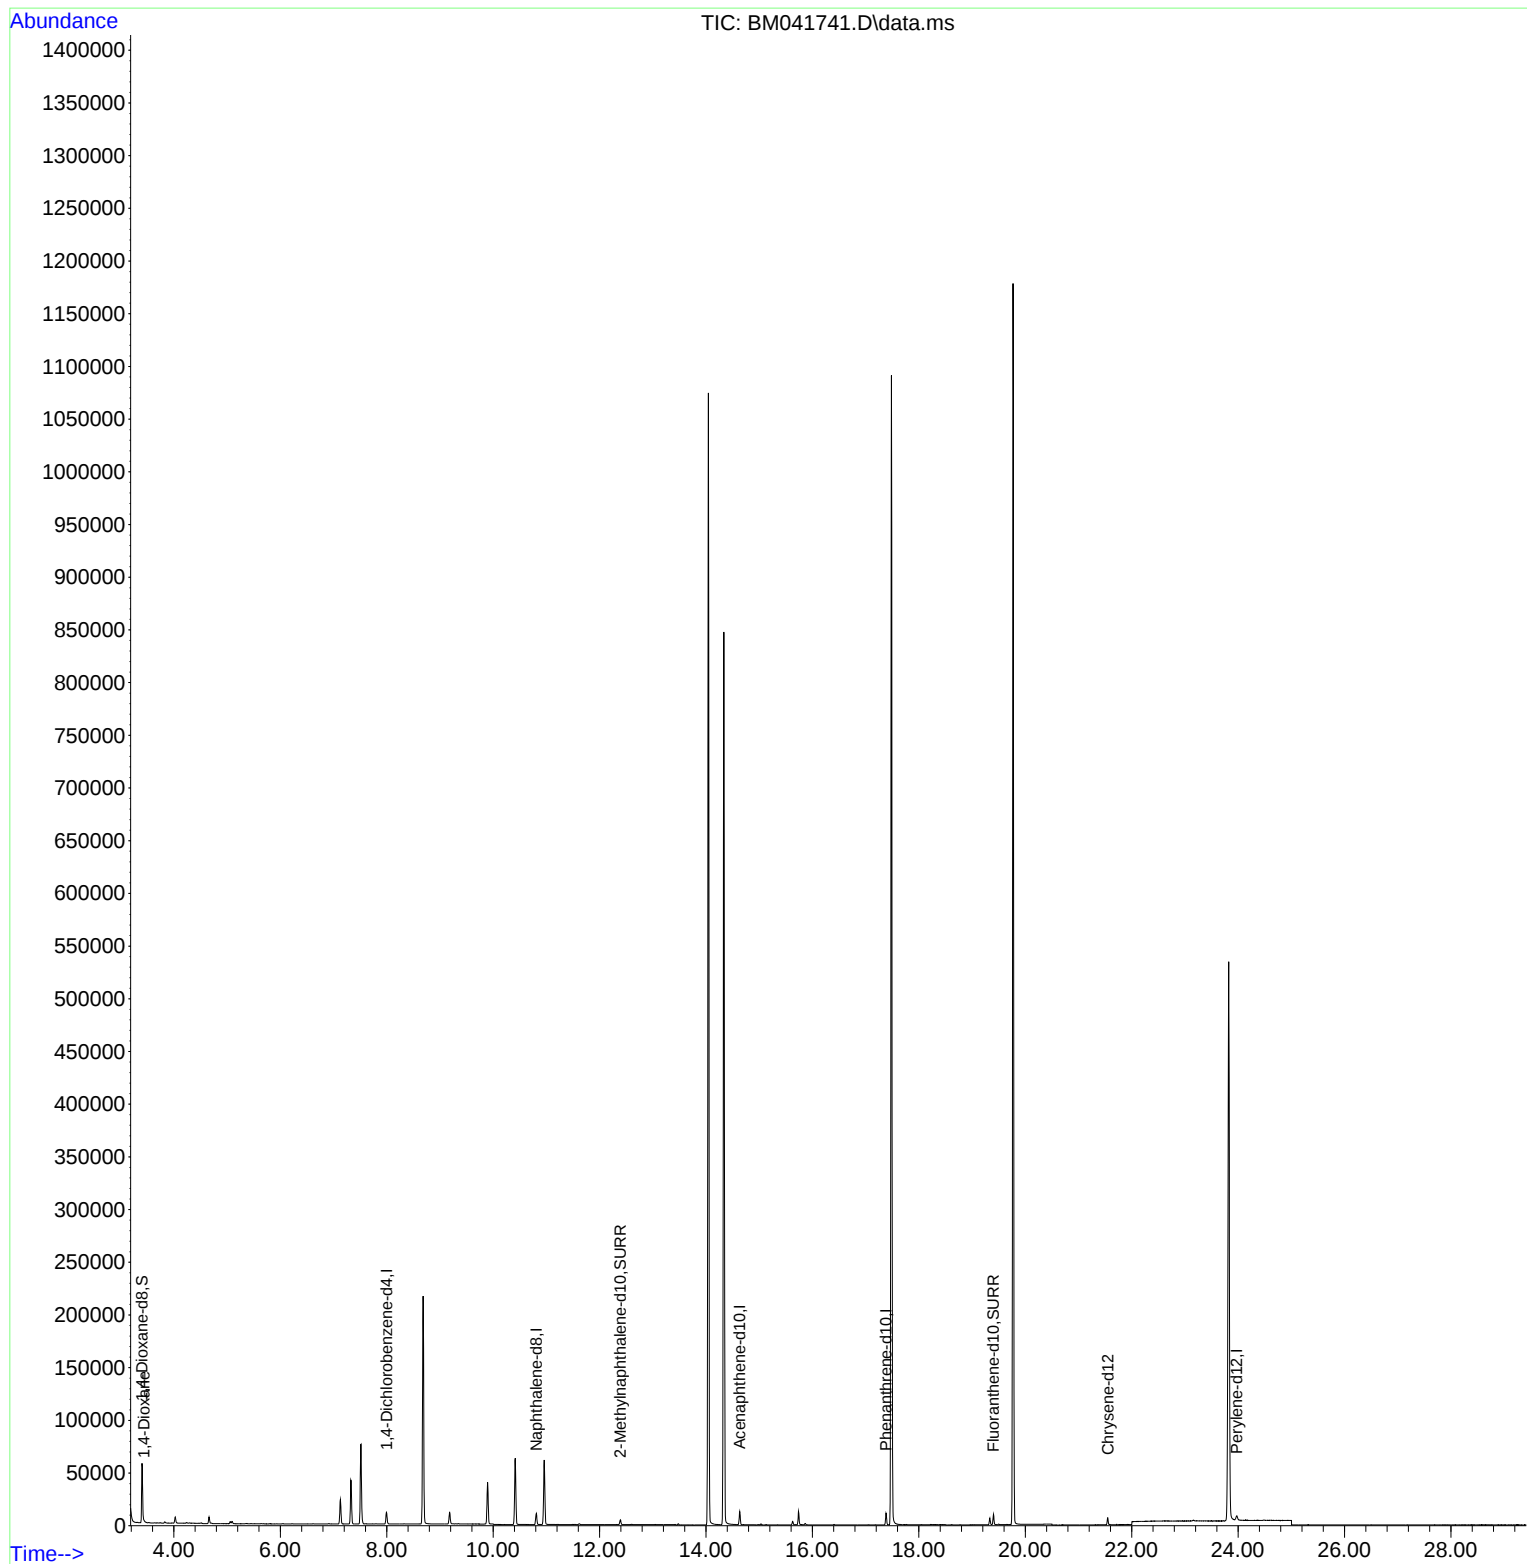


Abundance Scan 61 (3.440 min): BM041732.D\data.ms (-53)

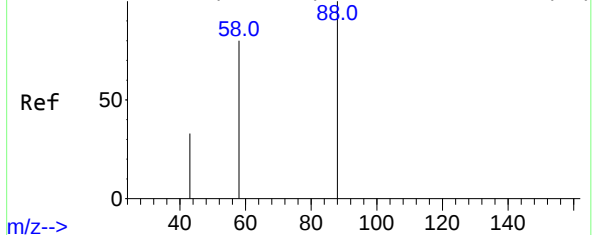


m/z-->

Abundance Scan 61 (3.440 min): BM041741.D\data.ms

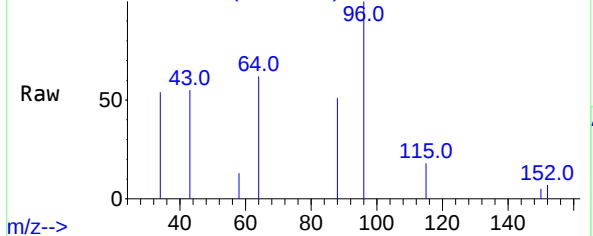

m/z-->

Abundance Scan 61 (3.440 min): BM041741.D\data.ms (-47)

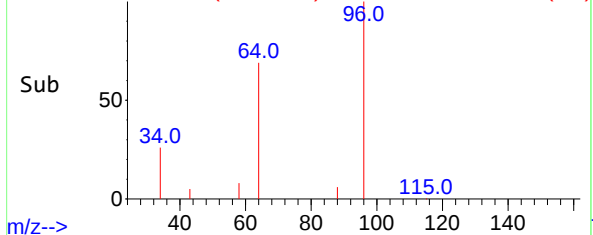

m/z-->

#2

1,4-Dioxane

Concen: 0.029 ng/ul

RT: 3.440 min Scan# 61

Delta R.T. 0.000 min

Lab File: BM041741.D

Acq: 08 Sep 2023 21:47

Instrument :

BNA_M

ClientSampleId :

BBJ90

Tgt Ion: 88 Resp: 256


Ion Ratio Lower Upper

88 100

43 106.5 33.8 50.6#

58 25.3 54.2 81.2#

Abundance

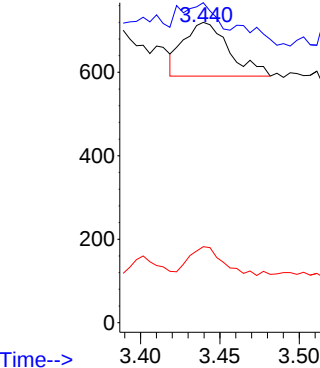

Time-->