

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090922\
 Data File : BM036533.D
 Acq On : 09 Sep 2022 10:41
 Operator : CG/JU
 Sample : PB147556BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK556

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	34	rVB	56916	85415	1.63%	0.159%
2	3.551	93	96	113	rBV	700887	1132512	21.58%	2.109%
3	3.869	146	150	159	rVB2	12080	22097	0.42%	0.041%
4	6.898	658	665	683	rBV	885269	1431910	27.28%	2.667%
5	7.057	686	692	704	rVB	756869	1193914	22.75%	2.224%
6	7.245	718	724	739	rBV	912478	1474813	28.10%	2.747%
7	7.716	797	804	817	rBV	726687	1136863	21.66%	2.118%
8	8.439	920	927	942	rBV	944650	1534100	29.23%	2.857%
9	8.886	993	1003	1019	rBV	793697	1286337	24.51%	2.396%
10	9.604	1118	1125	1139	rBV	737625	1237706	23.58%	2.305%
11	10.145	1209	1217	1234	rBV	1041947	1852781	35.30%	3.451%
12	10.516	1272	1280	1290	rBV	1074962	1776182	33.84%	3.308%
13	10.663	1298	1305	1327	rBV	1086620	1995181	38.02%	3.716%
14	12.127	1547	1554	1562	rBV2	14229	30143	0.57%	0.056%
15	13.792	1830	1837	1846	rBV	2086188	2743350	52.27%	5.110%
16	14.063	1876	1883	1895	rBV	2473213	3412238	65.02%	6.356%
17	14.368	1928	1935	1949	rBV	1724865	2373293	45.22%	4.421%
18	14.598	1968	1974	2001	rBV	704218	1282761	24.44%	2.389%
19	15.362	2096	2104	2118	rBV	3157346	4293532	81.81%	7.997%
20	15.498	2121	2127	2140	rVV	881329	1231134	23.46%	2.293%
21	15.604	2140	2145	2151	rVB2	26859	43181	0.82%	0.080%
22	16.151	2234	2238	2241	rBV5	5784	8148	0.16%	0.015%
23	16.574	2304	2310	2316	rBV6	4428	8499	0.16%	0.016%
24	16.798	2344	2348	2352	rVB6	4416	6227	0.12%	0.012%
25	17.115	2396	2402	2412	rBV	2099733	2720697	51.84%	5.068%
26	17.215	2412	2419	2435	rVV	3468444	4626551	88.16%	8.617%
27	17.645	2489	2492	2496	rVB5	4966	6890	0.13%	0.013%
28	18.598	2652	2654	2657	rVB3	5540	5625	0.11%	0.010%
29	19.074	2729	2735	2742	rBV2	37890	62100	1.18%	0.116%
30	19.150	2744	2748	2753	rVV	31871	44465	0.85%	0.083%
31	19.515	2803	2810	2823	rBV	4014373	5248003	100.00%	9.775%
32	20.521	2977	2981	2985	rBV	169455	195706	3.73%	0.365%
33	21.303	3109	3114	3122	rBV	2138651	2567676	48.93%	4.783%
34	23.450	3472	3479	3490	rVB2	2244868	4264771	81.26%	7.944%
35	23.591	3497	3503	3513	rVB2	1284424	2353480	44.85%	4.384%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090922\
Data File : BM036533.D
Acq On : 09 Sep 2022 10:41
Operator : CG/JU
Sample : PB147556BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK556

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Title : SVOA CALIBRATION




Sum of corrected areas: 53688281

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090922\
Data File : BM036533.D
Acq On : 09 Sep 2022 10:41
Operator : CG/JU
Sample : PB147556BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK556

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

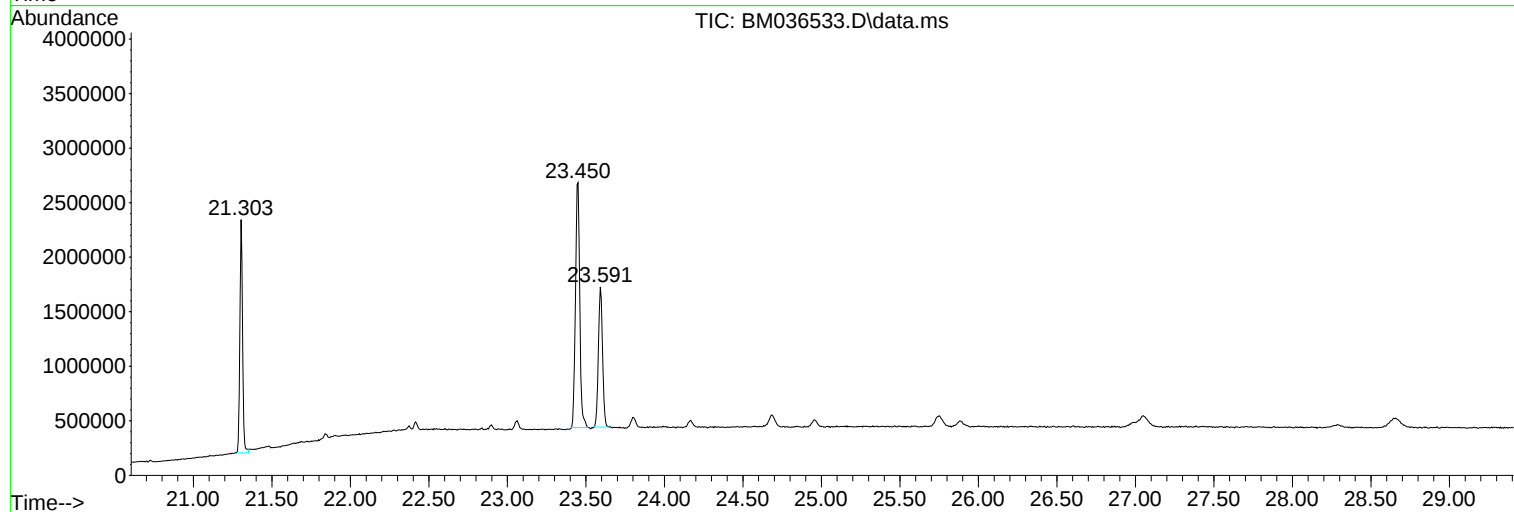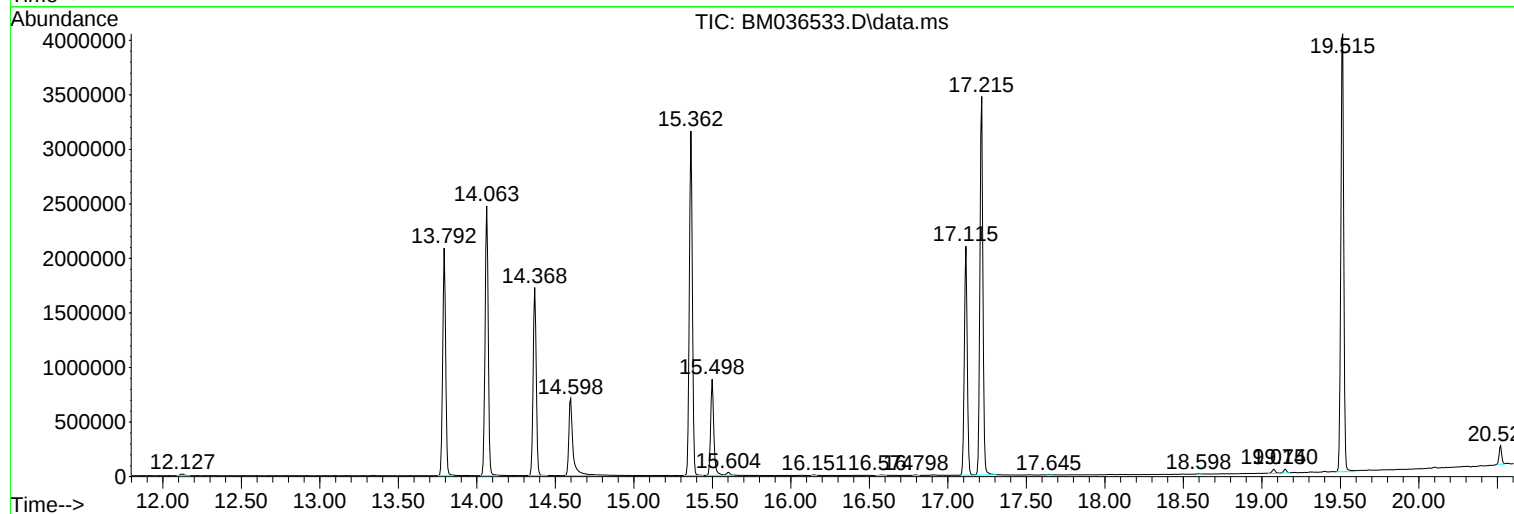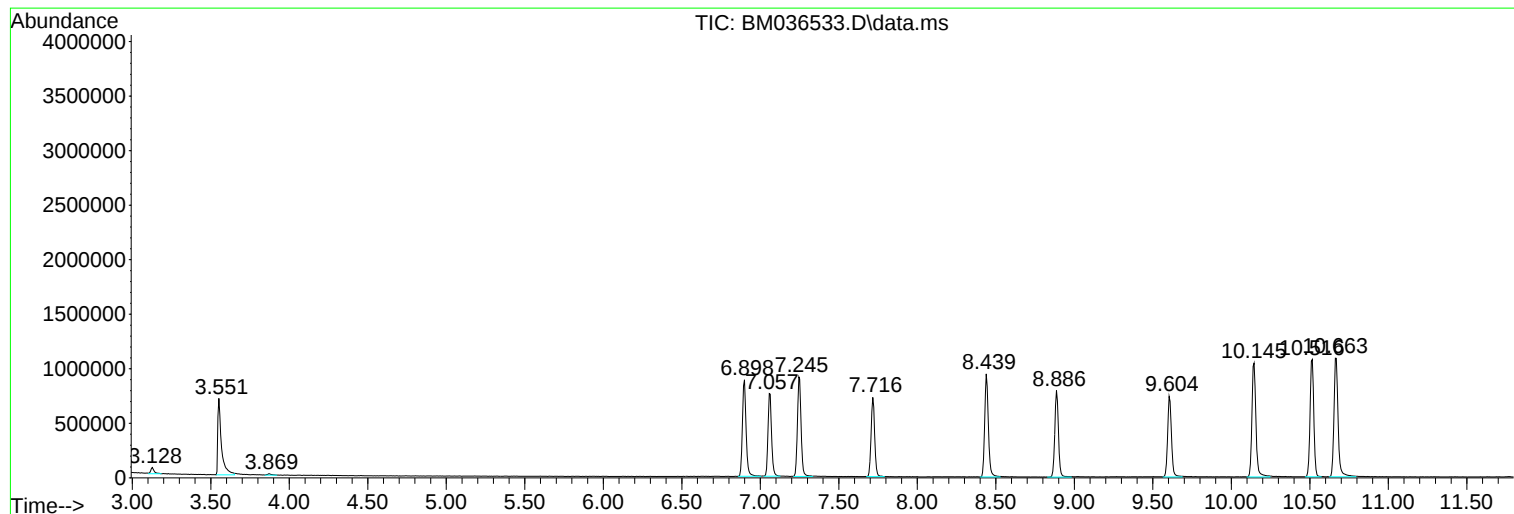

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090922\
Data File : BM036533.D
Acq On : 09 Sep 2022 10:41
Operator : CG/JU
Sample : PB147556BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK556

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090922\
Data File : BM036533.D
Acq On : 09 Sep 2022 10:41
Operator : CG/JU
Sample : PB147556BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK556

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc