

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090922\
 Data File : BM036535.D
 Acq On : 09 Sep 2022 12:32
 Operator : CG/JU
 Sample : N4546-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG6H4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036535.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	28	rBV	43659	60824	1.11%	0.120%
2	3.558	94	97	116	rBV	158490	290088	5.29%	0.574%
3	3.775	128	134	143	rBV	36904	64170	1.17%	0.127%
4	3.869	147	150	156	rVB	14141	20188	0.37%	0.040%
5	4.399	236	240	245	rBV6	5001	7677	0.14%	0.015%
6	6.899	658	665	676	rBV	161176	271988	4.96%	0.538%
7	7.057	683	692	705	rBV	708203	1090156	19.89%	2.158%
8	7.246	716	724	736	rBV	683866	1074351	19.60%	2.127%
9	7.328	736	738	743	rVB5	5872	7657	0.14%	0.015%
10	7.716	797	804	814	rBV	610947	947468	17.28%	1.875%
11	8.440	920	927	937	rBV	558247	917920	16.75%	1.817%
12	8.887	996	1003	1019	rBV	969779	1558323	28.43%	3.085%
13	9.604	1119	1125	1138	rBV	738102	1215208	22.17%	2.405%
14	10.145	1210	1217	1237	rBV	983981	1723007	31.43%	3.410%
15	10.516	1272	1280	1290	rBV	1096343	1806630	32.96%	3.576%
16	10.663	1297	1305	1321	rBV	945247	1734561	31.64%	3.433%
17	12.122	1545	1553	1561	rBV	15532	33785	0.62%	0.067%
18	12.728	1648	1656	1658	rBV7	2974	5871	0.11%	0.012%
19	13.339	1757	1760	1764	rBV4	3419	5655	0.10%	0.011%
20	13.792	1828	1837	1848	rBV	2138187	2826115	51.56%	5.594%
21	14.063	1876	1883	1896	rBV	2525020	3522237	64.25%	6.972%
22	14.369	1928	1935	1949	rBV	1740055	2397379	43.73%	4.745%
23	14.610	1971	1976	1992	rBV	73918	206999	3.78%	0.410%
24	15.216	2075	2079	2084	rVB6	3829	6662	0.12%	0.013%
25	15.363	2096	2104	2117	rBV	3332719	4482287	81.77%	8.872%
26	15.498	2122	2127	2141	rVV	946939	1294536	23.62%	2.562%
27	15.604	2141	2145	2154	rVB	28766	48132	0.88%	0.095%
28	16.086	2219	2227	2229	rBV7	6010	10483	0.19%	0.021%
29	16.145	2234	2237	2243	rVB5	7102	9584	0.17%	0.019%
30	16.580	2307	2311	2315	rBV5	6319	11954	0.22%	0.024%
31	16.798	2344	2348	2353	rVB7	3678	5836	0.11%	0.012%
32	16.874	2356	2361	2364	rBV6	7807	12526	0.23%	0.025%
33	17.116	2396	2402	2412	rBV	2007104	2728047	49.77%	5.400%
34	17.216	2412	2419	2434	rVV	3647535	4901824	89.42%	9.703%
35	17.521	2465	2471	2474	rBV8	4531	9963	0.18%	0.020%
36	17.786	2512	2516	2521	rBV7	3269	6332	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090922\
 Data File : BM036535.D
 Acq On : 09 Sep 2022 12:32
 Operator : CG/JU
 Sample : N4546-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG6H4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

37	18.021	2552	2556	2561	rBV6	16482	24987	0.46%	0.049%
38	18.092	2566	2568	2572	rVB3	7067	6801	0.12%	0.013%
39	18.598	2651	2654	2657	rBV5	4912	5603	0.10%	0.011%
40	19.074	2731	2735	2741	rBV3	36216	48432	0.88%	0.096%
41	19.145	2744	2747	2753	rVV	34081	46494	0.85%	0.092%
42	19.304	2772	2774	2778	rBV5	11955	15162	0.28%	0.030%
43	19.451	2796	2799	2803	rBV6	10136	13896	0.25%	0.028%
44	19.515	2804	2810	2817	rVV	4198665	5481706	100.00%	10.850%
45	20.521	2977	2981	2986	rBV	116630	127901	2.33%	0.253%
46	21.309	3110	3115	3122	rBV	2177147	2692635	49.12%	5.330%
47	23.450	3472	3479	3493	rVB2	2351808	4453864	81.25%	8.816%
48	23.597	3498	3504	3513	rVB	1252710	2287021	41.72%	4.527%




Sum of corrected areas: 50520925

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090922\
Data File : BM036535.D
Acq On : 09 Sep 2022 12:32
Operator : CG/JU
Sample : N4546-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG6H4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

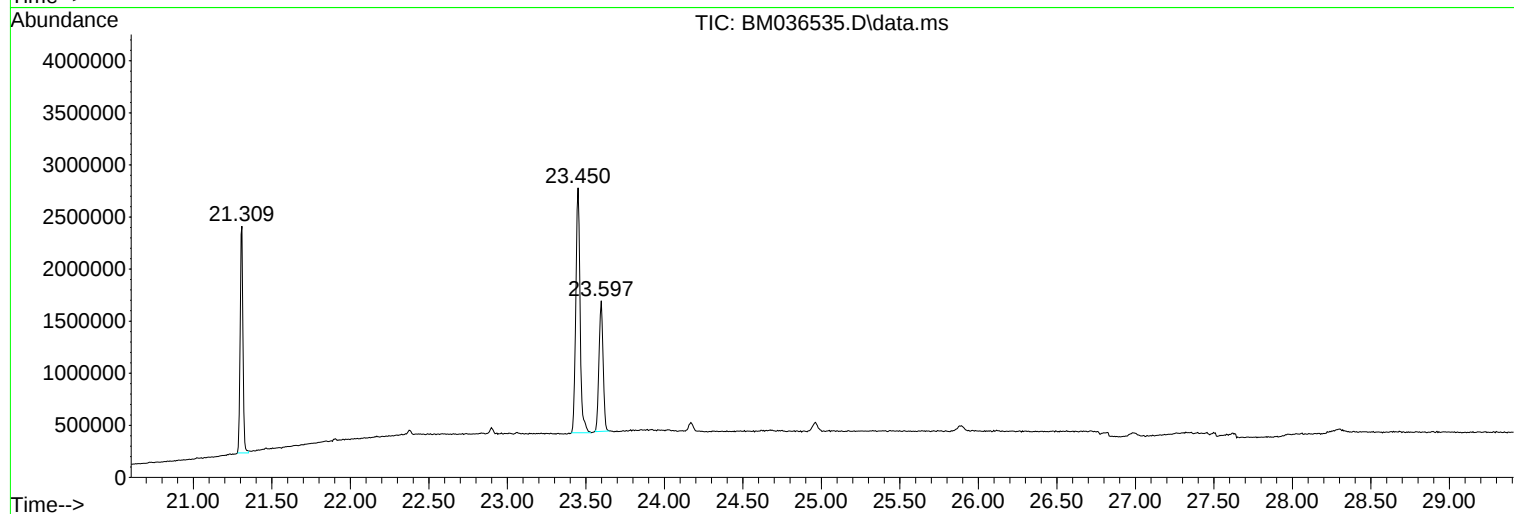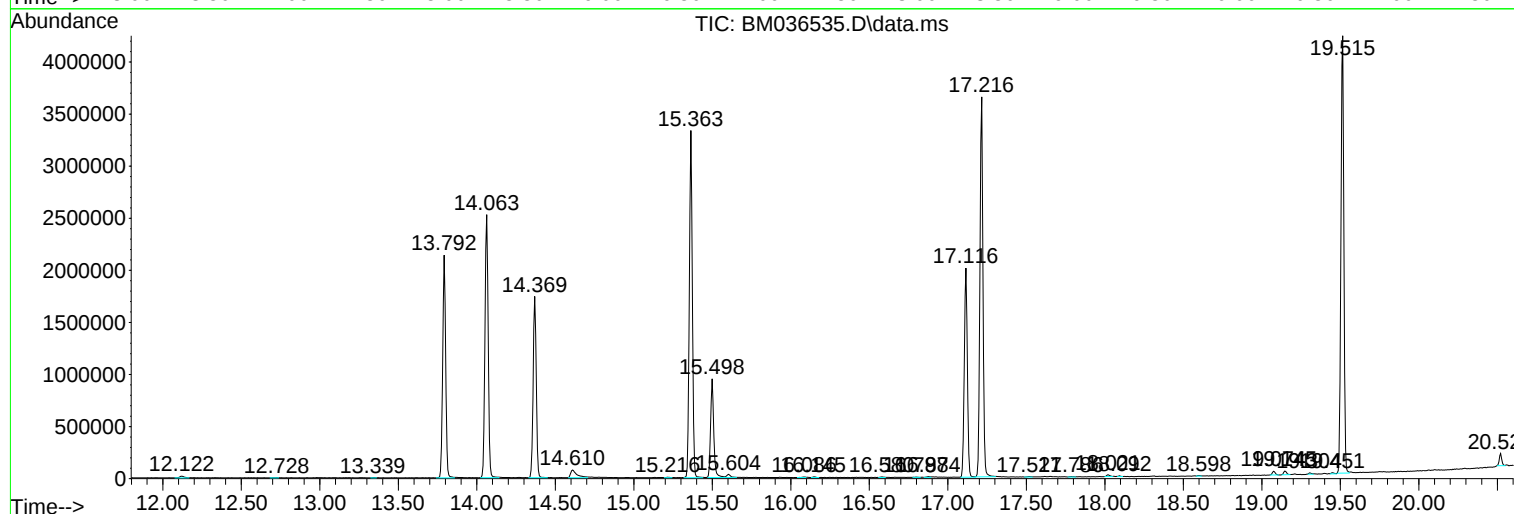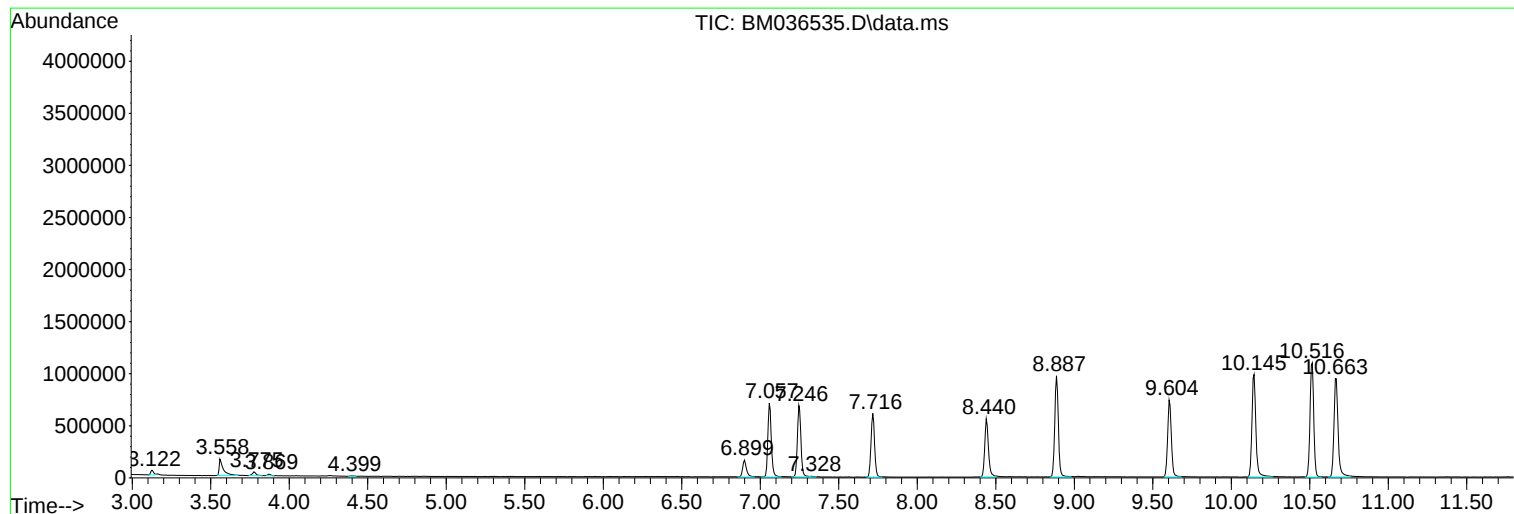

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090922\
Data File : BM036535.D
Acq On : 09 Sep 2022 12:32
Operator : CG/JU
Sample : N4546-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG6H4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090922\
Data File : BM036535.D
Acq On : 09 Sep 2022 12:32
Operator : CG/JU
Sample : N4546-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG6H4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc