




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090923\
Data File : BM041760.D
Acq On : 09 Sep 2023 21:48
Operator : MA/JU
Sample : 04247-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHA05

Manual IntegrationsAPPROVED

Quant Time: Sep 09 23:58:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :mohammad ahmed 09/11/2023

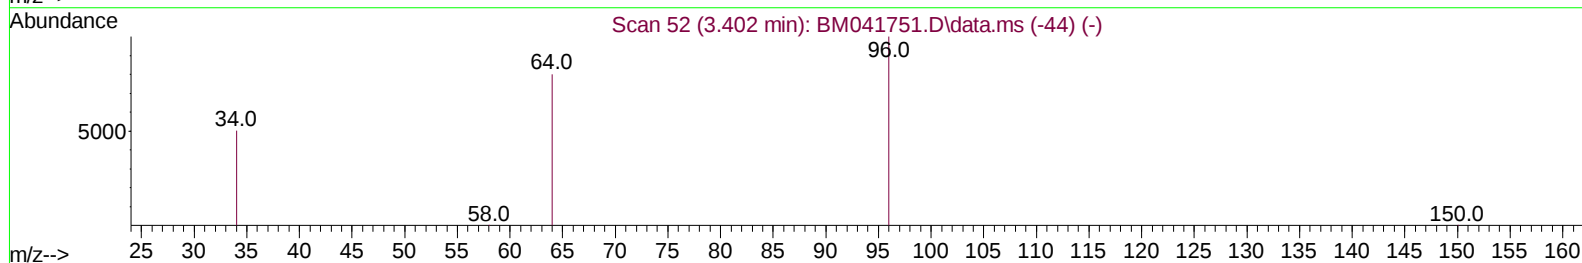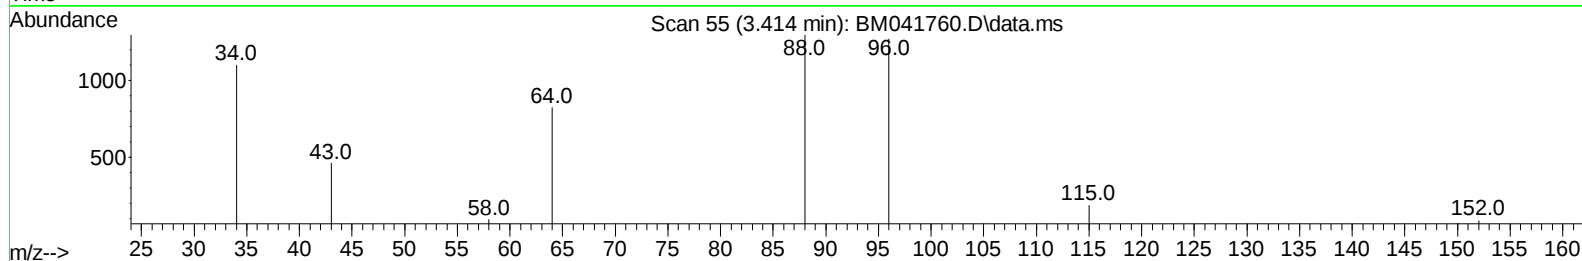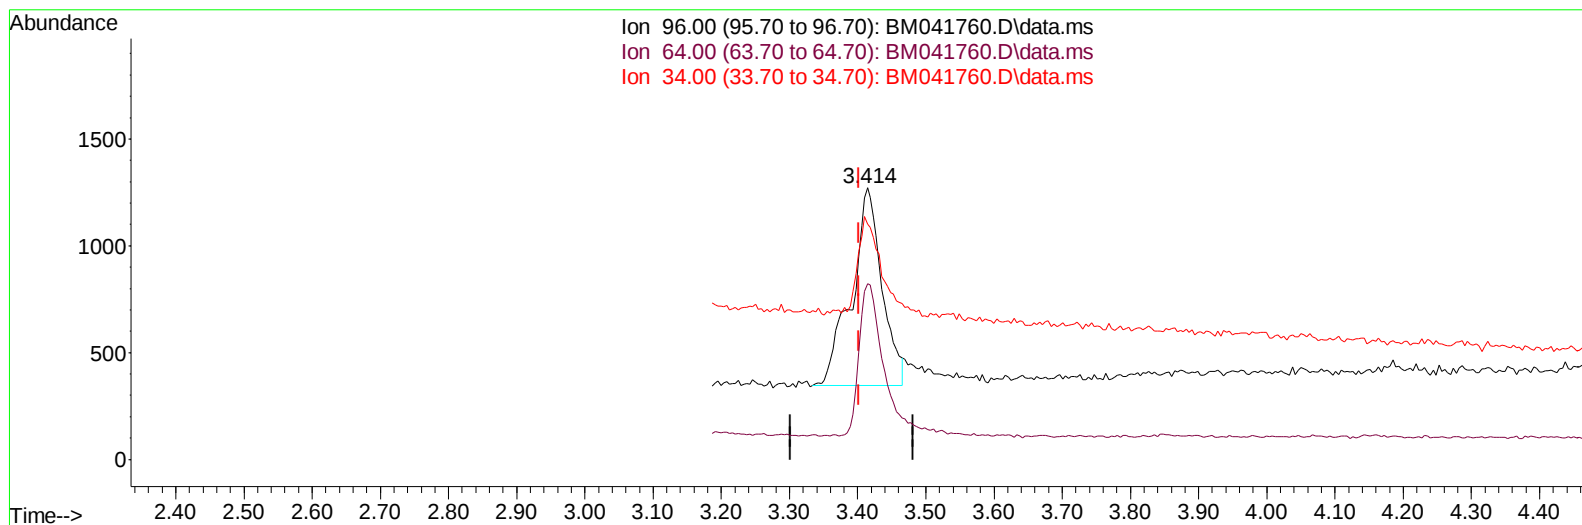

TIC: BM041760.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.414min (+ 0.013) 6.03 ng/u1

response 2856

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.30	64.75
34.00	53.80	86.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090923\
Data File : BM041760.D
Acq On : 09 Sep 2023 21:48
Operator : MA/JU
Sample : 04247-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHA05

Manual IntegrationsAPPROVED

Quant Time: Sep 09 23:58:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :mohammad ahmed 09/11/2023

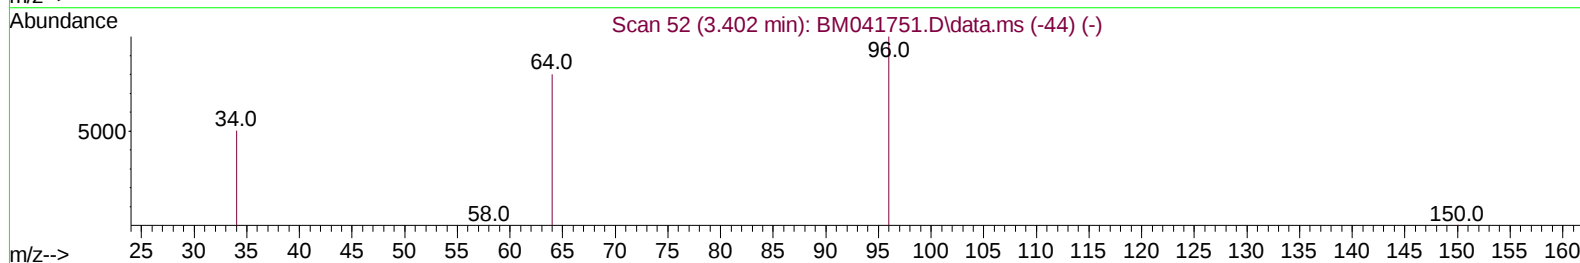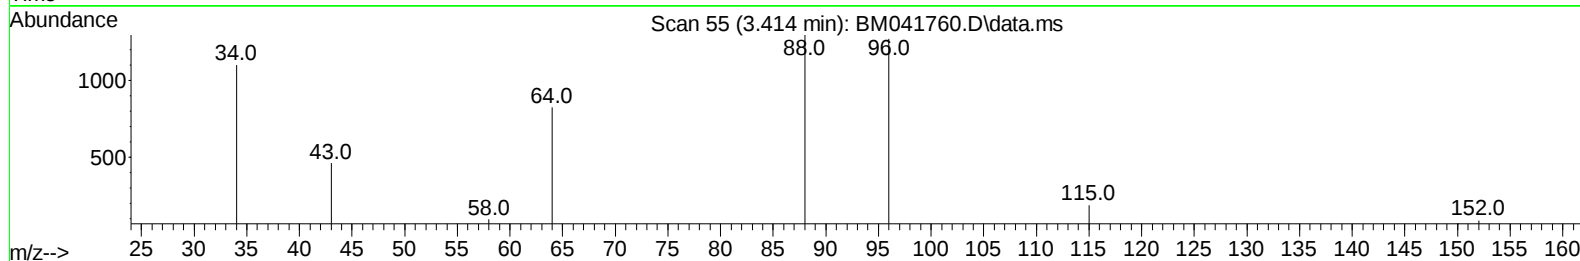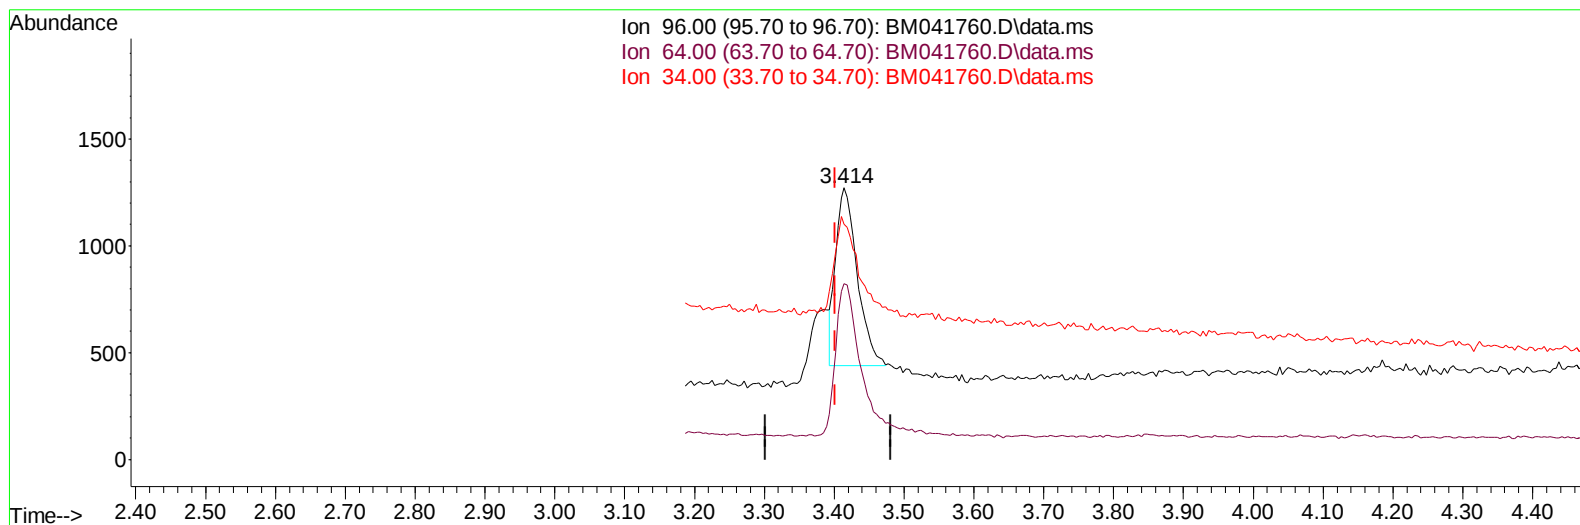

TIC: BM041760.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.414min (+ 0.013) 3.74 ng/ul m

response 1773

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.30	64.75
34.00	53.80	86.55#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090923\
 Data File : BM041760.D
 Acq On : 09 Sep 2023 21:48
 Operator : MA/JU
 Sample : 04247-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHA05

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :mohammad ahmed 09/11/2023

Quant Time: Sep 09 23:58:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.996	152		310	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.807	136		627	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.629	164		255	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.379	188		451	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.545	240		155	0.400	ng/ul	# 0.00
23) Perylene-d12	23.962	264		200	0.400	ng/ul	#-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.414	96		1773m	3.742	ng/ul	0.01
6) 2-Methylnaphthalene-d10	12.385	152		287	0.356	ng/ul	0.00
18) Fluoranthene-d10	19.399	212		251	0.334	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.448	88		4544	9.233	ng/ul	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090923\
Data File : BM041760.D
Acq On : 09 Sep 2023 21:48
Operator : MA/JU
Sample : 04247-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHA05

Manual IntegrationsAPPROVED

Quant Time: Sep 09 23:58:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :mohammad ahmed 09/11/2023

