




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090923\
 Data File : BM041771.D
 Acq On : 10 Sep 2023 04:38
 Operator : MA/JU
 Sample : 04247-17
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJ77

Manual IntegrationsAPPROVED

Quant Time: Sep 11 01:46:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :mohammad ahmed 09/11/2023

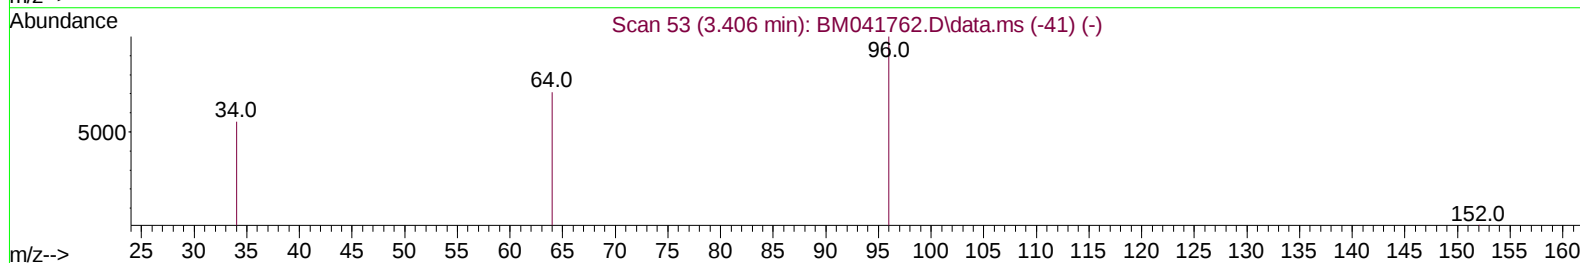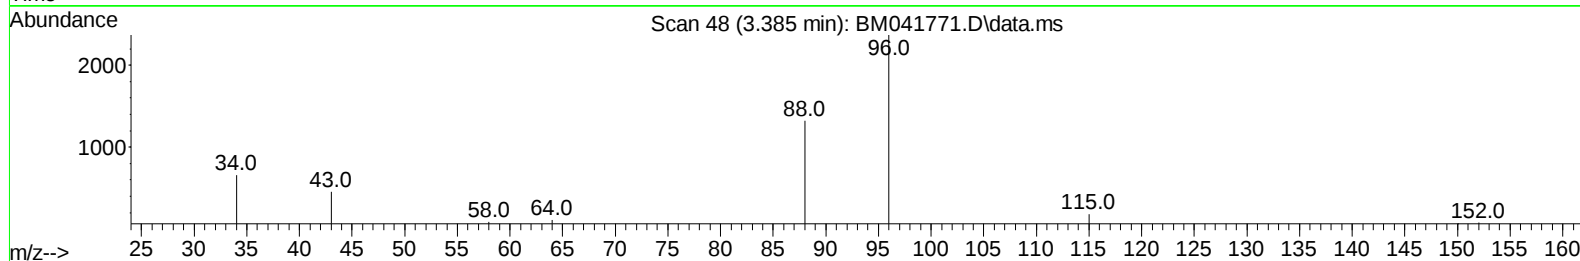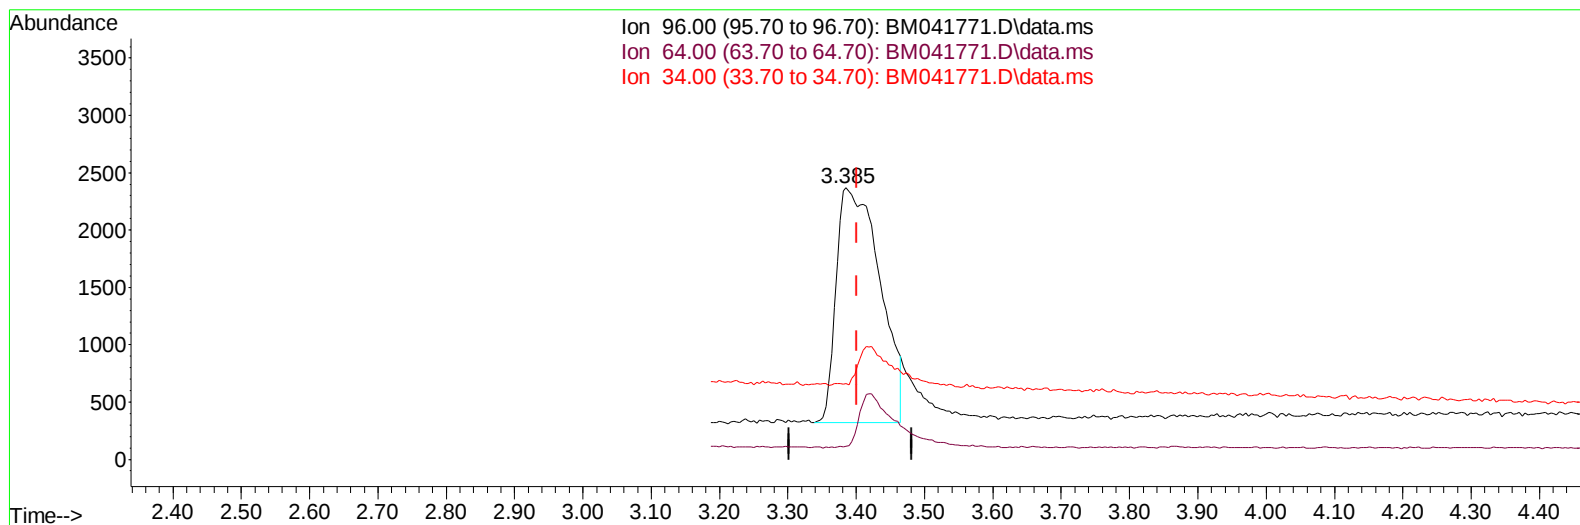

TIC: BM041771.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.385min (-0.017) 23.00 ng/u1

response 9104

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.30	4.86#
34.00	53.80	27.83#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090923\
 Data File : BM041771.D
 Acq On : 10 Sep 2023 04:38
 Operator : MA/JU
 Sample : 04247-17
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJ77

Manual IntegrationsAPPROVED

Quant Time: Sep 11 01:46:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :mohammad ahmed 09/11/2023

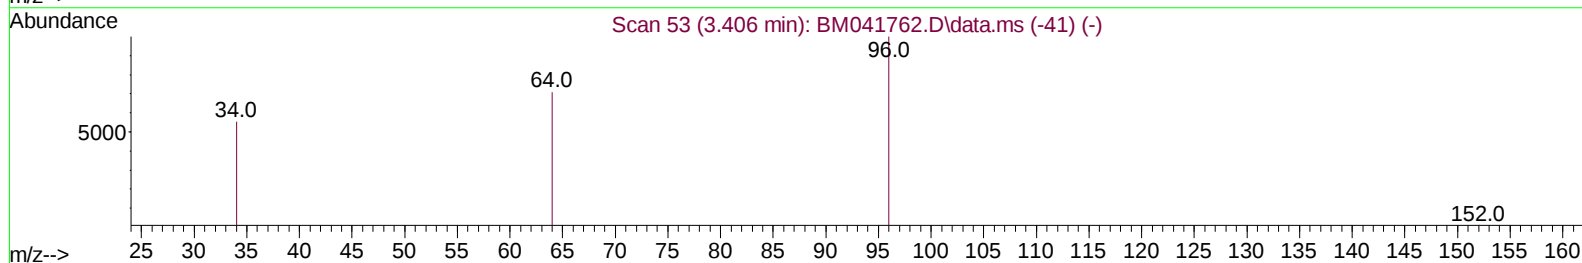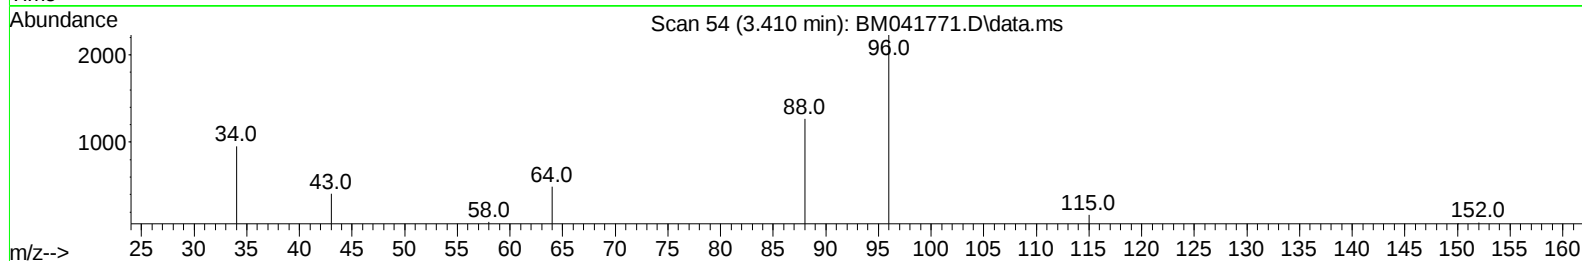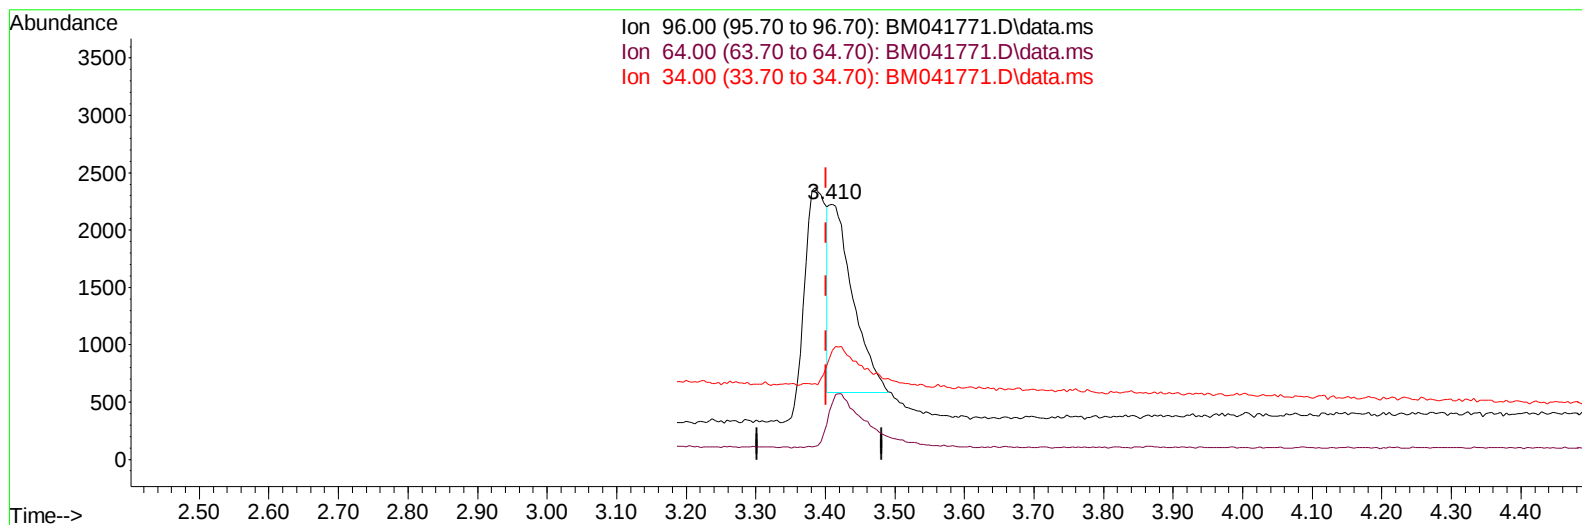

TIC: BM041771.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.410min (+ 0.008) 9.95 ng/ul m

response 3939

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.30	22.19#
34.00	53.80	42.81#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090923\
 Data File : BM041771.D
 Acq On : 10 Sep 2023 04:38
 Operator : MA/JU
 Sample : 04247-17
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJ77

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :mohammad ahmed 09/11/2023

Quant Time: Sep 11 01:46:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.996	152		259	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.807	136		512	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.629	164		204	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.379	188		324	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.542	240		106	0.400	ng/ul	# 0.00
23) Perylene-d12	23.962	264		115	0.400	ng/ul	#-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.410	96		3939m	9.951	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.385	152		232	0.352	ng/ul	0.00
18) Fluoranthene-d10	19.399	212		173	0.337	ng/ul	0.00
Target Compounds				Qvalue			
2) 1,4-Dioxane	3.452	88		848	2.062	ng/ul#	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090923\
Data File : BM041771.D
Acq On : 10 Sep 2023 04:38
Operator : MA/JU
Sample : 04247-17
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJ77

Manual IntegrationsAPPROVED

Quant Time: Sep 11 01:46:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :mohammad ahmed 09/11/2023

