

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090923\
 Data File : BM041760.D
 Acq On : 09 Sep 2023 21:48
 Operator : MA/JU
 Sample : 04247-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHA05

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :mohammad ahmed 09/11/2023

Quant Time: Sep 09 23:58:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	310	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.807	136	627	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.629	164	255	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.379	188	451	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.545	240	155	0.400	ng/ul	# 0.00
23) Perylene-d12	23.962	264	200	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.414	96	1773m	3.742	ng/ul	0.01
6) 2-Methylnaphthalene-d10	12.385	152	287	0.356	ng/ul	0.00
18) Fluoranthene-d10	19.399	212	251	0.334	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.448	88	4544	9.233	ng/ul	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090923\
Data File : BM041760.D
Acq On : 09 Sep 2023 21:48
Operator : MA/JU
Sample : 04247-11
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BHA05

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :mohammad ahmed 09/11/2023


Quant Time: Sep 09 23:58:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration

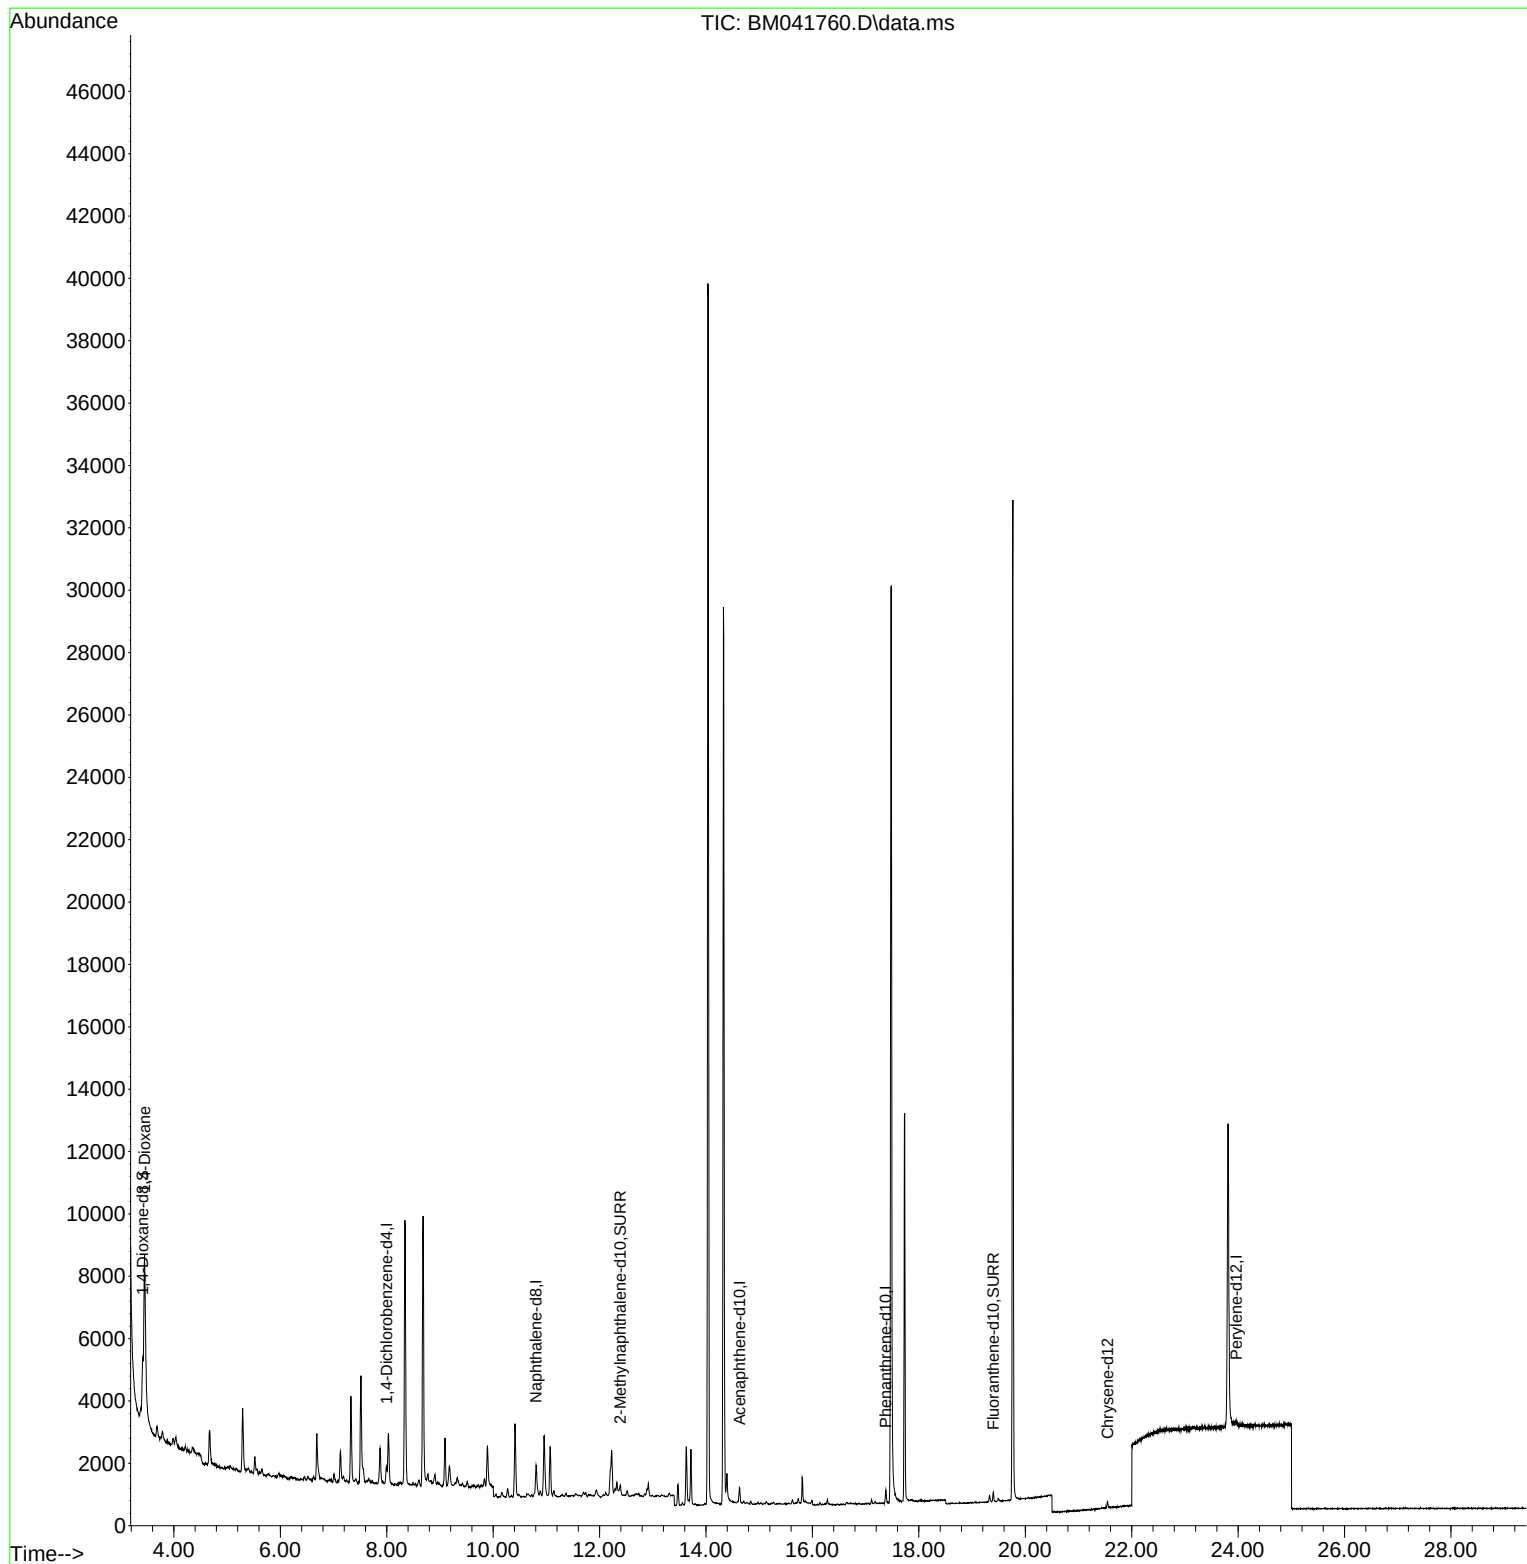

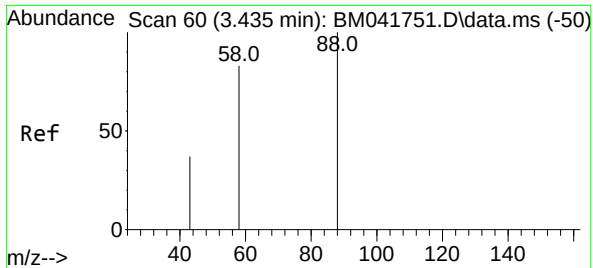

#2
 1,4-Dioxane
 Concen: 9.233 ng/ul
 RT: 3.448 min Scan# 61
 Delta R.T. 0.013 min
 Lab File: BM041760.D
 Acq: 09 Sep 2023 21:48

Instrument :
 BNA_M
 ClientSampleId :
 BHA05

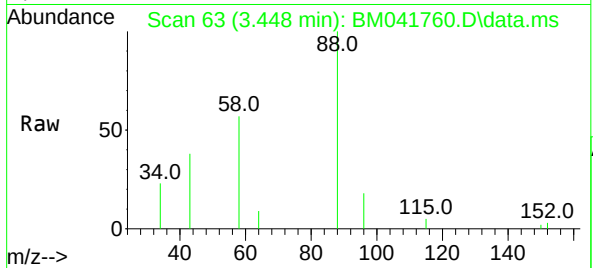

Tgt Ion: 88 Resp: 4544
 Ion Ratio Lower Upper
 88 100
 43 38.2 33.8 50.6
 58 57.2 54.2 81.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :mohammad ahmed 09/11/2023

