

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090923\
 Data File : BM041763.D
 Acq On : 09 Sep 2023 23:40
 Operator : MA/JU
 Sample : 04247-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBK19

Quant Time: Sep 10 00:10:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	491	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.807	136	1020	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.634	164	402	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.384	188	670	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.550	240	218	0.400	ng/ul	# 0.00
23) Perylene-d12	23.971	264	273	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	3087	4.114	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152	396	0.302	ng/ul	0.00
18) Fluoranthene-d10	19.399	212	398	0.376	ng/ul	0.00
Target Compounds				Qvalue		
2) 1,4-Dioxane	3.448	88	4006	5.139	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090923\
Data File : BM041763.D
Acq On : 09 Sep 2023 23:40
Operator : MA/JU
Sample : 04247-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBK19


Quant Time: Sep 10 00:10:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration

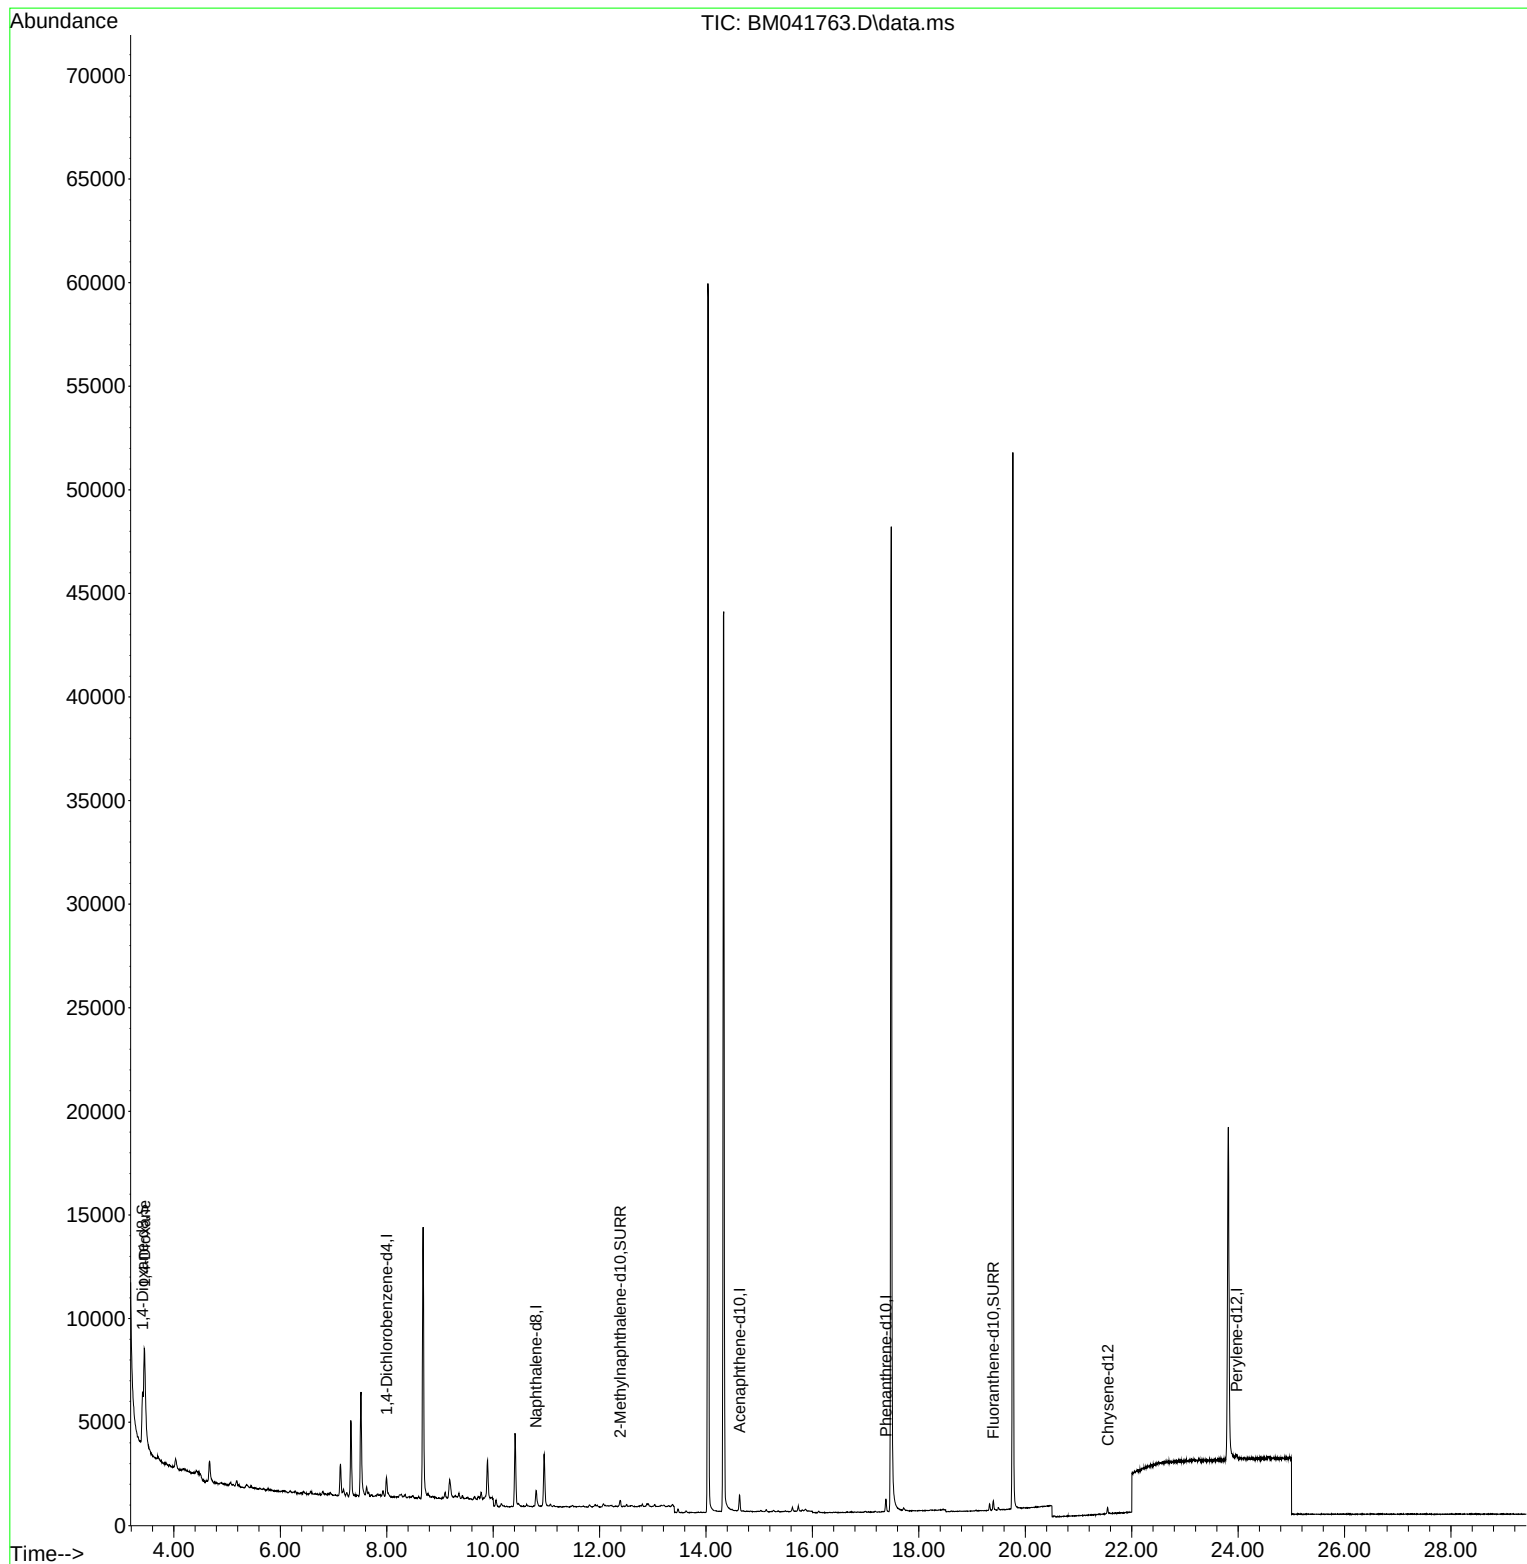

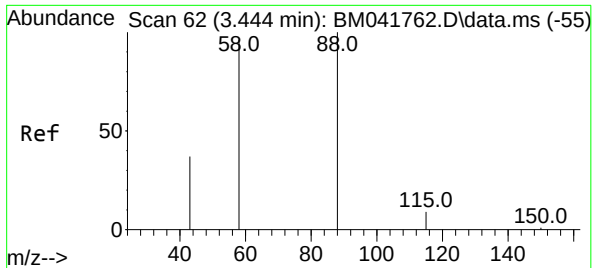

#2
 1,4-Dioxane
 Concen: 5.139 ng/ul
 RT: 3.448 min Scan# 61
 Delta R.T. 0.013 min
 Lab File: BM041763.D
 Acq: 09 Sep 2023 23:40

Instrument :
 BNA_M
 ClientSampleId :
 BBK19

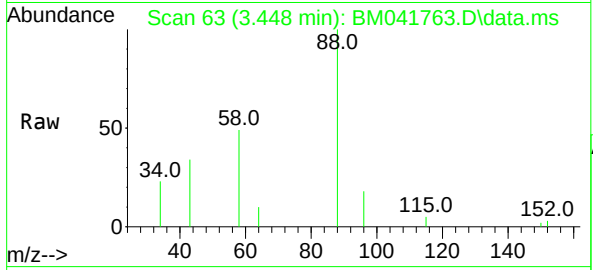

Tgt Ion: 88 Resp: 4006

Ion	Ratio	Lower	Upper
88	100		
43	34.2	33.8	50.6
58	48.6	54.2	81.2#

