


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM090923\  
Data File : BM041750.D  
Acq On : 09 Sep 2023 12:59  
Operator : MA/JU  
Sample : DFTPP161  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP161

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM090523.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Sat Sep 09 23:26:58 2023

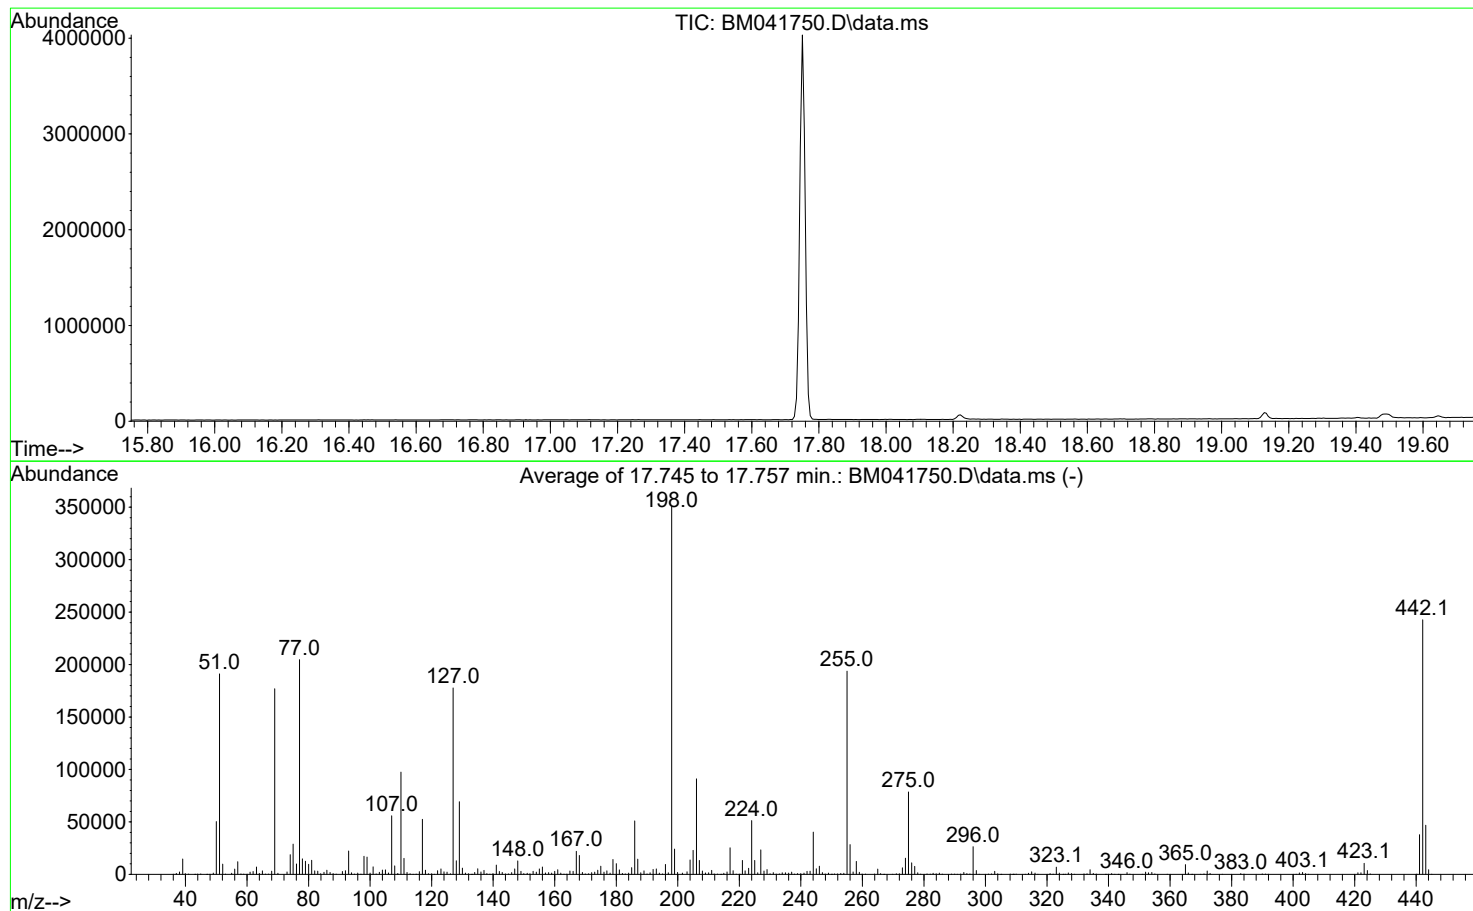

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 54.5         | 191165     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 3049       | PASS                |
| 69             | 198             | 0.00            | 100             | 50.5         | 176960     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 1013       | PASS                |
| 127            | 198             | 10              | 80              | 50.7         | 177664     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 1531       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 350677     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 24091      | PASS                |
| 275            | 198             | 10              | 60              | 22.4         | 78544      | PASS                |
| 365            | 198             | 1               | 100             | 2.7          | 9377       | PASS                |
| 441            | 198             | 0.01            | 100             | 10.8         | 37904      | PASS                |
| 442            | 198             | 50              | 100             | 69.2         | 242731     | PASS                |
| 443            | 442             | 15              | 24              | 19.3         | 46875      | PASS                |

| m/z    | Abundance |
|--------|-----------|
| 39.10  | 220.0     |
| 39.90  | 1725.0    |
| 40.90  | 270.0     |
| 41.90  | 161.0     |
| 43.00  | 197.0     |
| 44.00  | 6511.0    |
| 45.00  | 188.0     |
| 46.90  | 197.0     |
| 49.00  | 677.0     |
| 50.00  | 183.0     |
| 50.90  | 302.0     |
| 73.00  | 642.0     |
| 77.00  | 427.0     |
| 78.00  | 177.0     |
| 83.90  | 343.0     |
| 85.90  | 231.0     |
| 96.00  | 203.0     |
| 133.00 | 370.0     |
| 191.00 | 257.0     |
| 193.00 | 191.0     |
| 207.00 | 2091.0    |
| 208.00 | 476.0     |
| 209.00 | 229.0     |
| 281.00 | 377.0     |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP161

| m/z    | Abundance |
|--------|-----------|
| 36.00  | 392.0     |
| 37.00  | 970.0     |
| 38.00  | 2260.0    |
| 39.10  | 16416.0   |
| 40.00  | 2279.0    |
| 41.10  | 699.0     |
| 43.10  | 267.0     |
| 44.00  | 6860.0    |
| 45.00  | 702.0     |
| 46.90  | 255.0     |
| 47.90  | 213.0     |
| 49.00  | 1871.0    |
| 50.10  | 52264.0   |
| 51.10  | 196544.0  |
| 52.10  | 10148.0   |
| 53.00  | 418.0     |
| 55.00  | 1208.0    |
| 56.00  | 5114.0    |
| 57.00  | 12451.0   |
| 58.00  | 491.0     |
| 59.00  | 271.0     |
| 60.00  | 216.0     |
| 61.00  | 2267.0    |
| 62.00  | 2585.0    |
| 63.00  | 7457.0    |
| 64.00  | 842.0     |
| 65.00  | 3555.0    |
| 66.10  | 371.0     |
| 67.00  | 233.0     |
| 68.00  | 3443.0    |
| 69.00  | 176320.0  |
| 70.00  | 960.0     |
| 73.10  | 2560.0    |
| 74.00  | 18064.0   |
| 75.00  | 29104.0   |
| 76.10  | 10071.0   |
| 77.10  | 205632.0  |
| 78.00  | 15344.0   |
| 79.00  | 12053.0   |
| 80.00  | 9353.0    |
| 81.00  | 13041.0   |
| 82.00  | 3205.0    |
| 83.00  | 2955.0    |
| 84.00  | 905.0     |
| 85.00  | 2019.0    |
| 86.00  | 4088.0    |
| 87.00  | 1889.0    |
| 88.00  | 704.0     |
| 89.00  | 390.0     |
| 91.00  | 2947.0    |
| 92.00  | 3396.0    |
| 93.00  | 22720.0   |
| 93.90  | 1307.0    |
| 95.00  | 317.0     |
| 96.00  | 1431.0    |
| 97.00  | 420.0     |
| 98.00  | 16472.0   |
| 99.00  | 16344.0   |
| 100.00 | 1226.0    |
| 101.00 | 6530.0    |
| 101.90 | 442.0     |
| 103.00 | 2096.0    |
| 104.00 | 3579.0    |
| 105.00 | 4053.0    |
| 106.00 | 1366.0    |
| 107.00 | 53320.0   |
| 108.00 | 7272.0    |
| 108.90 | 1047.0    |
| 110.00 | 91456.0   |
| 111.00 | 14549.0   |
| 112.00 | 1760.0    |
| 113.00 | 794.0     |
| 114.00 | 151.0     |
| 115.00 | 269.0     |
| 116.00 | 2505.0    |
| 117.00 | 50104.0   |
| 118.00 | 4228.0    |
| 118.90 | 632.0     |
| 120.10 | 602.0     |
| 120.90 | 371.0     |
| 122.00 | 3217.0    |
| 123.00 | 4644.0    |
| 124.00 | 2149.0    |
| 125.00 | 1965.0    |
| 126.10 | 527.0     |
| 127.00 | 162880.0  |
| 128.00 | 12296.0   |
| 129.00 | 63768.0   |
| 130.00 | 5416.0    |
| 131.00 | 1086.0    |
| 132.00 | 751.0     |
| 133.00 | 437.0     |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP161

|        |          |
|--------|----------|
| 134.00 | 1677.0   |
| 135.00 | 4954.0   |
| 136.00 | 1937.0   |
| 137.00 | 3829.0   |
| 137.90 | 684.0    |
| 138.90 | 275.0    |
| 140.00 | 732.0    |
| 141.00 | 8247.0   |
| 142.00 | 2719.0   |
| 142.90 | 1466.0   |
| 144.00 | 484.0    |
| 145.00 | 421.0    |
| 146.00 | 1568.0   |
| 147.00 | 4316.0   |
| 148.00 | 11586.0  |
| 149.00 | 2938.0   |
| 149.90 | 834.0    |
| 151.00 | 925.0    |
| 152.00 | 642.0    |
| 153.00 | 2548.0   |
| 154.00 | 1772.0   |
| 155.00 | 4692.0   |
| 156.00 | 6755.0   |
| 157.00 | 1178.0   |
| 158.00 | 1503.0   |
| 159.00 | 973.0    |
| 160.00 | 2435.0   |
| 161.00 | 3670.0   |
| 162.00 | 1112.0   |
| 163.00 | 451.0    |
| 163.90 | 278.0    |
| 164.90 | 3030.0   |
| 166.00 | 2401.0   |
| 167.00 | 19448.0  |
| 168.00 | 17928.0  |
| 169.00 | 1704.0   |
| 169.90 | 460.0    |
| 171.10 | 609.0    |
| 172.00 | 1556.0   |
| 173.00 | 2073.0   |
| 174.00 | 3444.0   |
| 175.00 | 6165.0   |
| 176.00 | 2095.0   |
| 176.90 | 2838.0   |
| 178.00 | 1184.0   |
| 178.90 | 11711.0  |
| 180.00 | 9005.0   |
| 181.00 | 3772.0   |
| 182.00 | 712.0    |
| 182.90 | 345.0    |
| 184.00 | 1063.0   |
| 185.00 | 5594.0   |
| 186.00 | 42912.0  |
| 187.00 | 12616.0  |
| 188.00 | 1551.0   |
| 189.00 | 2883.0   |
| 189.90 | 325.0    |
| 191.00 | 1417.0   |
| 192.00 | 4225.0   |
| 193.00 | 4840.0   |
| 194.00 | 1005.0   |
| 195.10 | 343.0    |
| 196.00 | 8195.0   |
| 196.90 | 1166.0   |
| 198.00 | 296064.0 |
| 198.90 | 20168.0  |
| 199.90 | 1459.0   |
| 201.50 | 1054.0   |
| 203.00 | 1984.0   |
| 204.00 | 11604.0  |
| 205.00 | 19480.0  |
| 206.00 | 76704.0  |
| 207.10 | 13271.0  |
| 208.00 | 3052.0   |
| 209.00 | 1312.0   |
| 210.00 | 1334.0   |
| 211.00 | 3172.0   |
| 211.80 | 720.0    |
| 212.90 | 241.0    |
| 215.00 | 632.0    |
| 216.00 | 2134.0   |
| 217.00 | 20984.0  |
| 218.00 | 3207.0   |
| 218.90 | 267.0    |
| 220.00 | 239.0    |
| 221.00 | 11111.0  |
| 221.90 | 2945.0   |
| 223.00 | 4415.0   |
| 224.00 | 43136.0  |
| 225.00 | 11338.0  |
| 226.00 | 1267.0   |
| 227.00 | 19856.0  |
| 228.00 | 2727.0   |
| 229.00 | 3806.0   |
| 230.00 | 468.0    |
| 231.10 | 1145.0   |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP161

|        |          |
|--------|----------|
| 231.90 | 268.0    |
| 233.00 | 377.0    |
| 233.90 | 1312.0   |
| 235.00 | 1294.0   |
| 236.00 | 1094.0   |
| 237.00 | 2132.0   |
| 238.00 | 308.0    |
| 238.90 | 499.0    |
| 240.00 | 699.0    |
| 241.00 | 1126.0   |
| 242.00 | 2172.0   |
| 243.00 | 2597.0   |
| 244.00 | 30544.0  |
| 245.00 | 4204.0   |
| 246.00 | 5934.0   |
| 247.00 | 1468.0   |
| 247.90 | 278.0    |
| 249.00 | 872.0    |
| 249.90 | 150.0    |
| 250.90 | 271.0    |
| 251.90 | 358.0    |
| 253.00 | 933.0    |
| 254.00 | 857.0    |
| 255.00 | 152448.0 |
| 256.00 | 21808.0  |
| 257.00 | 1953.0   |
| 258.00 | 9619.0   |
| 259.00 | 1712.0   |
| 259.90 | 340.0    |
| 261.00 | 330.0    |
| 264.00 | 315.0    |
| 265.00 | 3784.0   |
| 266.00 | 757.0    |
| 271.00 | 571.0    |
| 272.00 | 472.0    |
| 273.00 | 4532.0   |
| 274.00 | 11596.0  |
| 275.00 | 59032.0  |
| 276.00 | 9129.0   |
| 277.00 | 6076.0   |
| 278.00 | 1066.0   |
| 279.00 | 274.0    |
| 281.00 | 577.0    |
| 282.10 | 447.0    |
| 283.00 | 925.0    |
| 283.90 | 499.0    |
| 285.00 | 821.0    |
| 285.90 | 154.0    |
| 288.90 | 214.0    |
| 290.00 | 184.0    |
| 292.00 | 274.0    |
| 292.90 | 1300.0   |
| 293.90 | 583.0    |
| 295.00 | 270.0    |
| 296.00 | 19488.0  |
| 297.00 | 2898.0   |
| 298.00 | 183.0    |
| 301.00 | 317.0    |
| 302.00 | 308.0    |
| 303.00 | 2255.0   |
| 304.00 | 532.0    |
| 308.00 | 302.0    |
| 309.90 | 259.0    |
| 313.00 | 188.0    |
| 314.00 | 885.0    |
| 315.00 | 1498.0   |
| 316.10 | 1136.0   |
| 321.00 | 451.0    |
| 322.00 | 164.0    |
| 323.00 | 4711.0   |
| 324.00 | 852.0    |
| 327.00 | 904.0    |
| 328.10 | 537.0    |
| 332.00 | 341.0    |
| 333.00 | 440.0    |
| 334.00 | 2901.0   |
| 335.00 | 730.0    |
| 341.00 | 548.0    |
| 342.10 | 151.0    |
| 346.00 | 1069.0   |
| 346.90 | 307.0    |
| 352.00 | 1543.0   |
| 353.00 | 956.0    |
| 354.10 | 1300.0   |
| 355.00 | 362.0    |
| 365.00 | 5880.0   |
| 365.90 | 927.0    |
| 370.00 | 168.0    |
| 371.00 | 373.0    |
| 372.10 | 2038.0   |
| 373.00 | 720.0    |
| 383.00 | 680.0    |
| 384.00 | 183.0    |
| 390.00 | 319.0    |
| 391.00 | 163.0    |
| 401.90 | 909.0    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP161

|        |          |
|--------|----------|
| 403.00 | 1102.0   |
| 404.00 | 476.0    |
| 405.00 | 184.0    |
| 421.00 | 772.0    |
| 422.00 | 992.0    |
| 423.10 | 6540.0   |
| 424.10 | 2749.0   |
| 425.00 | 449.0    |
| 441.00 | 20704.0  |
| 442.10 | 134272.0 |
| 443.10 | 27864.0  |
| 444.00 | 3002.0   |

|                  |
|------------------|
| Instrument :     |
| BNA_M            |
| ClientSampleId : |
| DFTPP161         |

| m/z    | Abundance |
|--------|-----------|
| 36.00  | 310.0     |
| 37.00  | 1051.0    |
| 38.10  | 2765.0    |
| 39.10  | 16768.0   |
| 40.00  | 2946.0    |
| 41.00  | 510.0     |
| 42.00  | 187.0     |
| 43.00  | 333.0     |
| 44.00  | 7189.0    |
| 45.00  | 689.0     |
| 46.90  | 272.0     |
| 48.00  | 315.0     |
| 49.00  | 2072.0    |
| 50.10  | 60144.0   |
| 51.10  | 226496.0  |
| 52.10  | 11407.0   |
| 53.00  | 478.0     |
| 55.00  | 1146.0    |
| 56.00  | 6060.0    |
| 57.00  | 13899.0   |
| 58.00  | 706.0     |
| 59.00  | 366.0     |
| 60.00  | 261.0     |
| 61.00  | 2574.0    |
| 62.00  | 3602.0    |
| 63.00  | 8317.0    |
| 64.00  | 1018.0    |
| 65.00  | 4046.0    |
| 66.00  | 392.0     |
| 67.00  | 312.0     |
| 68.00  | 3328.0    |
| 69.00  | 209856.0  |
| 70.10  | 1278.0    |
| 73.10  | 3156.0    |
| 74.00  | 22392.0   |
| 75.00  | 34408.0   |
| 76.00  | 11688.0   |
| 77.10  | 245184.0  |
| 78.10  | 17896.0   |
| 79.00  | 14811.0   |
| 80.00  | 11502.0   |
| 81.00  | 16040.0   |
| 82.00  | 4005.0    |
| 83.00  | 3850.0    |
| 83.90  | 1271.0    |
| 85.00  | 2477.0    |
| 86.00  | 5422.0    |
| 87.00  | 1815.0    |
| 88.00  | 1020.0    |
| 88.90  | 362.0     |
| 91.00  | 3172.0    |
| 92.00  | 4260.0    |
| 93.00  | 26176.0   |
| 94.00  | 1953.0    |
| 94.90  | 447.0     |
| 96.00  | 1723.0    |
| 97.00  | 324.0     |
| 98.00  | 21256.0   |
| 99.00  | 19504.0   |
| 100.00 | 1625.0    |
| 101.00 | 8593.0    |
| 102.00 | 430.0     |
| 103.00 | 2172.0    |
| 104.00 | 5578.0    |
| 105.00 | 5167.0    |
| 106.00 | 1497.0    |
| 107.00 | 67984.0   |
| 108.00 | 9916.0    |
| 109.10 | 1428.0    |
| 110.00 | 119912.0  |
| 111.00 | 18712.0   |
| 112.00 | 2233.0    |
| 113.00 | 736.0     |
| 114.00 | 168.0     |
| 114.90 | 342.0     |
| 116.00 | 3320.0    |
| 117.00 | 64664.0   |
| 118.00 | 4794.0    |
| 118.90 | 597.0     |
| 120.00 | 752.0     |
| 121.00 | 169.0     |
| 122.00 | 4309.0    |
| 123.00 | 6815.0    |
| 124.00 | 3094.0    |
| 125.00 | 2737.0    |
| 126.10 | 607.0     |
| 127.00 | 216832.0  |
| 128.00 | 15826.0   |
| 129.00 | 84944.0   |
| 130.00 | 7309.0    |
| 131.00 | 1527.0    |
| 131.90 | 710.0     |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP161

|        |          |
|--------|----------|
| 133.00 | 375.0    |
| 134.00 | 2245.0   |
| 135.00 | 6786.0   |
| 136.00 | 2949.0   |
| 137.00 | 4789.0   |
| 138.00 | 990.0    |
| 138.90 | 438.0    |
| 140.00 | 905.0    |
| 141.00 | 10714.0  |
| 142.00 | 3260.0   |
| 143.00 | 2388.0   |
| 144.00 | 665.0    |
| 144.90 | 713.0    |
| 146.00 | 2017.0   |
| 147.00 | 6833.0   |
| 148.00 | 15707.0  |
| 149.00 | 3333.0   |
| 150.00 | 770.0    |
| 151.10 | 1371.0   |
| 152.00 | 780.0    |
| 153.00 | 3743.0   |
| 154.00 | 2576.0   |
| 155.00 | 6381.0   |
| 156.00 | 8419.0   |
| 157.00 | 1843.0   |
| 158.00 | 2054.0   |
| 159.00 | 1413.0   |
| 160.00 | 3535.0   |
| 161.00 | 5556.0   |
| 162.00 | 1573.0   |
| 163.00 | 364.0    |
| 163.90 | 389.0    |
| 165.00 | 3771.0   |
| 166.00 | 3436.0   |
| 167.00 | 27032.0  |
| 168.00 | 20096.0  |
| 169.00 | 2254.0   |
| 170.00 | 582.0    |
| 171.00 | 968.0    |
| 172.00 | 2151.0   |
| 173.00 | 2526.0   |
| 174.00 | 4980.0   |
| 175.00 | 9776.0   |
| 176.00 | 2102.0   |
| 177.00 | 3677.0   |
| 178.00 | 1458.0   |
| 179.00 | 17416.0  |
| 180.00 | 11937.0  |
| 181.00 | 4941.0   |
| 182.00 | 888.0    |
| 183.00 | 553.0    |
| 184.00 | 1491.0   |
| 185.00 | 7936.0   |
| 186.00 | 62768.0  |
| 187.00 | 18480.0  |
| 188.00 | 1793.0   |
| 189.00 | 3789.0   |
| 190.00 | 836.0    |
| 191.00 | 2082.0   |
| 192.00 | 5851.0   |
| 193.00 | 6445.0   |
| 194.00 | 1300.0   |
| 195.00 | 602.0    |
| 196.00 | 11650.0  |
| 196.80 | 1777.0   |
| 198.00 | 430144.0 |
| 199.00 | 30248.0  |
| 200.00 | 2552.0   |
| 201.40 | 1480.0   |
| 203.00 | 3320.0   |
| 204.00 | 17016.0  |
| 205.00 | 27592.0  |
| 206.10 | 111808.0 |
| 207.00 | 18952.0  |
| 208.00 | 4490.0   |
| 209.00 | 1891.0   |
| 210.00 | 1597.0   |
| 211.00 | 4554.0   |
| 212.90 | 320.0    |
| 213.90 | 174.0    |
| 215.00 | 1387.0   |
| 216.00 | 2914.0   |
| 217.00 | 31016.0  |
| 218.00 | 4329.0   |
| 218.90 | 358.0    |
| 220.20 | 691.0    |
| 221.00 | 17352.0  |
| 221.90 | 3905.0   |
| 223.00 | 7496.0   |
| 224.00 | 61952.0  |
| 225.00 | 16880.0  |
| 226.00 | 1864.0   |
| 227.00 | 28576.0  |
| 228.00 | 4198.0   |
| 229.00 | 5748.0   |
| 230.00 | 820.0    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP161

|        |          |
|--------|----------|
| 231.00 | 2504.0   |
| 232.00 | 374.0    |
| 233.10 | 548.0    |
| 234.00 | 1546.0   |
| 235.00 | 1917.0   |
| 236.00 | 1412.0   |
| 237.00 | 2746.0   |
| 238.00 | 353.0    |
| 239.00 | 976.0    |
| 240.00 | 796.0    |
| 241.00 | 1634.0   |
| 242.00 | 3586.0   |
| 243.00 | 3733.0   |
| 244.10 | 49864.0  |
| 245.00 | 6915.0   |
| 246.00 | 9430.0   |
| 247.00 | 1924.0   |
| 247.90 | 445.0    |
| 248.90 | 1670.0   |
| 250.10 | 404.0    |
| 250.90 | 470.0    |
| 252.00 | 529.0    |
| 253.00 | 1124.0   |
| 253.90 | 1476.0   |
| 255.00 | 241344.0 |
| 256.00 | 35880.0  |
| 257.00 | 3082.0   |
| 258.00 | 14934.0  |
| 259.00 | 2456.0   |
| 259.90 | 305.0    |
| 261.00 | 440.0    |
| 264.00 | 334.0    |
| 265.00 | 6381.0   |
| 266.00 | 819.0    |
| 269.90 | 256.0    |
| 271.00 | 821.0    |
| 272.00 | 758.0    |
| 273.00 | 7813.0   |
| 274.00 | 19088.0  |
| 275.00 | 97920.0  |
| 276.00 | 13503.0  |
| 277.00 | 9237.0   |
| 278.00 | 1986.0   |
| 279.00 | 339.0    |
| 281.10 | 769.0    |
| 282.00 | 388.0    |
| 283.00 | 1268.0   |
| 284.00 | 688.0    |
| 285.00 | 1599.0   |
| 285.90 | 339.0    |
| 289.00 | 225.0    |
| 289.90 | 421.0    |
| 290.90 | 327.0    |
| 292.00 | 292.0    |
| 293.00 | 2236.0   |
| 294.00 | 886.0    |
| 295.00 | 473.0    |
| 296.00 | 32480.0  |
| 297.00 | 4736.0   |
| 297.90 | 282.0    |
| 301.00 | 424.0    |
| 301.90 | 690.0    |
| 303.00 | 3672.0   |
| 304.00 | 730.0    |
| 305.00 | 158.0    |
| 308.10 | 317.0    |
| 308.90 | 253.0    |
| 309.90 | 372.0    |
| 313.00 | 308.0    |
| 314.00 | 1184.0   |
| 315.00 | 3046.0   |
| 316.10 | 1315.0   |
| 317.10 | 271.0    |
| 321.00 | 1031.0   |
| 322.00 | 425.0    |
| 323.10 | 8384.0   |
| 324.00 | 1599.0   |
| 325.20 | 160.0    |
| 326.00 | 212.0    |
| 326.90 | 1646.0   |
| 327.90 | 1030.0   |
| 329.00 | 171.0    |
| 332.00 | 683.0    |
| 333.00 | 848.0    |
| 334.00 | 5477.0   |
| 335.00 | 1154.0   |
| 335.80 | 162.0    |
| 336.20 | 164.0    |
| 339.00 | 219.0    |
| 339.90 | 164.0    |
| 341.00 | 988.0    |
| 342.00 | 229.0    |
| 343.10 | 172.0    |
| 346.00 | 2050.0   |
| 347.00 | 334.0    |
| 350.90 | 164.0    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP161

|        |          |
|--------|----------|
| 352.10 | 2760.0   |
| 353.00 | 1716.0   |
| 354.10 | 2115.0   |
| 355.10 | 566.0    |
| 359.10 | 158.0    |
| 365.00 | 11695.0  |
| 366.00 | 1528.0   |
| 367.00 | 163.0    |
| 370.00 | 224.0    |
| 371.00 | 655.0    |
| 372.00 | 3595.0   |
| 373.00 | 985.0    |
| 376.90 | 186.0    |
| 383.00 | 873.0    |
| 384.00 | 291.0    |
| 389.90 | 493.0    |
| 391.10 | 294.0    |
| 392.00 | 317.0    |
| 401.00 | 252.0    |
| 402.00 | 1729.0   |
| 403.10 | 2250.0   |
| 404.00 | 899.0    |
| 405.00 | 288.0    |
| 421.00 | 1892.0   |
| 422.10 | 1939.0   |
| 423.10 | 12702.0  |
| 424.10 | 4506.0   |
| 425.10 | 580.0    |
| 440.00 | 218.0    |
| 441.10 | 45328.0  |
| 442.10 | 295488.0 |
| 443.10 | 57064.0  |
| 444.10 | 5271.0   |
| 445.00 | 371.0    |

**Instrument :**  
BNA\_M  
**ClientSampleId :**  
DFTPP161

| m/z    | Abundance |
|--------|-----------|
| 37.00  | 832.0     |
| 38.00  | 1958.0    |
| 39.10  | 11208.0   |
| 40.00  | 2443.0    |
| 41.10  | 645.0     |
| 42.10  | 181.0     |
| 42.90  | 226.0     |
| 44.00  | 6577.0    |
| 44.90  | 585.0     |
| 46.90  | 194.0     |
| 49.00  | 1777.0    |
| 50.00  | 39344.0   |
| 51.10  | 151360.0  |
| 52.10  | 7619.0    |
| 53.00  | 282.0     |
| 55.00  | 801.0     |
| 56.00  | 4114.0    |
| 57.00  | 9747.0    |
| 58.00  | 307.0     |
| 58.90  | 213.0     |
| 60.00  | 187.0     |
| 61.10  | 1410.0    |
| 62.00  | 1981.0    |
| 63.10  | 5369.0    |
| 64.00  | 804.0     |
| 65.00  | 2658.0    |
| 66.10  | 243.0     |
| 67.00  | 233.0     |
| 68.00  | 2377.0    |
| 69.00  | 144704.0  |
| 70.00  | 802.0     |
| 73.00  | 3111.0    |
| 74.10  | 15806.0   |
| 75.00  | 22864.0   |
| 76.00  | 8201.0    |
| 77.10  | 164672.0  |
| 78.10  | 11721.0   |
| 79.00  | 10519.0   |
| 80.00  | 8102.0    |
| 81.00  | 11222.0   |
| 82.00  | 2955.0    |
| 83.00  | 2466.0    |
| 84.00  | 880.0     |
| 85.00  | 1683.0    |
| 86.00  | 3178.0    |
| 87.00  | 1588.0    |
| 87.90  | 448.0     |
| 89.00  | 344.0     |
| 91.00  | 2274.0    |
| 92.00  | 2728.0    |
| 93.00  | 18144.0   |
| 94.00  | 1220.0    |
| 95.00  | 316.0     |
| 96.00  | 1103.0    |
| 97.00  | 410.0     |
| 98.00  | 13816.0   |
| 99.00  | 13477.0   |
| 100.00 | 1051.0    |
| 101.00 | 6540.0    |
| 102.00 | 397.0     |
| 103.00 | 1516.0    |
| 104.00 | 3379.0    |
| 105.00 | 3740.0    |
| 105.90 | 1304.0    |
| 107.00 | 46264.0   |
| 108.00 | 6932.0    |
| 108.90 | 974.0     |
| 110.00 | 81216.0   |
| 111.00 | 12675.0   |
| 112.00 | 1688.0    |
| 112.90 | 426.0     |
| 114.90 | 168.0     |
| 116.00 | 2050.0    |
| 117.00 | 42800.0   |
| 118.00 | 3071.0    |
| 119.00 | 420.0     |
| 119.90 | 415.0     |
| 121.00 | 166.0     |
| 121.90 | 2813.0    |
| 123.00 | 4340.0    |
| 124.00 | 2090.0    |
| 125.00 | 1965.0    |
| 126.10 | 562.0     |
| 127.00 | 153280.0  |
| 128.00 | 10719.0   |
| 129.00 | 58968.0   |
| 130.00 | 4957.0    |
| 130.90 | 846.0     |
| 132.00 | 615.0     |
| 132.90 | 496.0     |
| 134.00 | 1557.0    |
| 135.00 | 4249.0    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP161

|        |          |
|--------|----------|
| 136.00 | 2138.0   |
| 137.00 | 2967.0   |
| 138.00 | 559.0    |
| 139.00 | 264.0    |
| 139.90 | 805.0    |
| 141.00 | 7462.0   |
| 142.00 | 2286.0   |
| 143.00 | 1822.0   |
| 144.00 | 446.0    |
| 144.90 | 251.0    |
| 146.00 | 1380.0   |
| 147.00 | 4235.0   |
| 148.00 | 11313.0  |
| 149.00 | 2680.0   |
| 149.90 | 657.0    |
| 151.00 | 929.0    |
| 151.90 | 548.0    |
| 153.00 | 2547.0   |
| 154.00 | 2274.0   |
| 155.00 | 4520.0   |
| 156.00 | 6103.0   |
| 157.00 | 1102.0   |
| 158.00 | 1387.0   |
| 159.00 | 1099.0   |
| 160.00 | 2565.0   |
| 161.00 | 4005.0   |
| 162.00 | 872.0    |
| 162.90 | 267.0    |
| 164.00 | 506.0    |
| 165.00 | 3054.0   |
| 166.00 | 2710.0   |
| 167.00 | 19480.0  |
| 168.00 | 15876.0  |
| 169.00 | 1676.0   |
| 169.90 | 412.0    |
| 170.90 | 531.0    |
| 172.00 | 1487.0   |
| 173.00 | 2025.0   |
| 174.00 | 3506.0   |
| 175.00 | 7311.0   |
| 176.00 | 2069.0   |
| 177.00 | 3409.0   |
| 178.00 | 1048.0   |
| 179.00 | 13381.0  |
| 180.00 | 9636.0   |
| 181.00 | 3997.0   |
| 182.00 | 949.0    |
| 182.90 | 327.0    |
| 184.00 | 1080.0   |
| 185.00 | 5758.0   |
| 186.00 | 47344.0  |
| 187.00 | 12577.0  |
| 188.00 | 1203.0   |
| 189.00 | 3228.0   |
| 190.10 | 436.0    |
| 191.00 | 1843.0   |
| 192.00 | 4171.0   |
| 193.00 | 4952.0   |
| 194.00 | 1169.0   |
| 195.00 | 458.0    |
| 196.00 | 8508.0   |
| 197.00 | 1649.0   |
| 198.00 | 325824.0 |
| 199.00 | 21856.0  |
| 200.00 | 1746.0   |
| 201.60 | 1029.0   |
| 203.00 | 2218.0   |
| 204.00 | 12437.0  |
| 205.00 | 21584.0  |
| 206.00 | 84816.0  |
| 207.00 | 14060.0  |
| 208.00 | 3538.0   |
| 209.00 | 1453.0   |
| 210.10 | 1504.0   |
| 211.00 | 3825.0   |
| 212.00 | 581.0    |
| 213.00 | 240.0    |
| 214.90 | 1116.0   |
| 216.00 | 2022.0   |
| 217.00 | 23984.0  |
| 218.00 | 3060.0   |
| 219.00 | 225.0    |
| 219.90 | 307.0    |
| 221.00 | 11560.0  |
| 221.90 | 3088.0   |
| 223.00 | 5435.0   |
| 224.00 | 48648.0  |
| 225.00 | 11532.0  |
| 226.00 | 1536.0   |
| 227.00 | 21680.0  |
| 228.00 | 2890.0   |
| 229.00 | 4246.0   |
| 230.00 | 655.0    |
| 231.00 | 1559.0   |
| 232.00 | 288.0    |
| 232.90 | 358.0    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP161

|        |          |
|--------|----------|
| 234.00 | 1541.0   |
| 235.00 | 1450.0   |
| 236.00 | 1025.0   |
| 237.00 | 1666.0   |
| 237.90 | 235.0    |
| 238.90 | 813.0    |
| 240.00 | 668.0    |
| 241.00 | 989.0    |
| 242.00 | 3001.0   |
| 243.00 | 3052.0   |
| 244.10 | 40592.0  |
| 245.00 | 4869.0   |
| 246.00 | 7841.0   |
| 247.00 | 1487.0   |
| 248.10 | 374.0    |
| 249.00 | 1366.0   |
| 251.00 | 493.0    |
| 252.00 | 550.0    |
| 253.00 | 724.0    |
| 254.00 | 1097.0   |
| 255.00 | 187456.0 |
| 256.00 | 27680.0  |
| 257.00 | 2100.0   |
| 258.00 | 12311.0  |
| 259.00 | 1961.0   |
| 259.90 | 293.0    |
| 261.00 | 233.0    |
| 263.90 | 333.0    |
| 265.00 | 5060.0   |
| 265.90 | 540.0    |
| 266.90 | 180.0    |
| 269.90 | 393.0    |
| 271.00 | 512.0    |
| 272.00 | 512.0    |
| 273.00 | 6362.0   |
| 274.00 | 15347.0  |
| 275.00 | 78680.0  |
| 276.00 | 10104.0  |
| 277.00 | 7498.0   |
| 278.00 | 1413.0   |
| 279.00 | 212.0    |
| 281.00 | 998.0    |
| 282.00 | 272.0    |
| 283.00 | 962.0    |
| 284.00 | 529.0    |
| 285.00 | 1188.0   |
| 286.00 | 262.0    |
| 288.90 | 331.0    |
| 290.10 | 247.0    |
| 290.80 | 199.0    |
| 291.90 | 337.0    |
| 293.00 | 1874.0   |
| 294.00 | 676.0    |
| 294.90 | 495.0    |
| 296.00 | 27272.0  |
| 297.00 | 3190.0   |
| 297.90 | 252.0    |
| 301.00 | 405.0    |
| 302.00 | 553.0    |
| 303.00 | 2707.0   |
| 304.00 | 596.0    |
| 308.00 | 500.0    |
| 309.10 | 224.0    |
| 310.00 | 296.0    |
| 312.80 | 202.0    |
| 314.00 | 1073.0   |
| 315.00 | 2714.0   |
| 316.10 | 1386.0   |
| 317.00 | 208.0    |
| 321.00 | 829.0    |
| 322.00 | 475.0    |
| 323.10 | 7352.0   |
| 324.00 | 1381.0   |
| 326.00 | 170.0    |
| 327.00 | 1573.0   |
| 327.90 | 908.0    |
| 329.00 | 217.0    |
| 332.00 | 493.0    |
| 333.00 | 582.0    |
| 334.00 | 5003.0   |
| 335.10 | 1097.0   |
| 336.10 | 153.0    |
| 340.00 | 206.0    |
| 341.00 | 953.0    |
| 342.00 | 260.0    |
| 346.00 | 1834.0   |
| 346.90 | 331.0    |
| 351.00 | 178.0    |
| 352.00 | 2326.0   |
| 353.00 | 1750.0   |
| 354.00 | 1981.0   |
| 355.00 | 441.0    |
| 359.00 | 163.0    |
| 365.00 | 10555.0  |
| 366.00 | 1591.0   |
| 370.00 | 189.0    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP161

|        |          |
|--------|----------|
| 371.00 | 507.0    |
| 372.10 | 4123.0   |
| 373.00 | 1011.0   |
| 377.00 | 150.0    |
| 383.00 | 851.0    |
| 384.00 | 384.0    |
| 390.00 | 507.0    |
| 391.00 | 275.0    |
| 391.90 | 325.0    |
| 400.90 | 224.0    |
| 402.10 | 1316.0   |
| 403.00 | 2329.0   |
| 404.10 | 796.0    |
| 405.00 | 204.0    |
| 421.10 | 1905.0   |
| 422.00 | 1861.0   |
| 423.10 | 12486.0  |
| 424.10 | 3742.0   |
| 425.00 | 550.0    |
| 441.10 | 47680.0  |
| 442.10 | 298432.0 |
| 443.10 | 55696.0  |
| 444.10 | 4902.0   |
| 445.10 | 251.0    |

**Instrument :**  
BNA\_M  
**ClientSampleId :**  
DFTPP161