

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091019\
 Data File : BM022642.D
 Acq On : 11 Sep 2019 05:19
 Operator : HP/JU
 Sample : K4682-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 11 06:46:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 11 05:39:50 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	18331	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	78139	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	44826	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	6097844	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.39
20) Perylene-d12	23.67	264	68295	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	30651	0.24	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.53	252	20077	0.077	ng/ul#	Ovalue 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091019\
Data File : BM022642.D
Acq On : 11 Sep 2019 05:19
Operator : HP/JU
Sample : K4682-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 11 06:46:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 11 05:39:50 2019
Response via : Initial Calibration

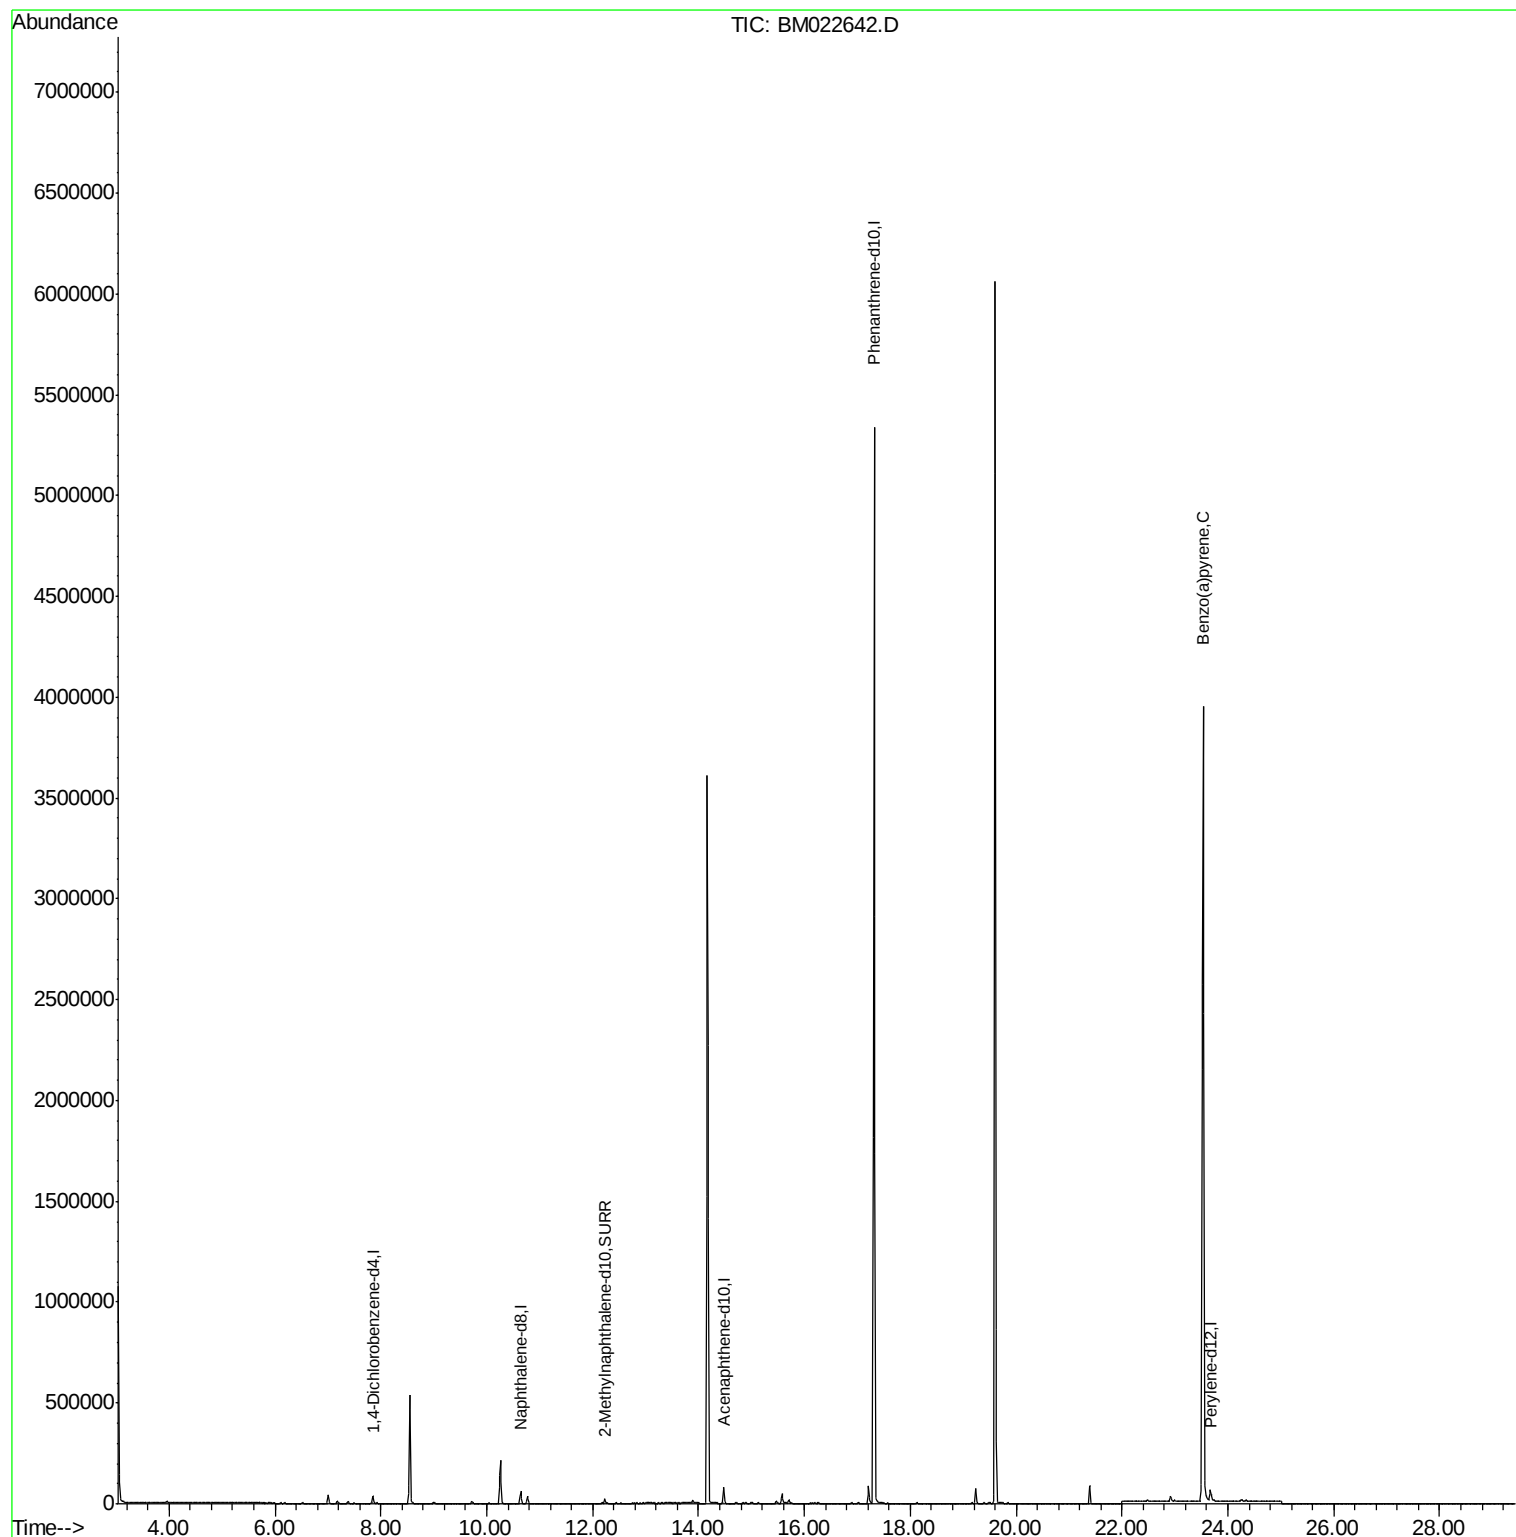

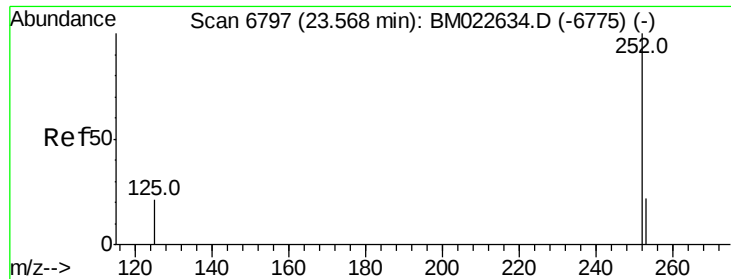

#23

Benzo(a)pyrene

Concen: 0.077 ng/ul

RT: 23.53 min Scan# 6781

Delta R.T. -0.04 min

Lab File: BM022642.D

Acq: 11 Sep 2019 05:19

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 252 Resp: 20077

Ion Ratio Lower Upper

252 100

253 38.3 20.2 30.2#

125 33.2 15.7 23.5#

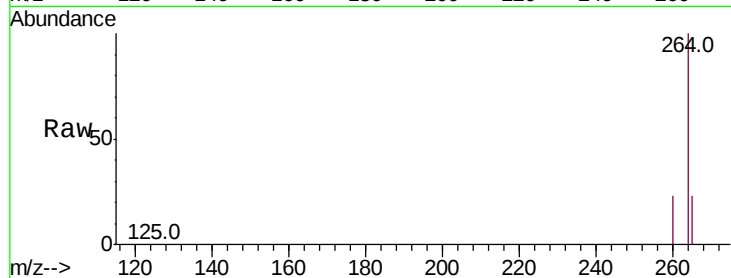

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

