

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091019\
 Data File : BM022645.D
 Acq On : 11 Sep 2019 07:09
 Operator : HP/JU
 Sample : K4682-12
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 11 07:47:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 11 07:37:53 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	20998	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	89081	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	50099	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	6781124	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.39
20) Perylene-d12	23.67	264	74064	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	33425	0.23	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	1640	0.00	ng/ul	0.06
Target Compounds						
23) Benzo(a)pyrene	23.53	252	22391	0.080	ng/ul#	Ovalue 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091019\
Data File : BM022645.D
Acq On : 11 Sep 2019 07:09
Operator : HP/JU
Sample : K4682-12
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 11 07:47:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 11 07:37:53 2019
Response via : Initial Calibration

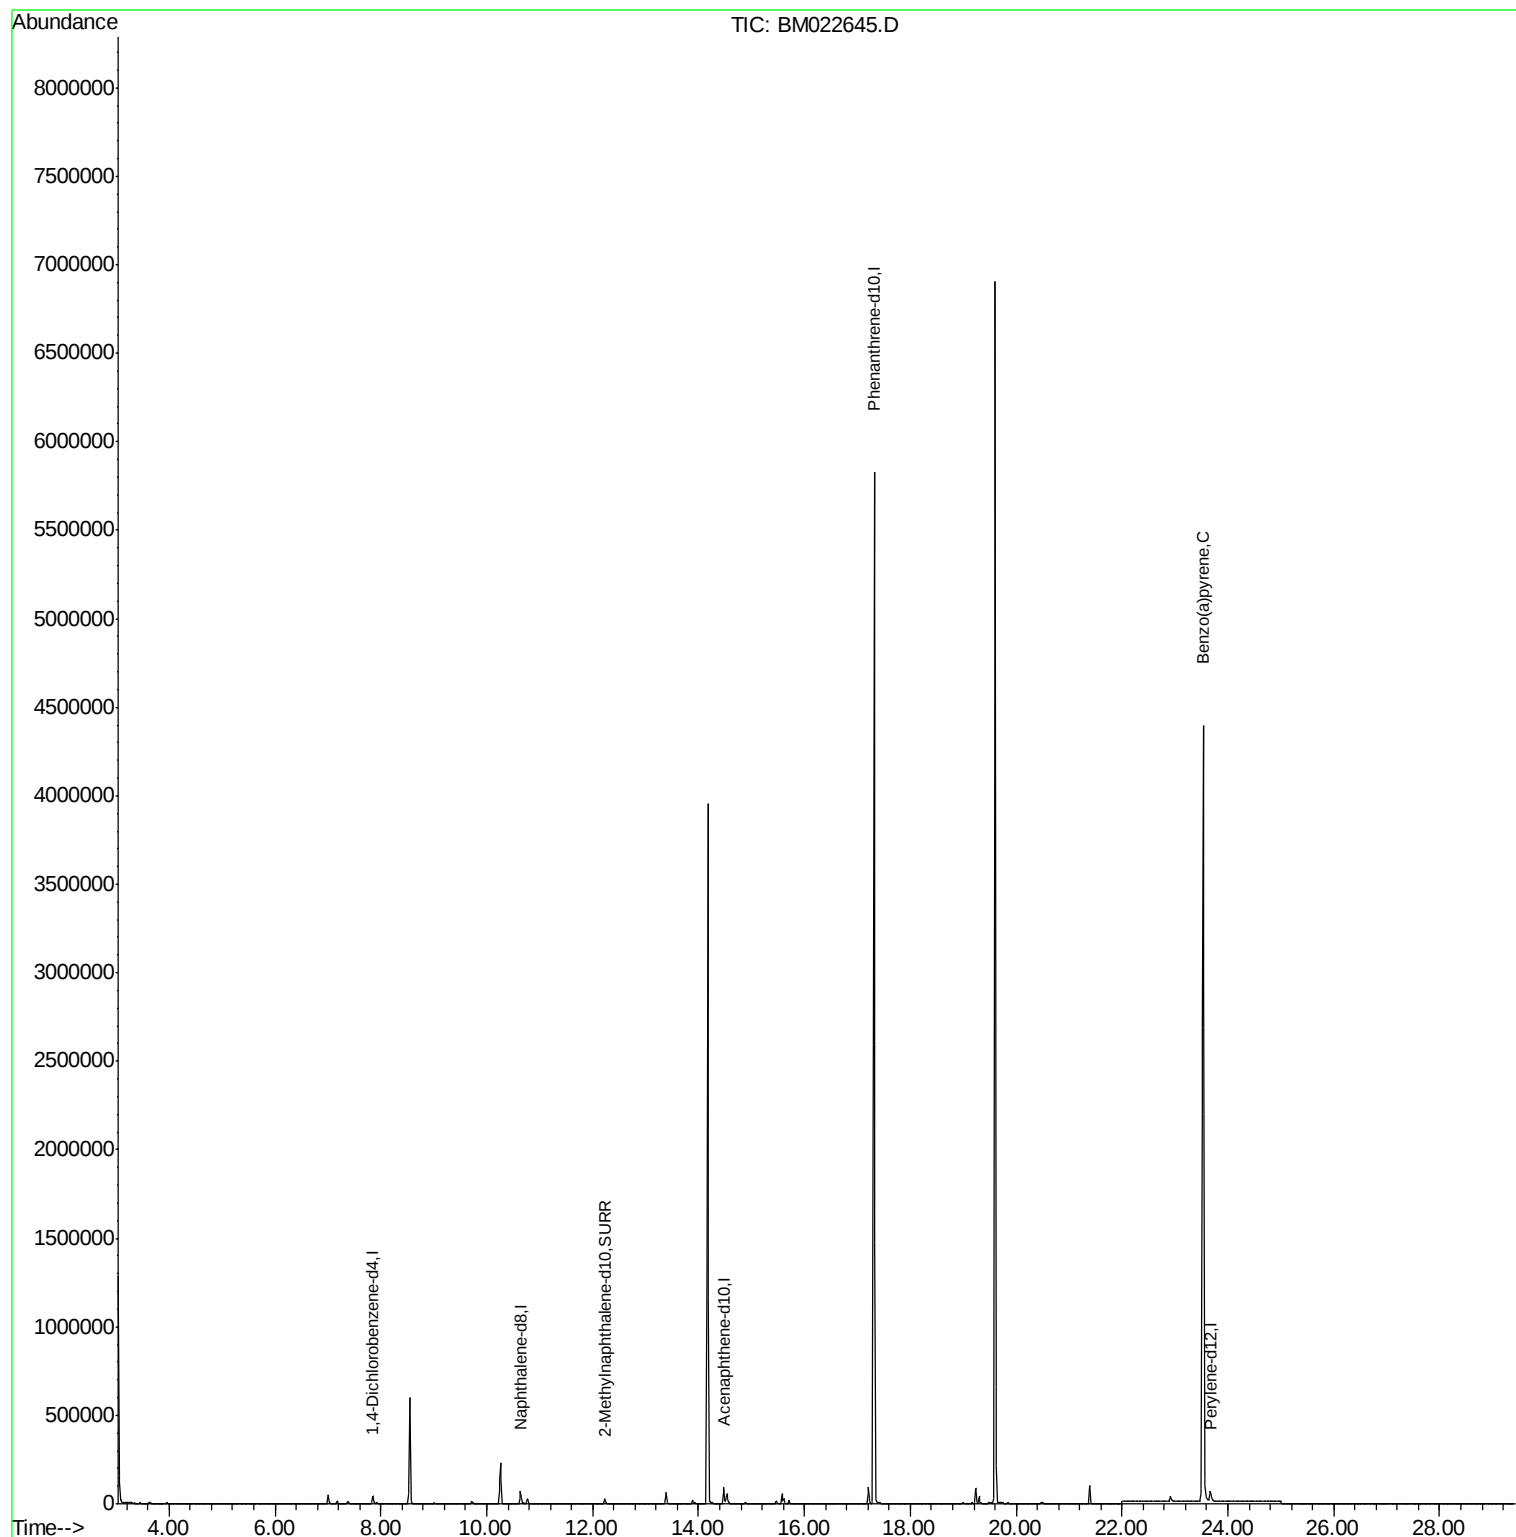

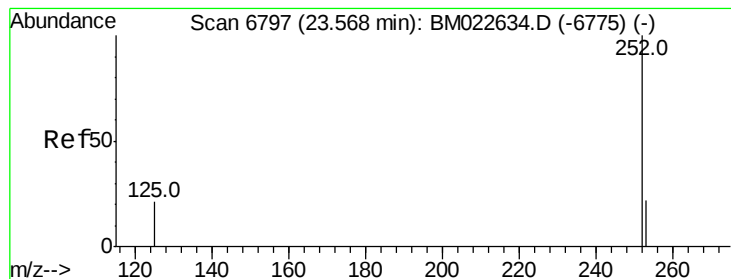

#23

Benzo(a)pyrene

Concen: 0.080 ng/ul

RT: 23.53 min Scan# 6782

Delta R.T. -0.04 min


Lab File: BM022645.D

Acq: 11 Sep 2019 07:09

Instrument :

BNA_M

ClientSampleId :

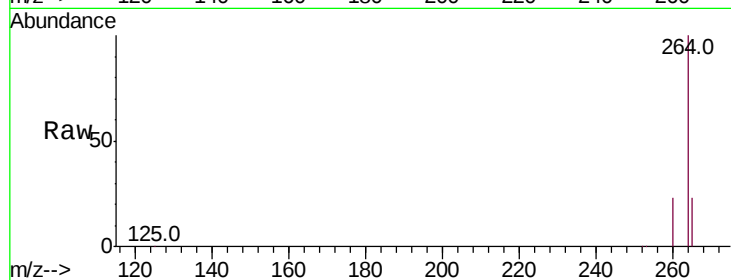


Tot Ion: 252 Resp: 22391

Ion Ratio Lower Upper

252 100

253 36.5 20.2 30.2#

125 30.5 15.7 23.5#

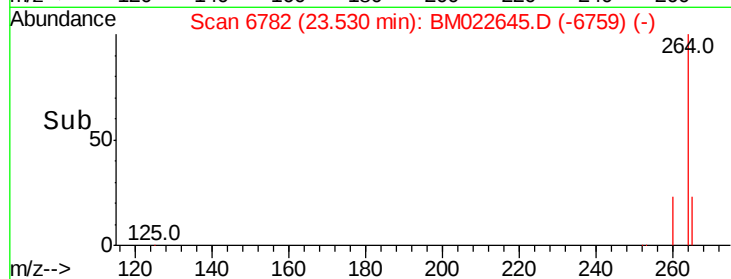

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

