

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091019\
 Data File : BM022646.D
 Acq On : 11 Sep 2019 07:45
 Operator : HP/JU
 Sample : PB122838BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 11 08:20:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 11 07:37:53 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	19528	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	84299	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	46979	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	6838465	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.39
20) Perylene-d12	23.67	264	66046	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	39684	0.29	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.69	128	10732	0.045	ng/ul#	96
23) Benzo(a)pyrene	23.53	252	21700	0.086	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091019\
Data File : BM022646.D
Acq On : 11 Sep 2019 07:45
Operator : HP/JU
Sample : PB122838BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 11 08:20:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 11 07:37:53 2019
Response via : Initial Calibration

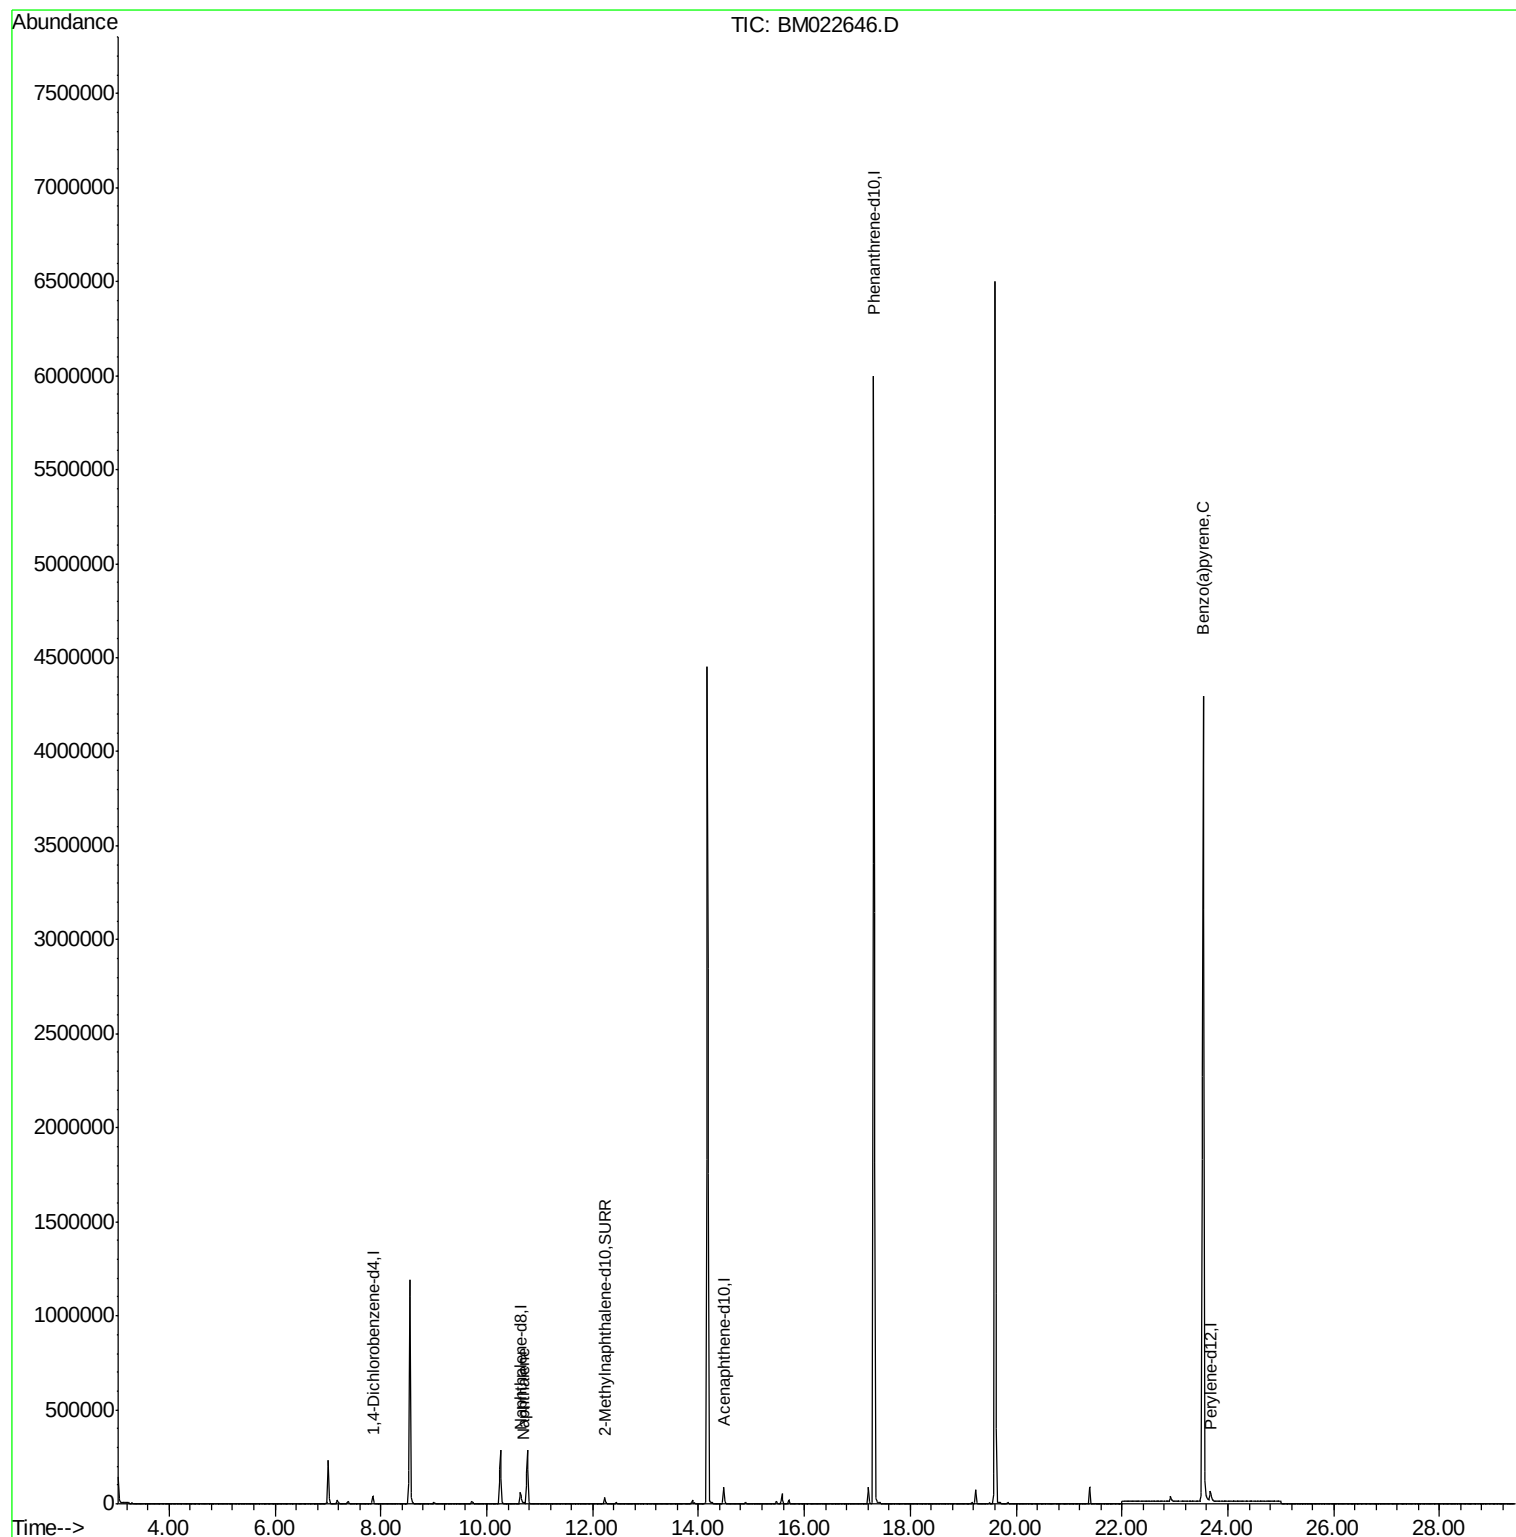

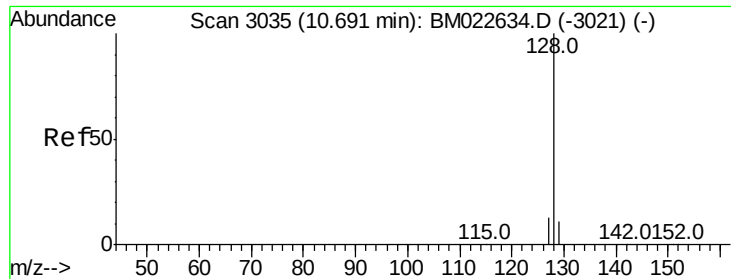

#3

Naphthalene

Concen: 0.045 ng/ul

RT: 10.69 min Scan# 3035

Delta R.T. -0.00 min

Lab File: BM022646.D

Acq: 11 Sep 2019 07:45

Instrument :

BNA_M

ClientSampled :





Tot Ion:128 Resp: 10732

Ion Ratio Lower Upper

128 100

129 13.6 8.8 13.2#

127 14.0 10.4 15.6

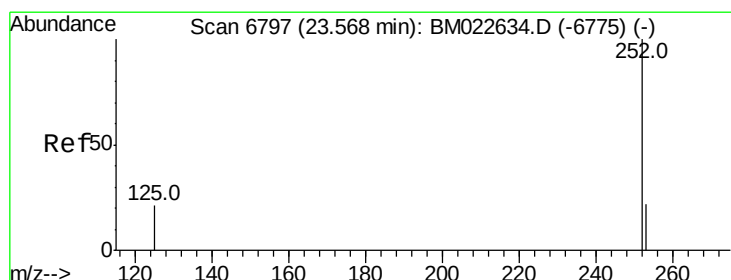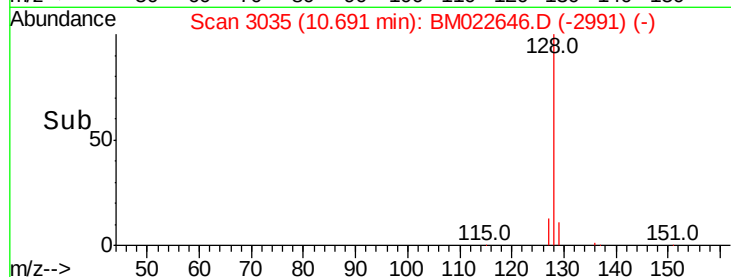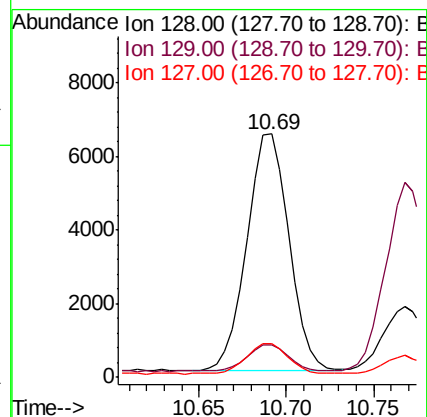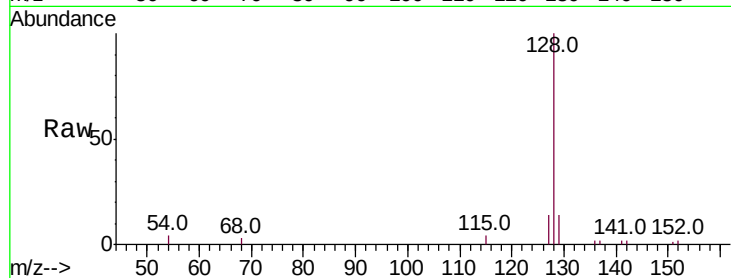

#23

Benzo(a)pyrene

Concen: 0.086 ng/ul

RT: 23.53 min Scan# 6782

Delta R.T. -0.04 min

Lab File: BM022646.D

Acq: 11 Sep 2019 07:45

Tgt Ion:252 Resp: 21700

Ion Ratio Lower Upper

252 100

253 36.0 20.2 30.2#

125 29.6 15.7 23.5#

