

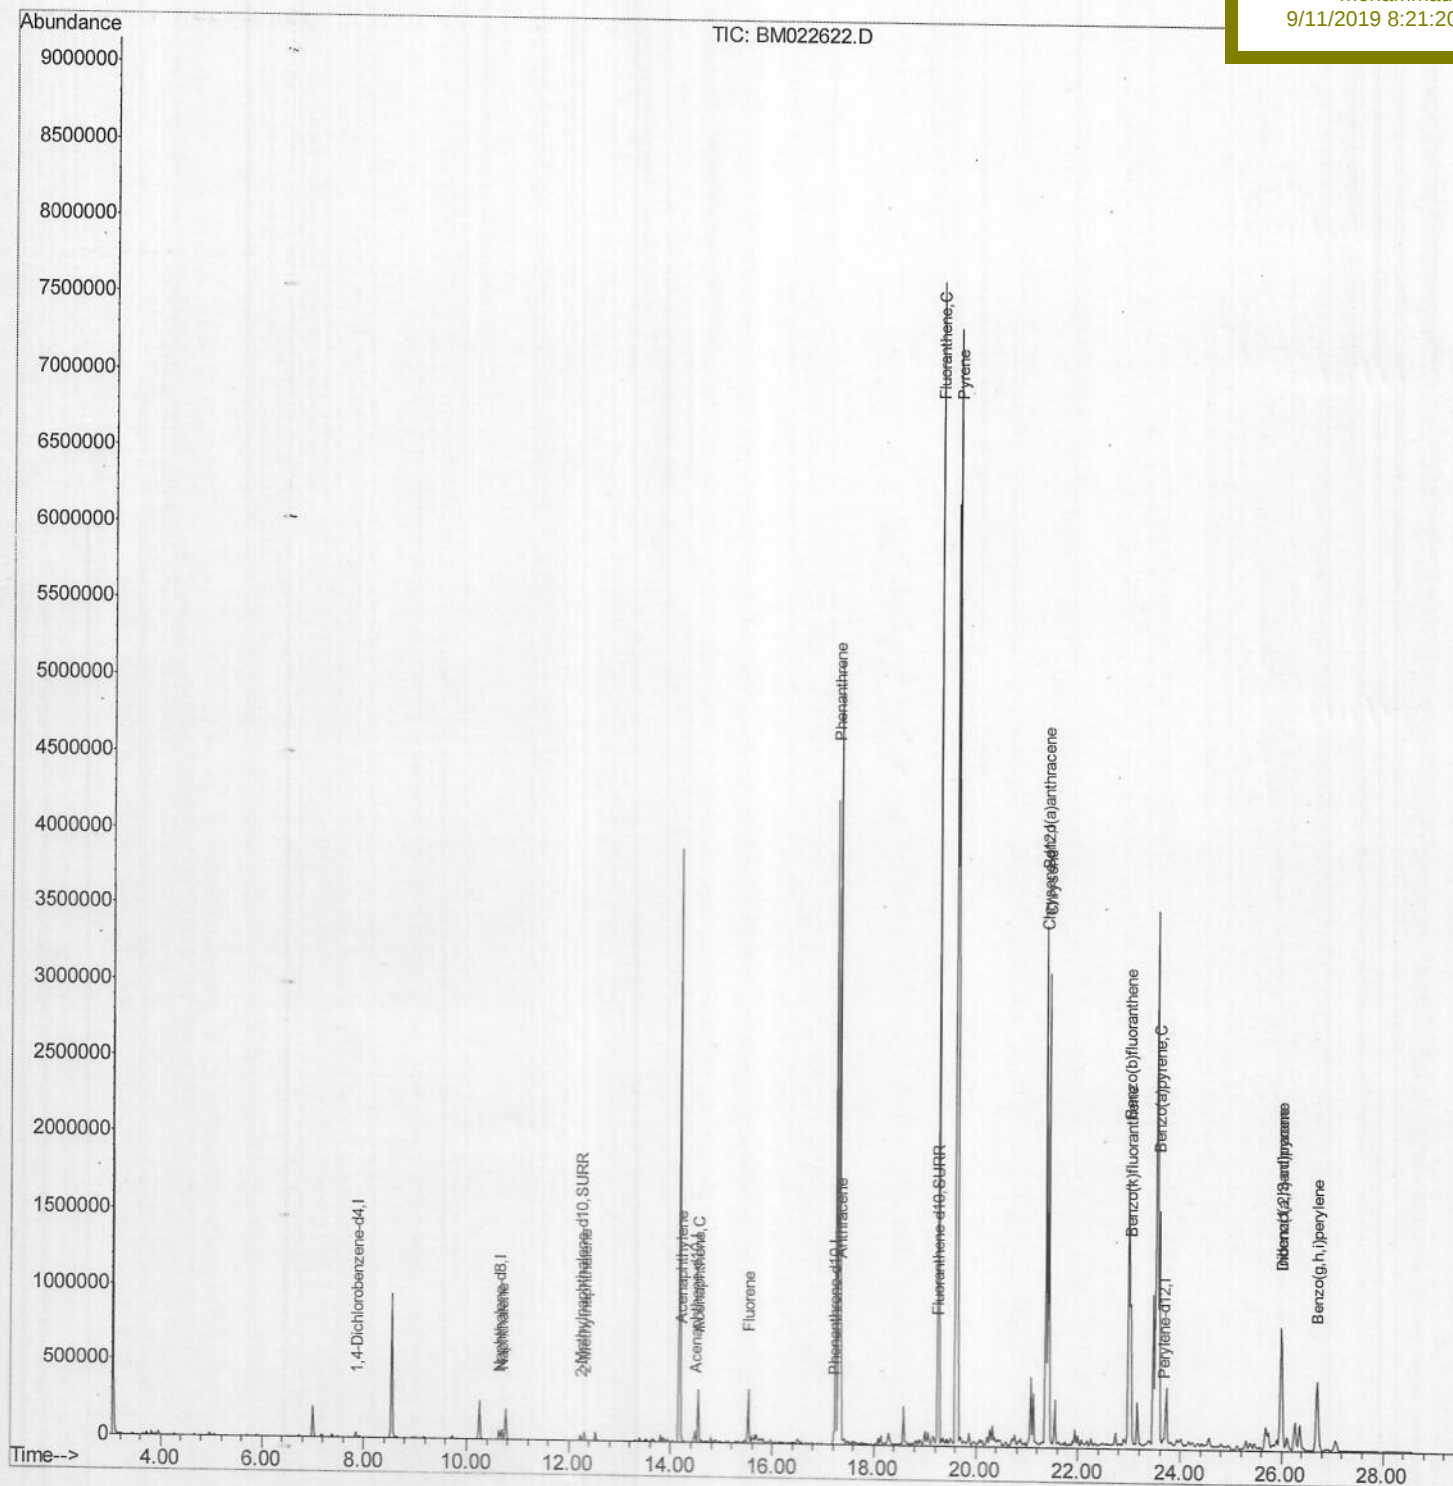
Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
Data File : BM022622.D
Acq On : 10 Sep 2019 16:31
Operator : HP/JU
Sample : K4708-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:16:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 15:06:45 2019
Response via : Initial Calibration

Instrument :
BNA_M
Client Sample ID :
CB5P8

Manual Integrations
APPROVED

mohammad
9/11/2019 8:21:20 AM



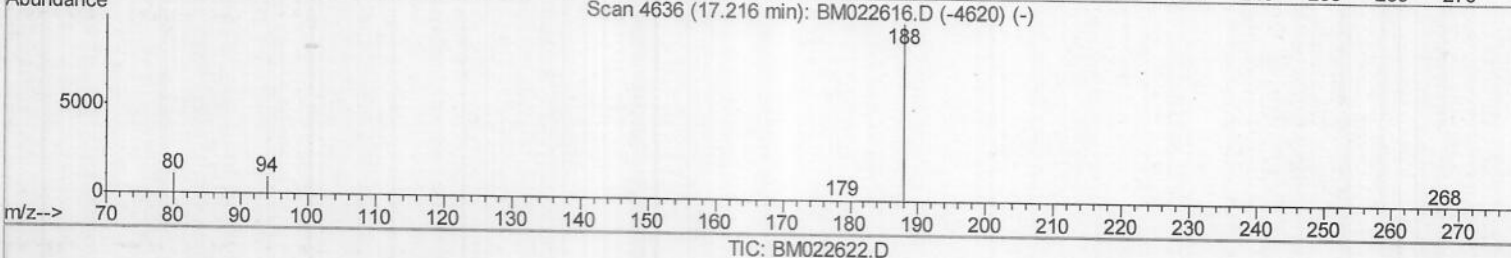
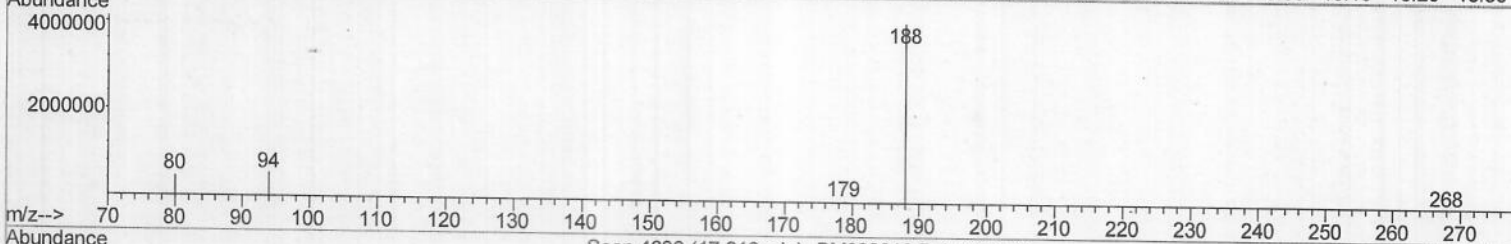
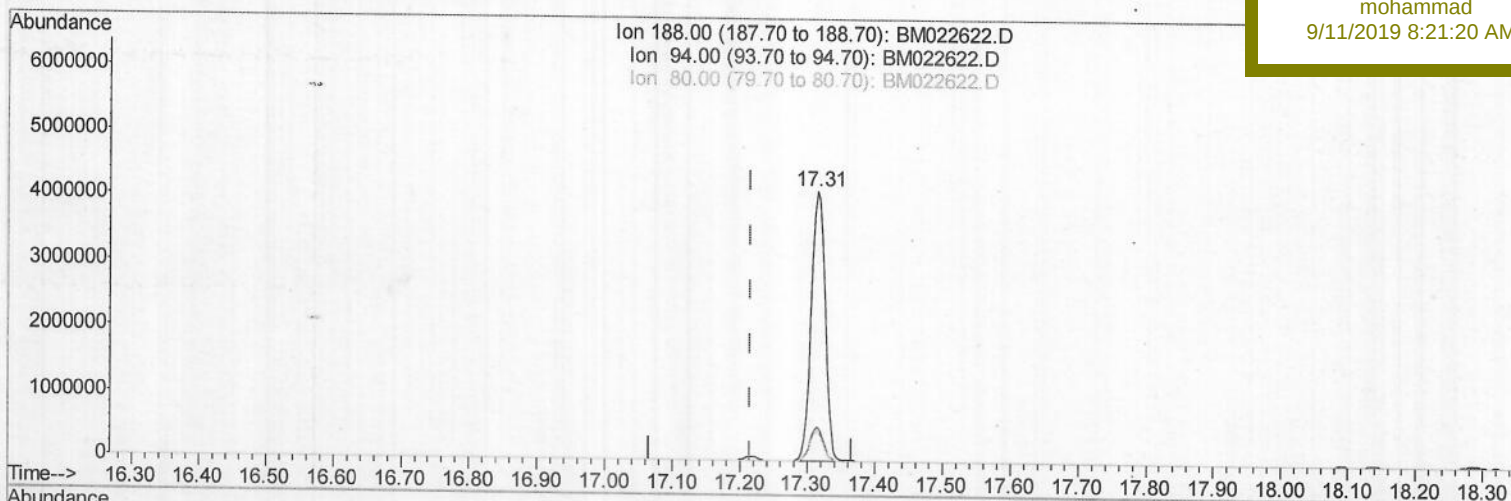
Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
Data File : BM022622.D
Acq On : 10 Sep 2019 16:31
Operator : HP/JU
Sample : K4708-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:08:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 15:06:45 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
CB5P8

Manual Integrations
APPROVED

mohammad
9/11/2019 8:21:20 AM



(10) Phenanthrene-d10 (I)
17.315min (+0.099) 0.40ng/ul
response 5870350

Ion	Exp%	Act%
188.00	100	100
94.00	9.80	12.70#
80.00	11.00	11.23
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:08:45 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

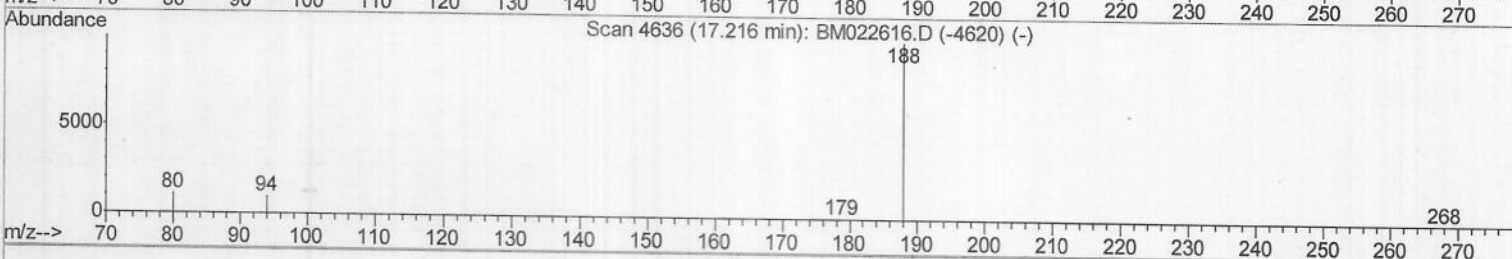
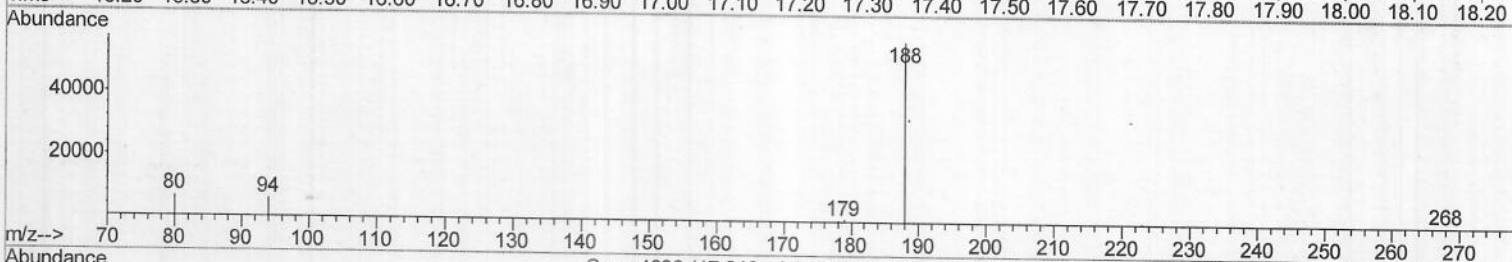
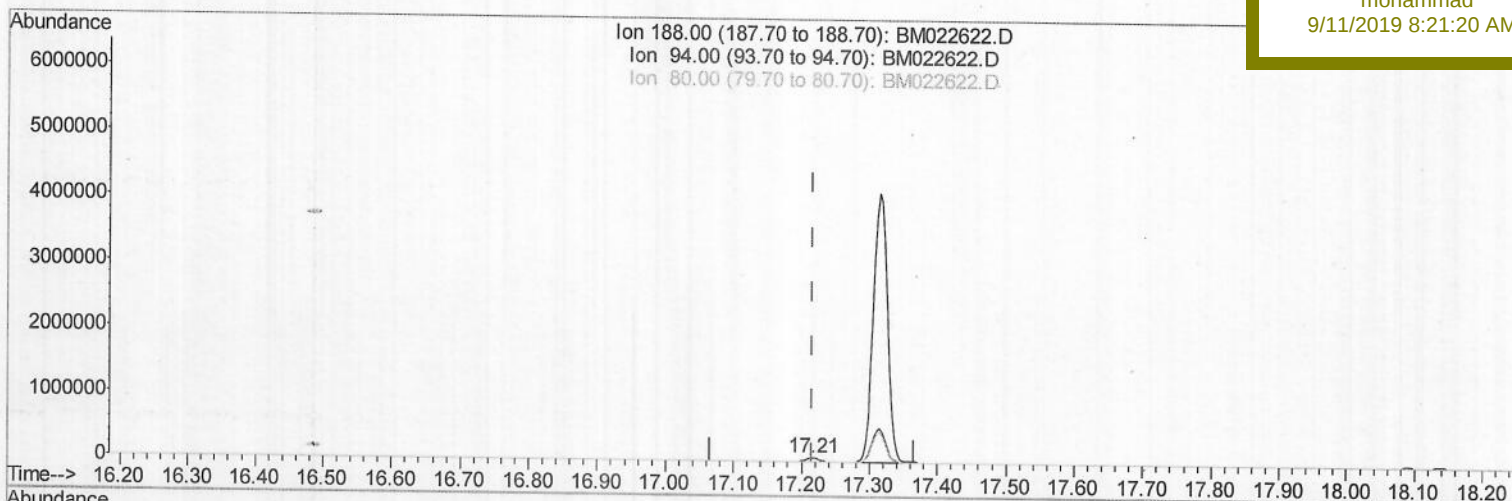
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

TIC: BM022622.D

(10) Phenanthrene-d10 (I)

17.214min (-0.002) 0.40ng/ul m

response 81568

Ion	Exp%	Act%
188.00	100	100
94.00	9.80	10.27
80.00	11.00	11.37
0.00	0.00	0.00

JU
09/11/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:09:30 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

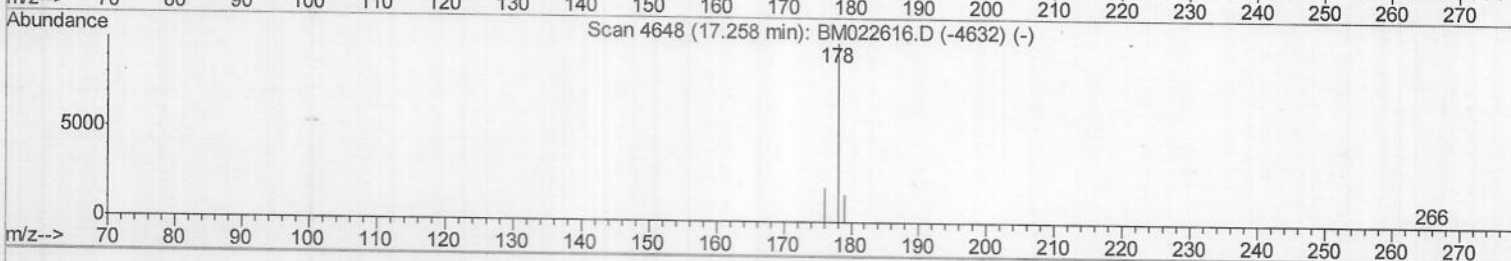
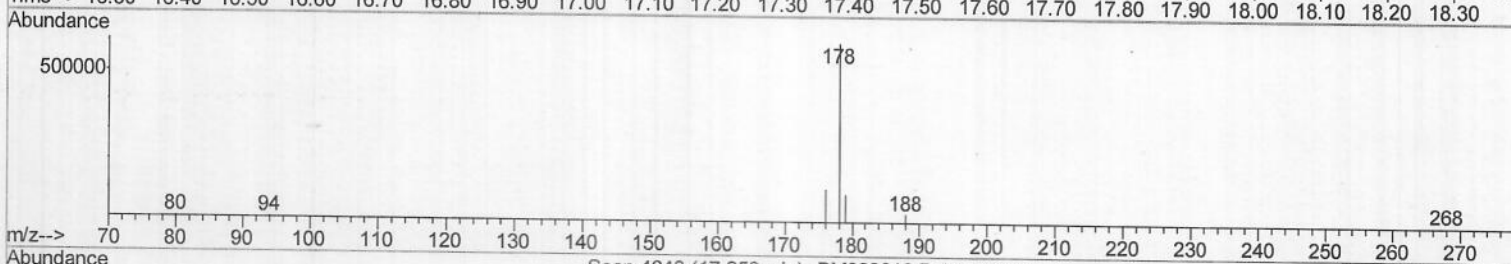
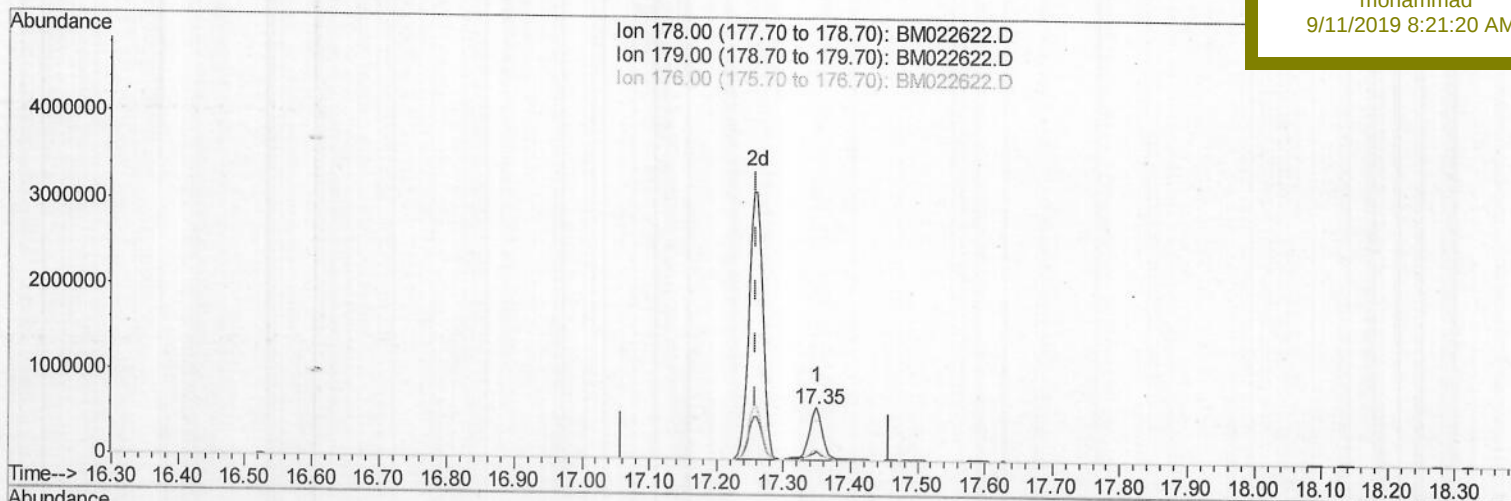
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

TIC: BM022622.D

(12) Phenanthrene

17.350min (+0.092) 3.19ng/ul

response 828782

Ion	Exp%	Act%
178.00	100	100
179.00	15.50	15.62
176.00	19.10	18.35
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:09:30 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

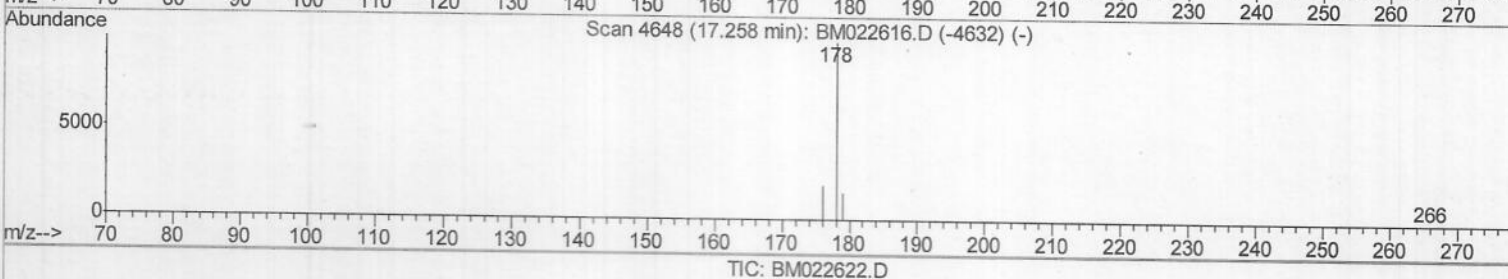
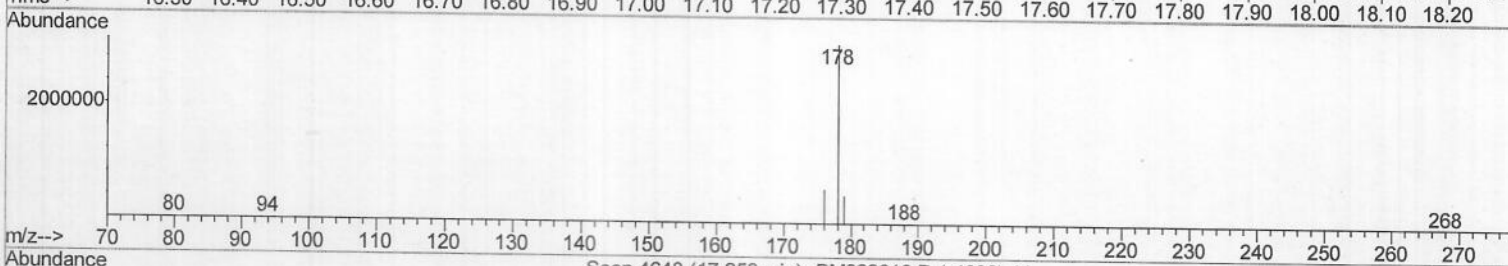
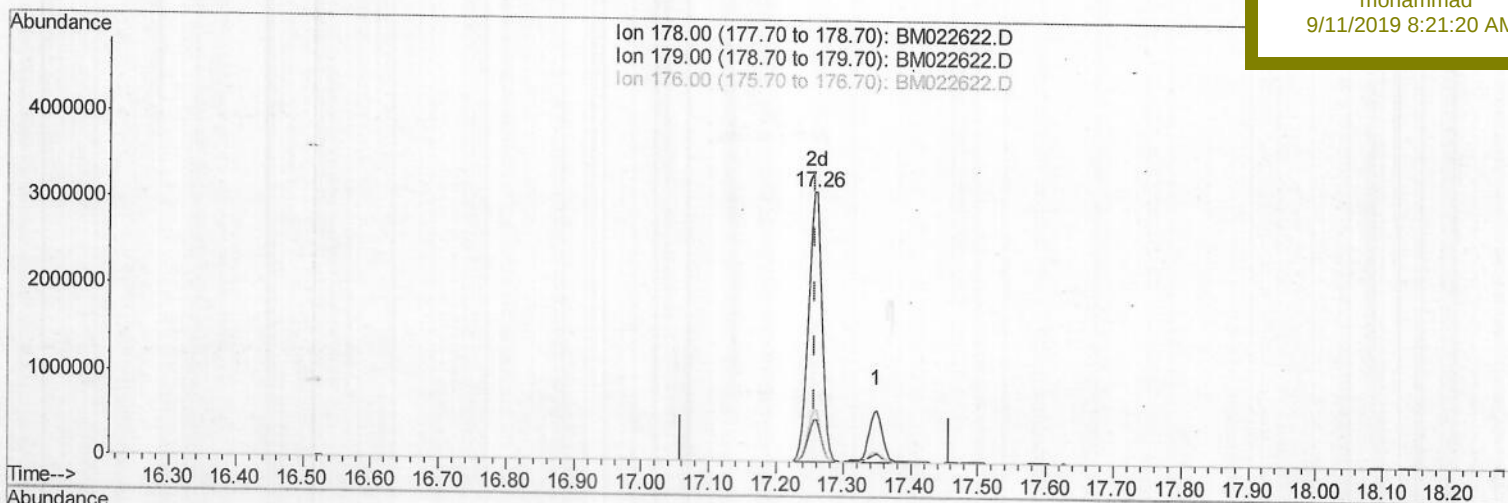
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

(12) Phenanthrene

17.259min (+0.001) 17.10ng/ul m

response 4444216

Ion	Exp%	Act%
178.00	100	100
179.00	15.50	16.03
176.00	19.10	19.37
0.00	0.00	0.00

JU
09/11/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:09:30 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

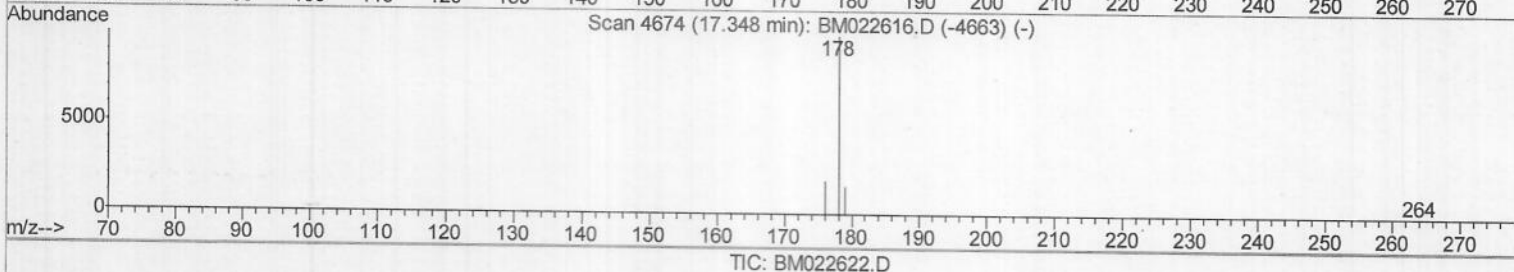
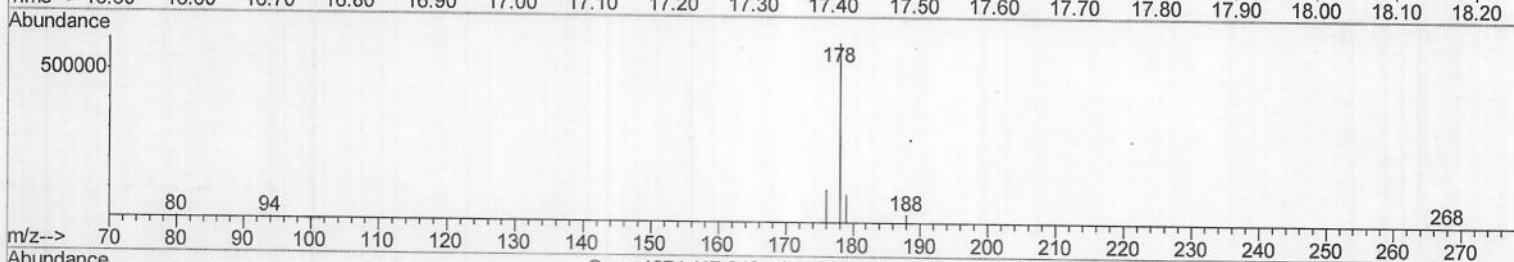
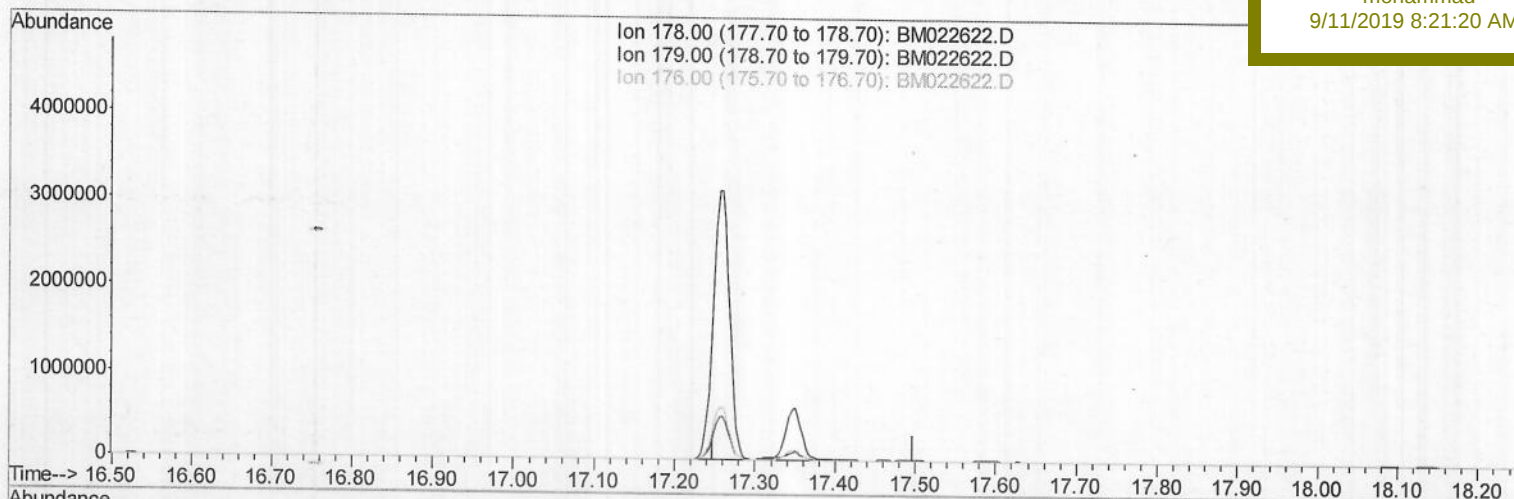
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

(13) Anthracene

17.348min (-17.348) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	15.60	0.00#
176.00	18.50	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:09:30 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

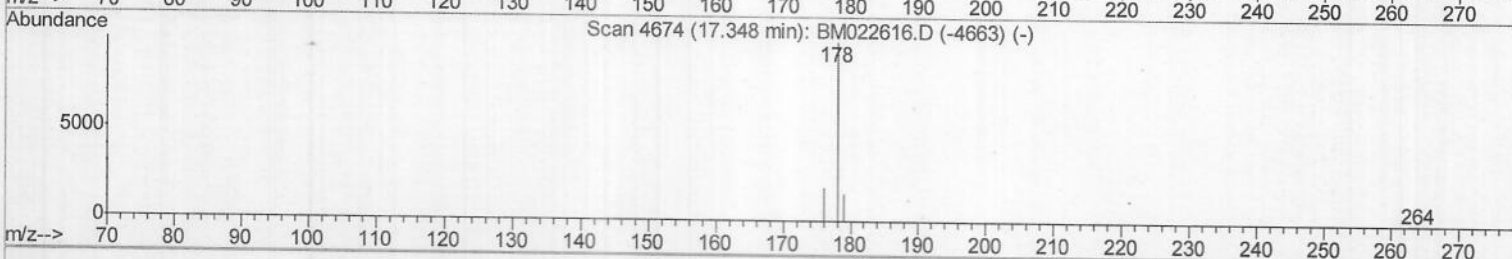
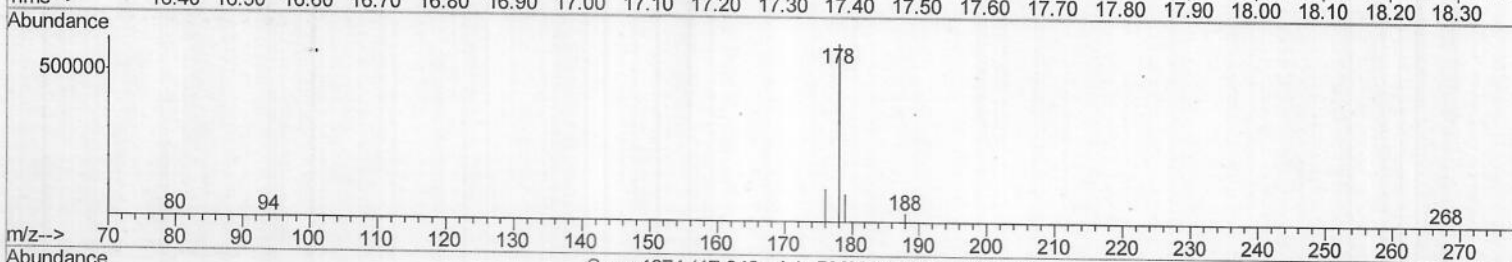
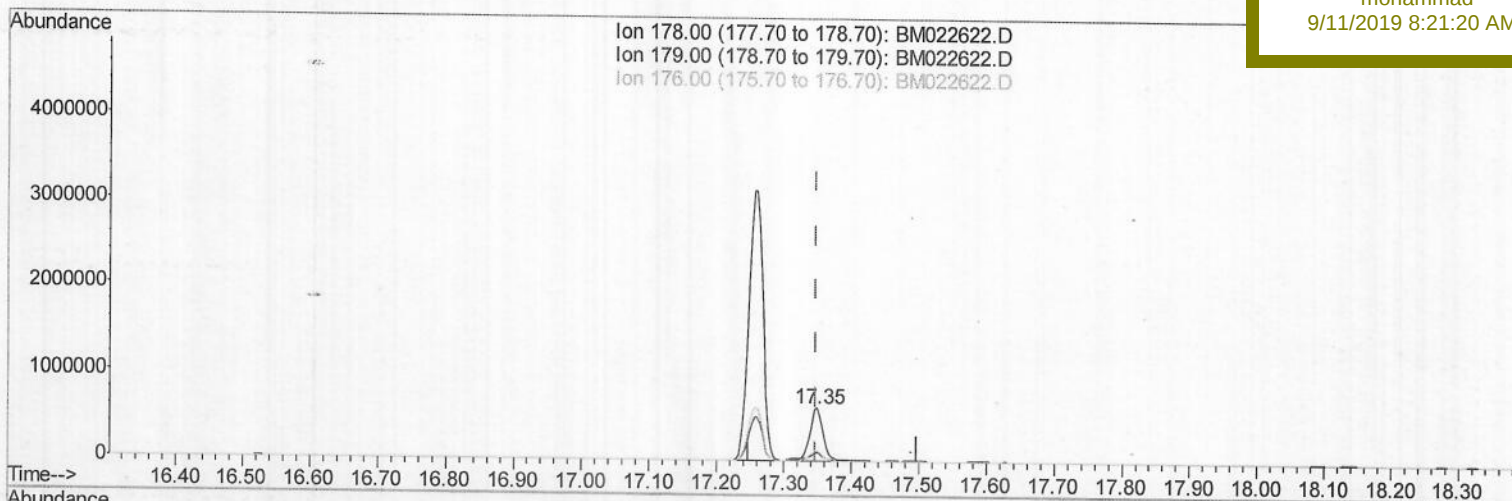
CB5P8

Manual Integrations

APPROVED

mohammad

9/11/2019 8:21:20 AM



TIC: BM022622.D

(13) Anthracene

17.350min (+0.001) 3.81ng/ul m

response 850423

Ion	Exp%	Act%
178.00	100	100
179.00	15.60	15.62
176.00	18.50	18.35
0.00	0.00	0.00

JU
09111119

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:09:30 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

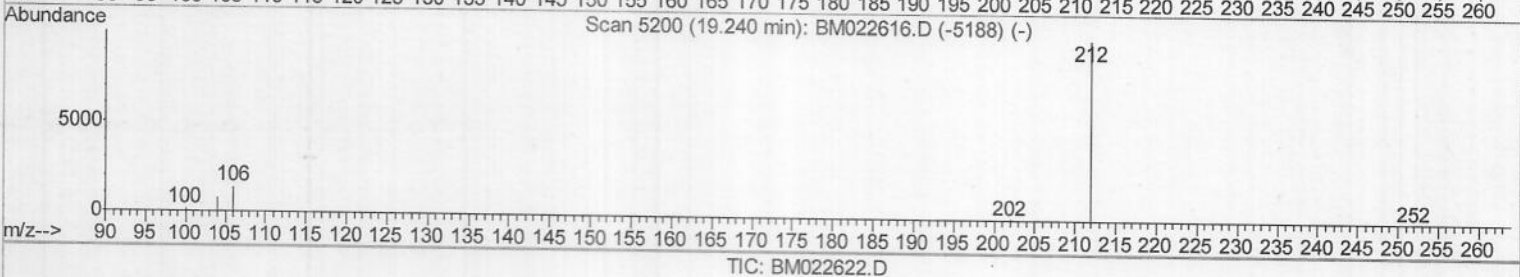
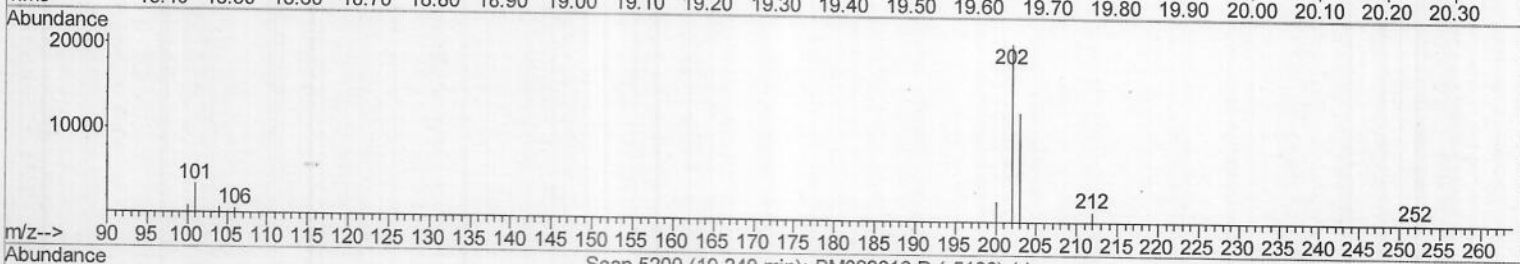
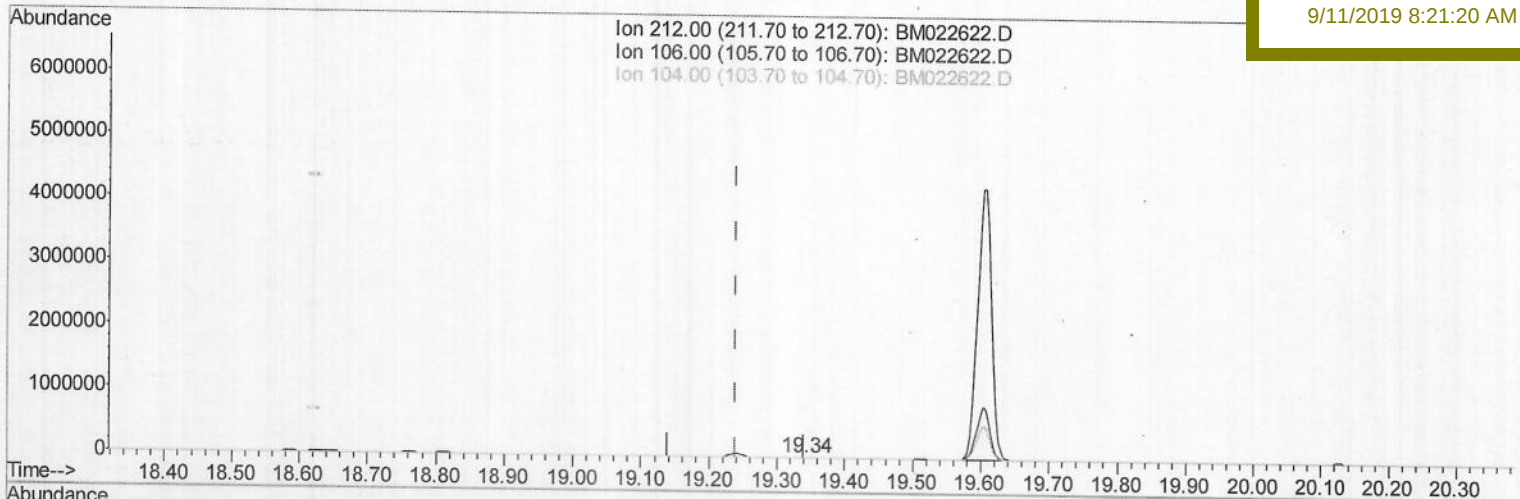
CB5P8

Manual Integrations

APPROVED

mohammad

9/11/2019 8:21:20 AM



(14) Fluoranthene-d10 (SURR)

19.340min (+0.101) 0.01ng/ul

response 1986

Ion	Exp%	Act%
212.00	100	100
106.00	14.00	22.05#
104.00	8.00	23.46#
0.00	0.00	0.00

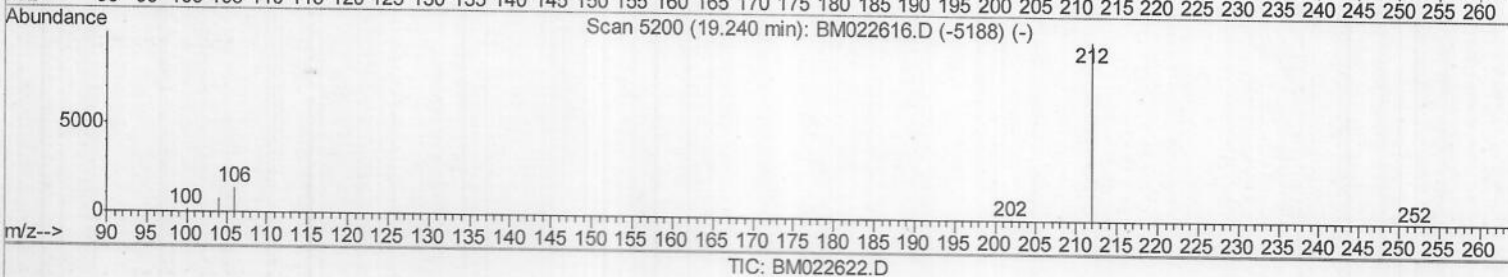
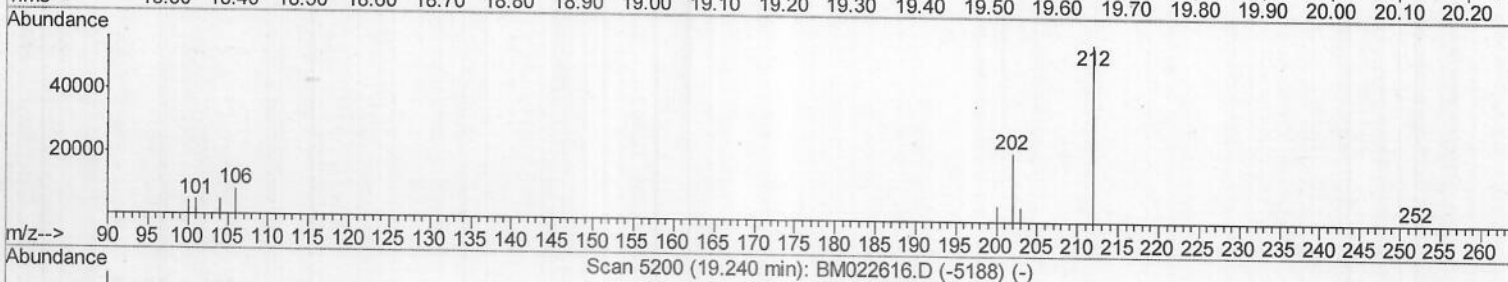
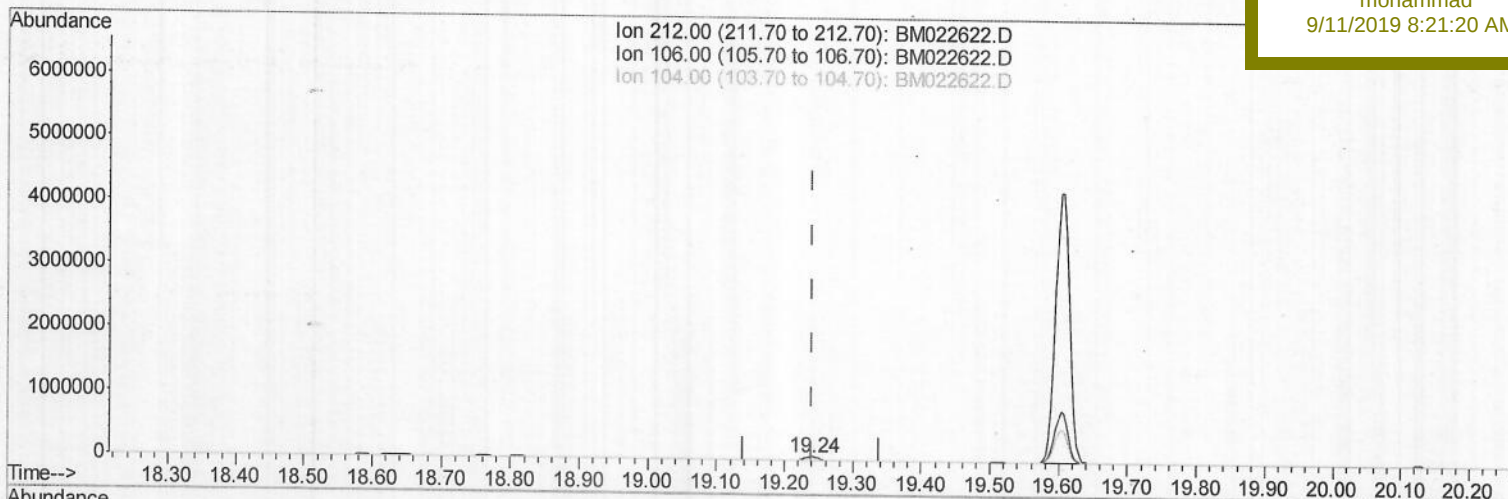
Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
Data File : BM022622.D
Acq On : 10 Sep 2019 16:31
Operator : HP/JU
Sample : K4708-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:09:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 15:06:45 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
CB5P8

Manual Integrations
APPROVED

mohammad
9/11/2019 8:21:20 AM



(14) Fluoranthene-d10 (SURR)

19.241min (+0.001) 0.35ng/ul m) JU
response 77325 09/11/19

Ion	Exp%	Act%
212.00	100	100
106.00	14.00	0.57#
104.00	8.00	0.60#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:09:30 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

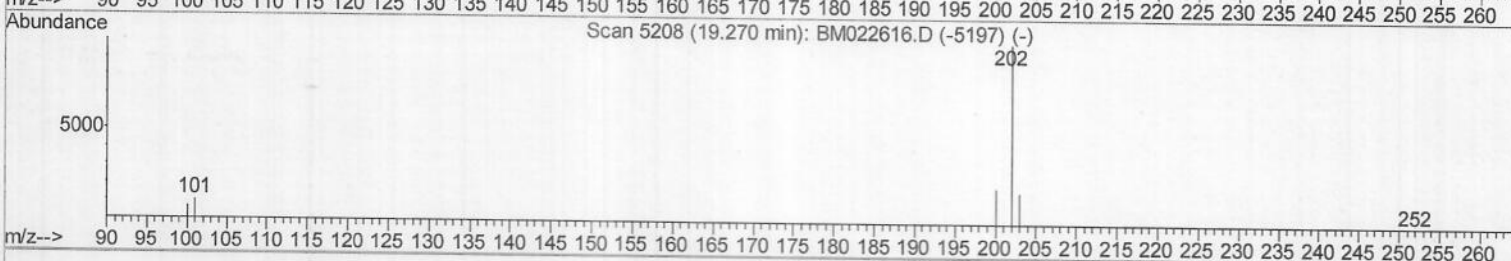
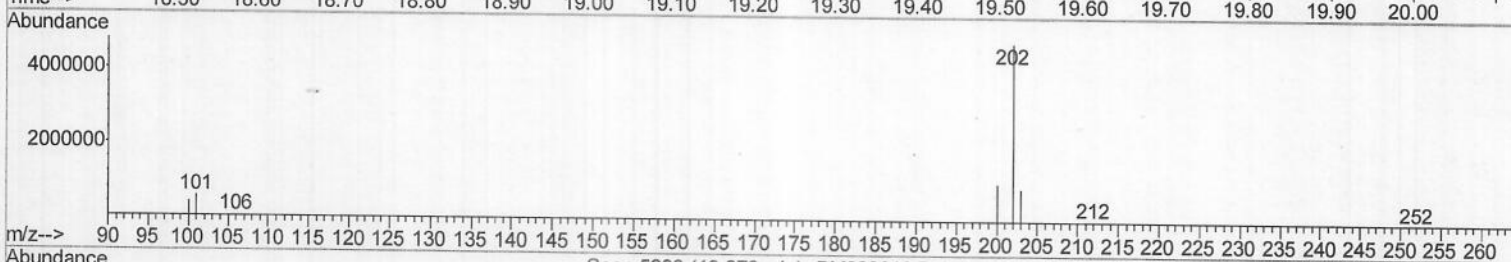
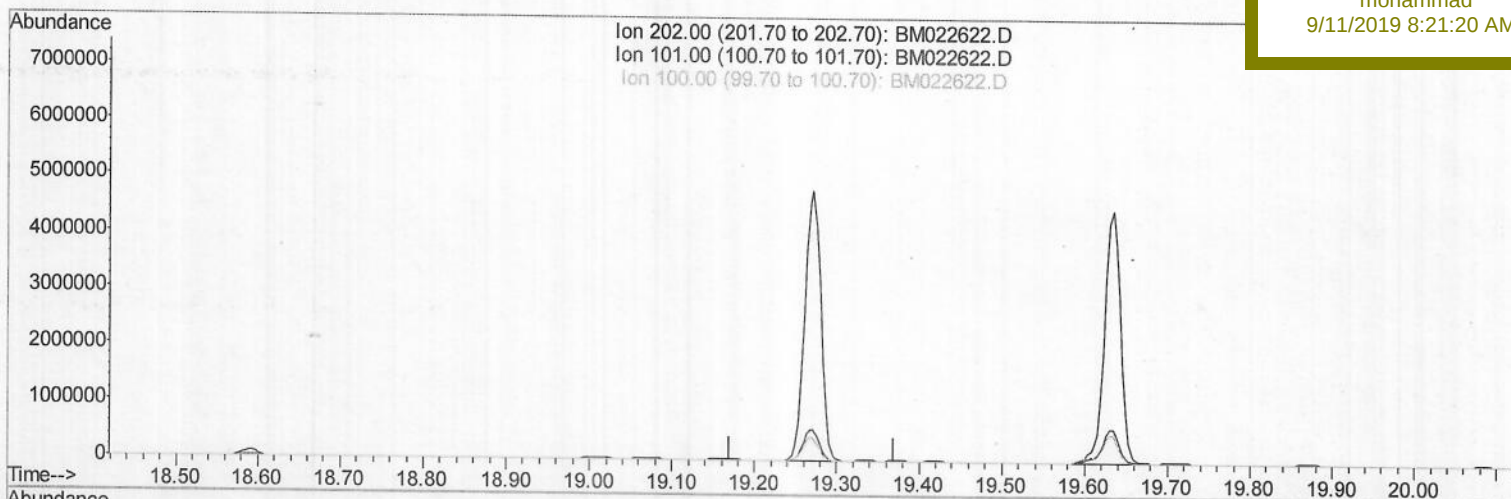
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

(15) Fluoranthene (C)

19.270min (-19.270) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	10.50	0.00
100.00	8.00	0.00
0.00	0.00	0.00

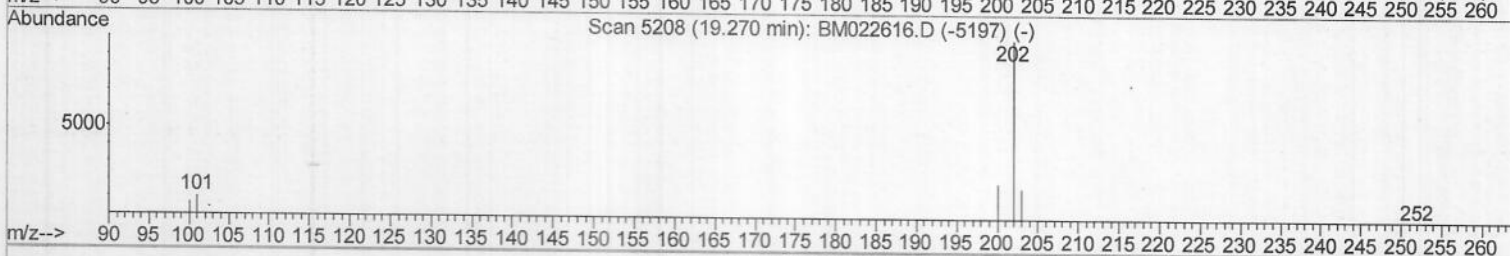
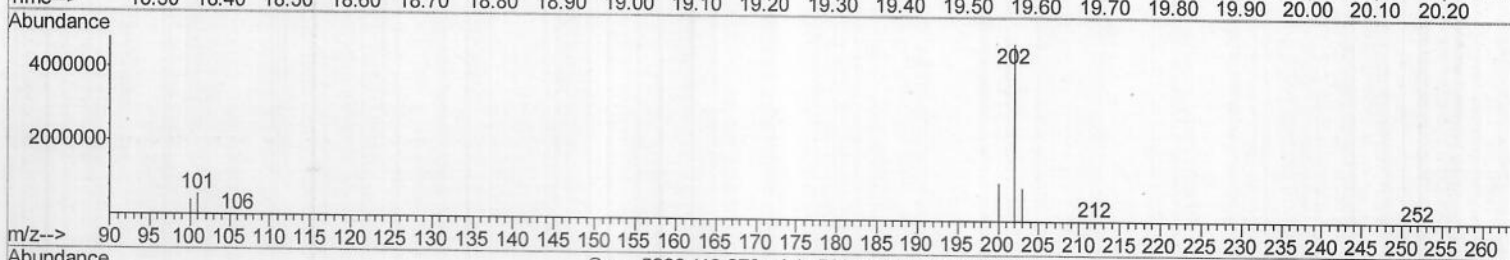
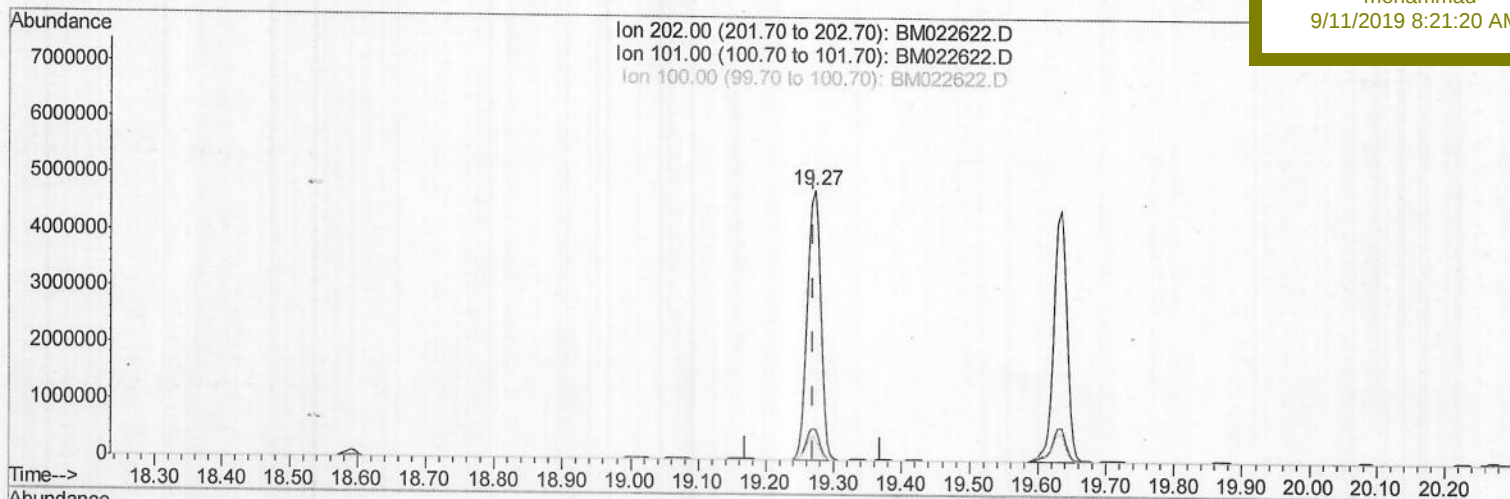
Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
Data File : BM022622.D
Acq On : 10 Sep 2019 16:31
Operator : HP/JU
Sample : K4708-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:09:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 15:06:45 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
CB5P8

Manual Integrations
APPROVED

mohammad
9/11/2019 8:21:20 AM



TIC: BM022622.D

(15) Fluoranthene (C)

19.272min (+0.001) 22.98ng/ul m

response 6445190

Ion	Exp%	Act%
202.00	100	100
101.00	10.50	11.37
100.00	8.00	8.39
0.00	0.00	0.00

JU
09/11/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:09:30 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

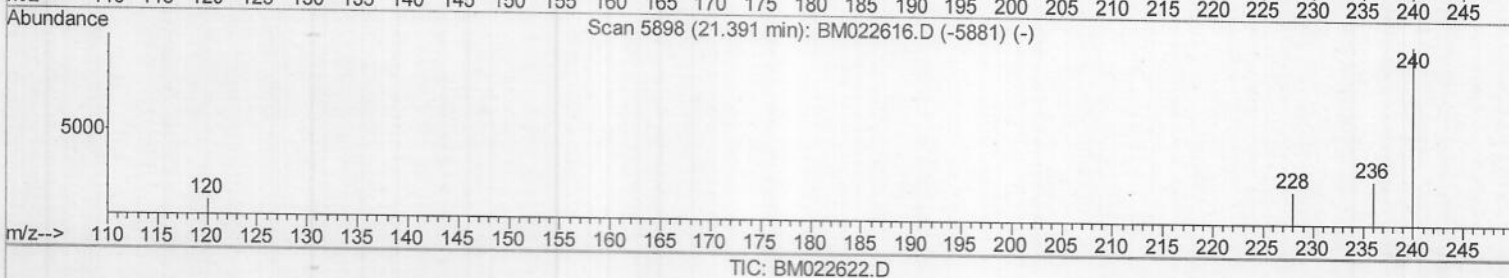
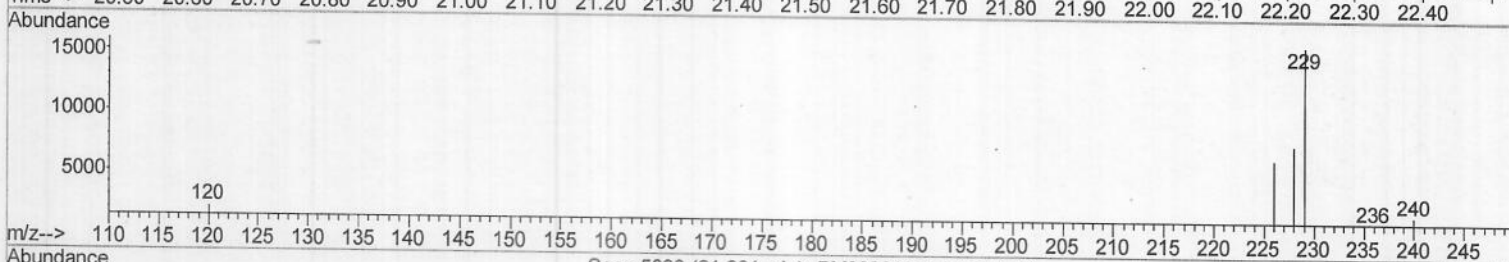
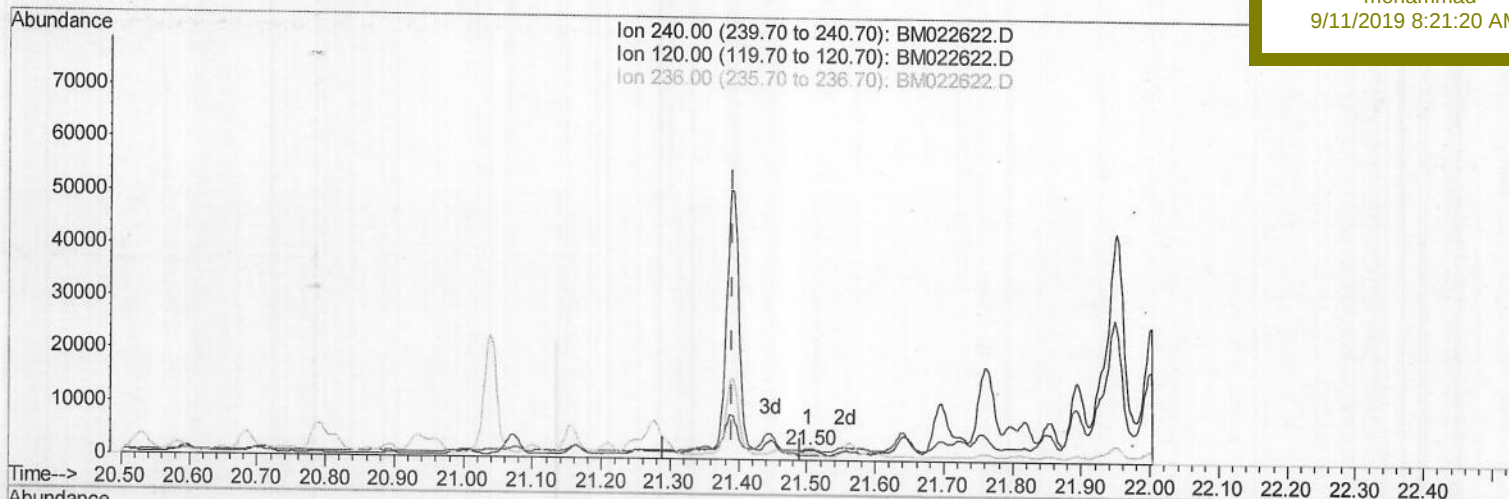
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

(16) Chrysene-d12 (I)

21.503min (+0.111) 0.40ng/ul

response 1535

Ion	Exp%	Act%
240.00	100	100
120.00	14.60	108.07#
236.00	28.80	70.17#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:09:30 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

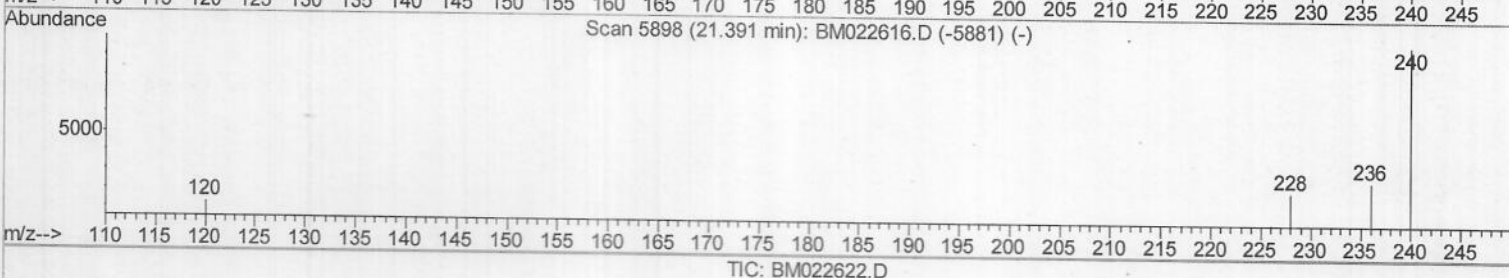
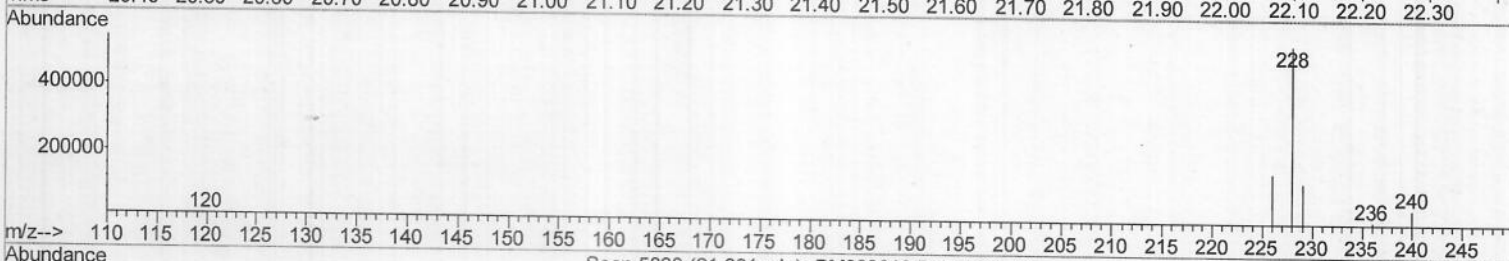
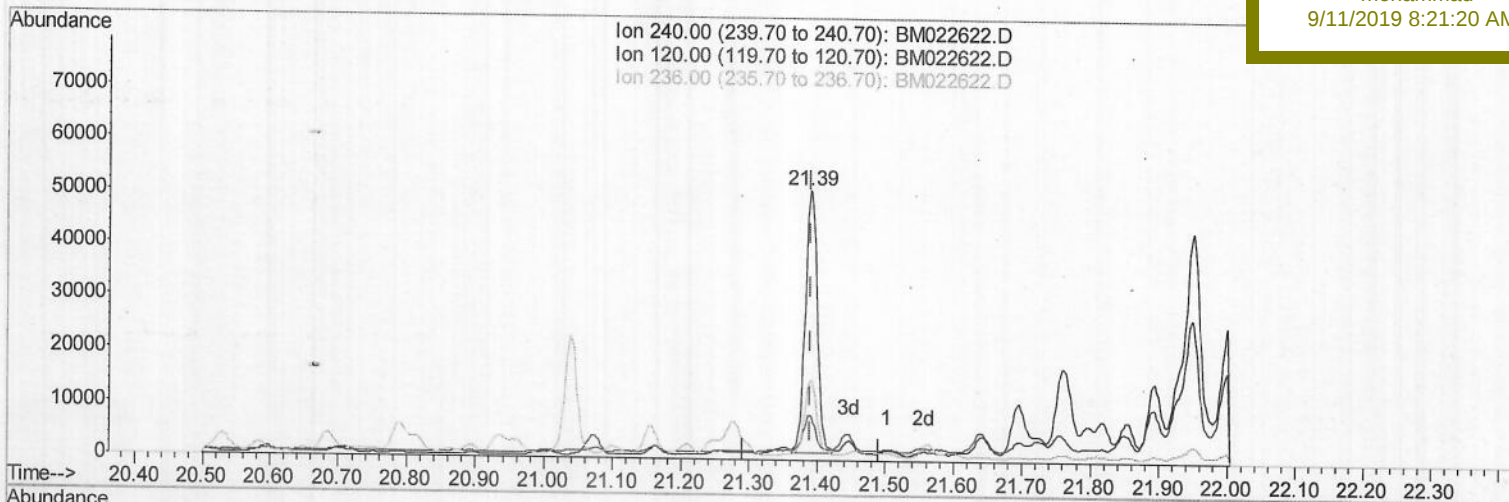
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

(16) Chrysene-d12 (I)

21.389min (-0.002) 0.40ng/ul m) JU
09/11/19

response 61021

Ion	Exp%	Act%
240.00	100	100
120.00	14.60	16.24
236.00	28.80	29.67
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:12:21 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

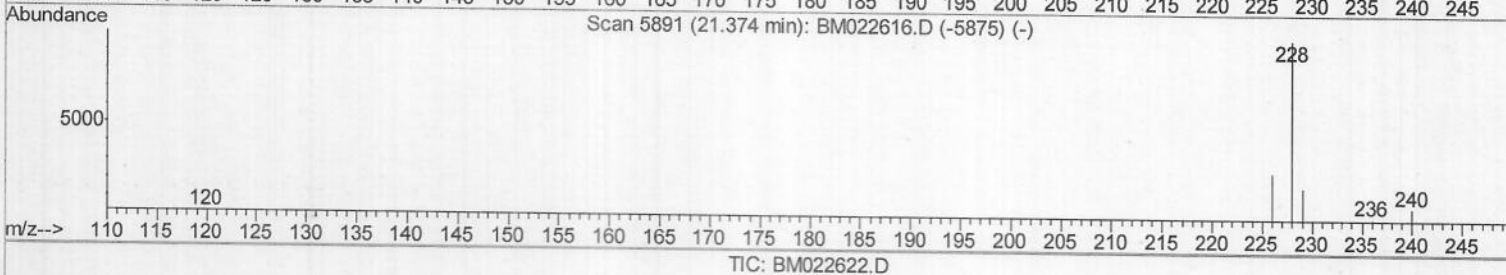
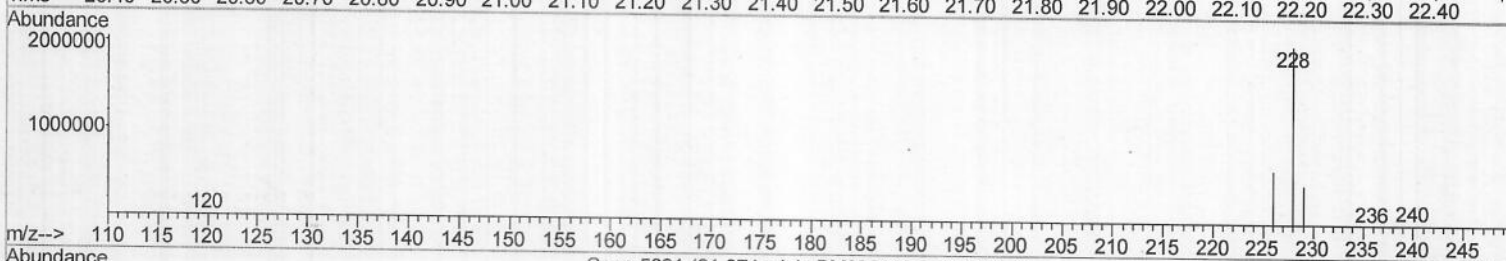
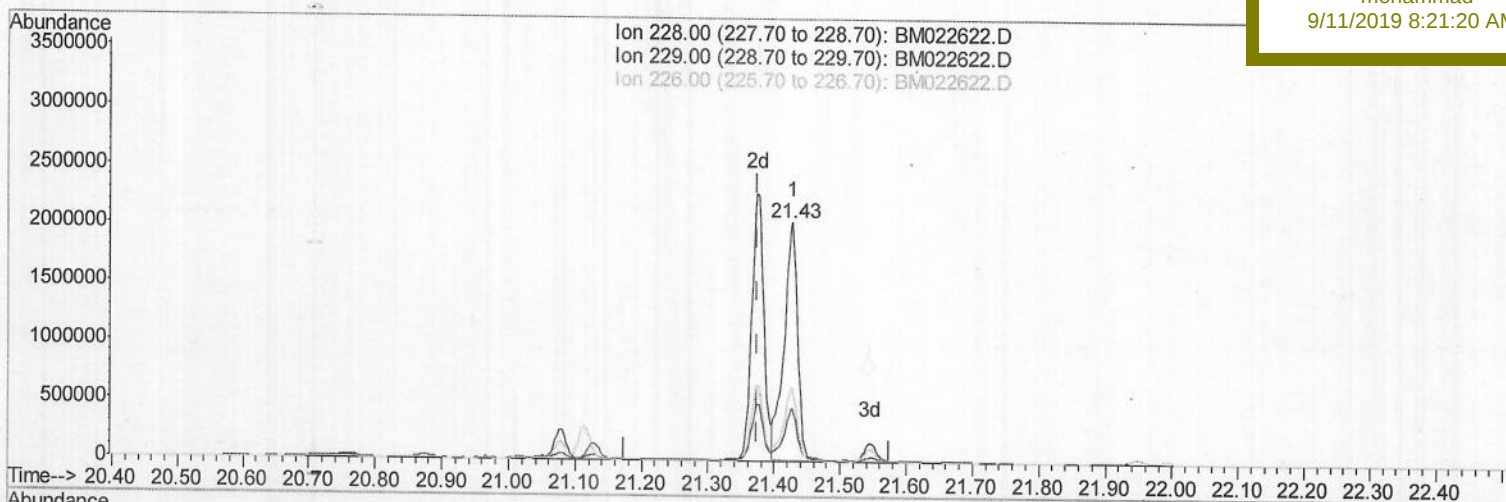
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

(18) Benzo(a)anthracene

21.428min (+0.053) 12.56ng/ul

response 2932487

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	21.71
226.00	27.50	30.36
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:12:21 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

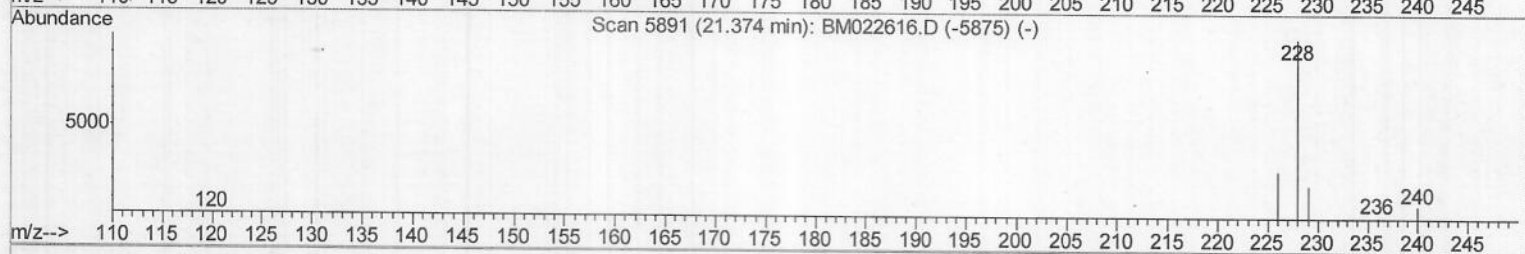
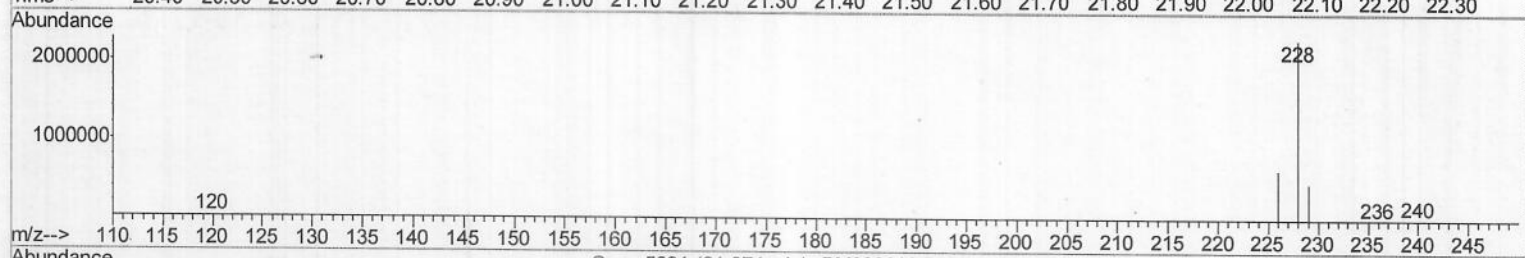
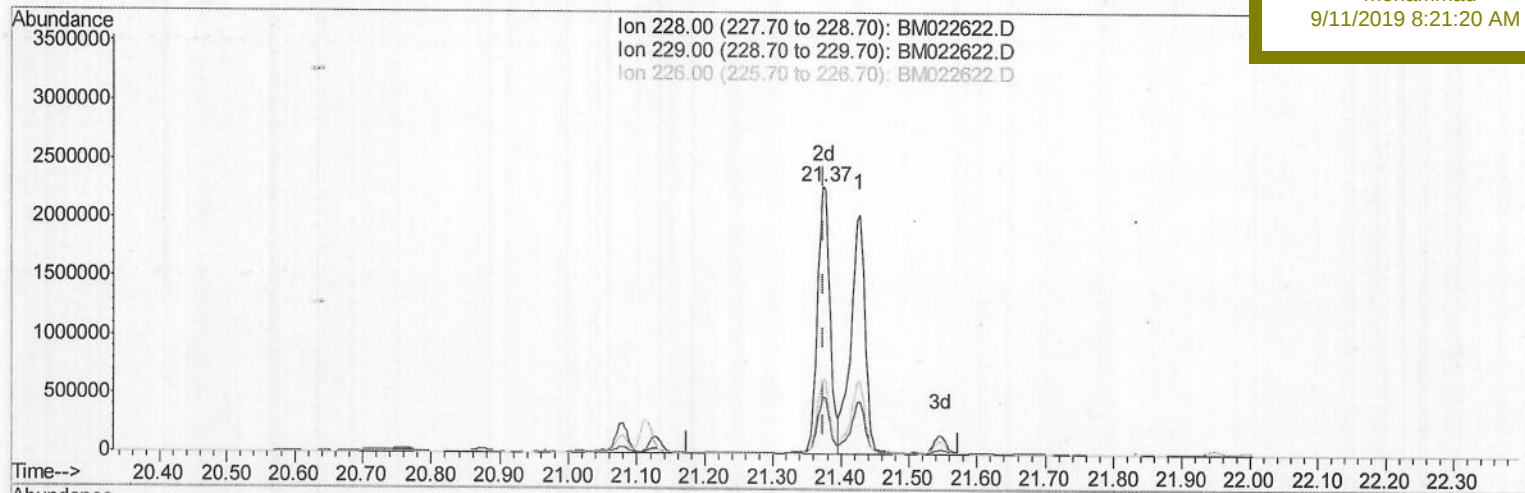
ClientSampleId :

CB5P8

Manual Integrations
APPROVED

mohammad

9/11/2019 8:21:20 AM



TIC: BM022622.D

(18) Benzo(a)anthracene

21.374min (+0.000) 12.58ng/ul m > 50
09/11/19

response 2937706

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	20.85
226.00	27.50	28.17
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:12:21 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

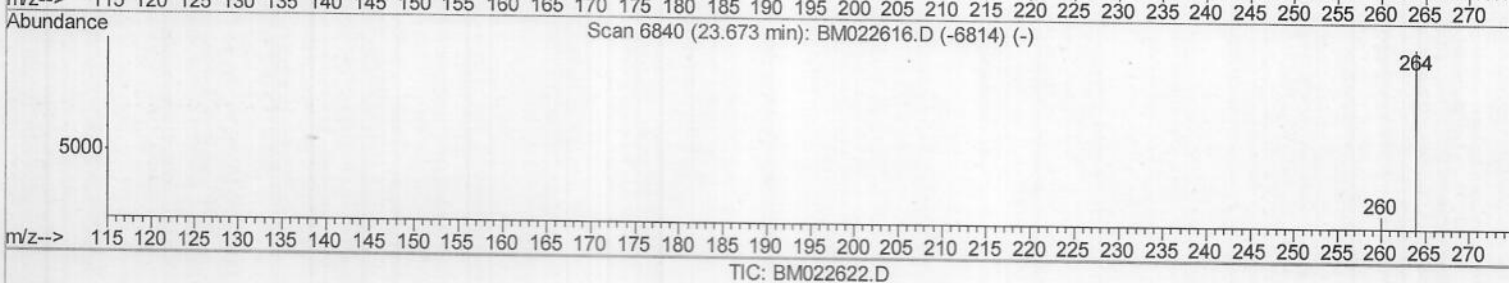
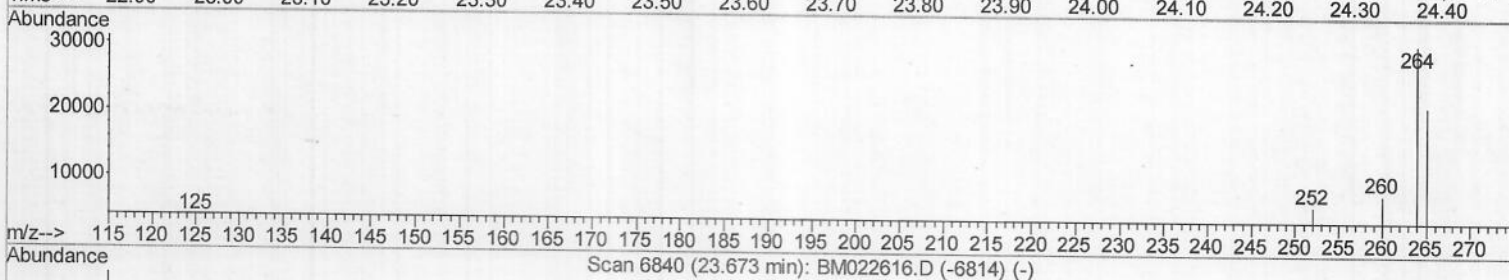
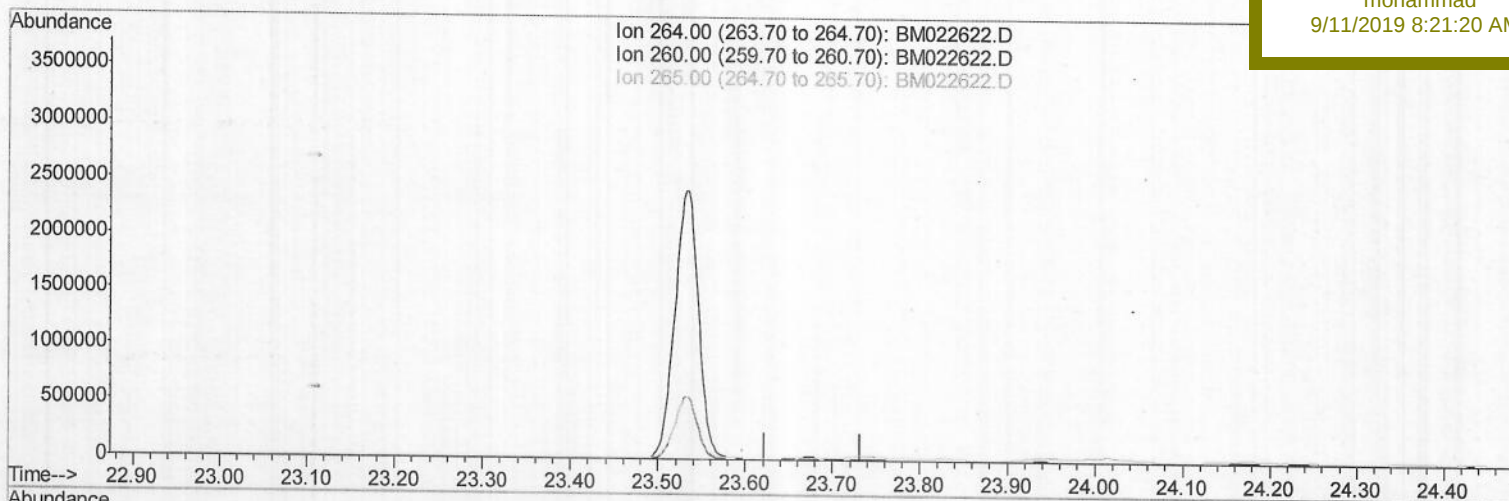
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

(20) Perylene-d12 (I)

23.673min (-23.673) 0.00ng/ul

response 0

Ion	Exp%	Act%
264.00	100	0.00
260.00	25.60	0.00#
265.00	59.90	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:12:21 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

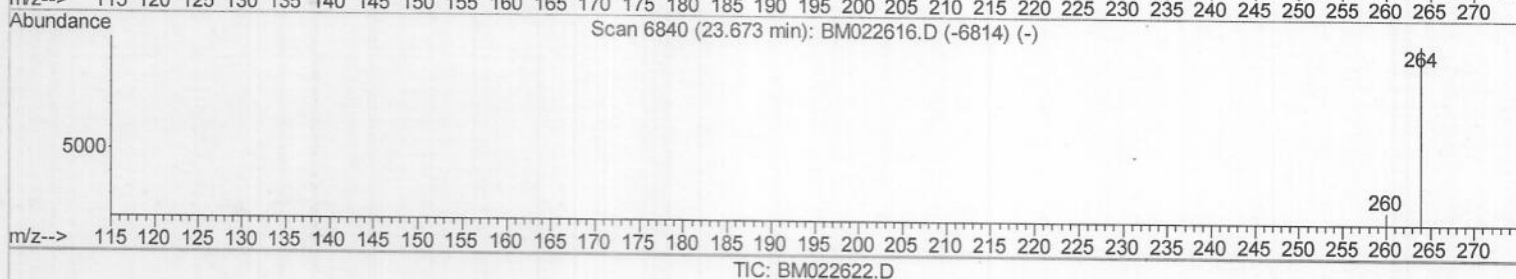
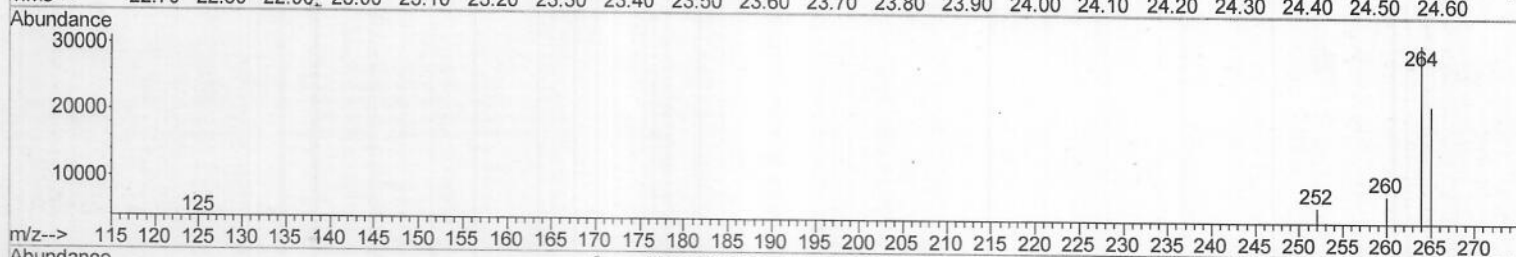
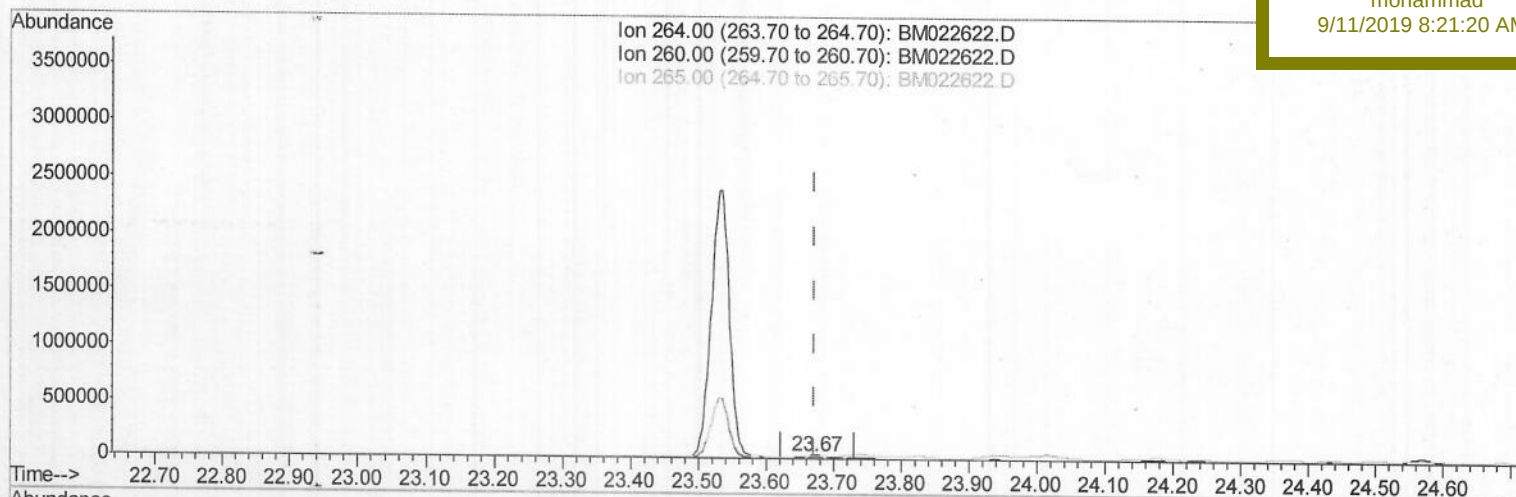
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

(20) Perylene-d12 (I)

23.673min (+0.000) 0.40ng/ul m) 50
09/11/19

response 48920

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	26.28
265.00	59.90	70.23
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:14:39 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

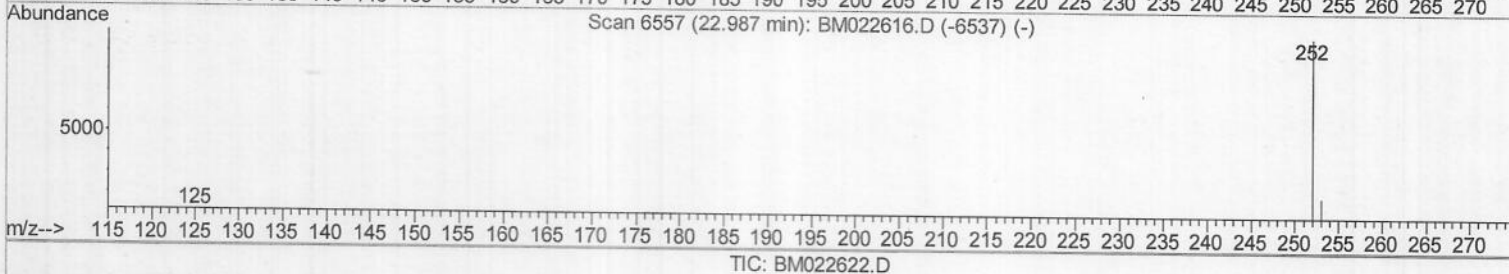
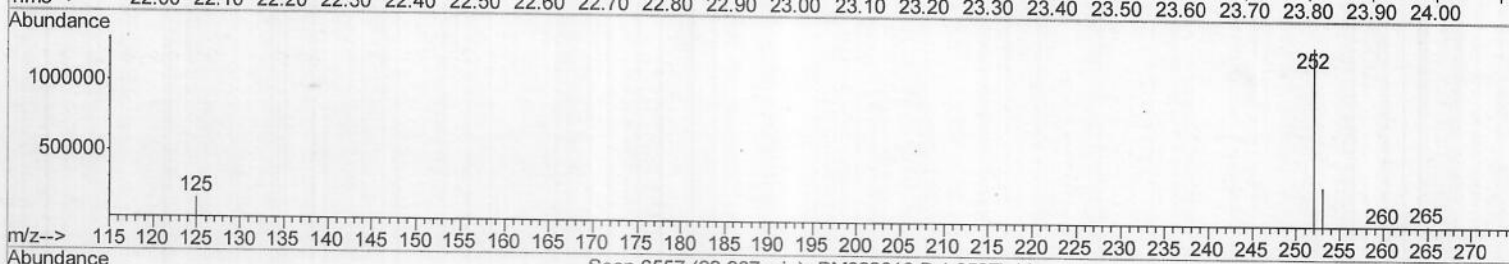
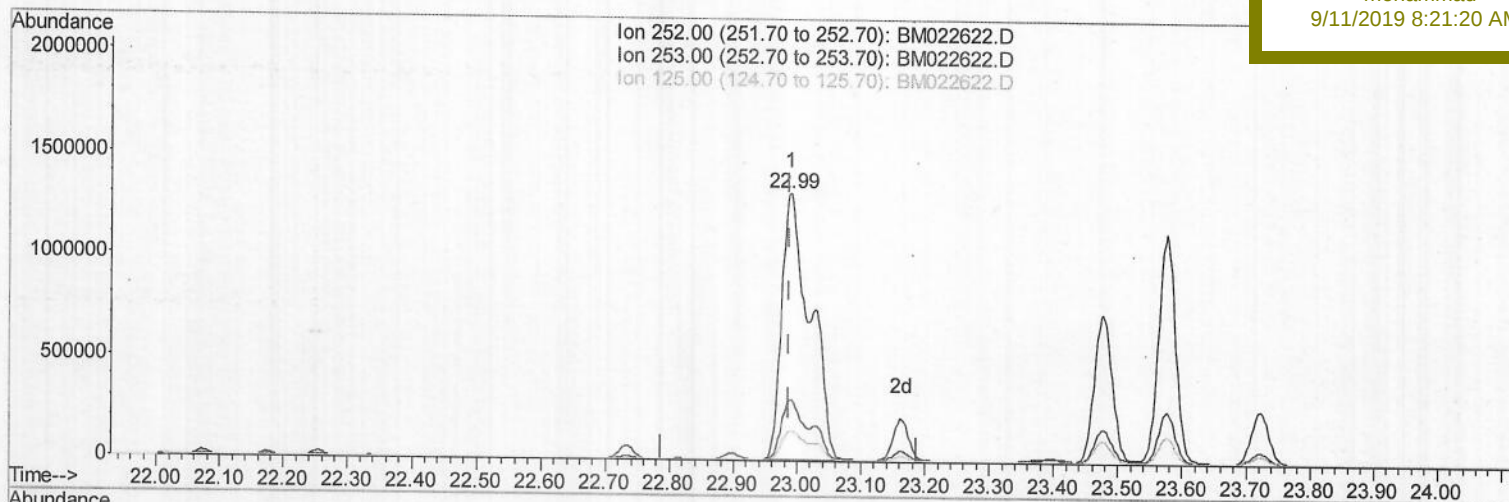
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

TIC: BM022622.D

(21) Benzo(b)fluoranthene

22.990min (+0.002) 19.12ng/ul

response 4063740

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	22.76
125.00	15.60	11.04
0.00	0.00	0.00

Quantitation Report (Qedit)

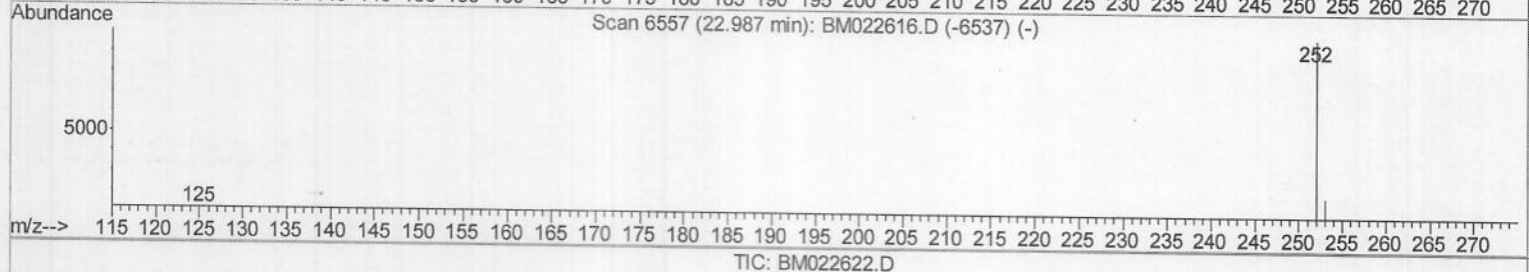
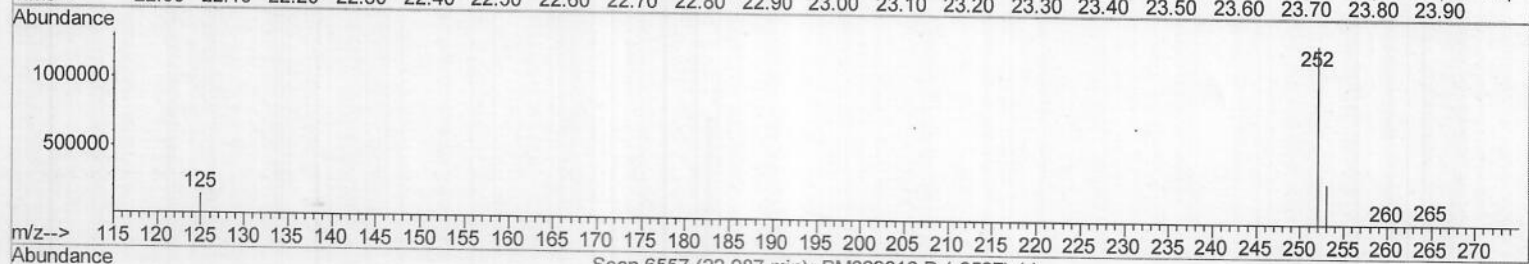
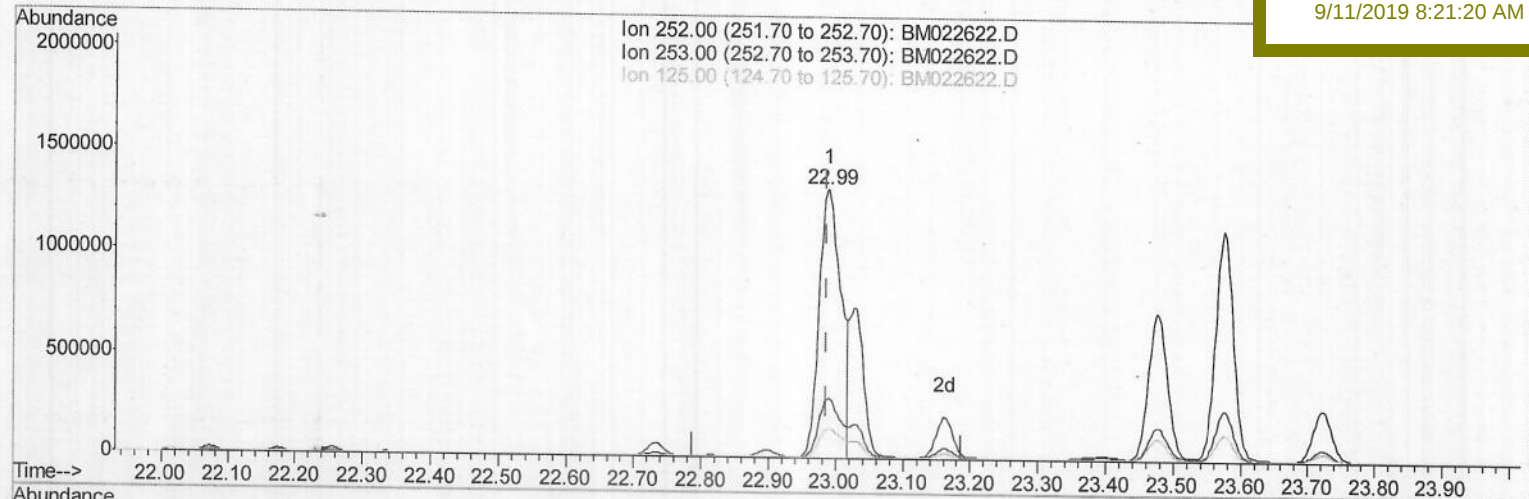
Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
 Data File : BM022622.D
 Acq On : 10 Sep 2019 16:31
 Operator : HP/JU
 Sample : K4708-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:14:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 CB5P8

Manual Integrations
 APPROVED

mohammad
 9/11/2019 8:21:20 AM



(21) Benzo(b)fluoranthene

22.990min (+0.002) 13.77ng/ul m } JU
 response 2927807 09/11/19

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	22.76
125.00	15.60	11.04
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:14:39 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

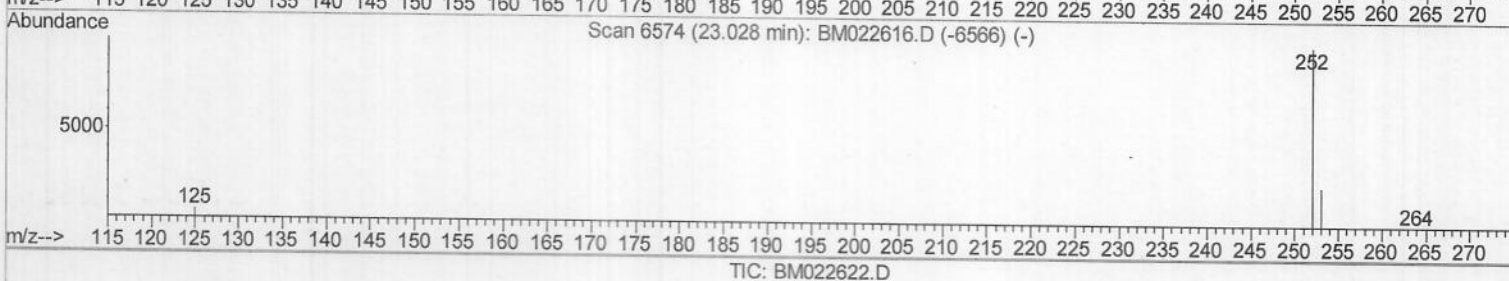
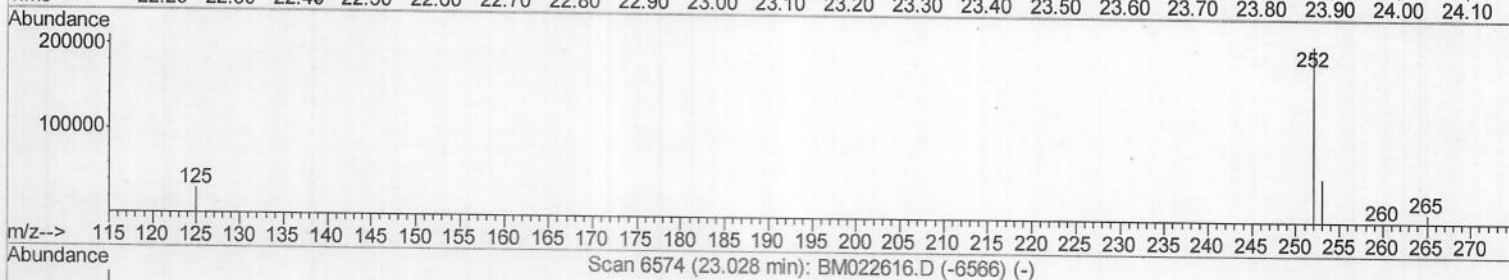
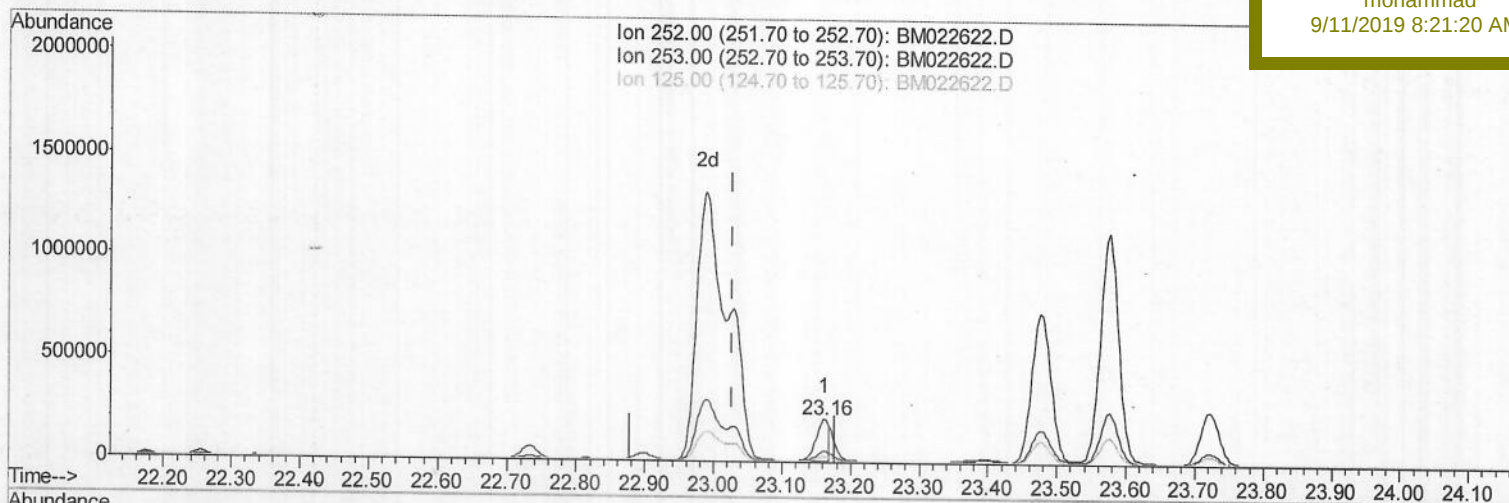
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

(22) Benzo(k)fluoranthene

23.162min (+0.133) 1.18ng/ul

response 256614

Ion	Exp%	Act%
252.00	100	100
253.00	24.40	24.91
125.00	14.00	13.81
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022622.D

Acq On : 10 Sep 2019 16:31

Operator : HP/JU

Sample : K4708-01

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 10 17:14:39 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

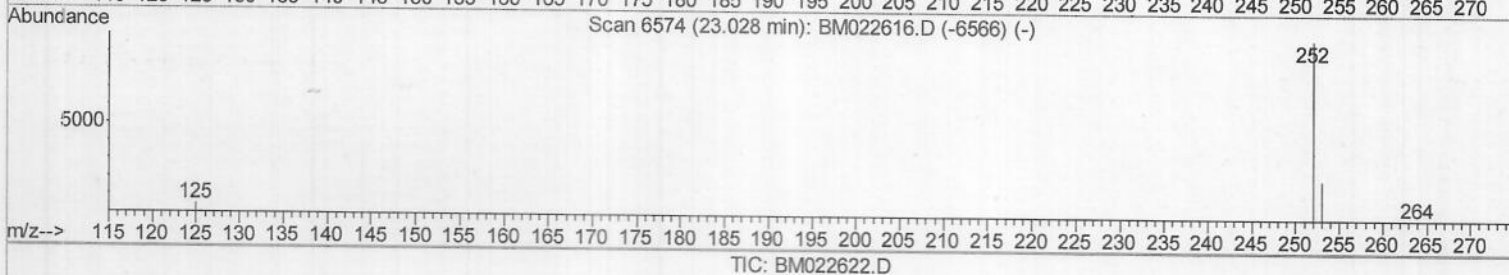
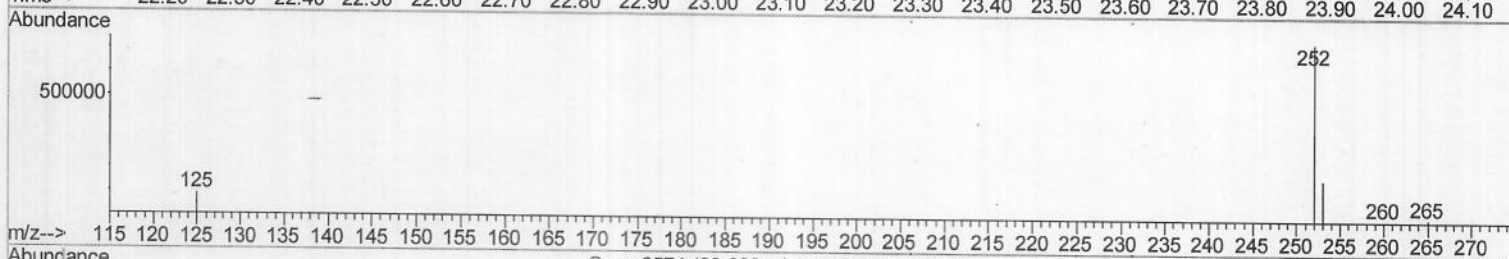
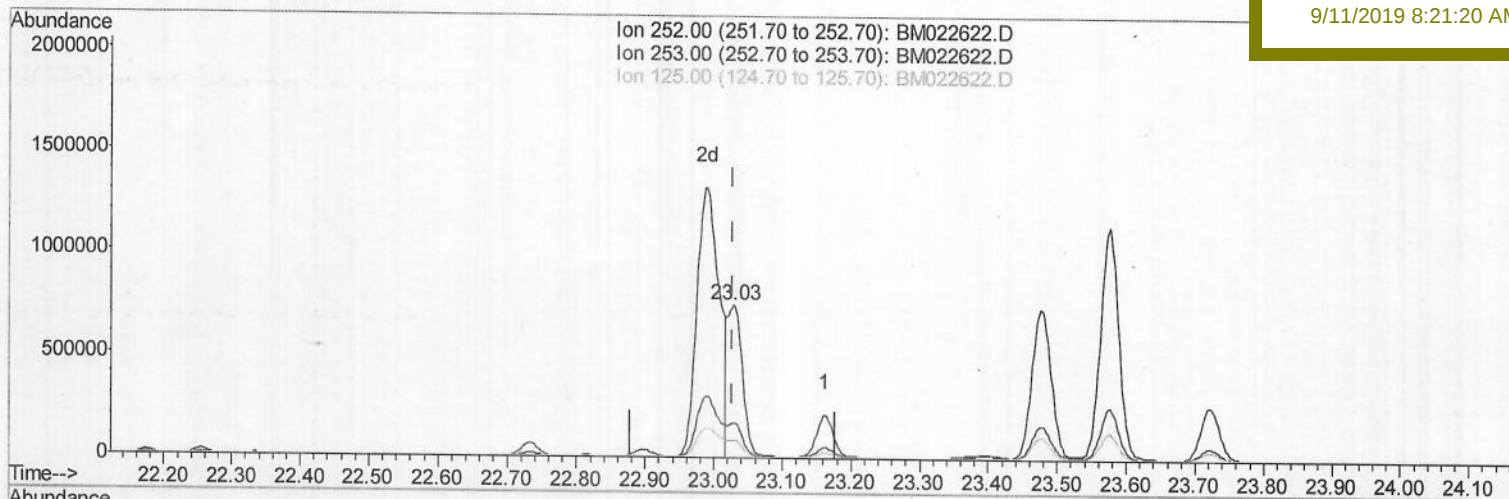
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5P8

Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:20 AM

(22) Benzo(k)fluoranthene

23.028min (+0.000) 5.36ng/ul m) JU
09/11/19

response 1162757

Ion	Exp%	Act%
252.00	100	100
253.00	24.40	22.91
125.00	14.00	11.56
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
 Data File : BM022622.D
 Acq On : 10 Sep 2019 16:31
 Operator : HP/JU
 Sample : K4708-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 CB5P8

Quant Time: Sep 10 17:16:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 9/11/2019 8:21:20 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	16076	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	67447	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	37229	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	81568m)	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	61021m)	0.40	ng/ul	0.00
20) Perylene-d12	23.67	264	48920m)	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.23	152	33978	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	77325m)	0.35	ng/ul	0.00

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.69	128	84664	0.441	ng/ul	99
5) 2-Methylnaphthalene	12.30	142	36207	0.275	ng/ul	100
7) Acenaphthylene	14.20	152	52600	0.305	ng/ul	97
8) Acenaphthene	14.54	153	188216	1.305	ng/ul	98
9) Fluorene	15.52	166	208256	1.260	ng/ul	99
12) Phenanthrene	17.26	178	4444216m)	17.101	ng/ul	
13) Anthracene	17.35	178	850423m)	3.814	ng/ul	
15) Fluoranthene	19.27	202	6445190m)	22.983	ng/ul	
17) Pyrene	19.63	202	5948587	21.503	ng/ul	98
18) Benzo(a)anthracene	21.37	228	2937706m)	12.579	ng/ul	
19) Chrysene	21.43	228	2931931	11.933	ng/ul	97
21) Benzo(b)fluoranthene	22.99	252	2927807m)	13.774	ng/ul	
22) Benzo(k)fluoranthene	23.03	252	1162757m)	5.362	ng/ul	
23) Benzo(a)pyrene	23.58	252	2077935	11.172	ng/ul#	89
24) Indeno(1,2,3-cd)pyrene	25.99	276	1267954	5.589	ng/ul#	90
25) Dibenzo(a,h)anthracene	26.00	278	356610	1.945	ng/ul	97
26) Benzo(g,h,i)perylene	26.70	276	991396	5.485	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed