

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
Data File : BM022625.D
Acq On : 10 Sep 2019 18:21
Operator : HP/JU
Sample : K4708-03
Misc :
ALS Vial : 13 Sample Multiplier: 1


Quant Time: Sep 10 19:00:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 15:06:45 2019
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5Q0

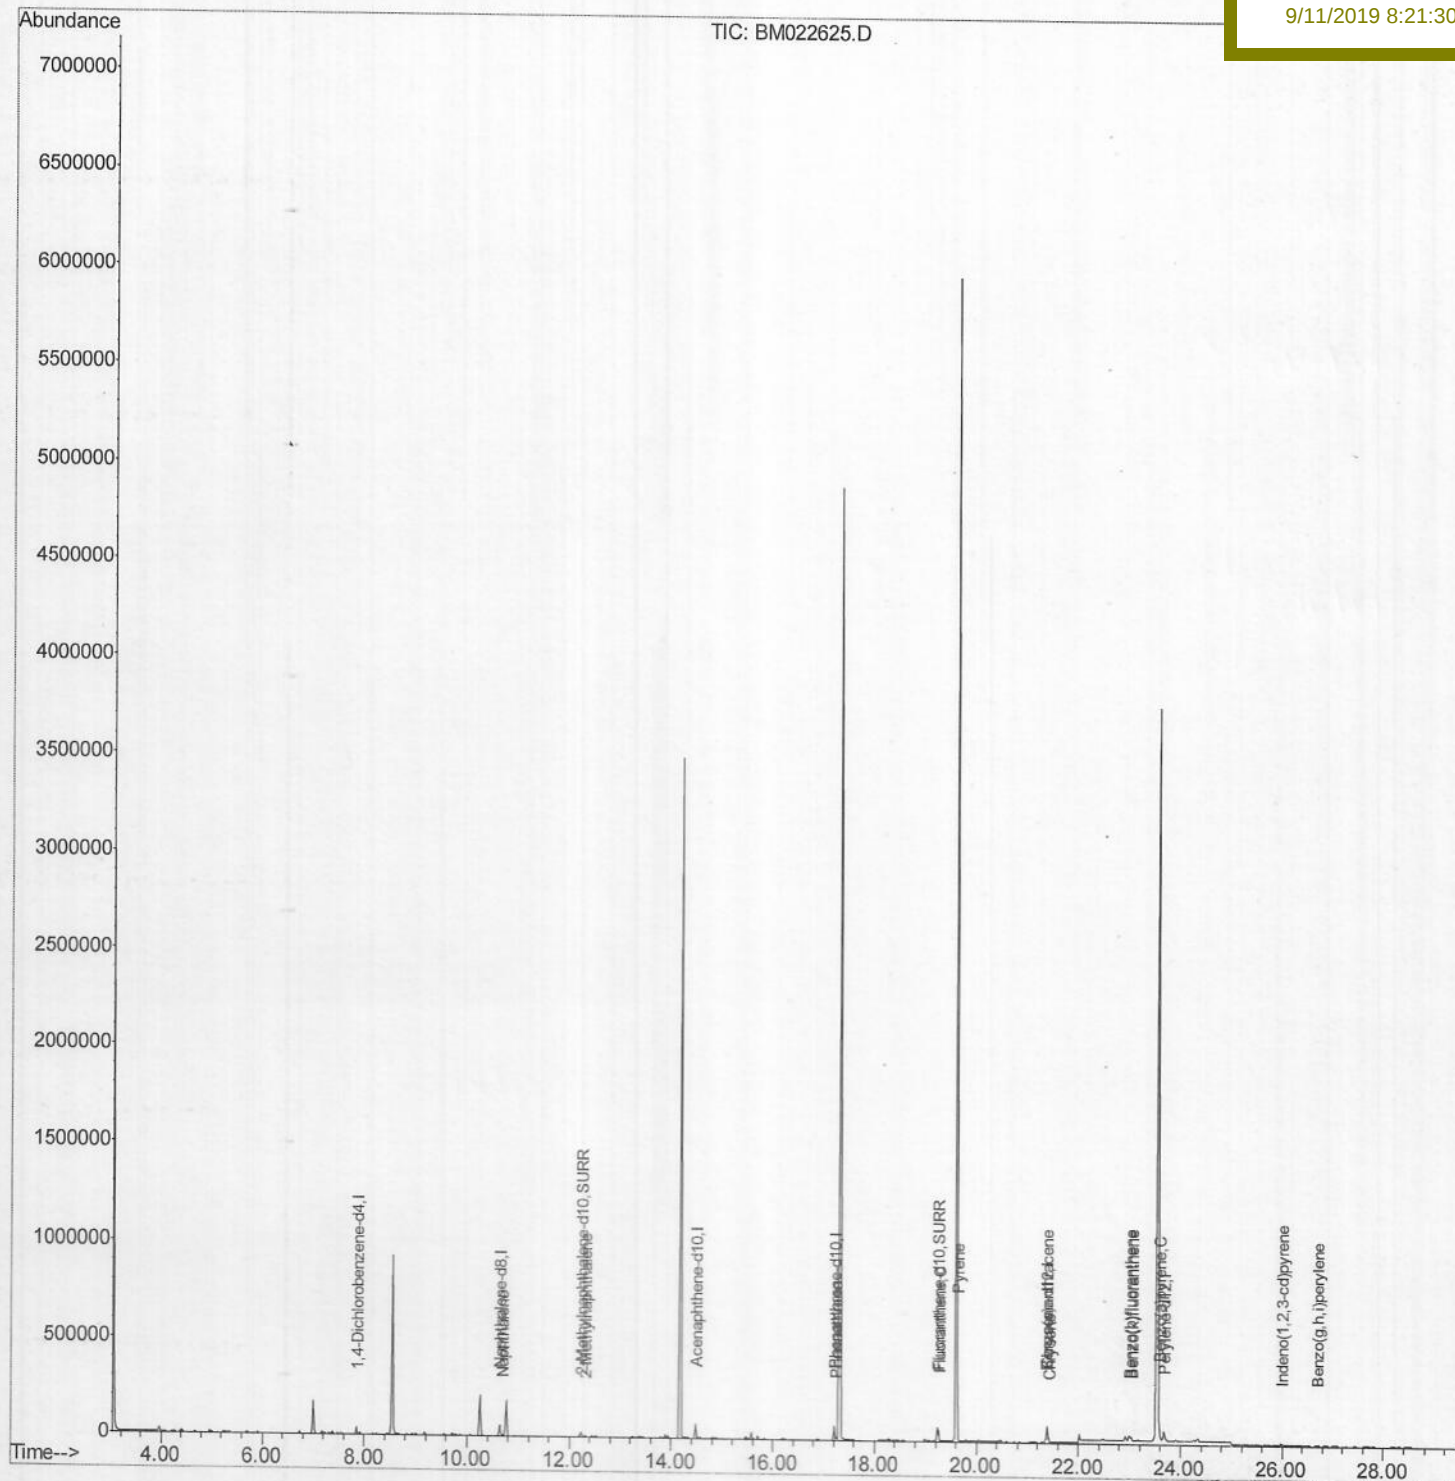Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:30 AM

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:54:34 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5Q0

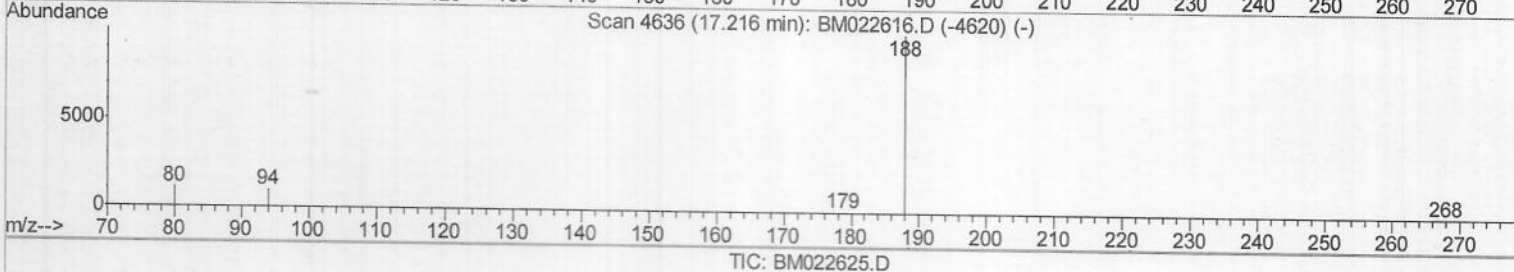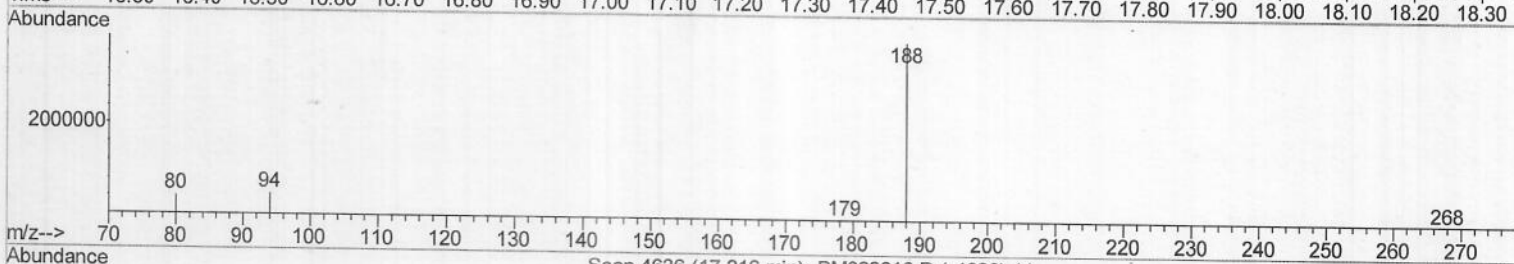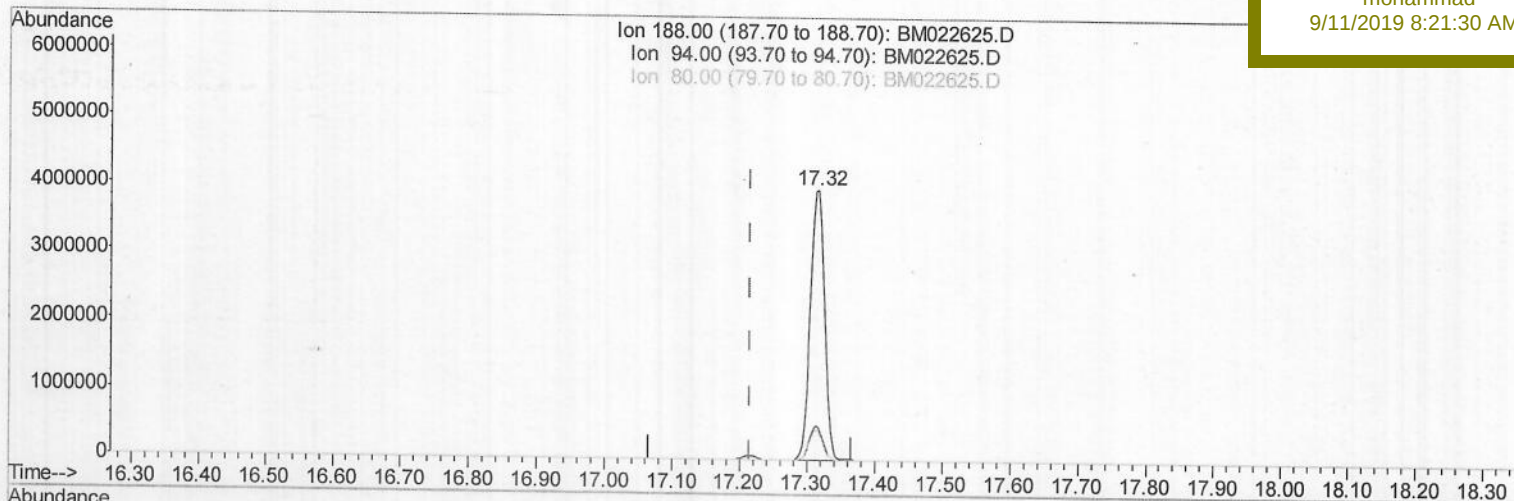Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:30 AM

(10) Phenanthrene-d10 (I)

17.317min (+0.100) 0.40ng/ul

response 5700926

Ion	Exp%	Act%
188.00	100	100
94.00	9.80	11.91#
80.00	11.00	10.43
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:54:34 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




CB5Q0

Manual Integrations

APPROVED

mohammad

9/11/2019 8:21:30 AM

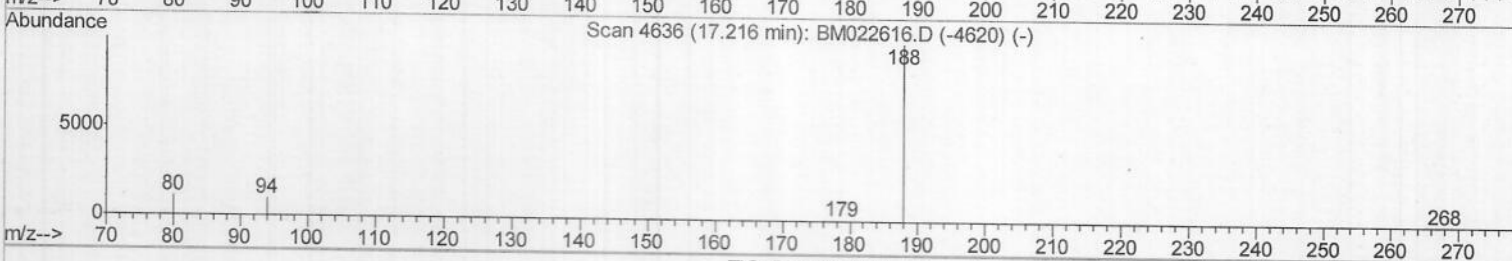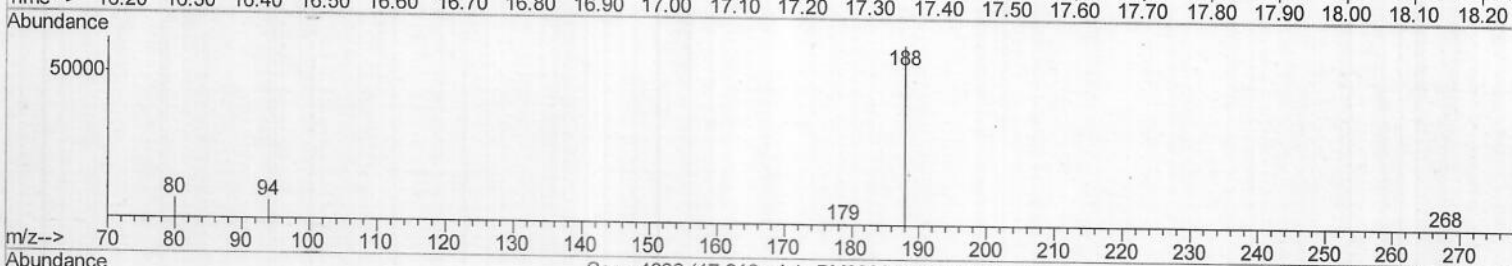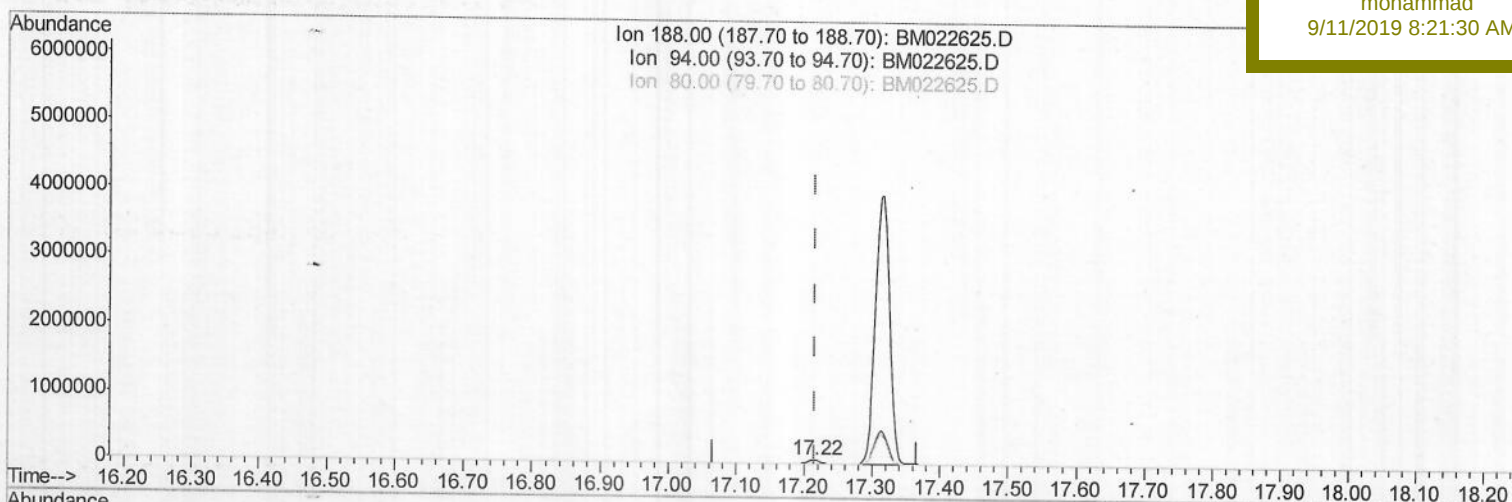

TIC: BM022625.D

(10) Phenanthrene-d10 (I)

17.216min (-0.000) 0.40ng/ul m) 30
09/11/19

response 85362

Ion	Exp%	Act%
188.00	100	100
94.00	9.80	10.08
80.00	11.00	10.89
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
 Data File : BM022625.D
 Acq On : 10 Sep 2019 18:21
 Operator : HP/JU
 Sample : K4708-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:55:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 CB5Q0

Manual Integrations
 APPROVED

mohammad
 9/11/2019 8:21:30 AM

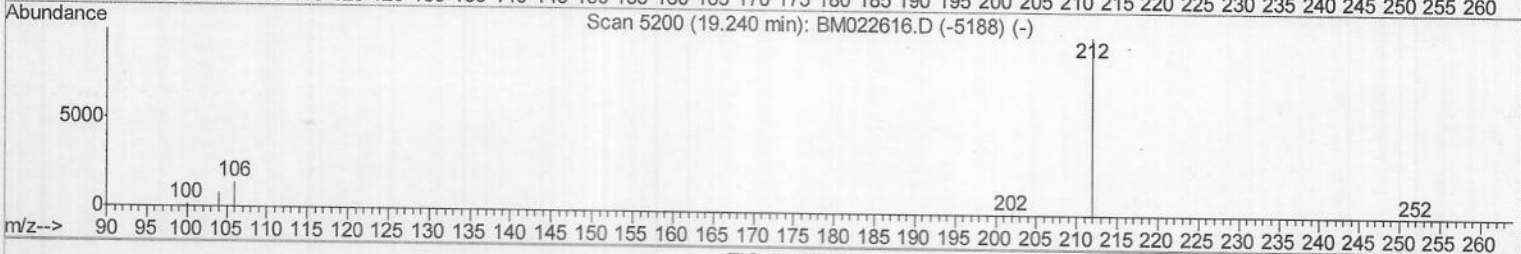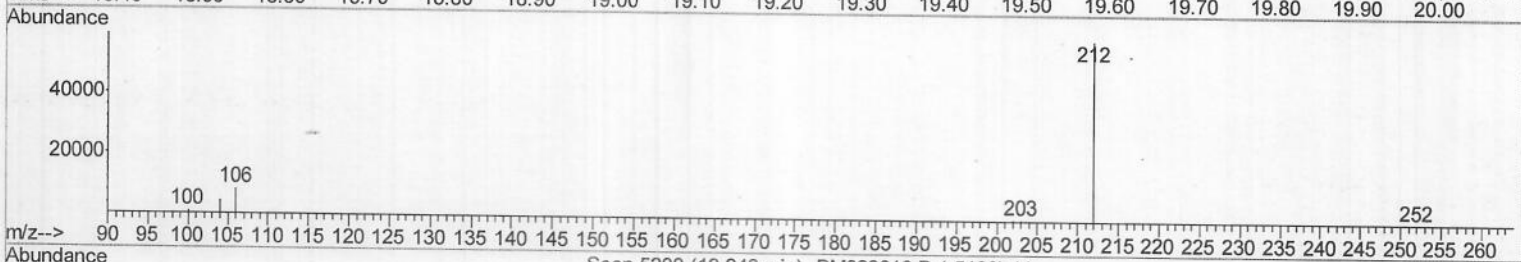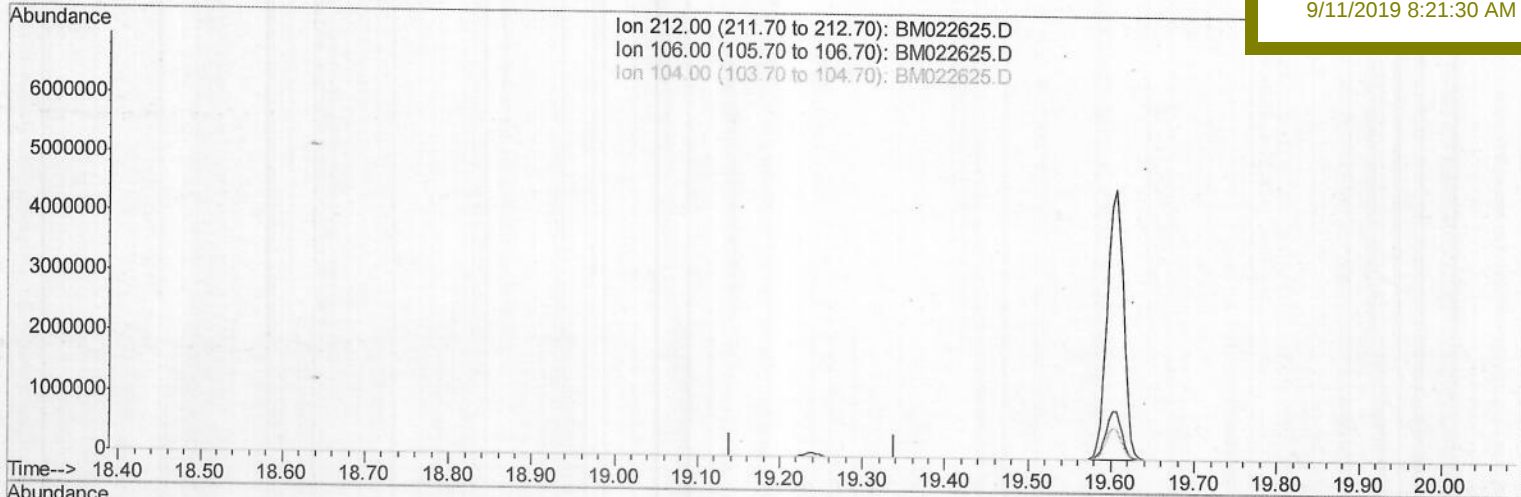

(14) Fluoranthene-d10 (SURR)

19.240min (-19.240) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.00	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:55:13 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5Q0

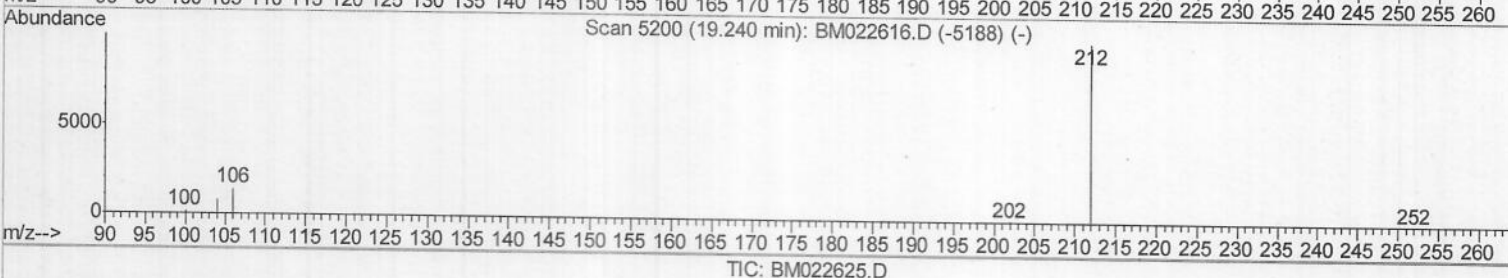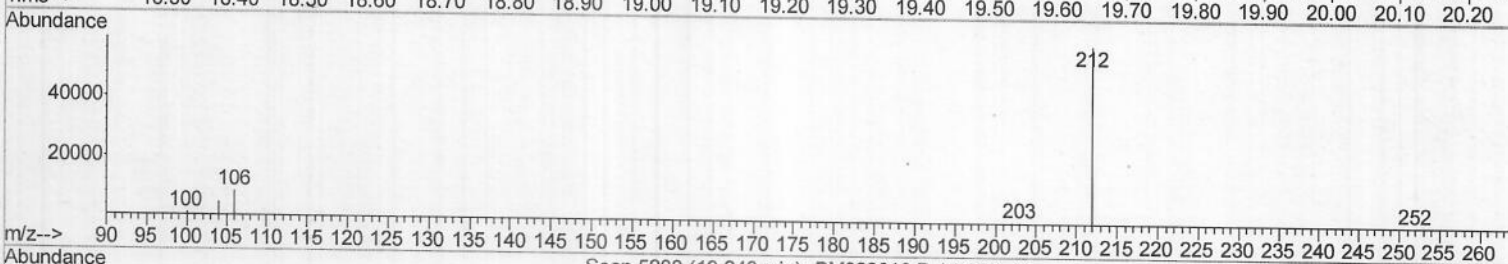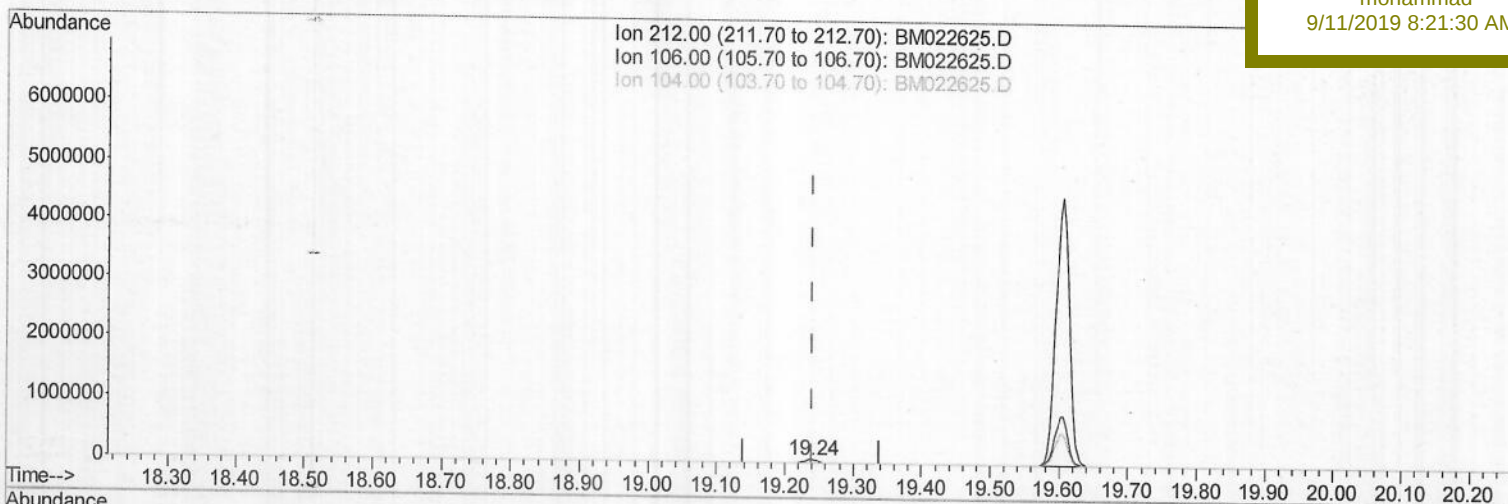Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:30 AM

(14) Fluoranthene-d10 (SURR)

19.239min (-0.000) 0.33ng/ul m) JU
09/11/19

response 77534

Ion	Exp%	Act%
212.00	100	100
106.00	14.00	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:55:13 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5Q0

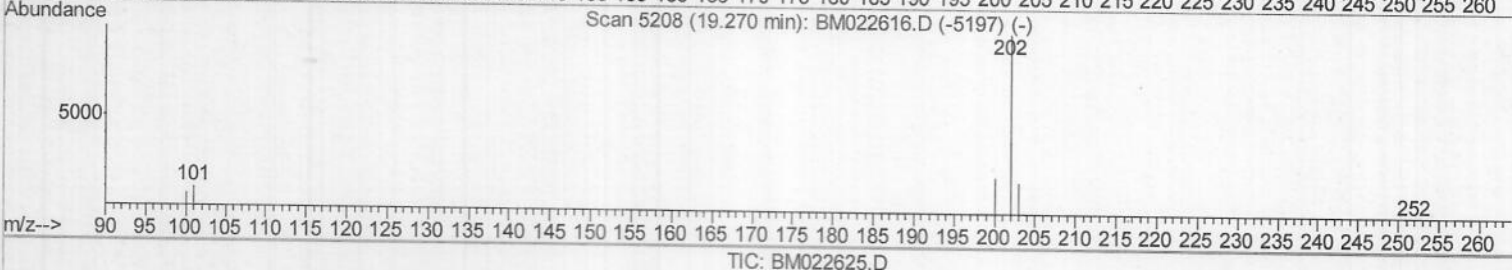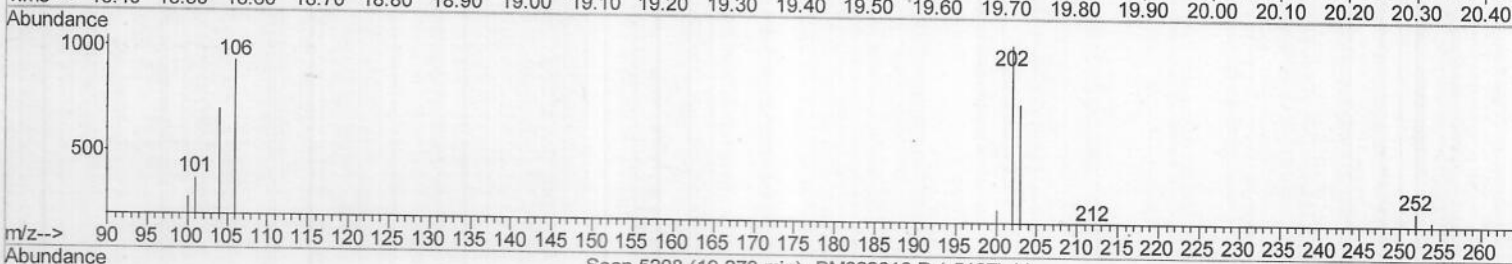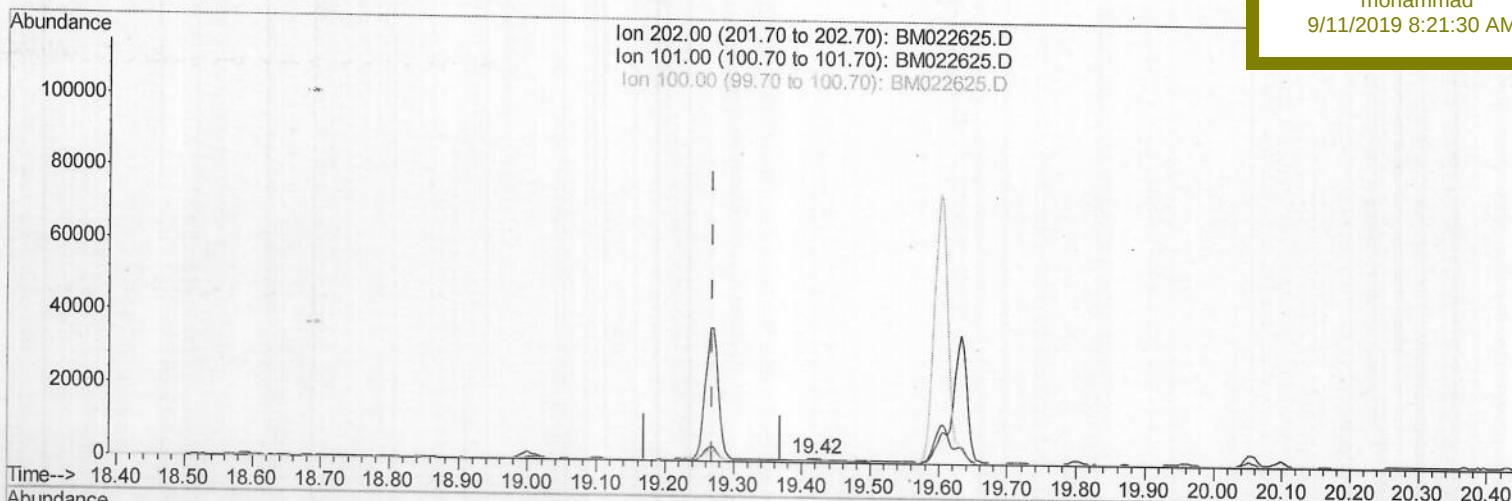Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:30 AM

(15) Fluoranthene (C)

19.419min (+0.148) 0.00ng/ul

response 628

Ion	Exp%	Act%
202.00	100	100
101.00	10.50	35.16#
100.00	8.00	26.69
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:55:13 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




CB5Q0

Manual Integrations

APPROVED

mohammad

9/11/2019 8:21:30 AM

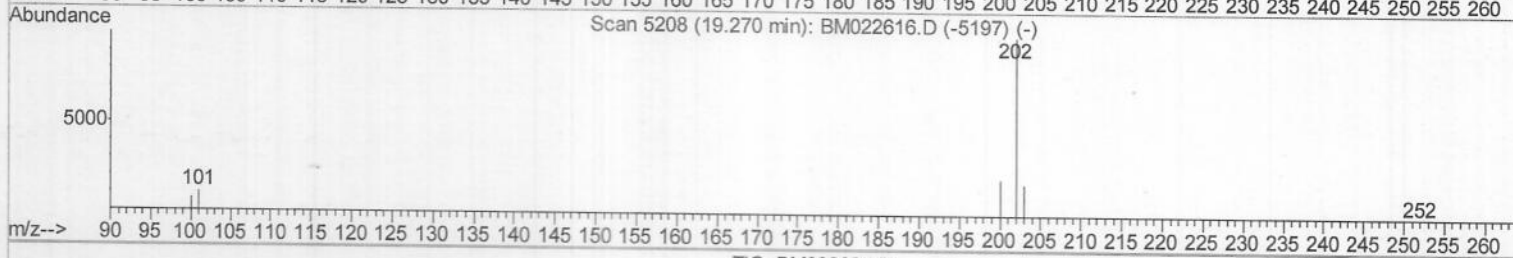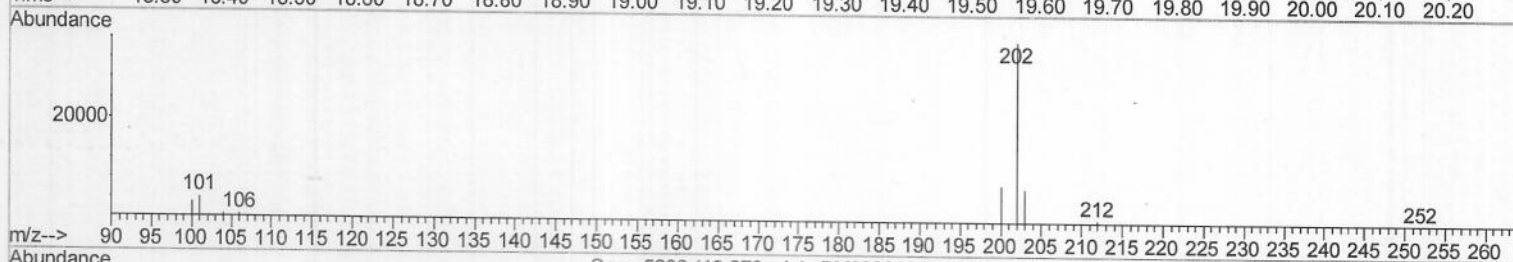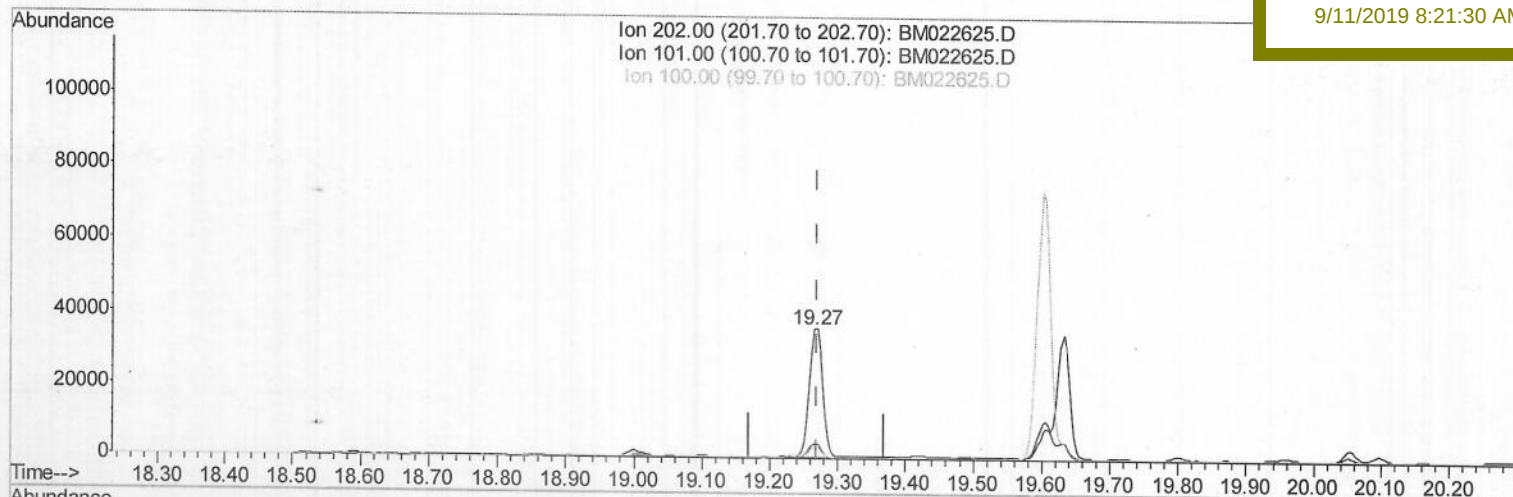

TIC: BM022625.D

(15) Fluoranthene (C)

19.266min (-0.004) 0.16ng/ul m 09/11/19

response 48323

Ion	Exp%	Act%
202.00	100	100
101.00	10.50	11.60
100.00	8.00	8.82
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:55:13 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5Q0

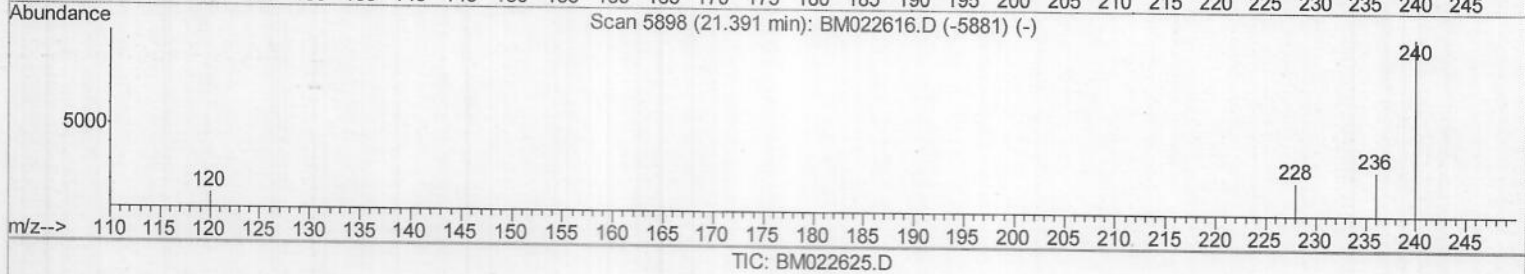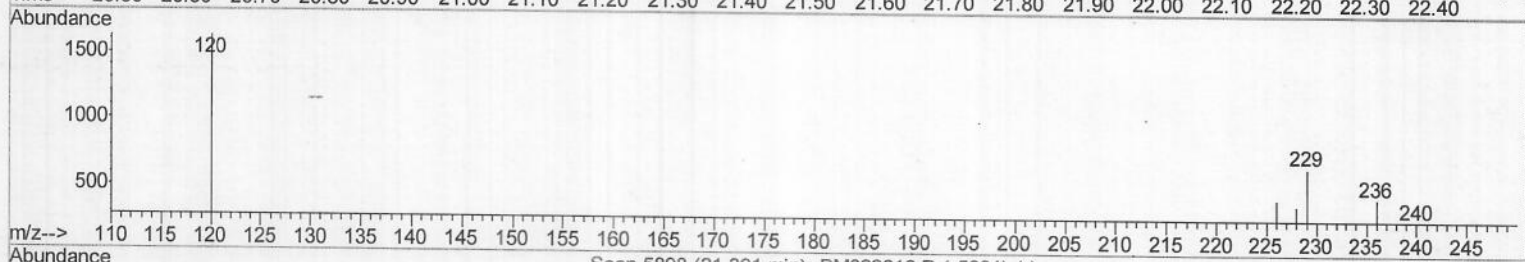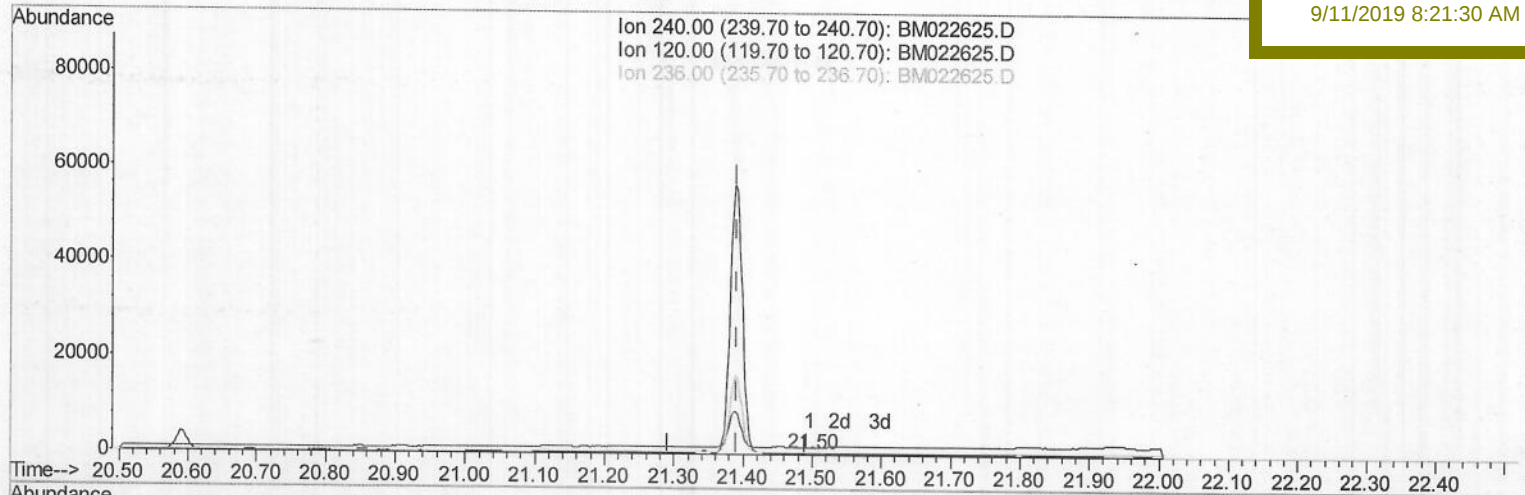Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:30 AM

(16) Chrysene-d12 (I)

21.497min (+0.106) 0.40ng/ul

response 39

Ion	Exp%	Act%
240.00	100	100
120.00	14.60	571.83#
236.00	28.80	157.04#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
 Data File : BM022625.D
 Acq On : 10 Sep 2019 18:21
 Operator : HP/JU
 Sample : K4708-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 CB5Q0

Quant Time: Sep 10 18:55:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
 9/11/2019 8:21:30 AM

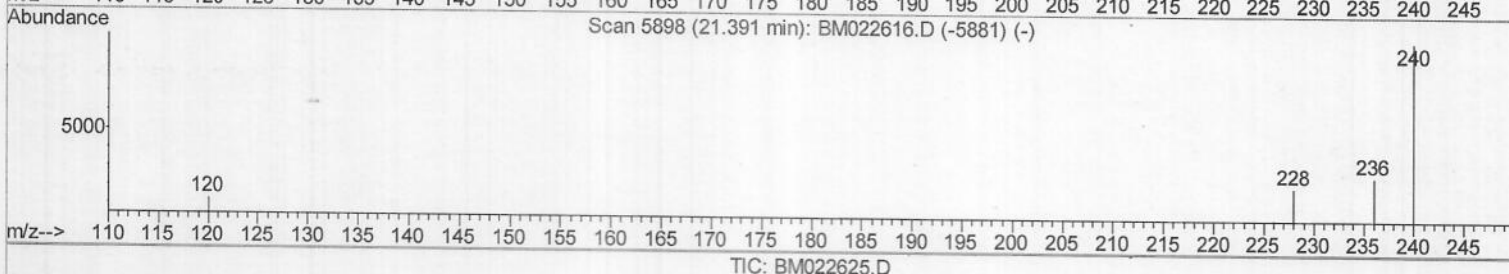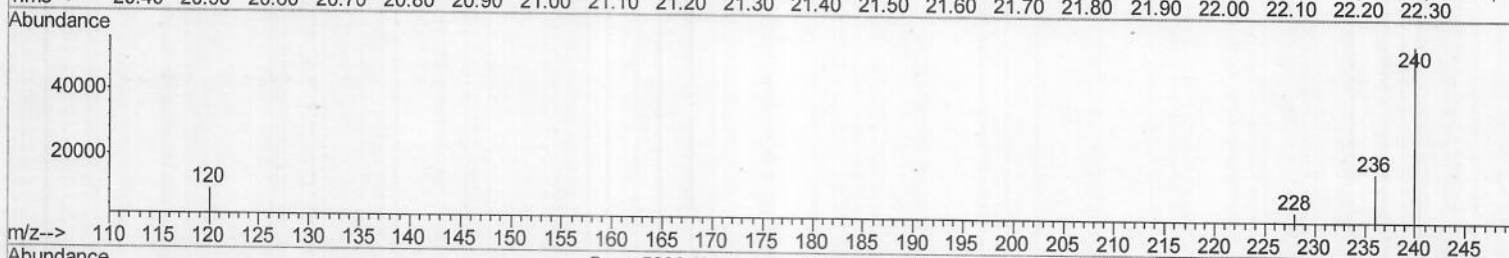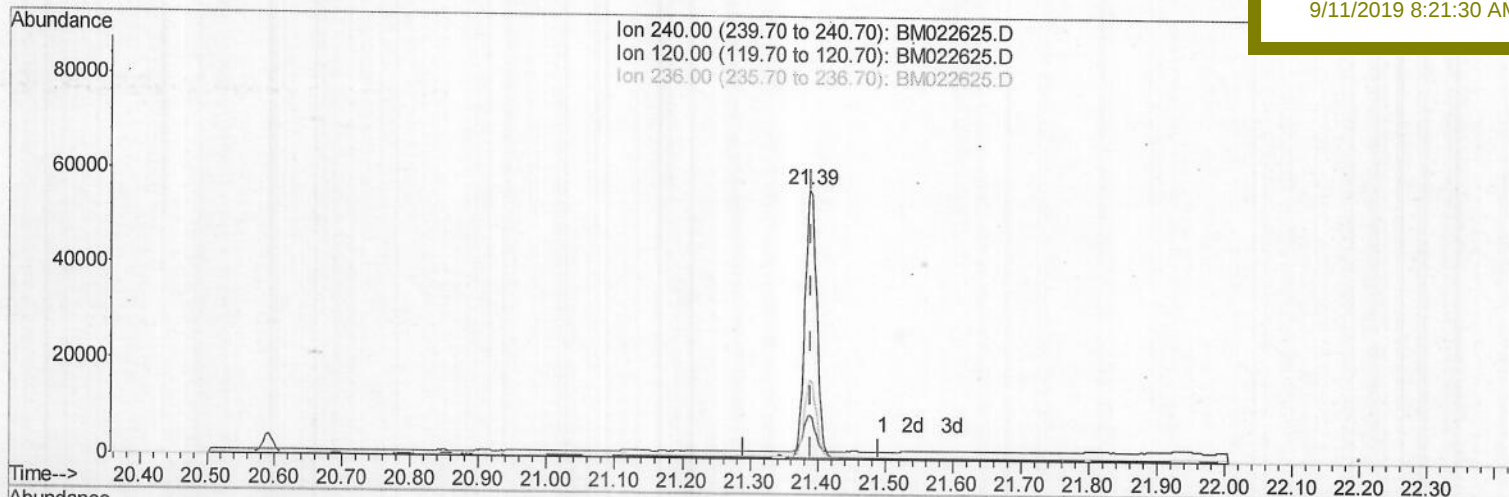

TIC: BM022625.D

(16) Chrysene-d12 (I)

21.389min (-0.003) 0.40ng/ul m

response 68233

JU
 09/11/19

Ion	Exp%	Act%
240.00	100	100
120.00	14.60	15.89
236.00	28.80	28.99
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:57:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5Q0

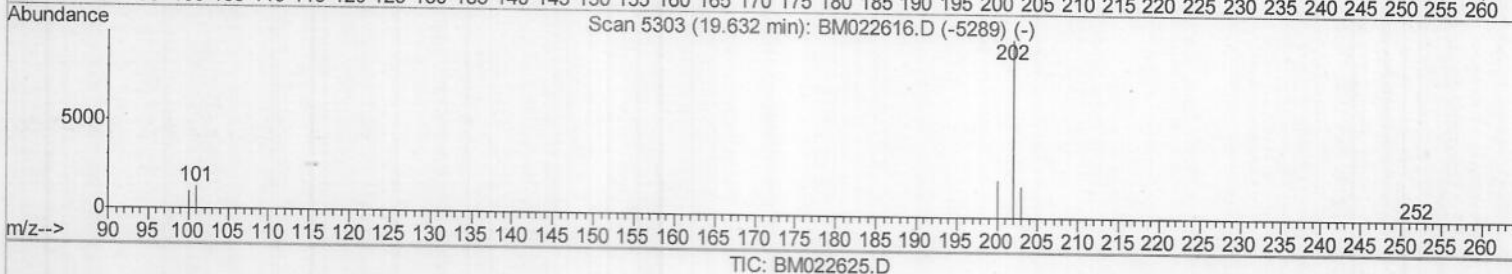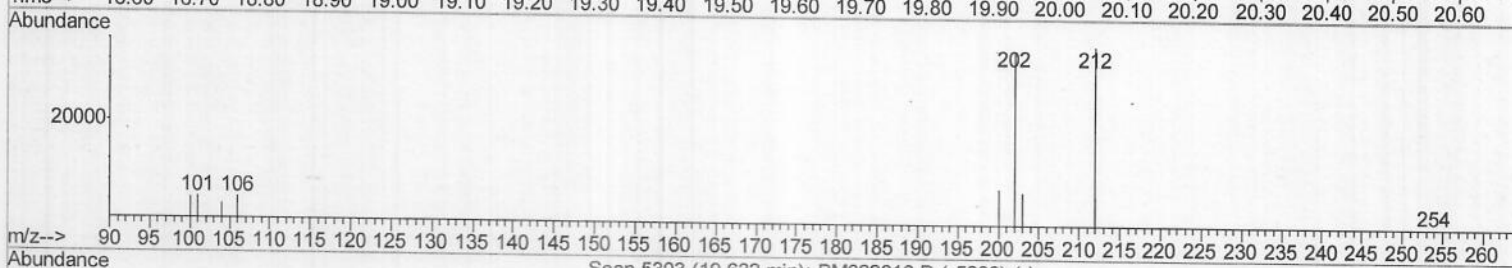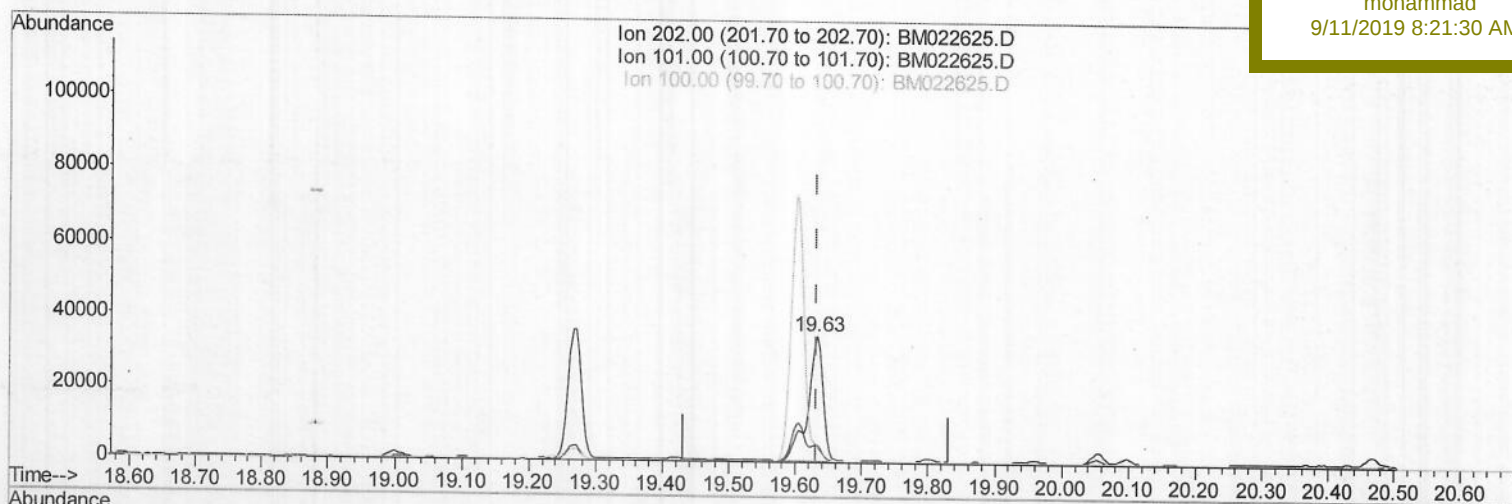Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:30 AM

(17) Pyrene

19.632min (-0.000) 0.17ng/ul

response 53406

Ion	Exp%	Act%
202.00	100	100
101.00	12.50	13.30
100.00	10.10	12.43#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:57:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




CB5Q0

Manual Integrations

APPROVED

mohammad

9/11/2019 8:21:30 AM

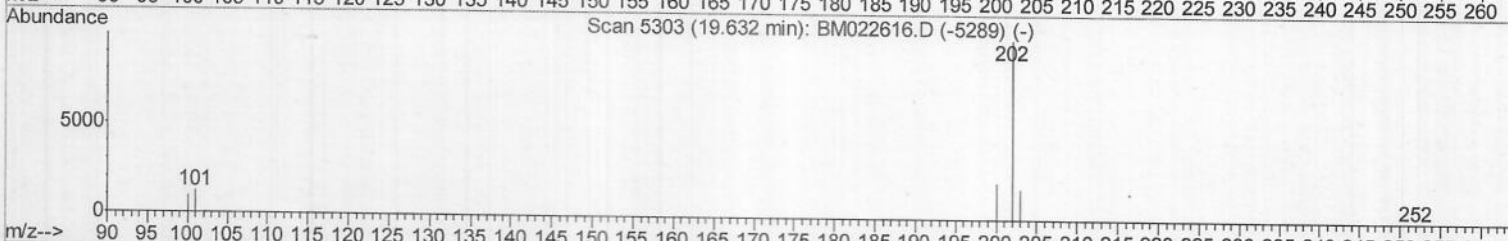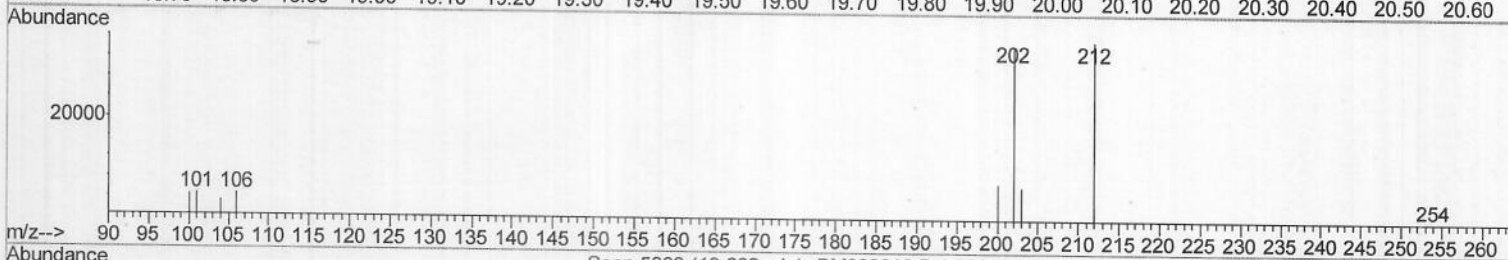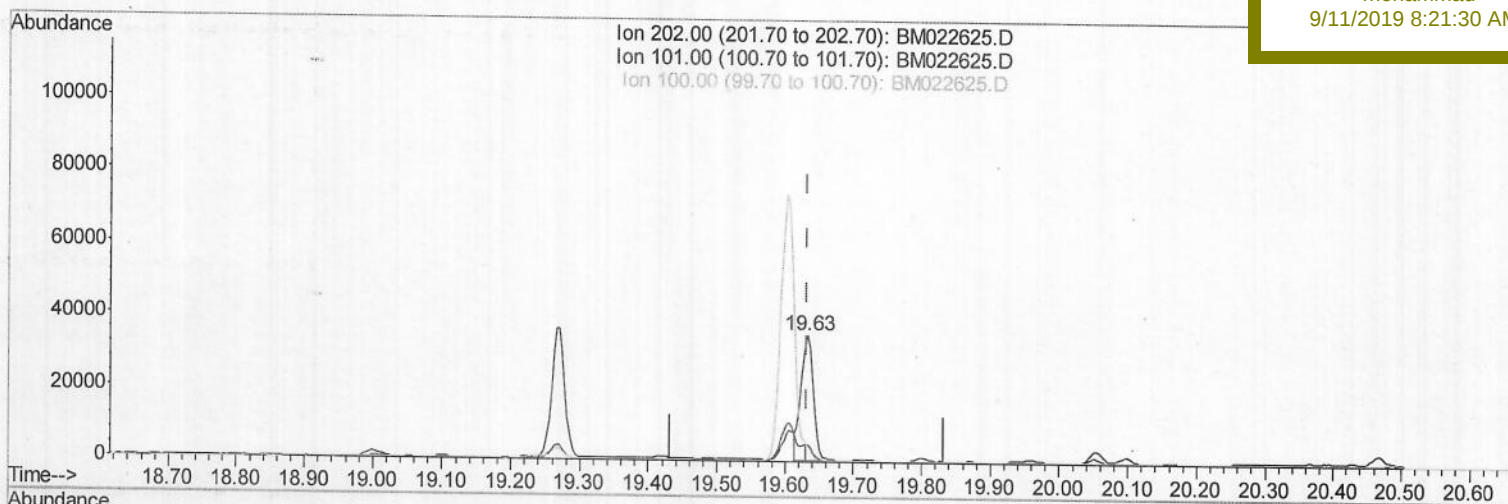

(17) Pyrene

19.632min (-0.000) 0.14ng/ul m) JU
09/11/19

response 43629

Ion	Exp%	Act%
202.00	100	100
101.00	12.50	13.30
100.00	10.10	12.43#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:57:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




CB5Q0

Manual Integrations

APPROVED

mohammad

9/11/2019 8:21:30 AM

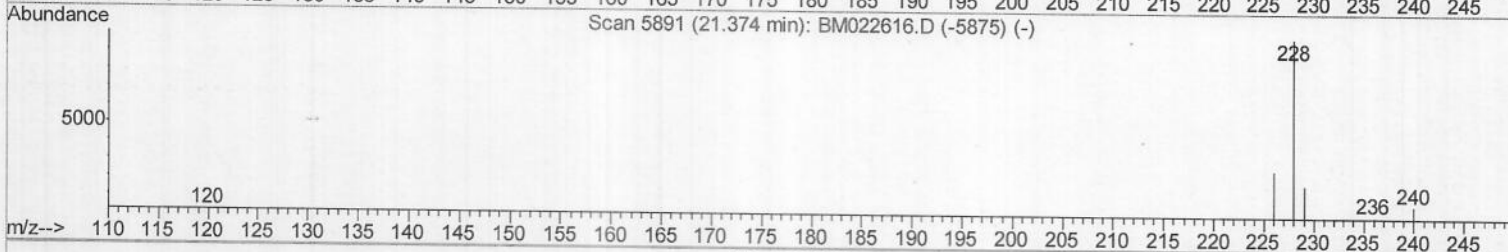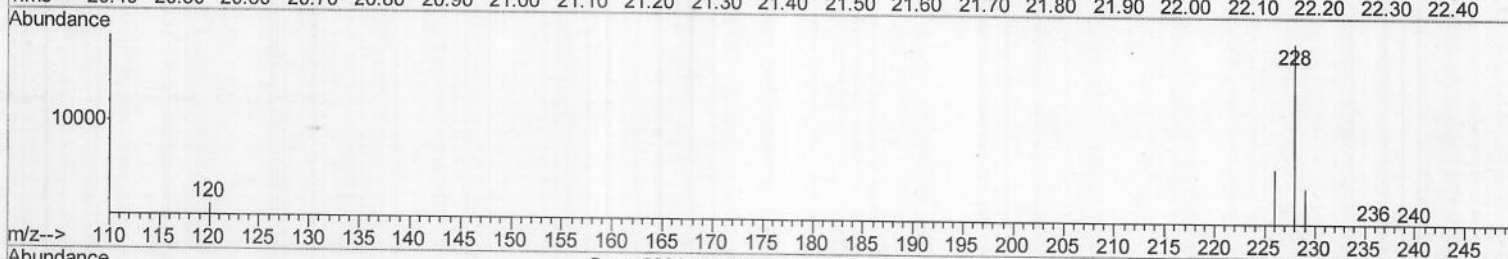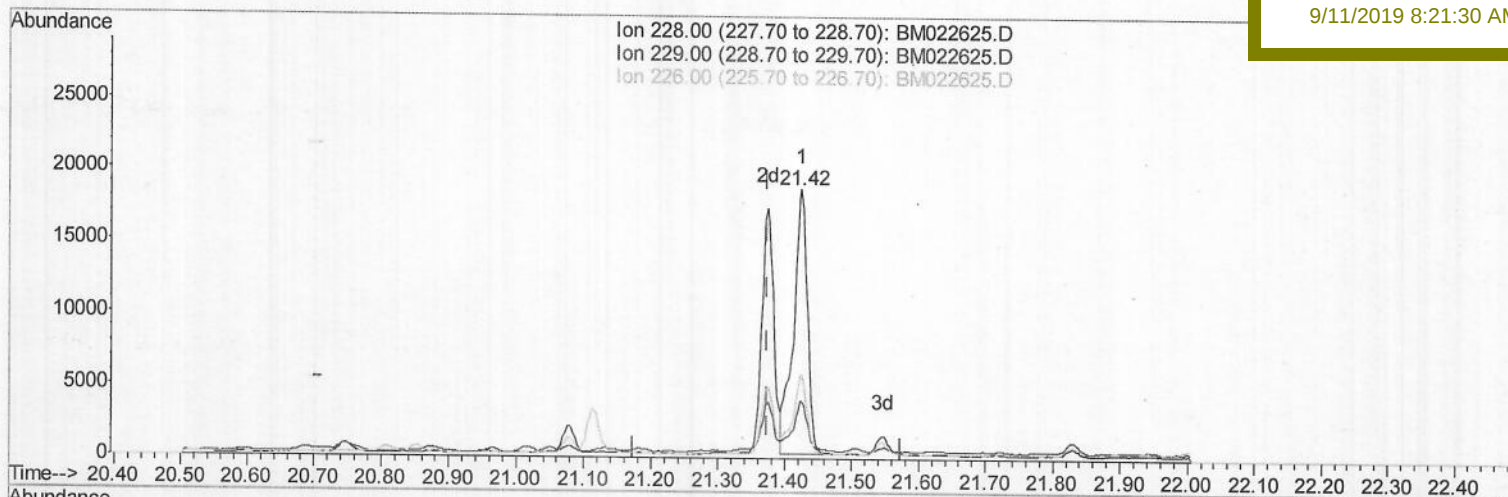

(18) Benzo(a)anthracene

21.425min (+0.051) 0.10ng/ul

response 26853

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	21.97
226.00	27.50	31.64
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:57:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5Q0

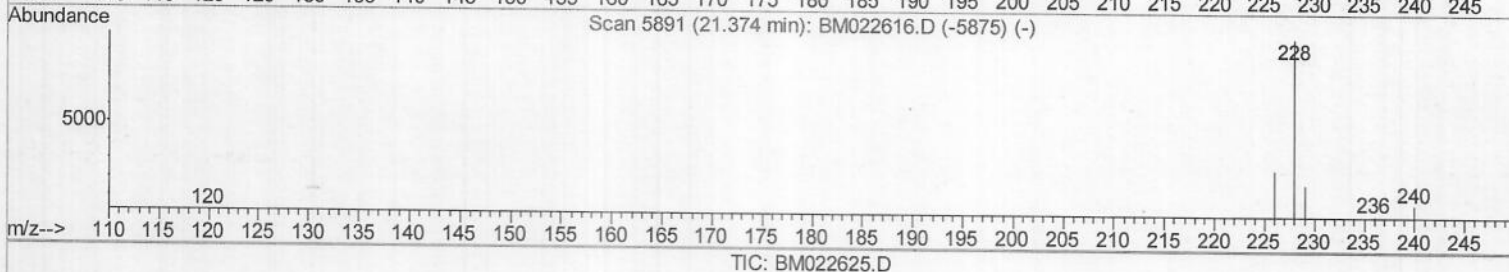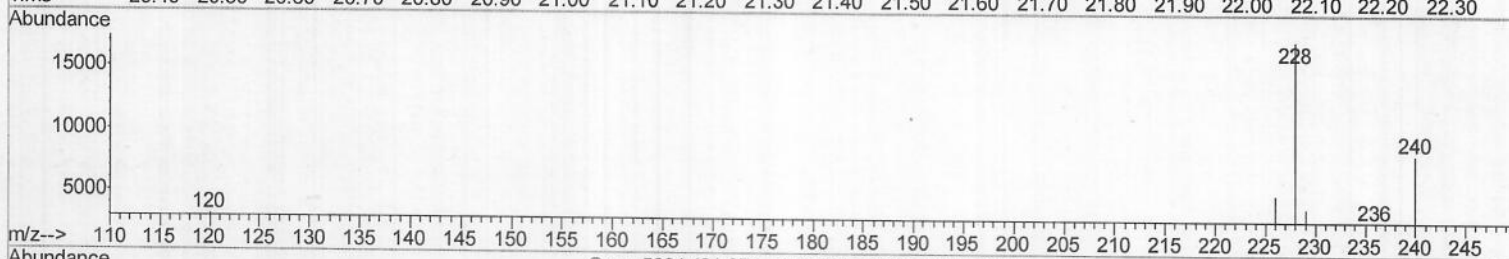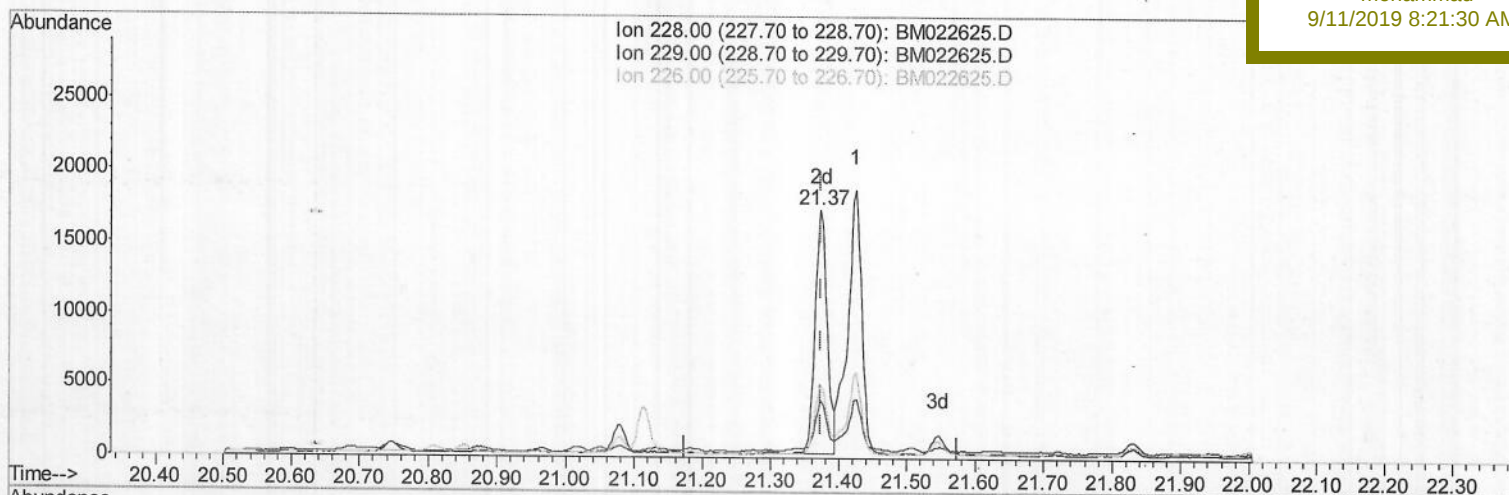Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:30 AM

(18) Benzo(a)anthracene

21.374min (-0.000) 0.08ng/ul m) JU
09/11/19

response 21150

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	22.88
226.00	27.50	29.04
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
Data File : BM022625.D
Acq On : 10 Sep 2019 18:21
Operator : HP/JU
Sample : K4708-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:57:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 15:06:45 2019
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




CB5Q0

Manual Integrations

APPROVED

mohammad

9/11/2019 8:21:30 AM

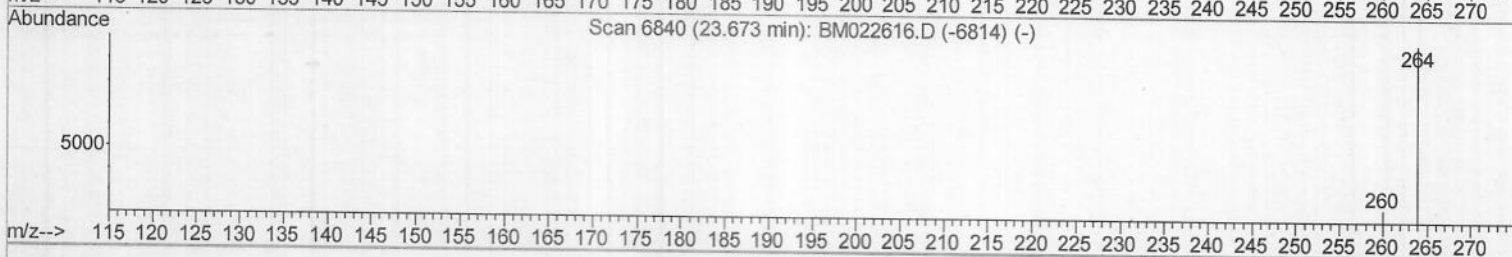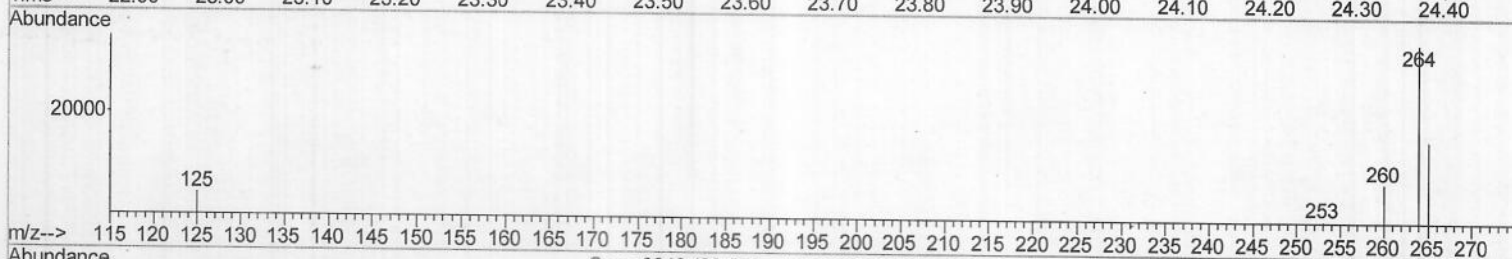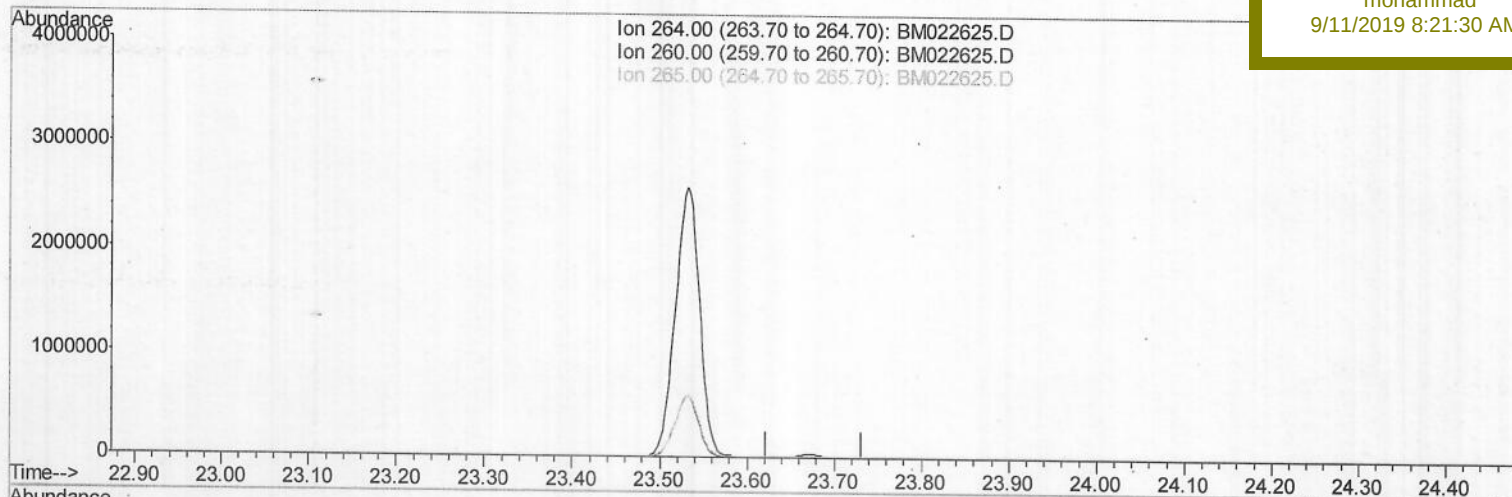

(20) Perylene-d12 (I)

23.673min (-23.673) 0.00ng/ul

response 0

Ion	Exp%	Act%
264.00	100	0.00
260.00	25.60	0.00#
265.00	59.90	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:57:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

CB5Q0

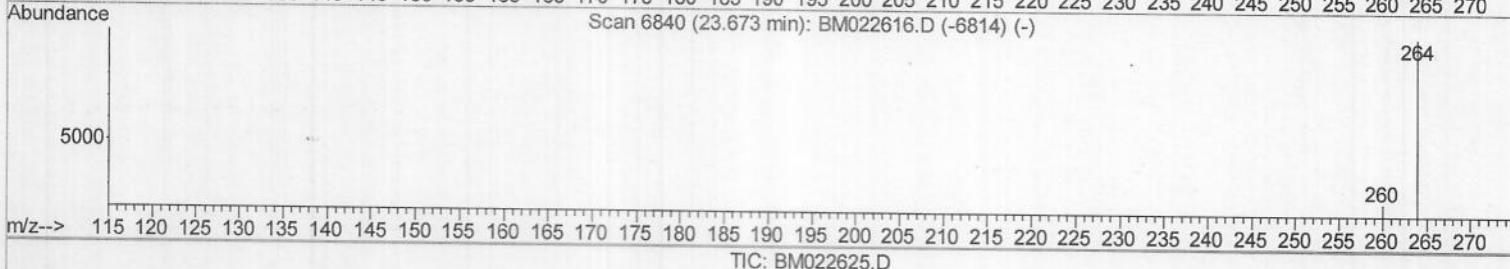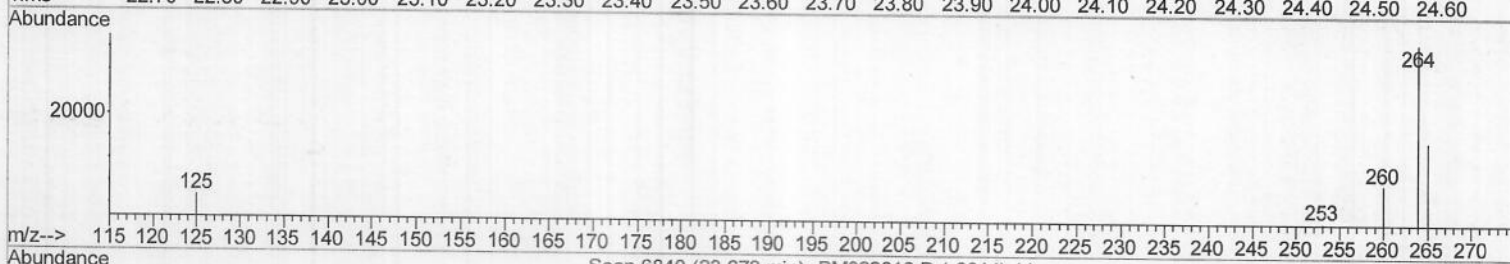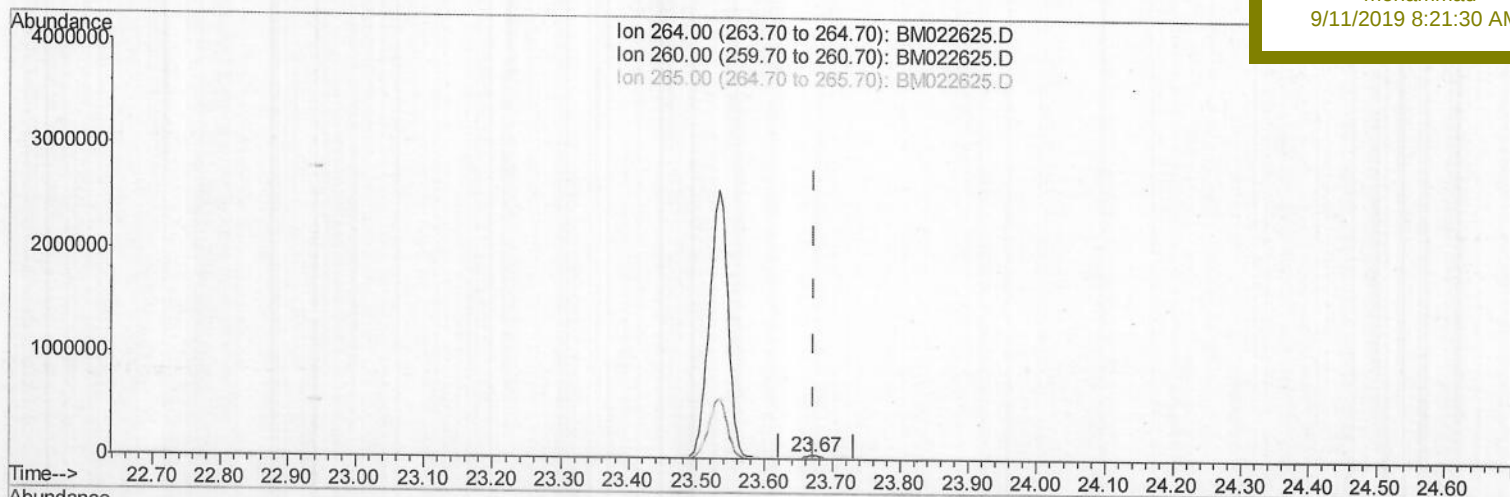Manual Integrations
APPROVEDmohammad
9/11/2019 8:21:30 AM

(20) Perylene-d12 (I)

23.672min (-0.000) 0.40ng/ul m) JU

response 53244

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	25.32
265.00	59.90	48.30
0.00	0.00	0.00

09/11/19

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
 Data File : BM022625.D
 Acq On : 10 Sep 2019 18:21
 Operator : HP/JU
 Sample : K4708-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:59:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 CB5Q0

Manual Integrations
 APPROVED

mohammad
 9/11/2019 8:21:30 AM

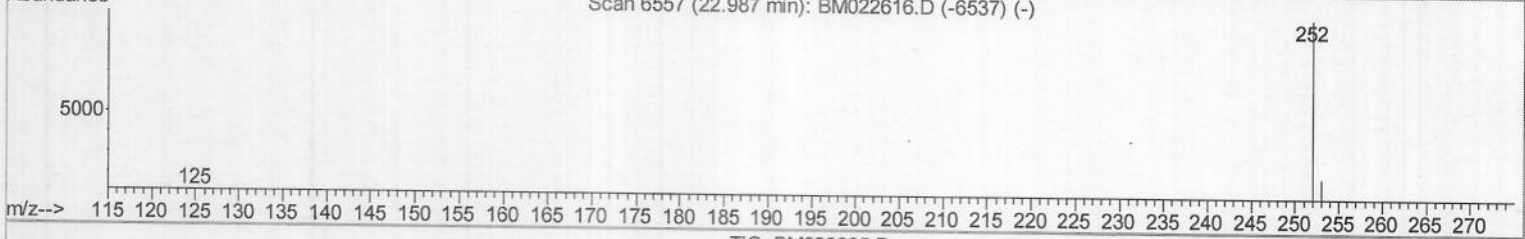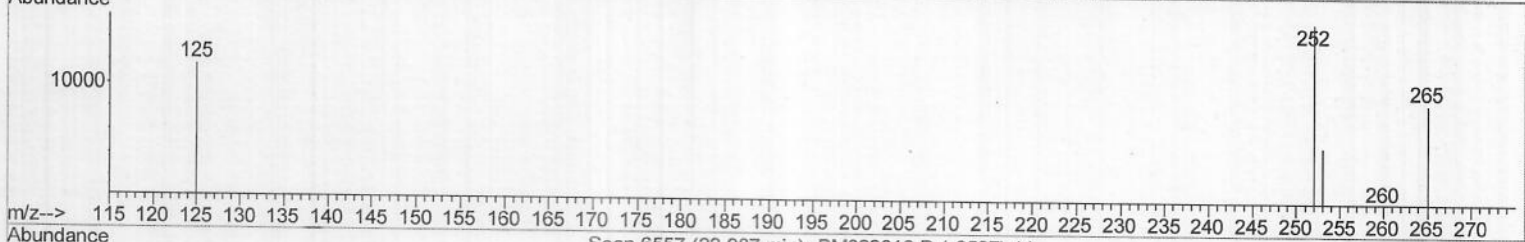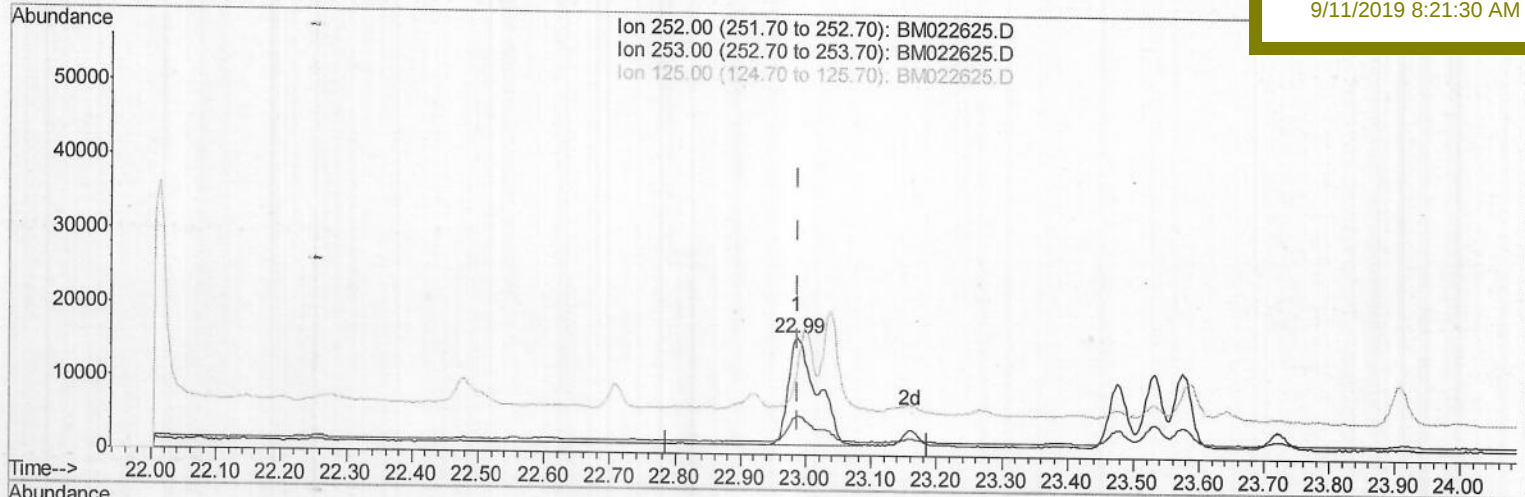

TIC: BM022625.D

(21) Benzo(b)fluoranthene
 22.987min (-0.000) 0.19ng/ul
 response 44857

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	32.60
125.00	15.60	73.31#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
 Data File : BM022625.D
 Acq On : 10 Sep 2019 18:21
 Operator : HP/JU
 Sample : K4708-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB5Q0

Manual Integrations
 APPROVED

mohammad
 9/11/2019 8:21:30 AM

Quant Time: Sep 10 18:59:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

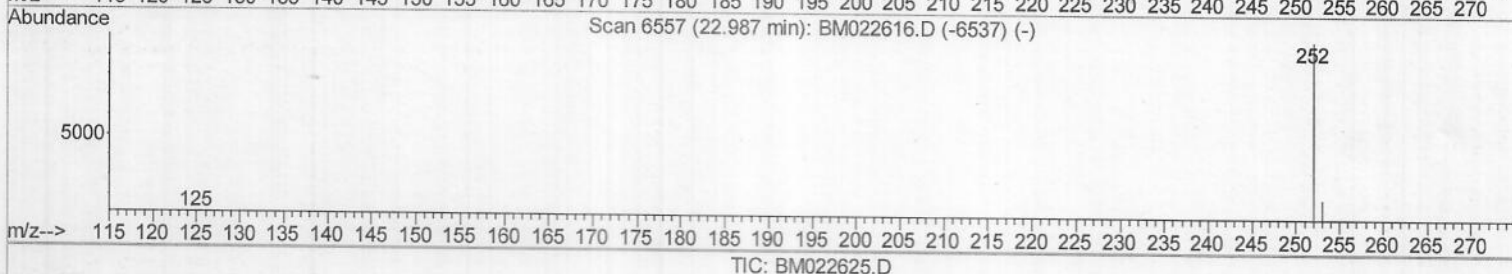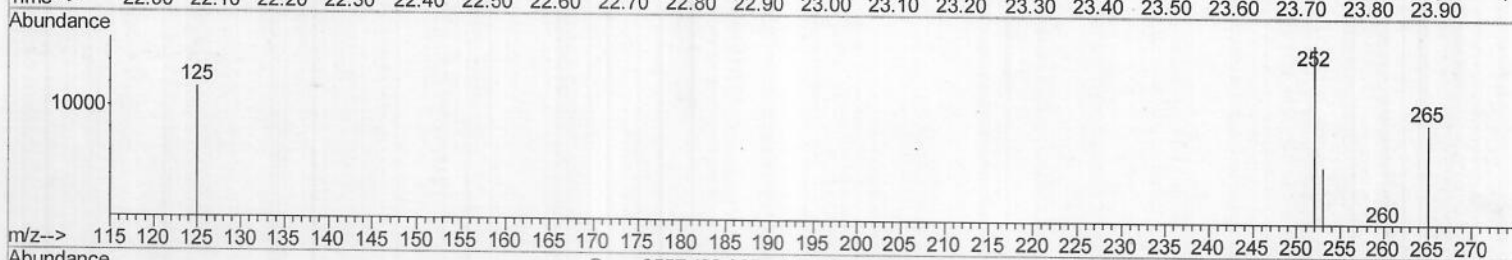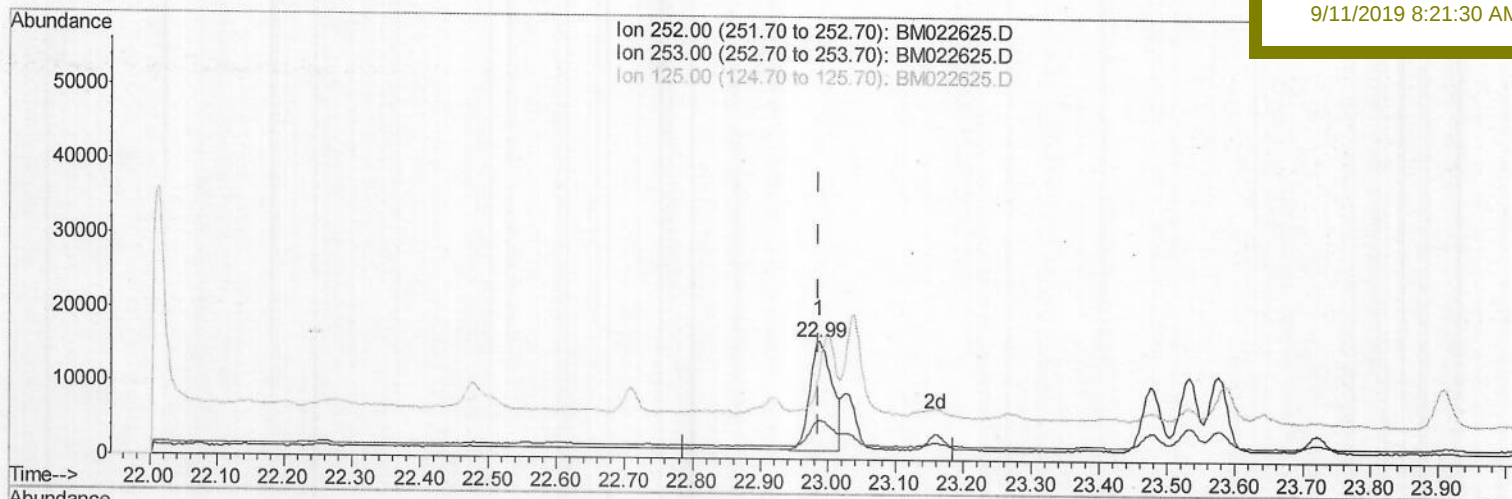

(21) Benzo(b)fluoranthene

22.987min (-0.000) 0.14ng/ul m) JU
 09/11/19
 response 33333

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	32.60
125.00	15.60	73.31#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:59:16 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




CB5Q0

Manual Integrations

APPROVED

mohammad

9/11/2019 8:21:30 AM

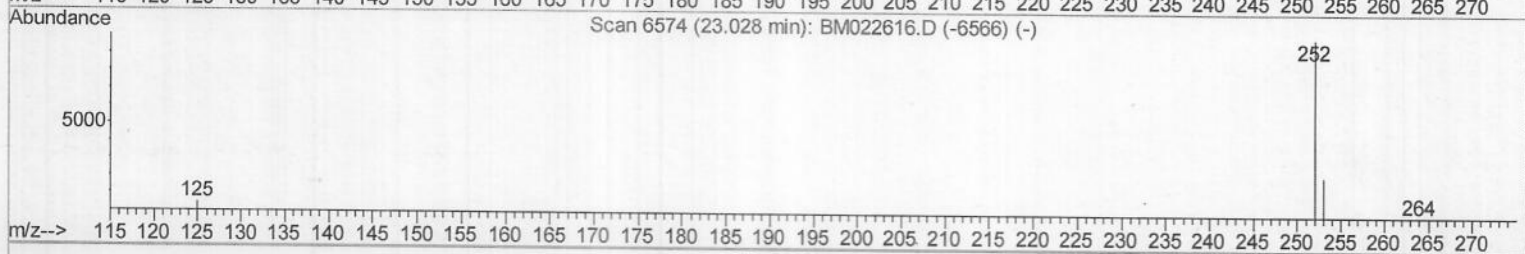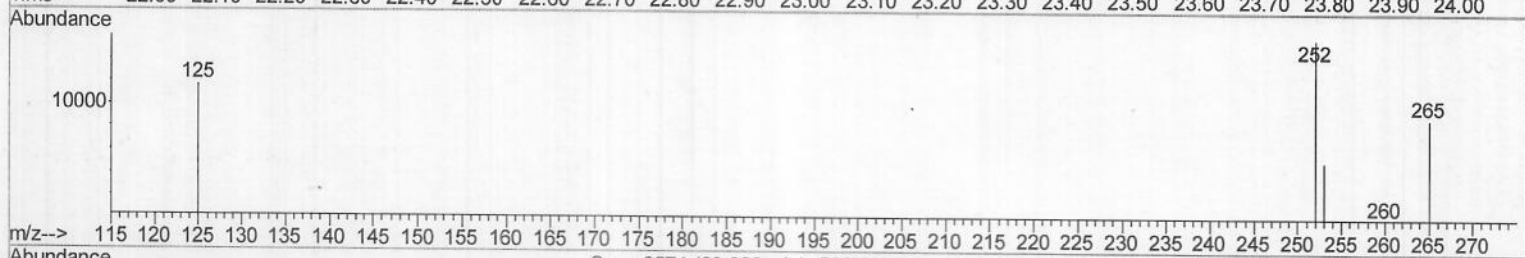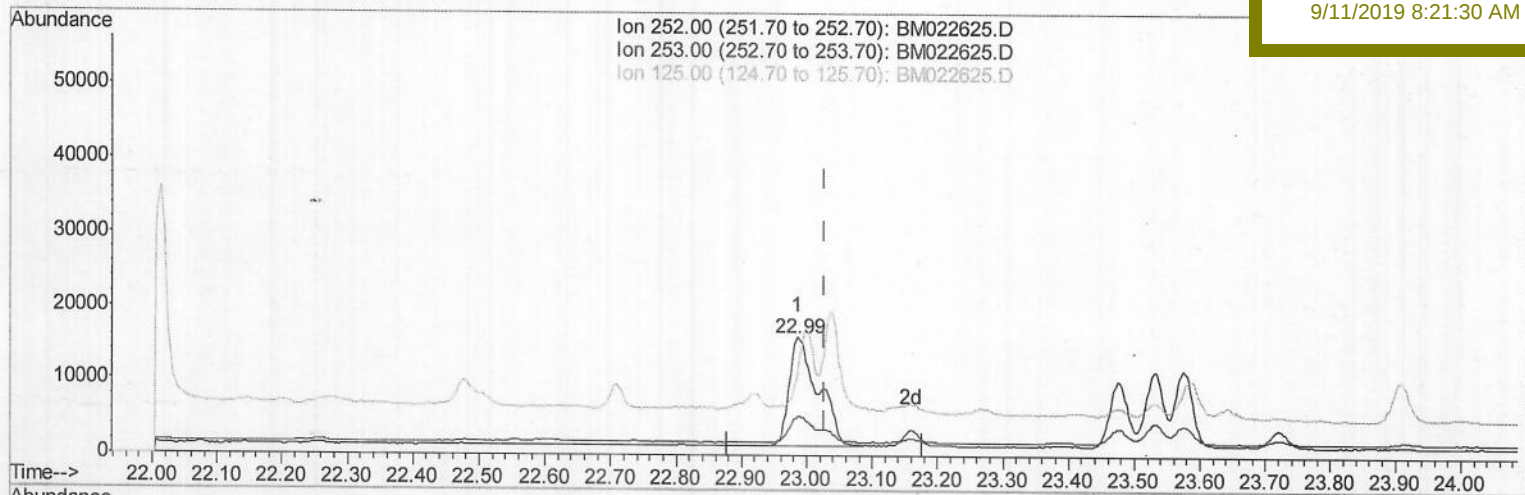

TIC: BM022625.D

(22) Benzo(k)fluoranthene

22.987min (-0.041) 0.19ng/ul

response 44857

Ion	Exp%	Act%
252.00	100	100
253.00	24.40	32.60#
125.00	14.00	73.31#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\

Data File : BM022625.D

Acq On : 10 Sep 2019 18:21

Operator : HP/JU

Sample : K4708-03

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 10 18:59:16 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




CB5Q0

Manual Integrations

APPROVED

mohammad

9/11/2019 8:21:30 AM

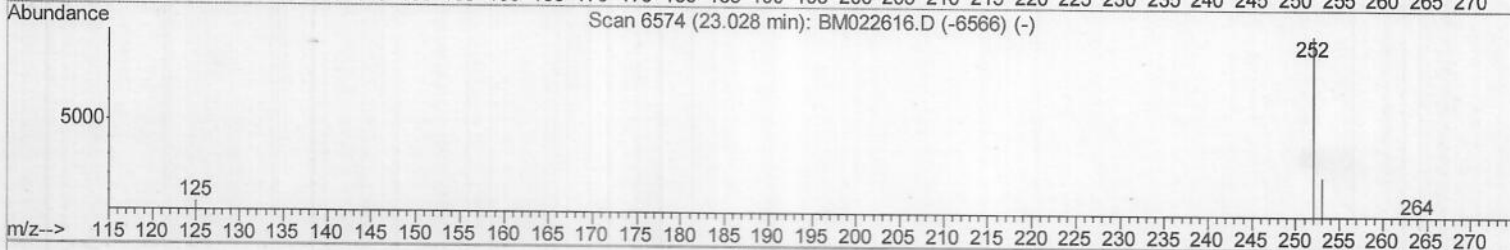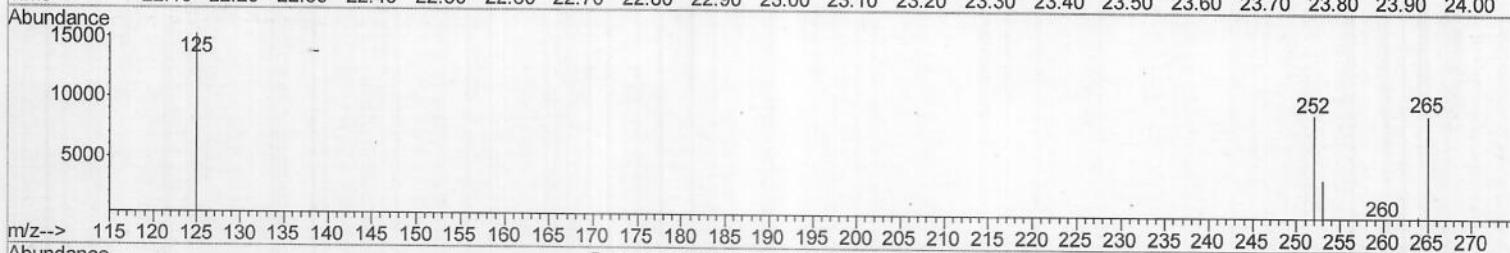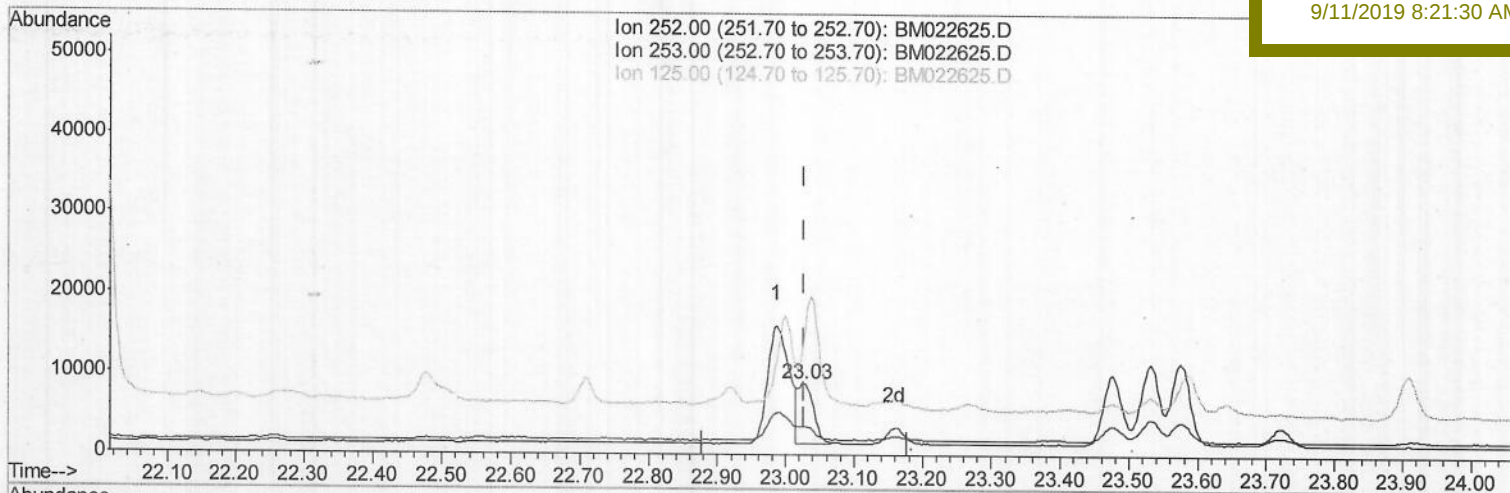

TIC: BM022625.D

(22) Benzo(k)fluoranthene

23.028min (-0.000) 0.05ng/ul m) JU
09/11/19

response 12816

Ion	Exp%	Act%
252.00	100	100
253.00	24.40	39.43#
125.00	14.00	170.32#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091019\
 Data File : BM022625.D
 Acq On : 10 Sep 2019 18:21
 Operator : HP/JU
 Sample : K4708-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB5Q0

Quant Time: Sep 10 19:00:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP.BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 9/11/2019 8:21:30 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	16317	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	69076	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	37864	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	85362m)	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	68233m)	0.40	ng/ul	0.00
20) Perylene-d12	23.67	264	53244m)	0.40	ng/ul	0.00

System Monitoring Compounds
 4) 2-Methylnaphthalene-d10
 14) Fluoranthene-d10

4) 2-Methylnaphthalene-d10	12.23	152	30453	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	77534m)	0.33	ng/ul	0.00

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.69	128	5391	0.027	ng/ul#	92
5) 2-Methylnaphthalene	12.31	142	2845	0.021	ng/ul	98
12) Phenanthrene	17.25	178	19988	0.073	ng/ul	96
15) Fluoranthene	19.27	202	48323m)	0.165	ng/ul	
17) Pyrene	19.63	202	43629m)	0.141	ng/ul	
18) Benzo(a)anthracene	21.37	228	21150m)	0.081	ng/ul	
19) Chrysene	21.42	228	26770	0.097	ng/ul	96
21) Benzo(b)fluoranthene	22.99	252	33333m)	0.144	ng/ul	
22) Benzo(k)fluoranthene	23.03	252	12816m)	0.054	ng/ul	
23) Benzo(a)pyrene	23.58	252	18771	0.093	ng/ul#	33
24) Indeno(1,2,3-cd)pyrene	25.99	276	13975	0.057	ng/ul#	81
26) Benzo(g,h,i)perylene	26.69	276	11890	0.060	ng/ul#	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed