


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
Data File : BM022655.D
Acq On : 11 Sep 2019 13:52
Operator : HP/JU
Sample : K4706-07
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:48:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 15:06:45 2019
Response via : Initial Calibration

Instrument :
BNA_M
Client Sample ID :
BF573

Manual Integrations
APPROVED

mohammad
9/16/2019 8:54:54 AM

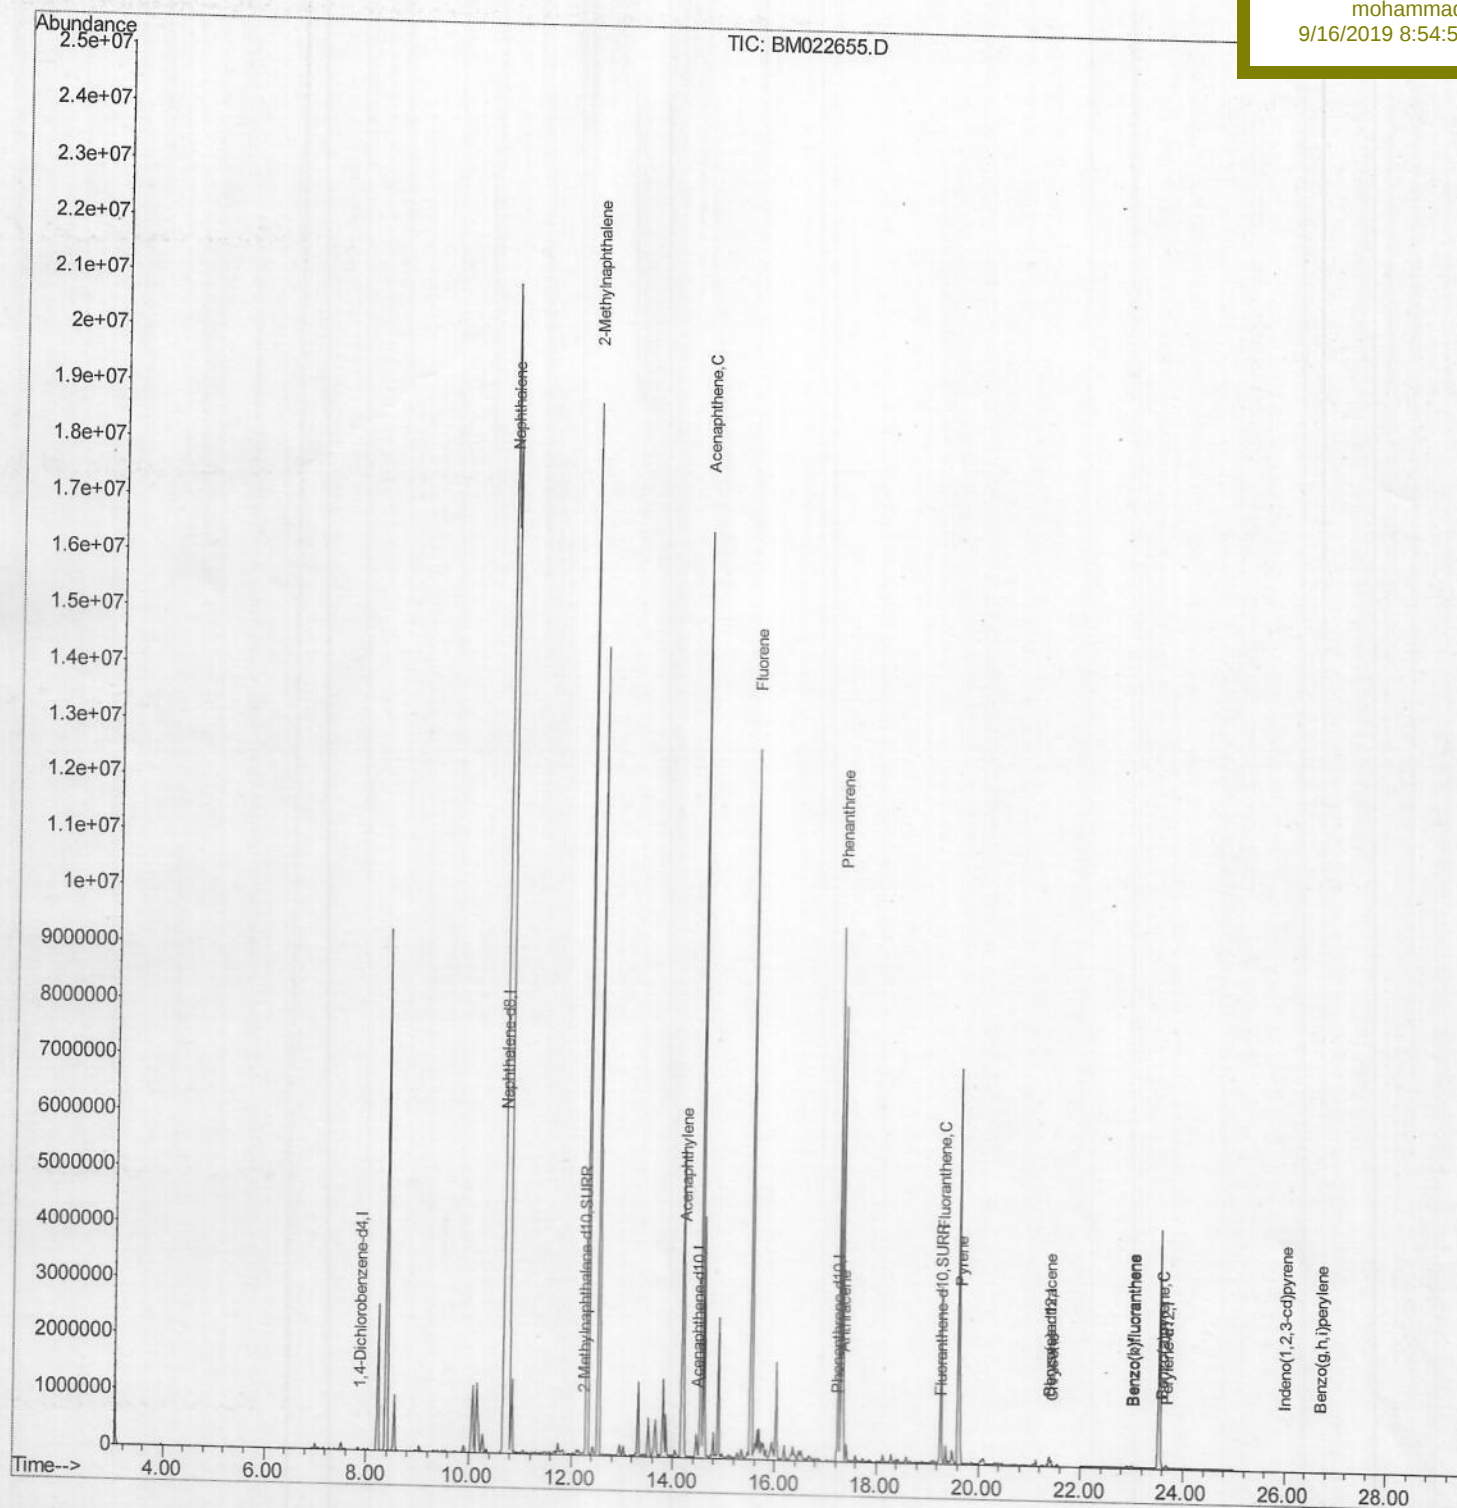

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:44:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BF573

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:54 AM

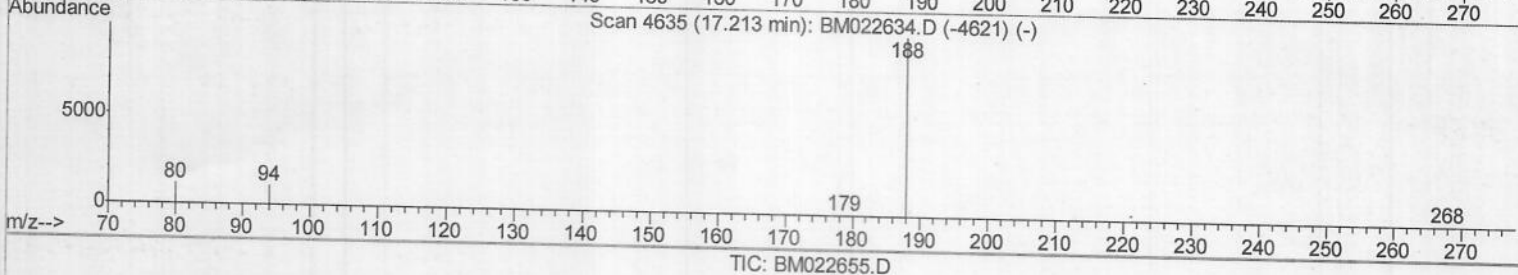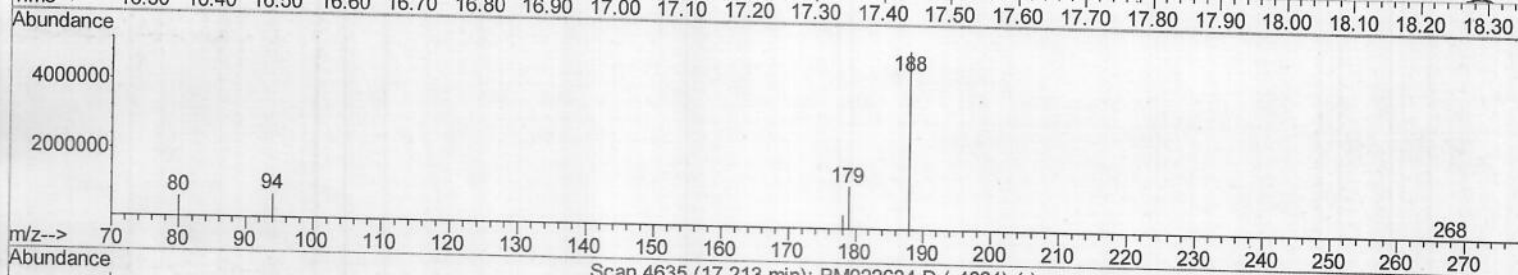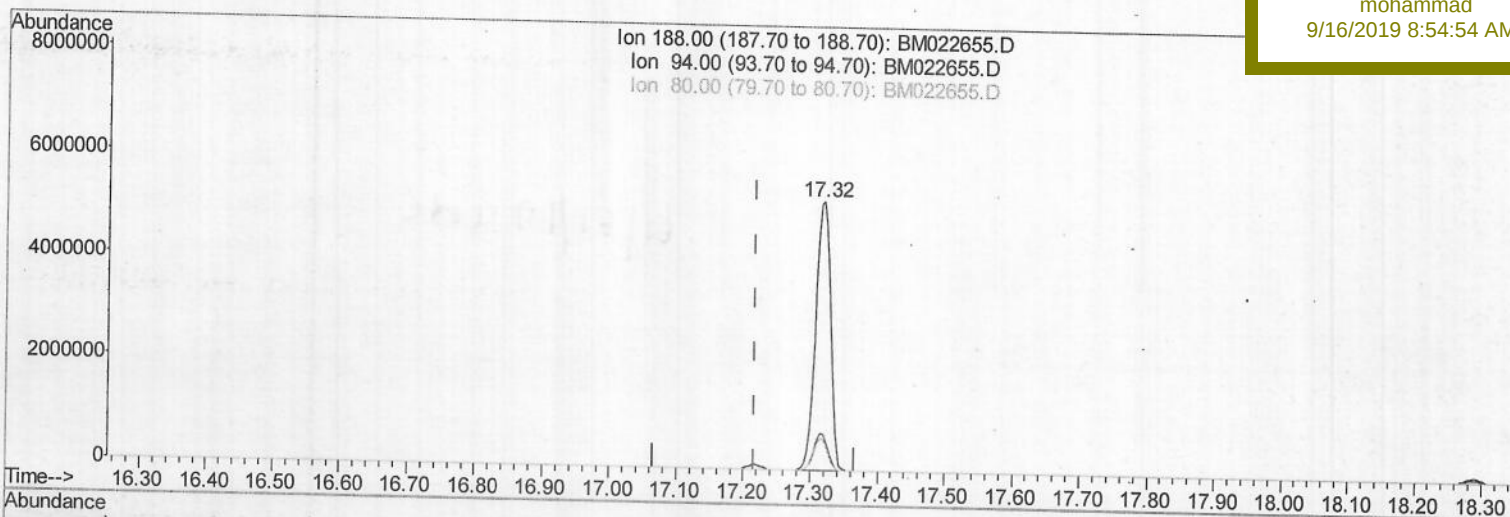

(10) Phenanthrene-d10 (I)
 17.319min (+0.102) 0.40ng/ul
 response 7884279

Ion	Exp%	Act%
188.00	100	100
94.00	9.80	13.02#
80.00	11.00	11.37
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BF573

Manual Integrations
APPROVED

mohammad
 9/16/2019 8:54:54 AM

Quant Time: Sep 11 15:44:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

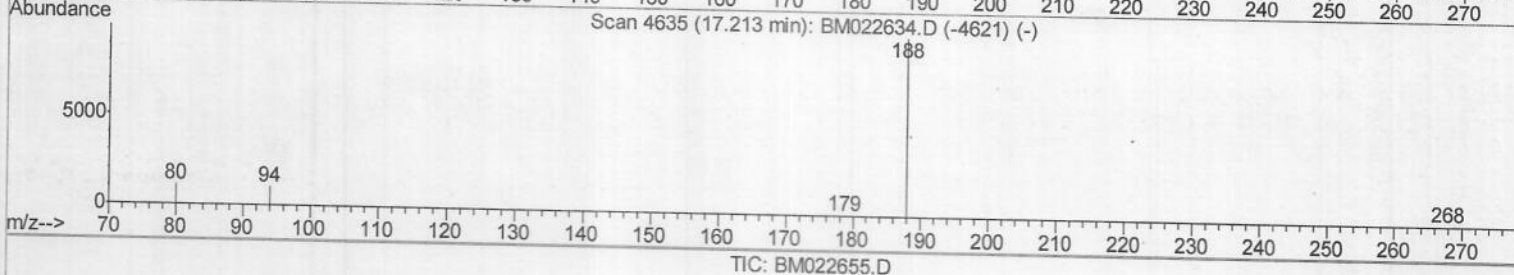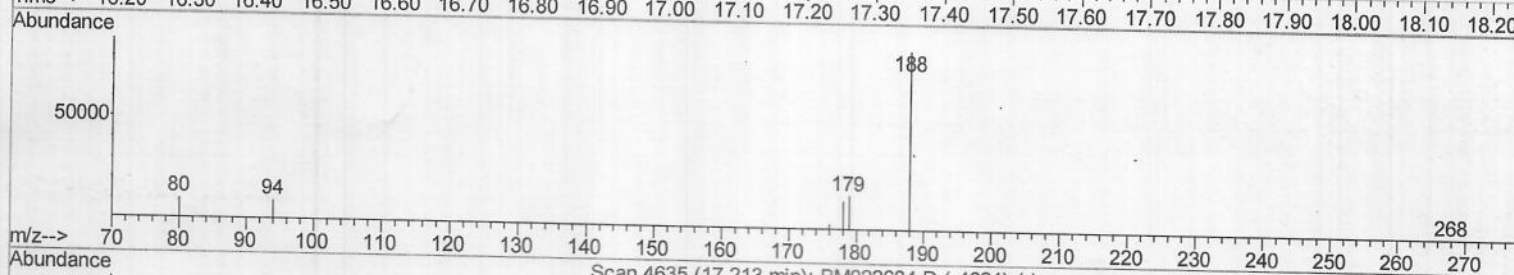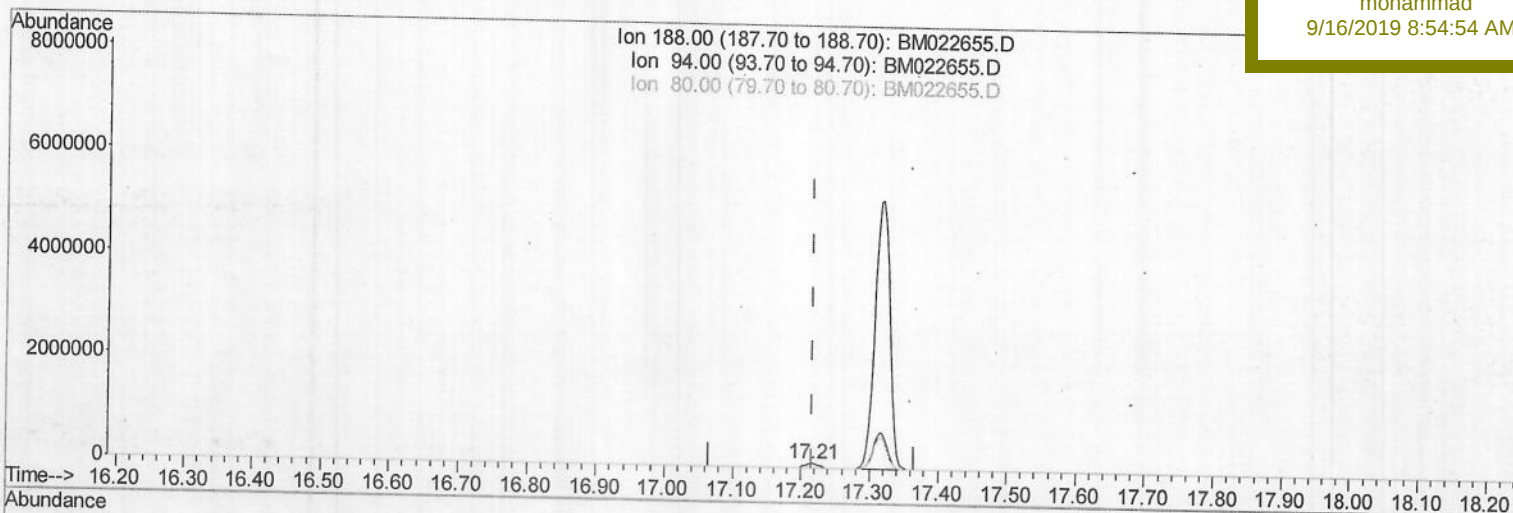

(10) Phenanthrene-d10 (I)

17.215min (-0.002) 0.40ng/ul.m > JU 09/14/19

response 126480

Ion	Exp%	Act%
188.00	100	100
94.00	9.80	10.64
80.00	11.00	11.08
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:44:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BF573

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:54 AM

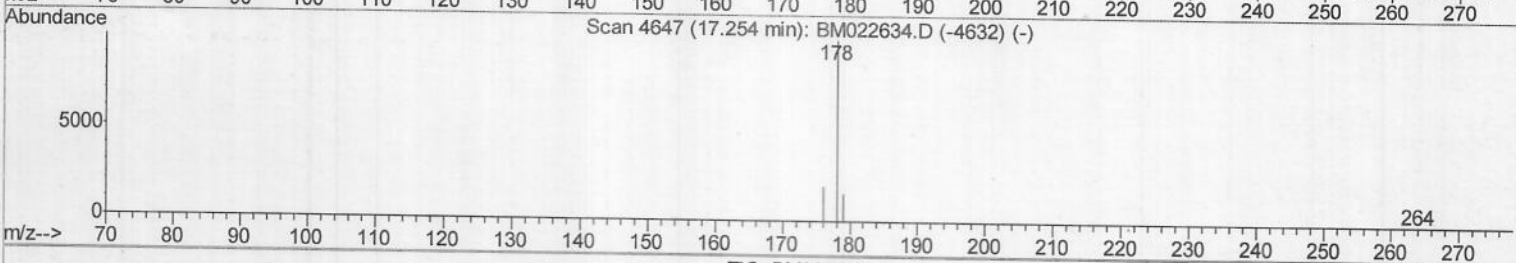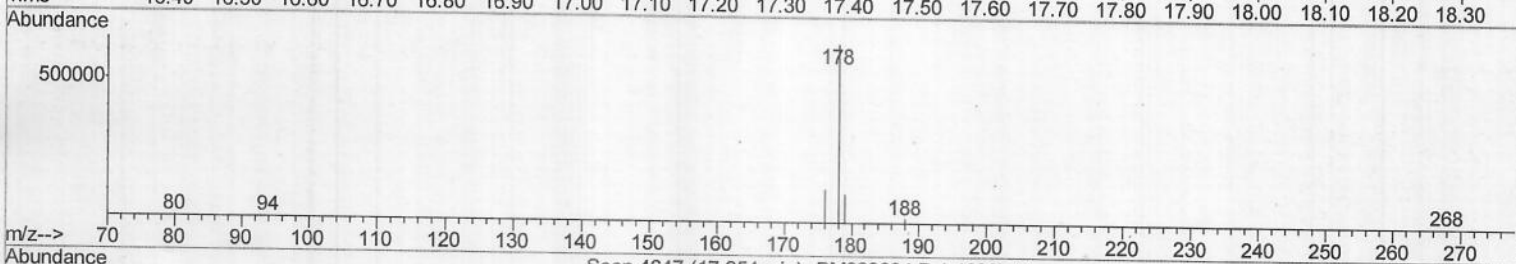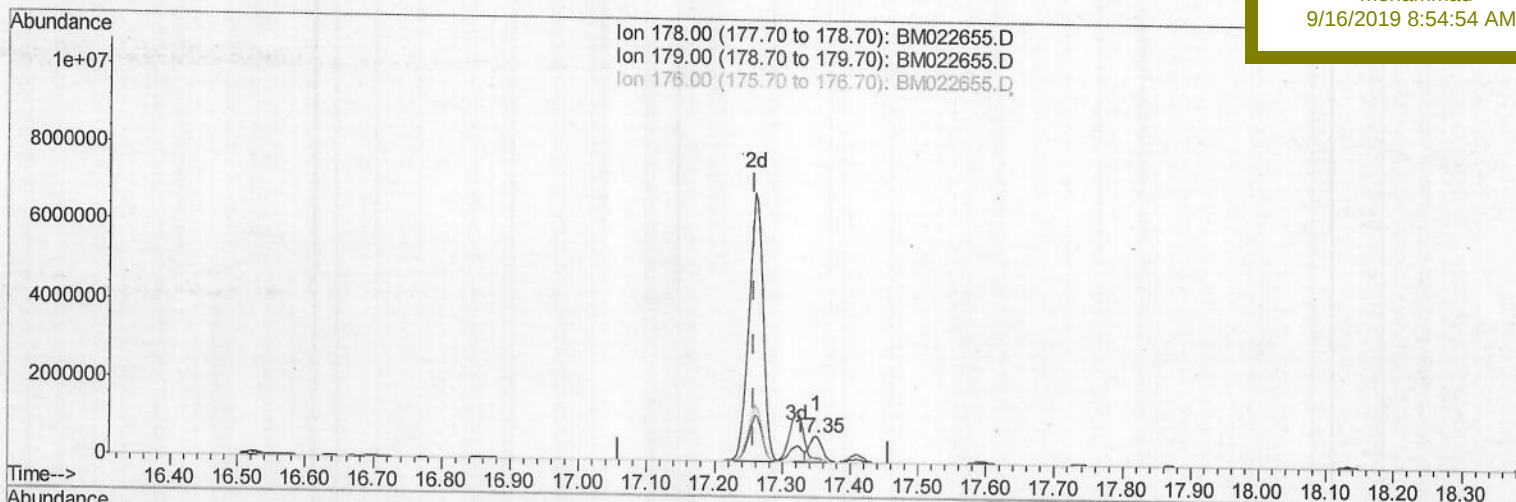

TIC: BM022655.D

(12) Phenanthrene

17.350min (+0.092) 2.06ng/ul

response 828944

Ion	Exp%	Act%
178.00	100	100
179.00	15.50	16.52
176.00	19.10	18.95
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:44:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BF573

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:54 AM

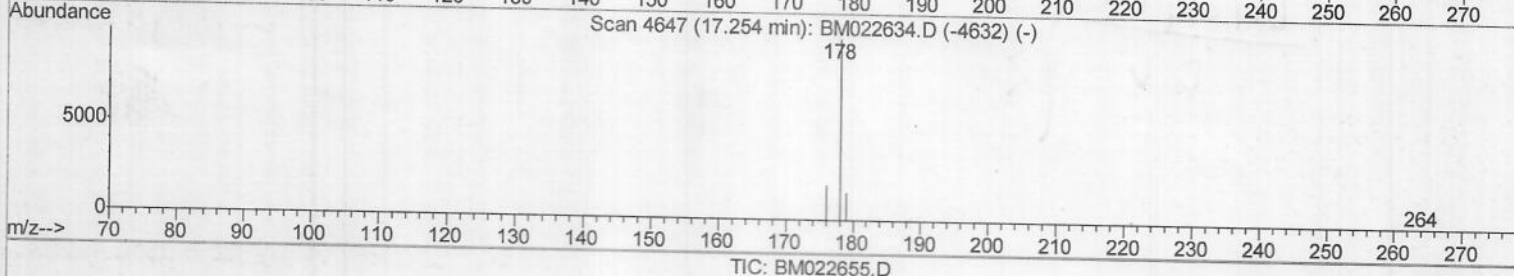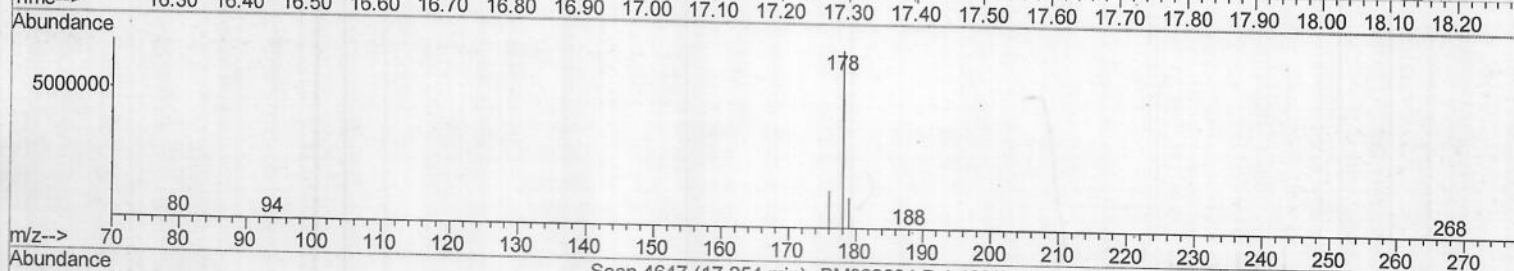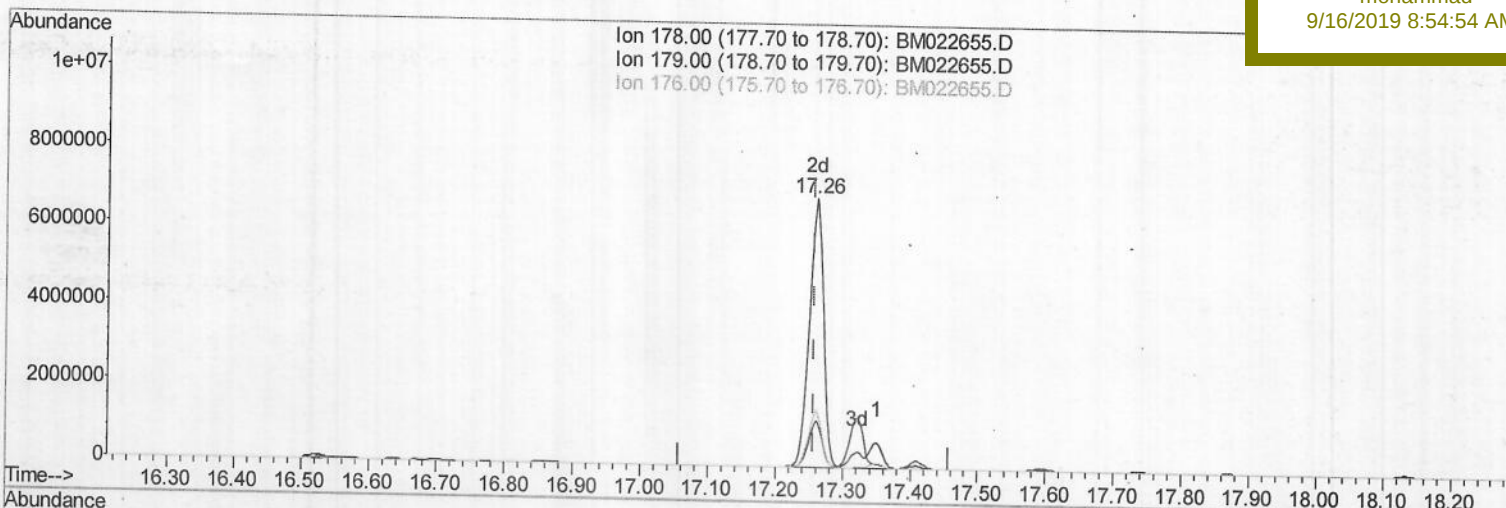

(12) Phenanthrene

17.260min (+0.002) 25.33ng/ul m > JU 09/24/29

response 10207361

Ion	Exp%	Act%
178.00	100	100
179.00	15.50	17.47
176.00	19.10	21.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\

Data File : BM022655.D

Acq On : 11 Sep 2019 13:52

Operator : HP/JU

Sample : K4706-07

Misc :

ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:44:34 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

BF573

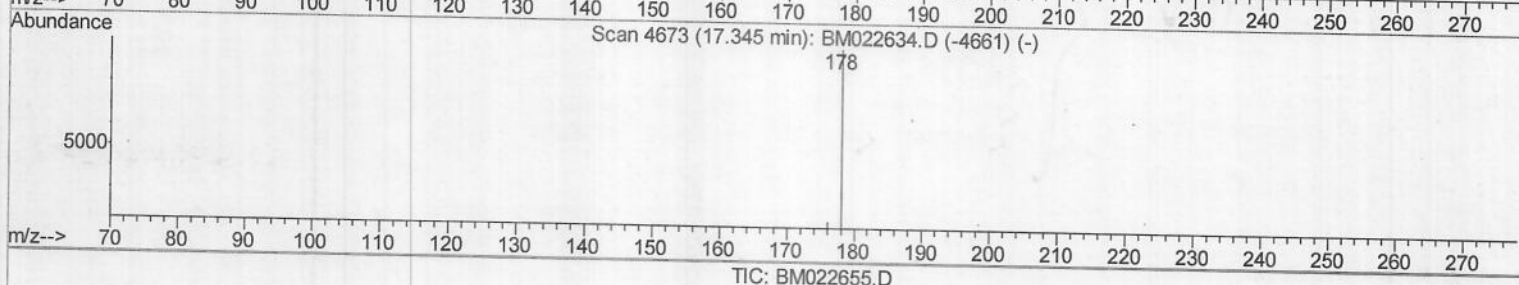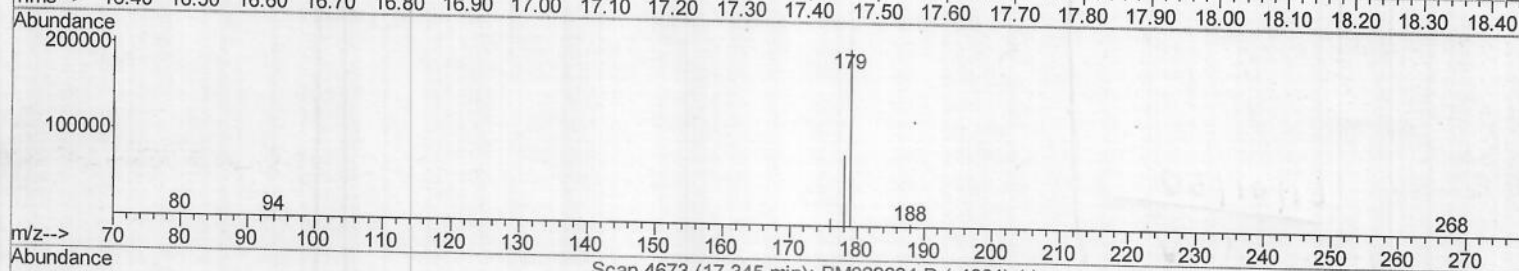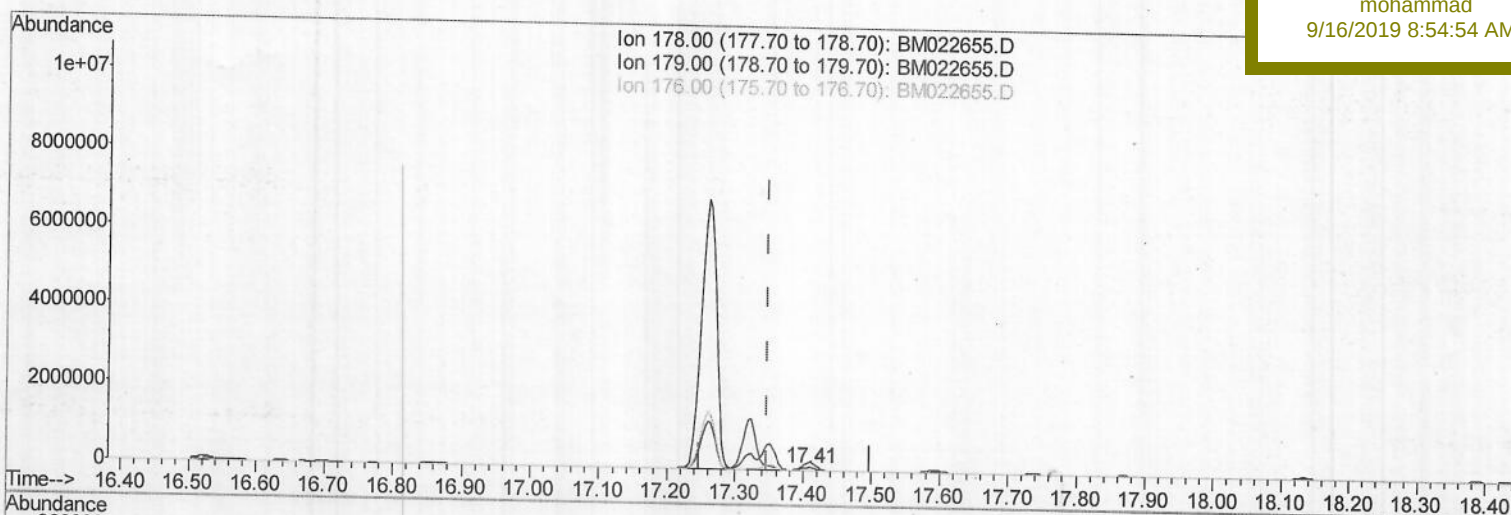Manual Integrations
APPROVEDmohammad
9/16/2019 8:54:54 AM

TIC: BM022655.D

(13) Anthracene

17.409min (+0.061) 0.33ng/ul

response 114344

Ion	Exp%	Act%
178.00	100	100
179.00	15.60	249.53#
176.00	18.50	10.20#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF573

Quant Time: Sep 11 15:44:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:54 AM

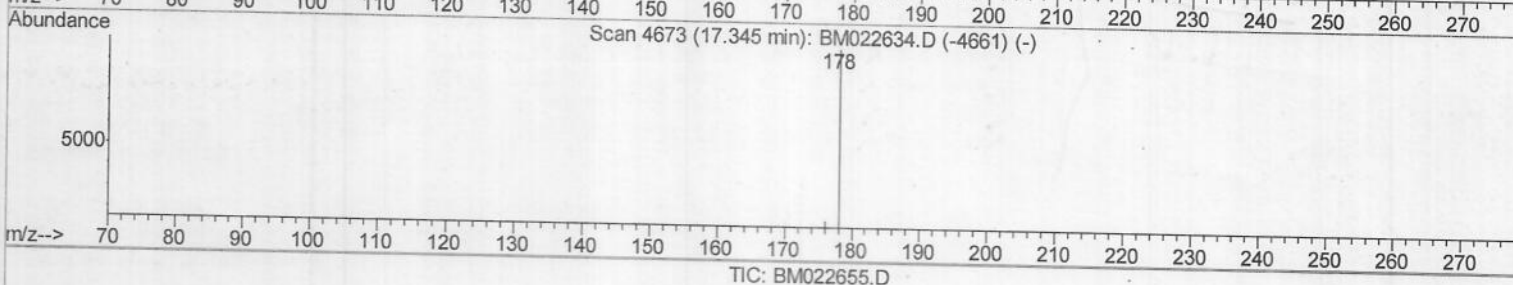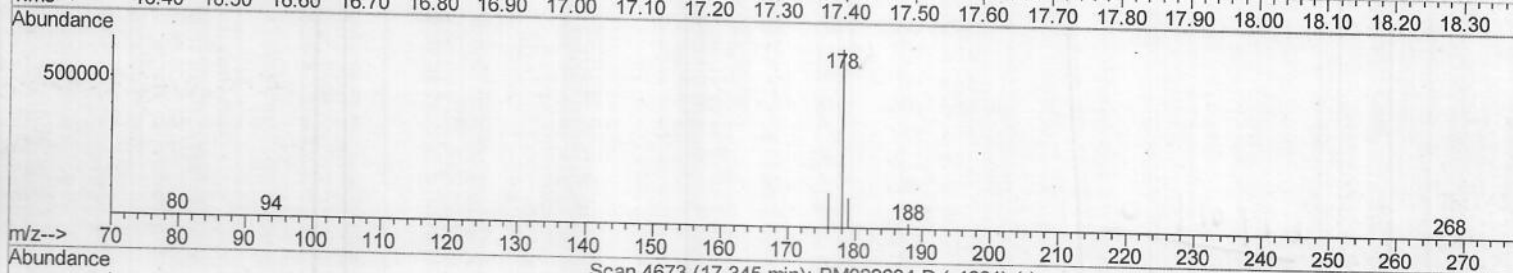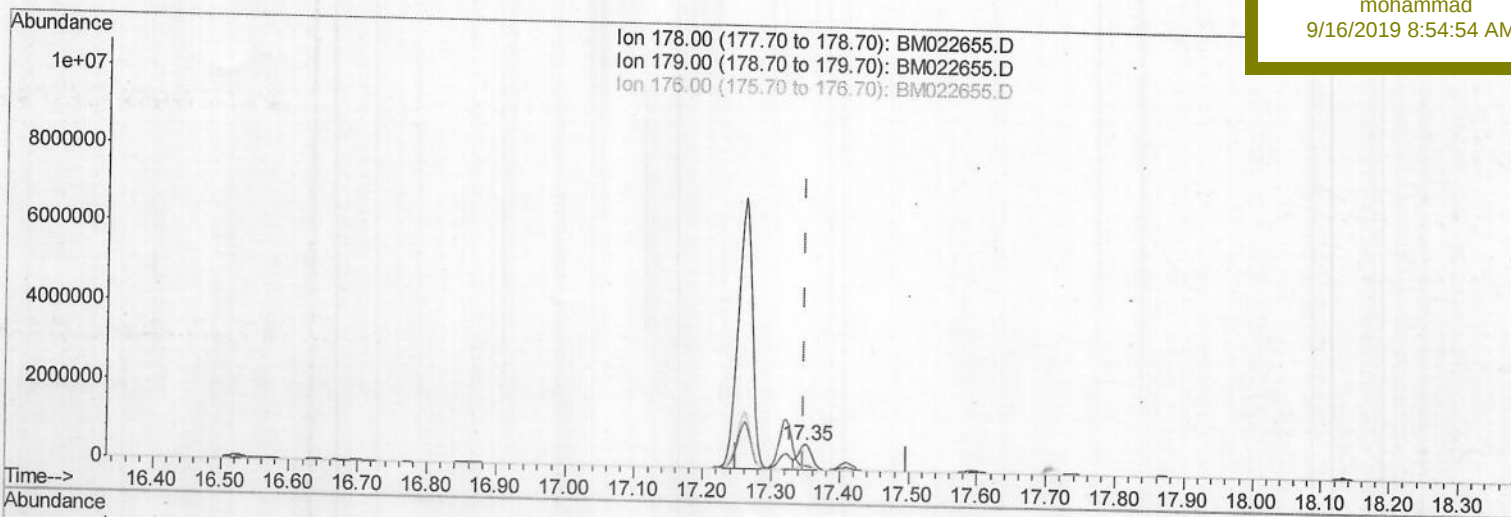

(13) Anthracene

17.350min (+0.002) 2.47ng/ul m > JU 09/14/19

response 854415

Ion	Exp%	Act%
178.00	100	100
179.00	15.60	16.52
176.00	18.50	18.95
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:44:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BF573

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:54 AM

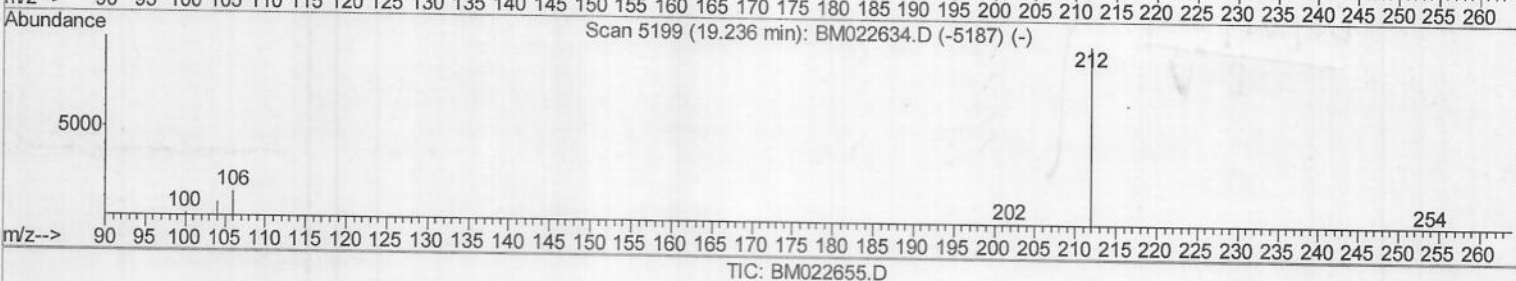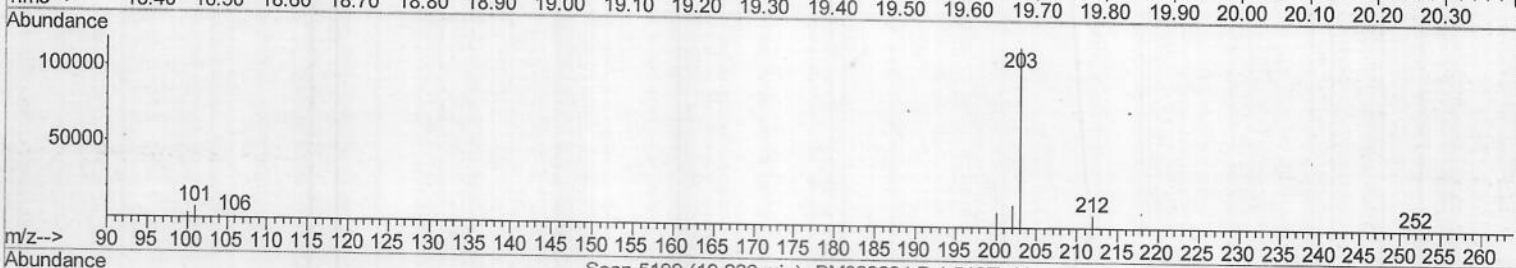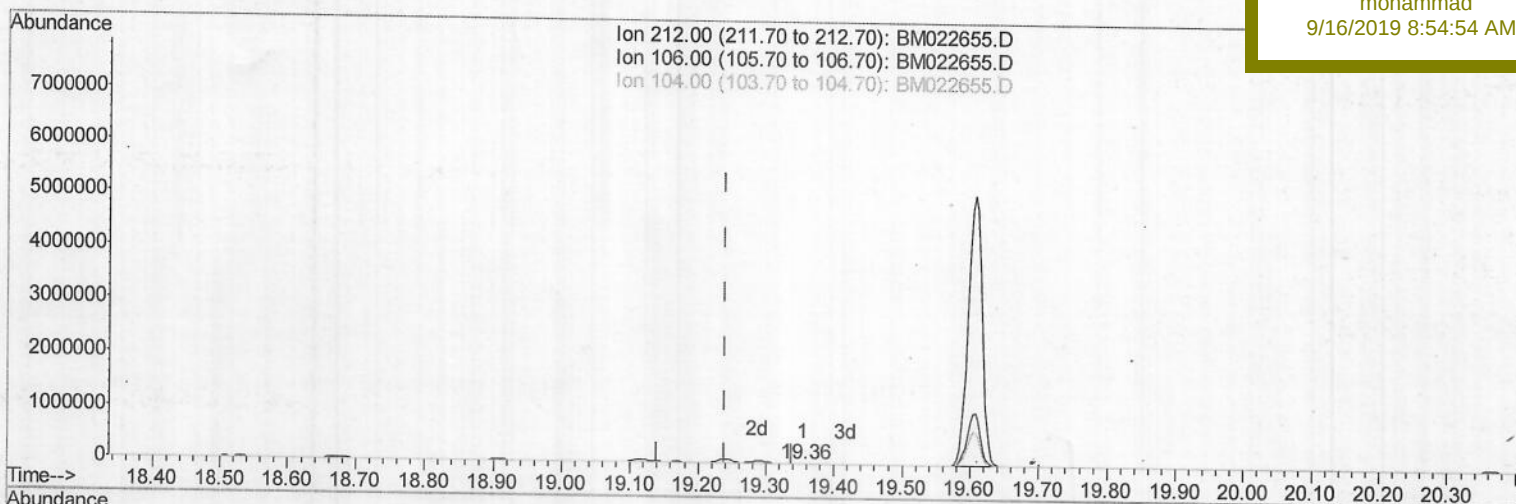

TIC: BM022655.D

(14) Fluoranthene-d10 (SURR)

19.356min (+0.116) 0.03ng/ul

response 10706

Ion	Exp%	Act%
212.00	100	100
106.00	14.00	4.54#
104.00	8.00	7.49
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\

Data File : BM022655.D

Acq On : 11 Sep 2019 13:52

Operator : HP/JU

Sample : K4706-07

Misc :

ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:44:34 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampled :




BF573

Manual Integrations

APPROVED

mohammad

9/16/2019 8:54:54 AM

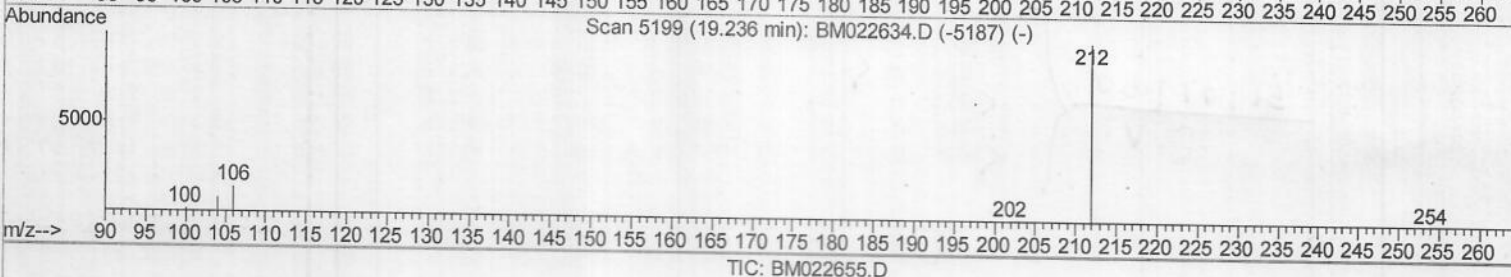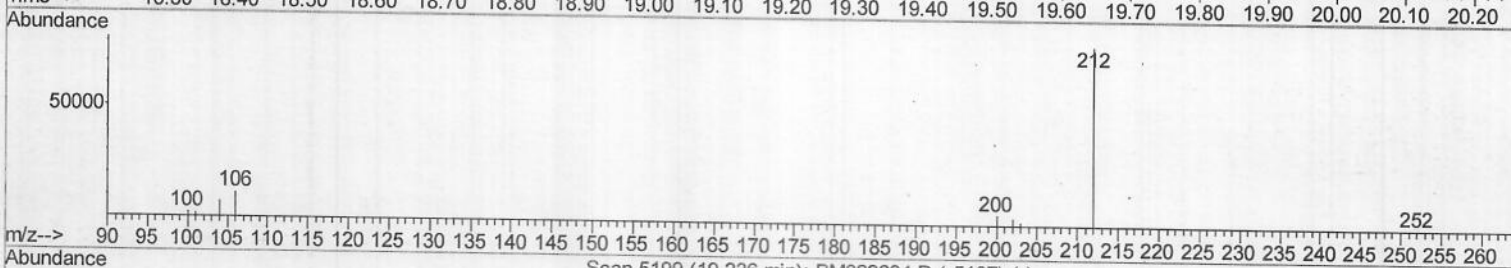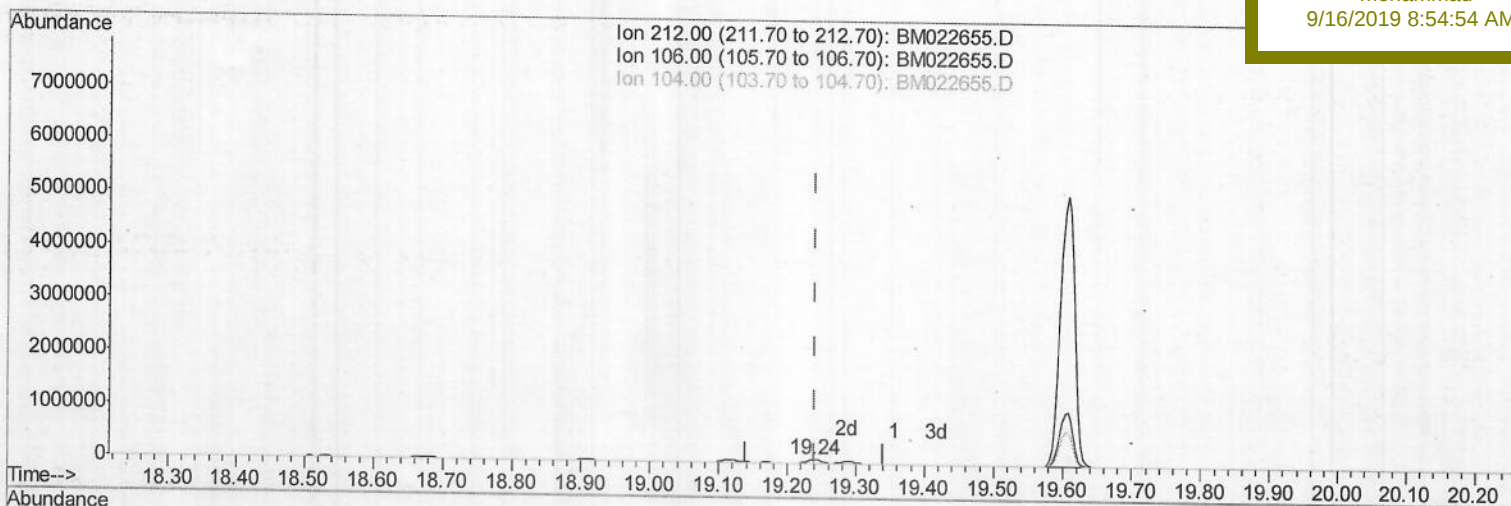

(14) Fluoranthene-d10 (SURR)

19.238min (-0.002) 0.32ng/ul m² JU 09/24/19

response 111603

Ion	Exp%	Act%
212.00	100	100
106.00	14.00	0.44#
104.00	8.00	0.72#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:44:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BF573

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:54 AM

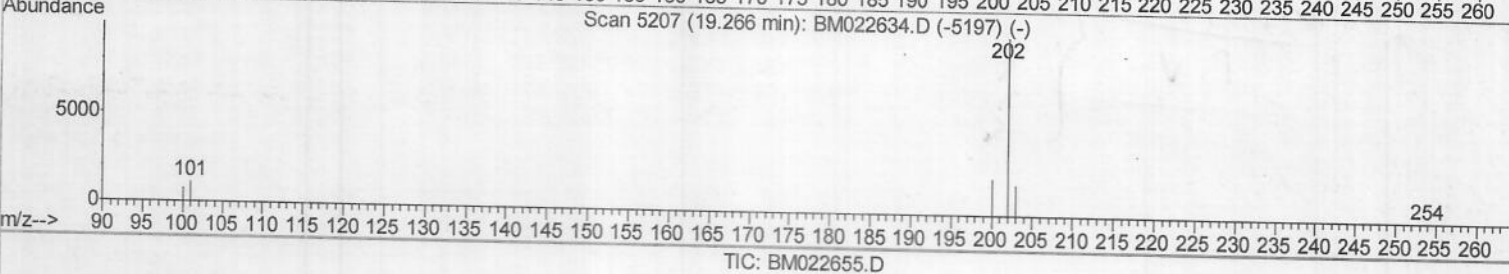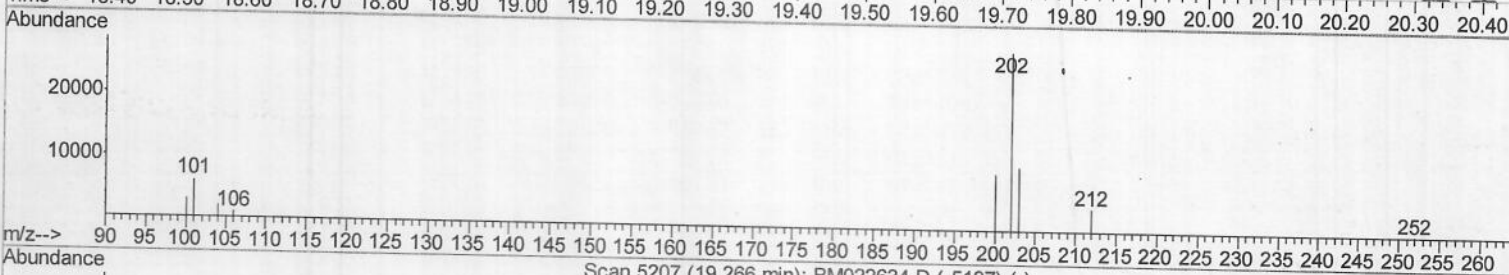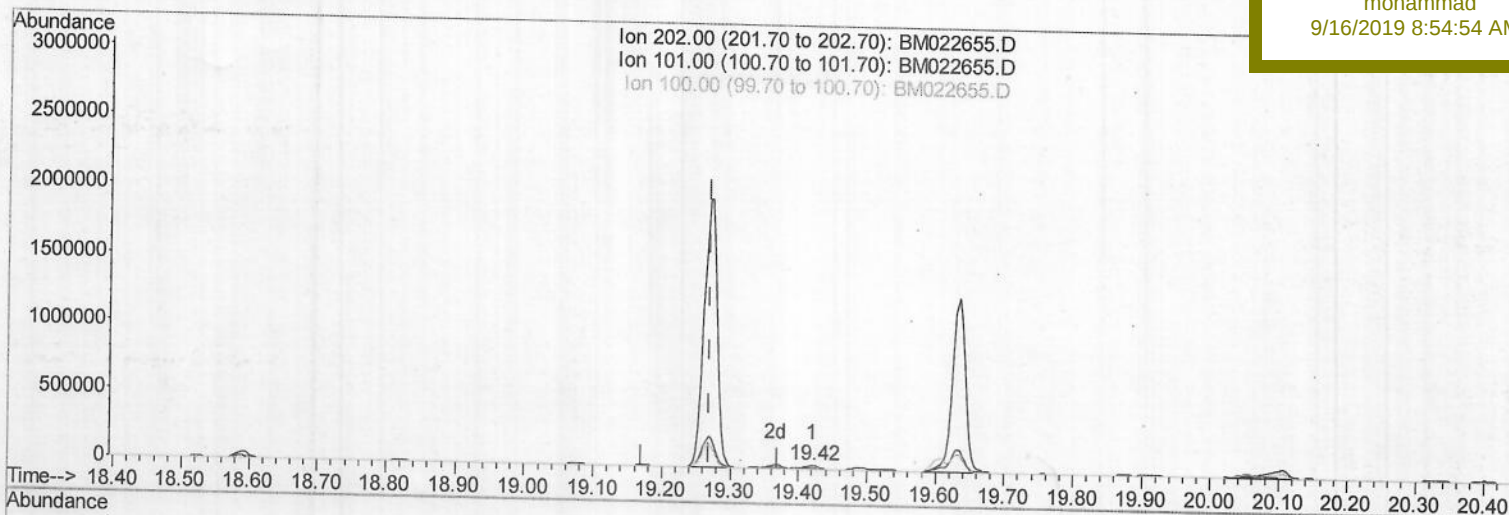

(15) Fluoranthene (C)

19.421min (+0.150) 0.08ng/ul

response 32998

Ion	Exp%	Act%
202.00	100	100
101.00	10.50	21.69
100.00	8.00	11.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\

Data File : BM022655.D

Acq On : 11 Sep 2019 13:52

Operator : HP/JU

Sample : K4706-07

Misc :

ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:44:34 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




BF573

Manual Integrations

APPROVED

mohammad

9/16/2019 8:54:54 AM

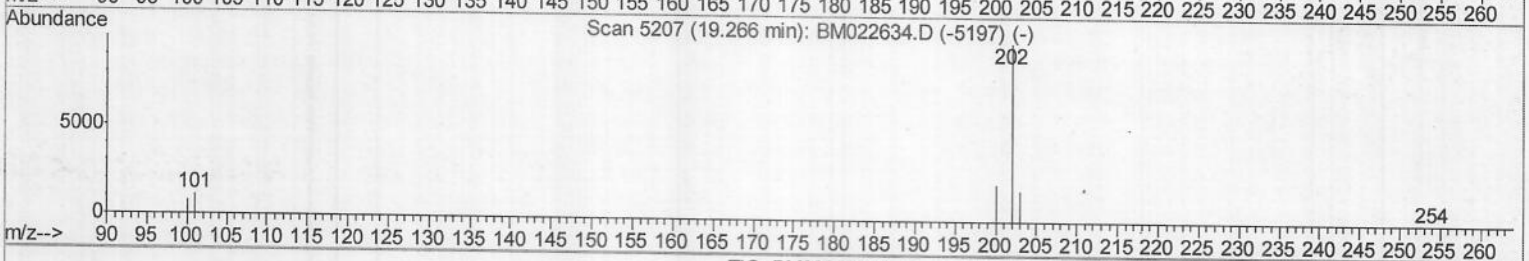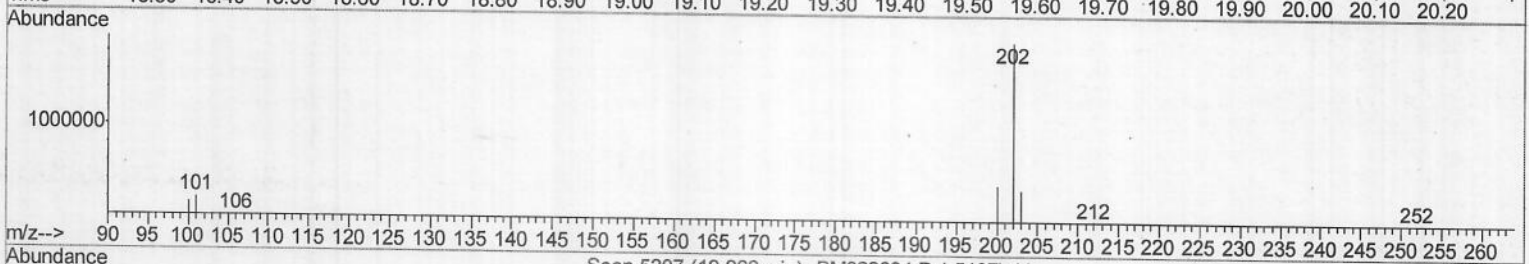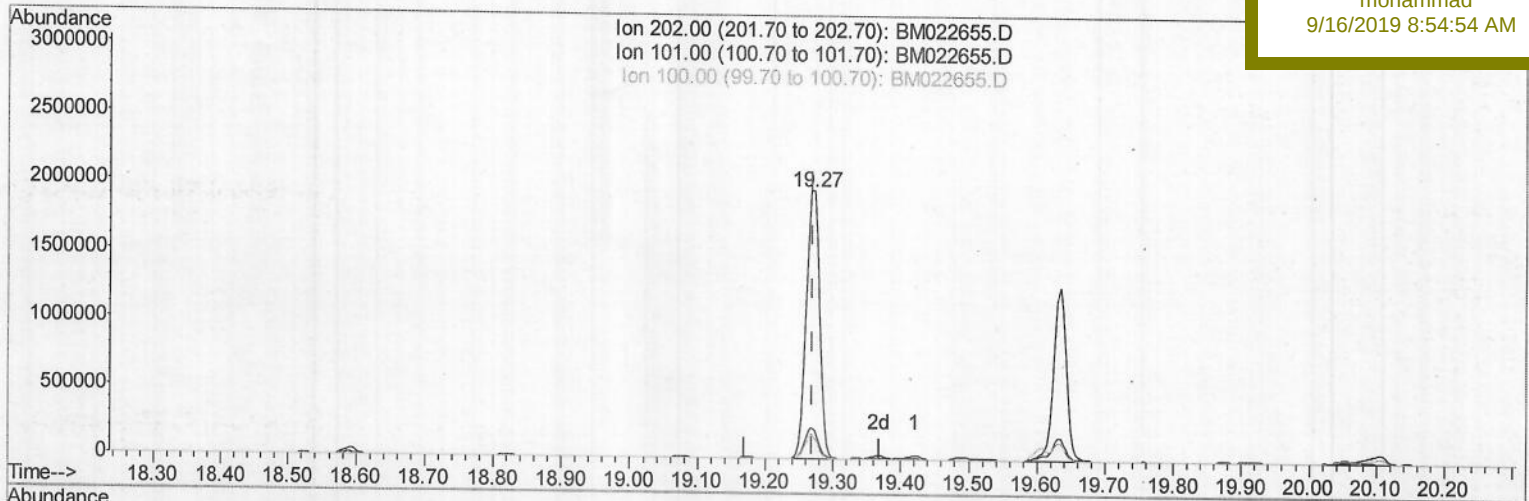

TIC: BM022655.D

(15) Fluoranthene (C)

19.272min (+0.002) 6.00ng/ul m > JU 09/14/19

response 2608788

Ion	Exp%	Act%
202.00	100	100
101.00	10.50	10.45
100.00	8.00	7.68
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:44:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BF573

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:54 AM

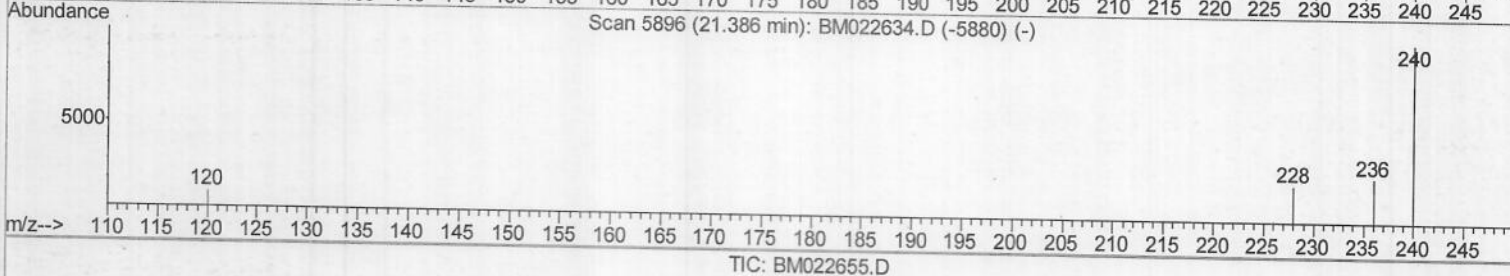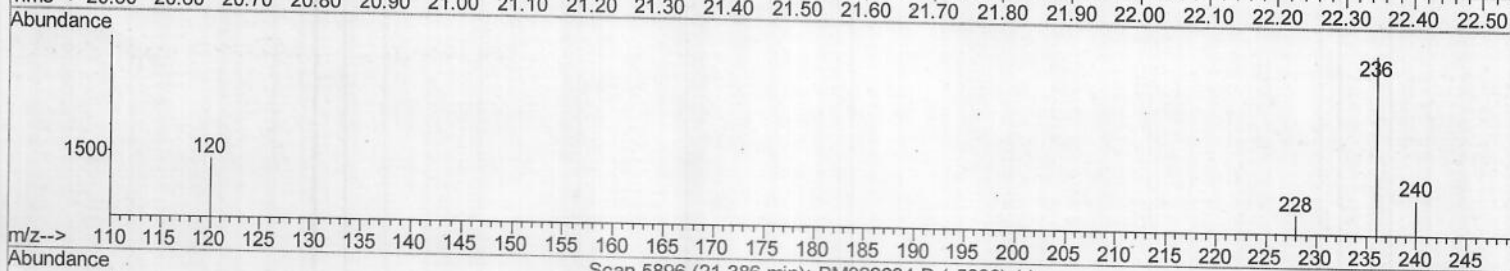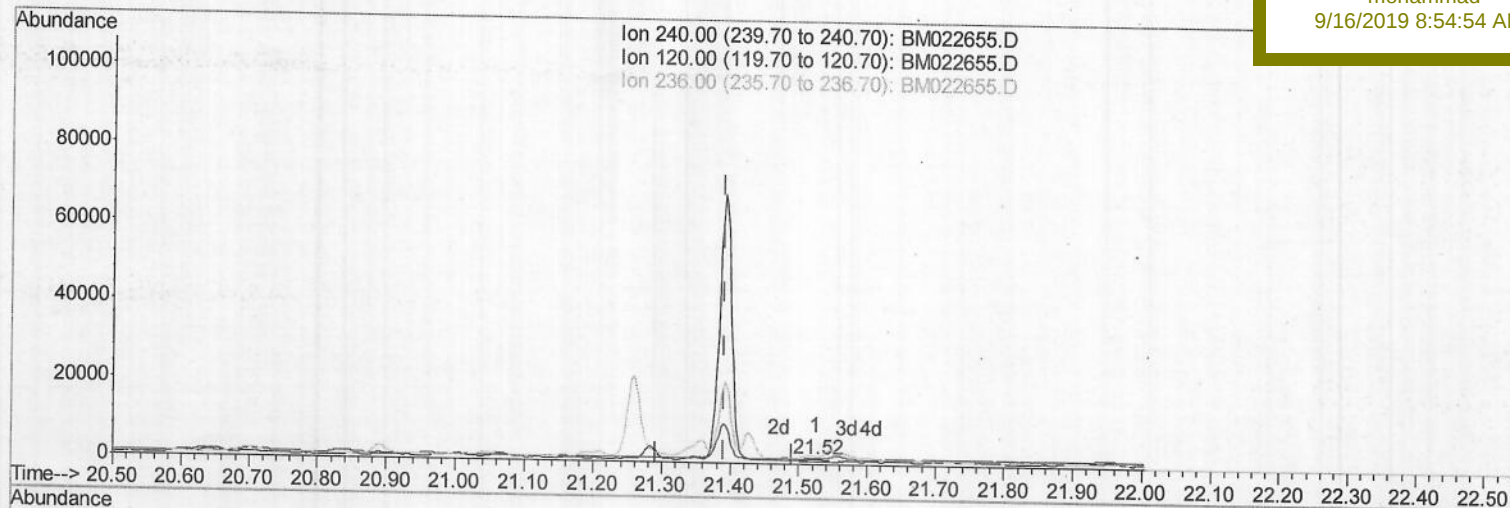

(16) Chrysene-d12 (I)
 21.525min (+0.133) 0.40ng/ul
 response 963

Ion	Exp%	Act%
240.00	100	100
120.00	14.60	106.19#
236.00	28.80	139.09#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:44:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BF573

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:54 AM

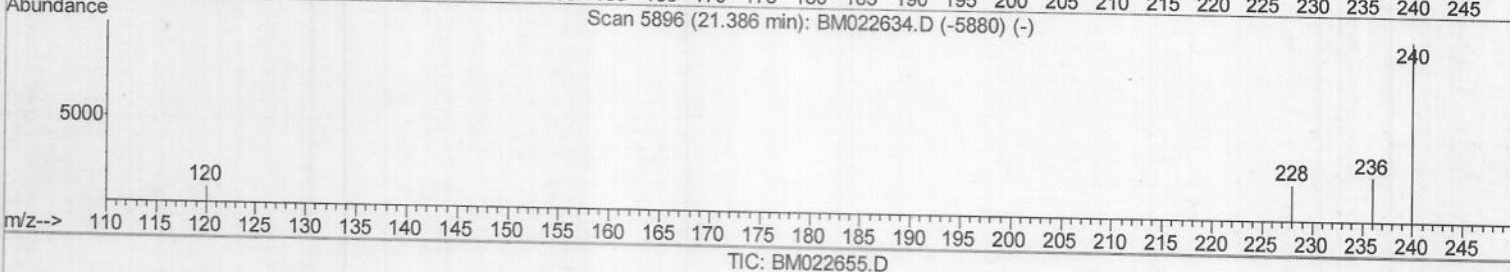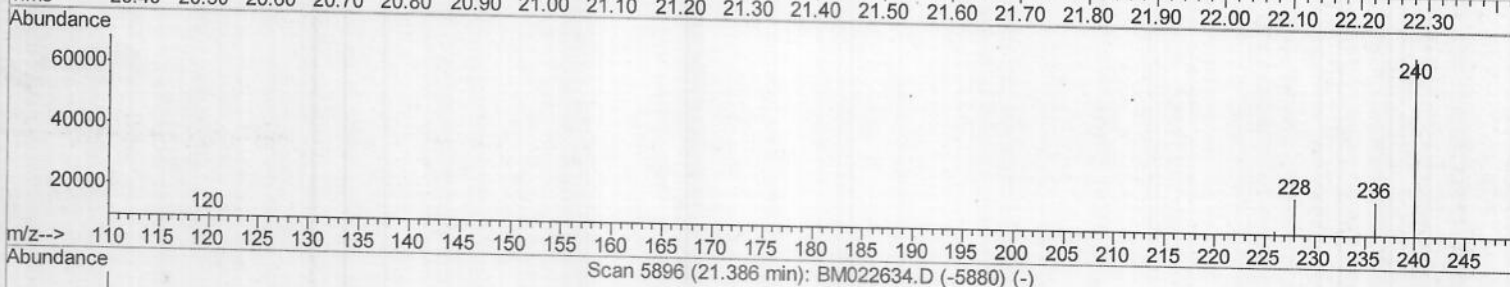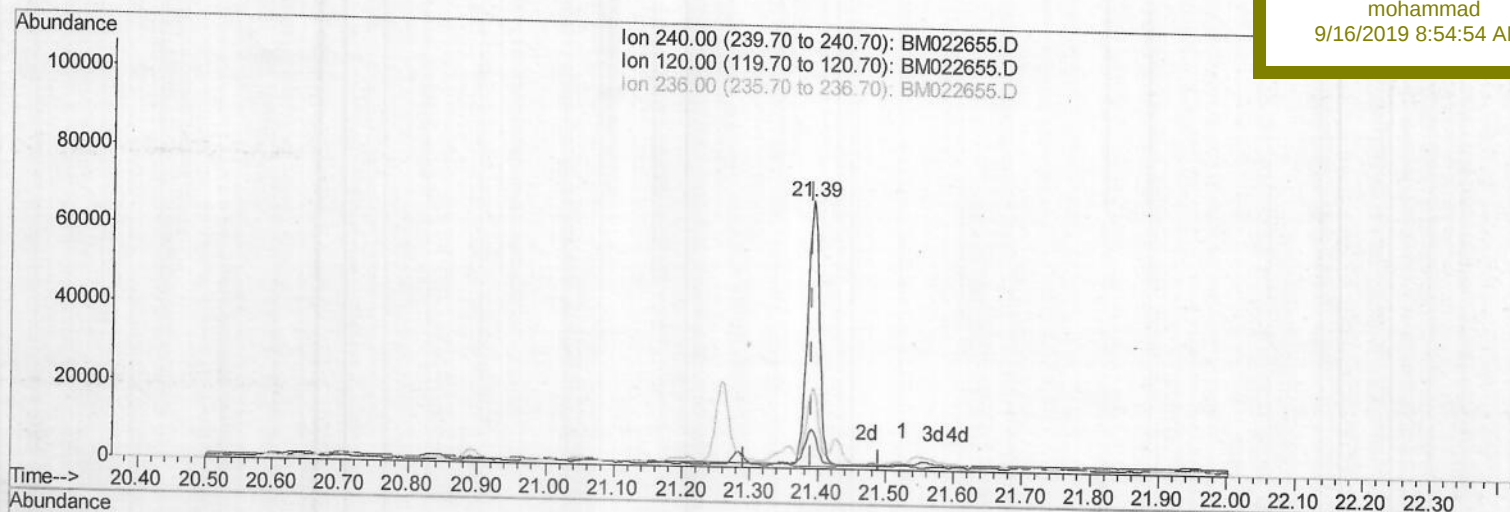

(16) Chrysene-d12 (I)

21.391min (+0.000) 0.40ng/ul m > JU 09/14/19

response 84020

Ion	Exp%	Act%
240.00	100	100
120.00	14.60	14.32
236.00	28.80	29.85
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:46:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BF573

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:54 AM

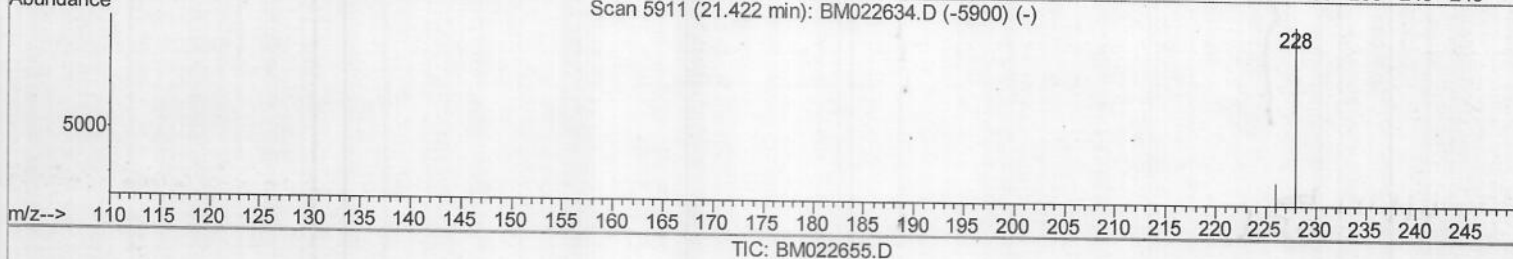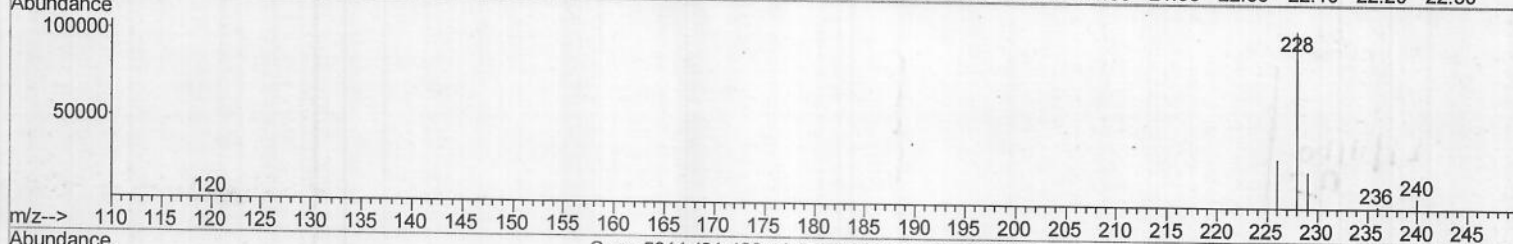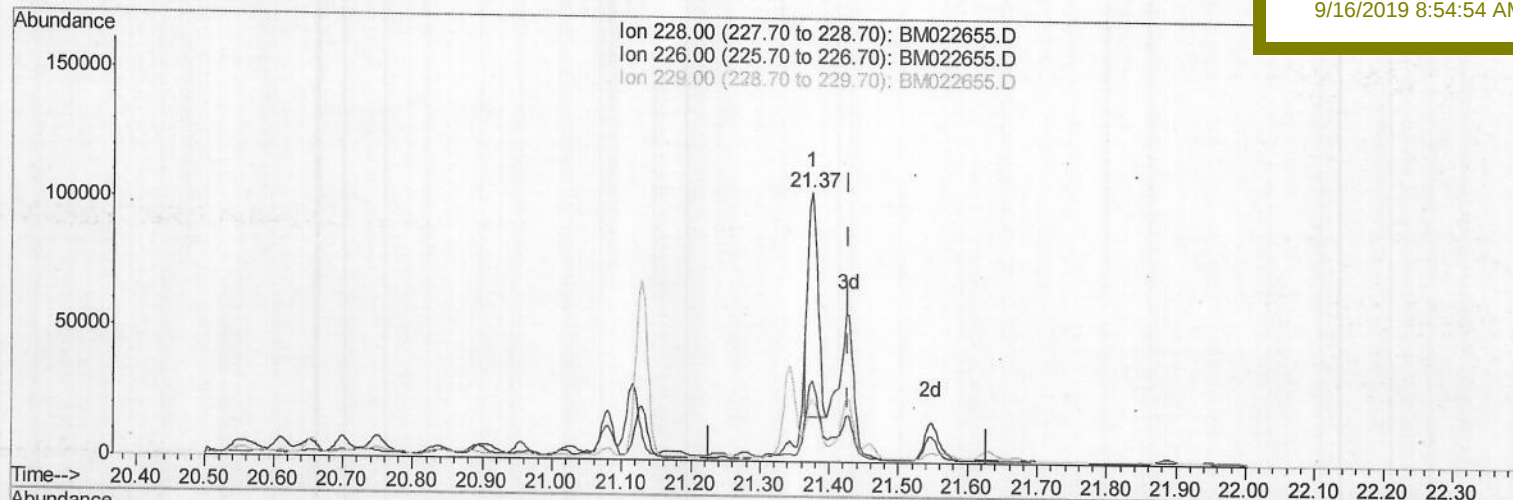

TIC: BM022655.D

(19) Chrysene

21.375min (-0.053) 0.25ng/ul

response 85048

Ion	Exp%	Act%
228.00	100	100
226.00	29.80	29.44
229.00	19.40	22.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
Data File : BM022655.D
Acq On : 11 Sep 2019 13:52
Operator : HP/JU
Sample : K4706-07
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:46:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 15:06:45 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BF573

Manual Integrations
APPROVED

mohammad
9/16/2019 8:54:54 AM

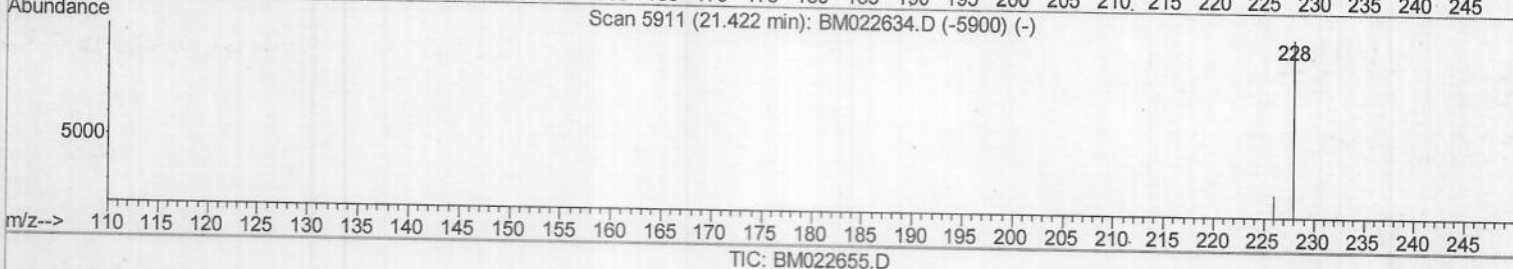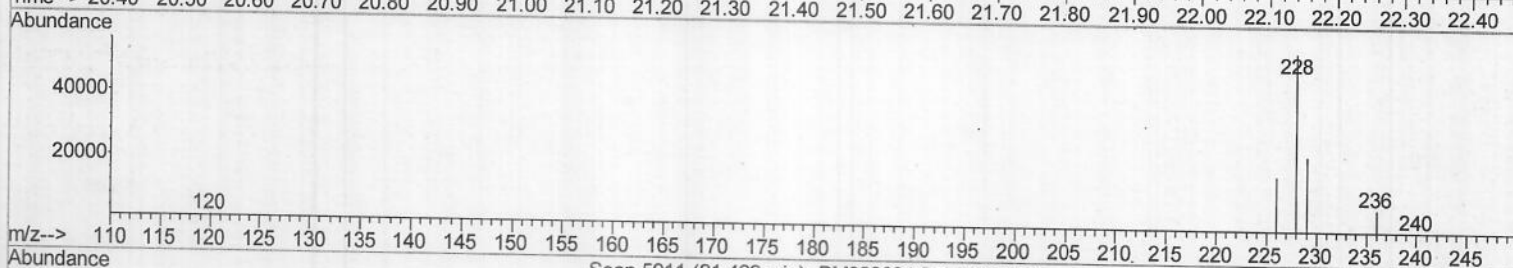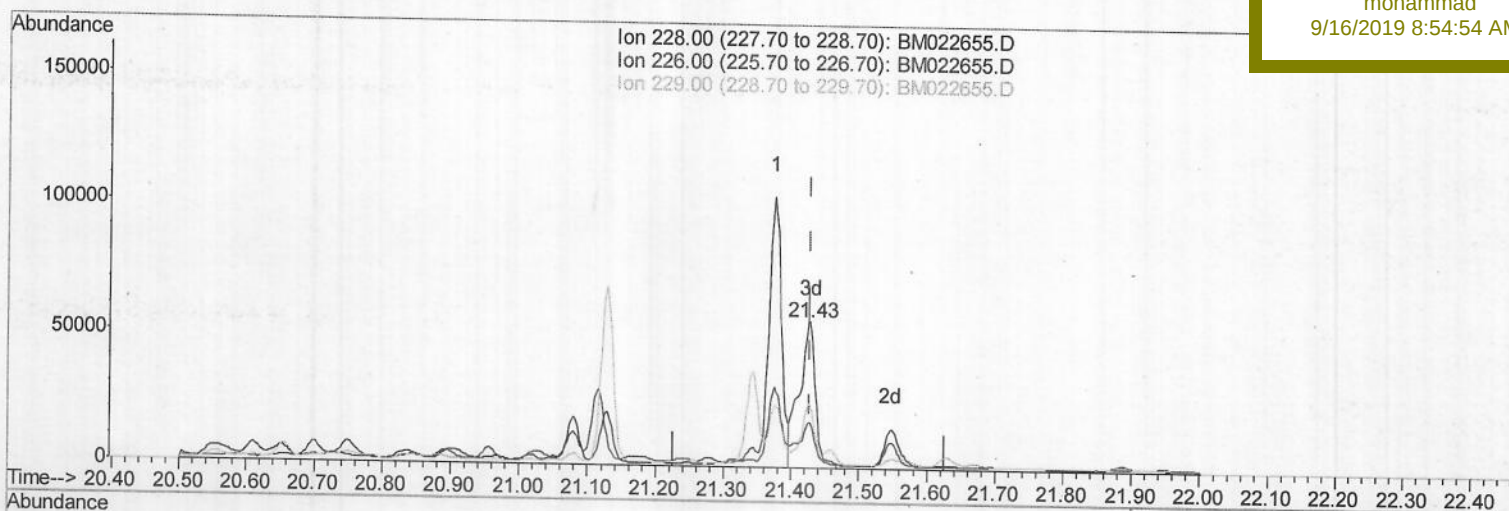

(19) Chrysene

21.428min (+0.000) 0.28ng/ul m > JU 09/14/19

response 94645

Ion	Exp%	Act%
228.00	100	100
226.00	29.80	31.28
229.00	19.40	42.73#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:46:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BF573

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:54 AM

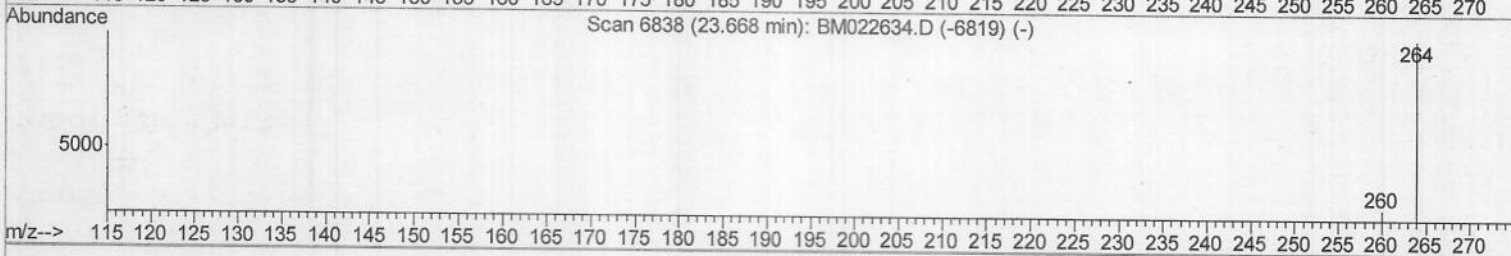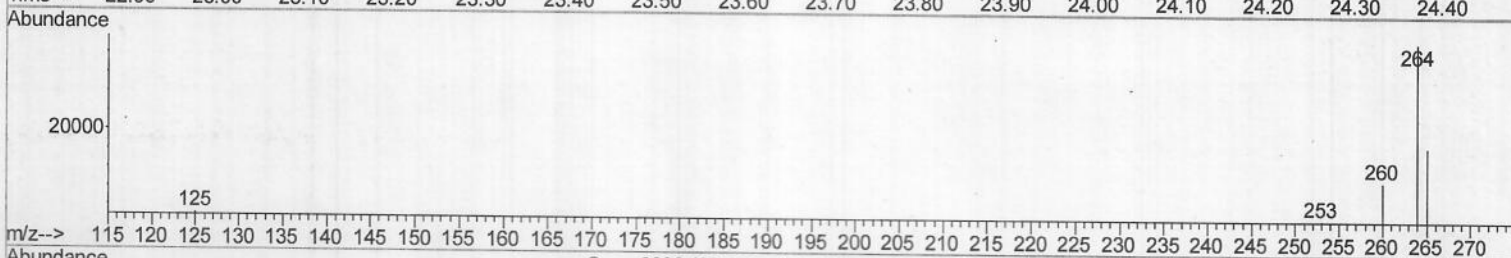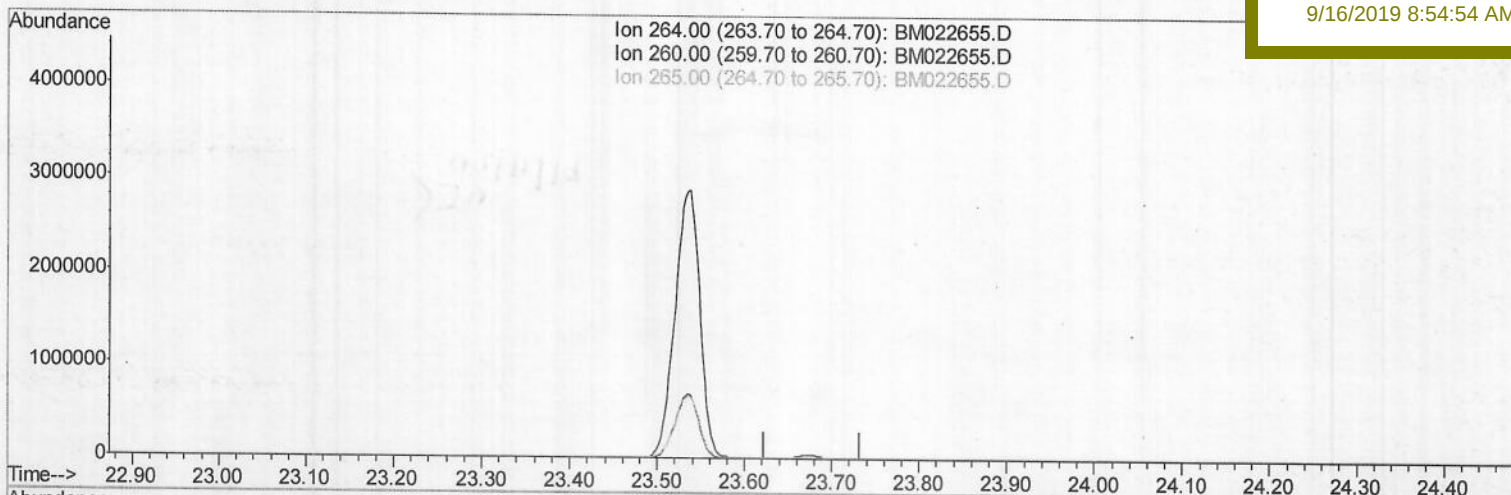

(20) Perylene-d12 (I)

23.673min (-23.673) 0.00ng/ul

response 0

Ion	Exp%	Act%
264.00	100	0.00
260.00	25.60	0.00#
265.00	59.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:46:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BF573

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:54 AM

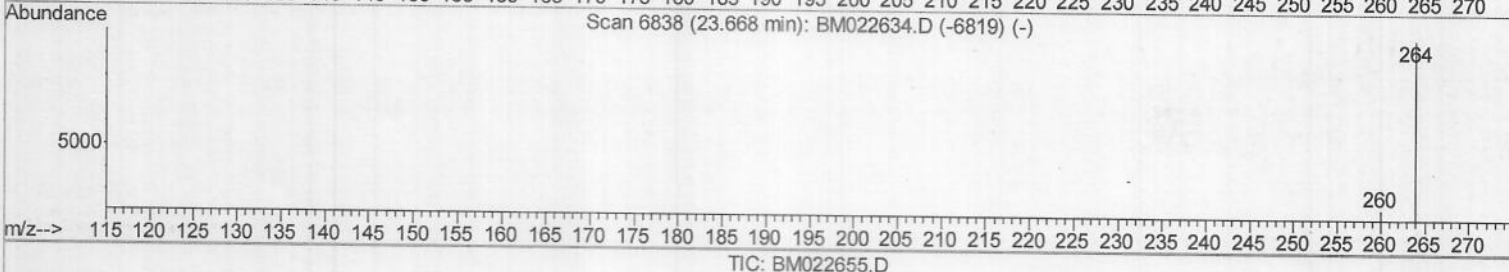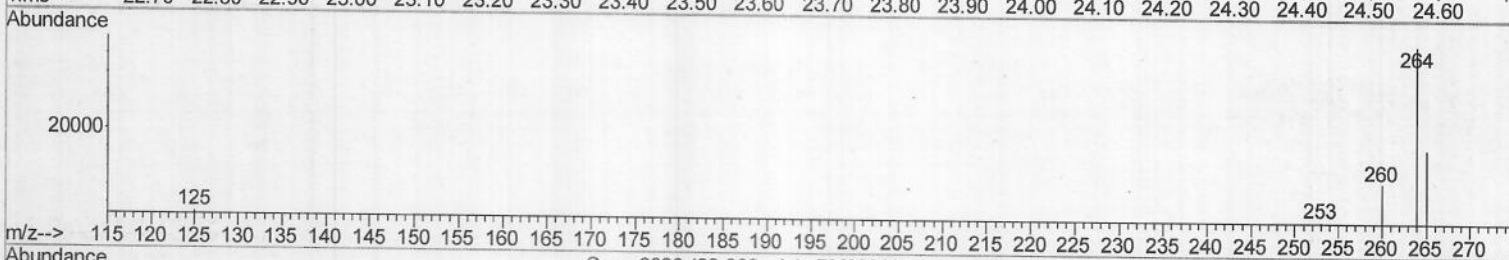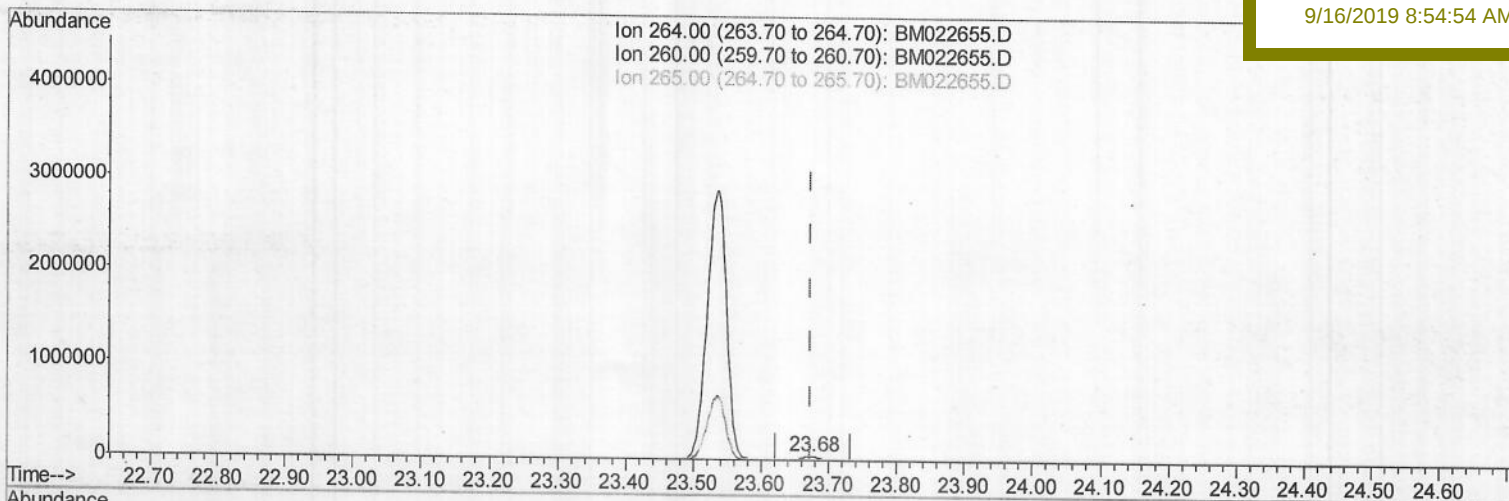

(20) Perylene-d12 (I)

23.675min (+0.003) 0.40ng/ul m > JU 09/14/19

response 67047

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	25.72
265.00	59.90	44.60#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BF573

Quant Time: Sep 11 15:47:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
 9/16/2019 8:54:54 AM

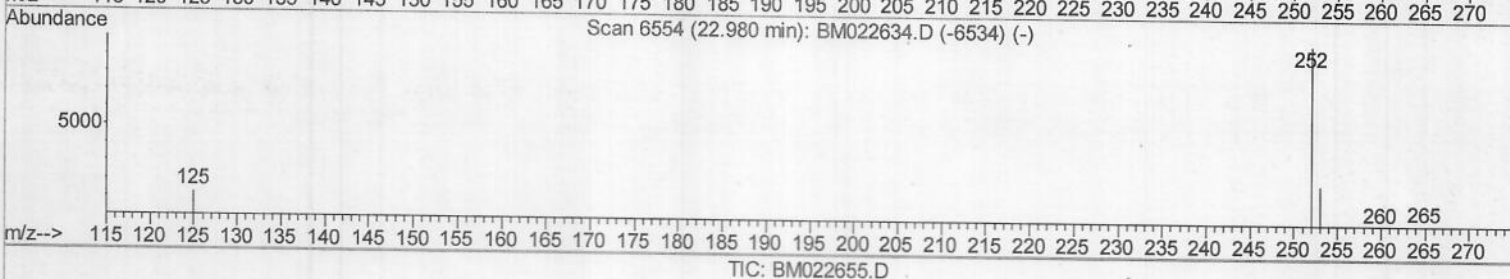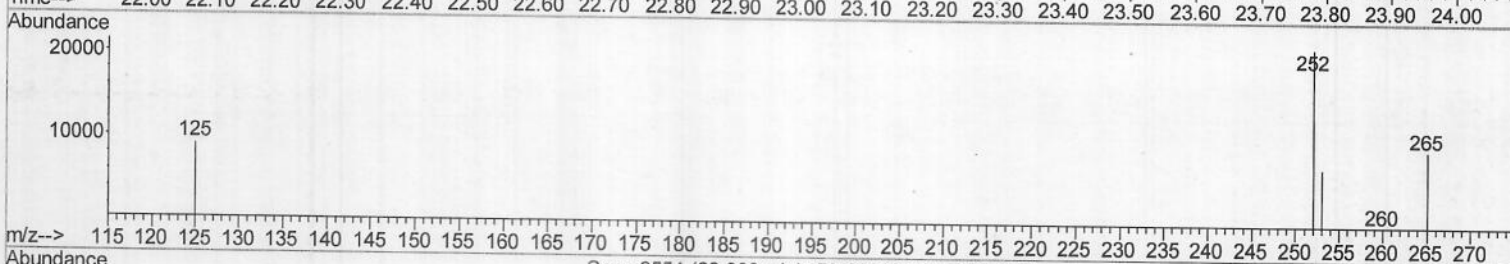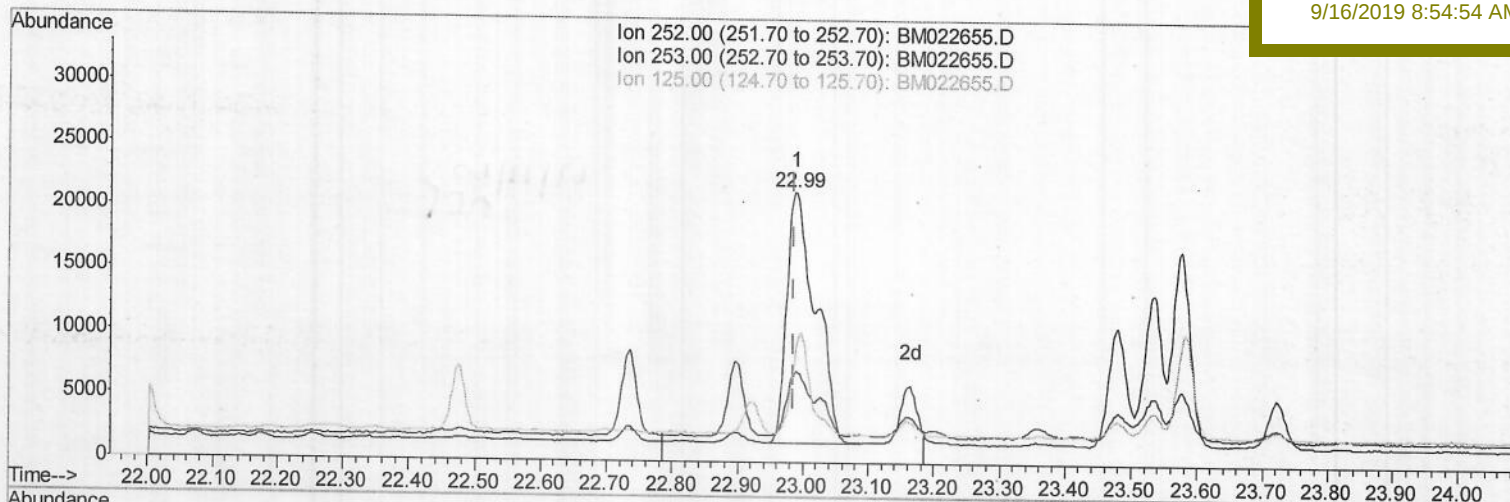

(21) Benzo(b)fluoranthene
 22.990min (+0.003) 0.21ng/ul
 response 60581

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	33.48
125.00	15.60	42.45#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\

Data File : BM022655.D

Acq On : 11 Sep 2019 13:52

Operator : HP/JU

Sample : K4706-07

Misc :

ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:47:20 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

BF573

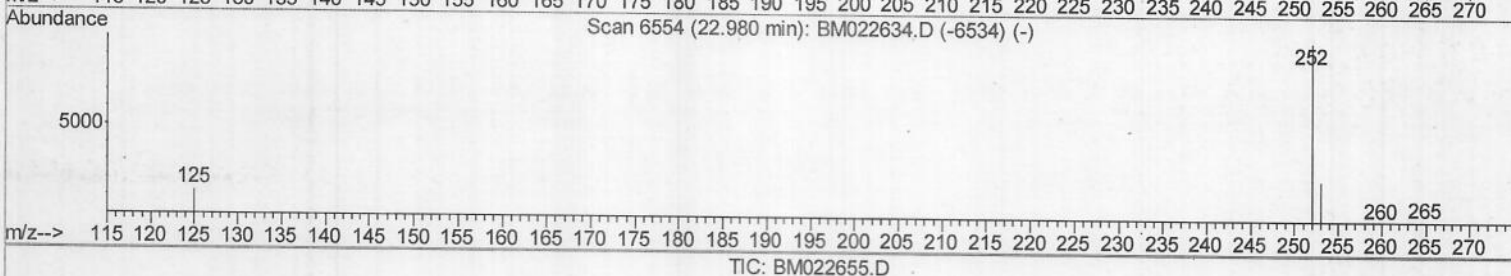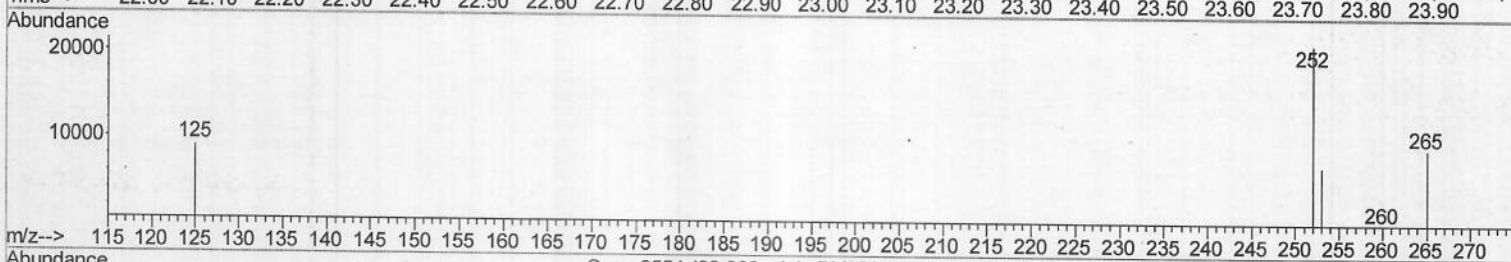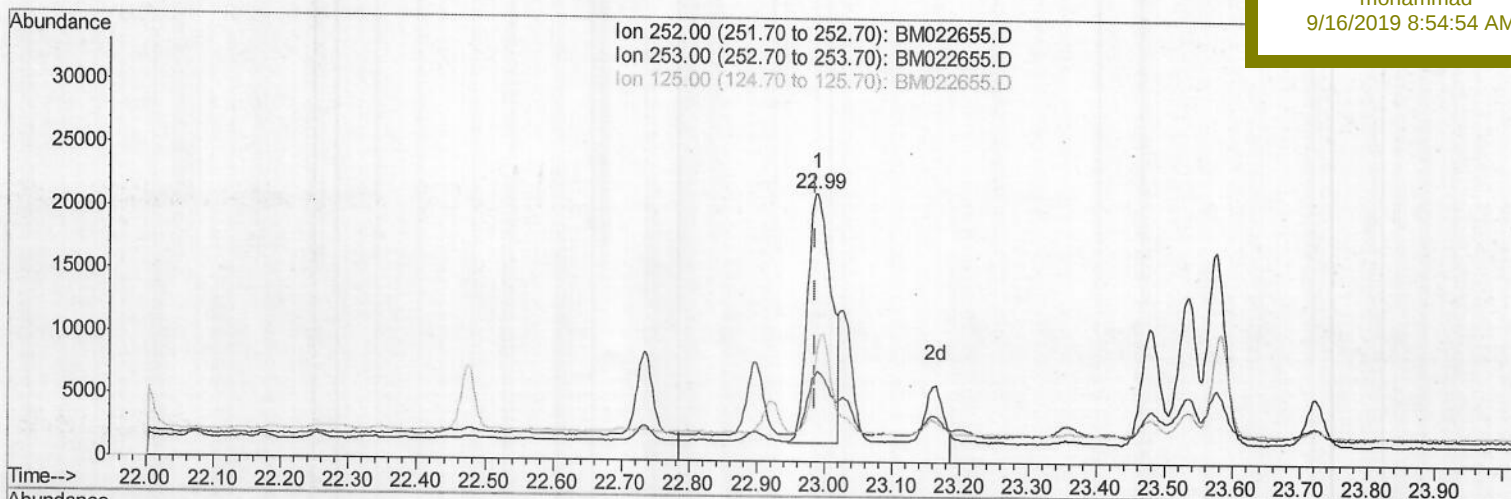Manual Integrations
APPROVEDmohammad
9/16/2019 8:54:54 AM

(21) Benzo(b)fluoranthene

22.990min (+0.003) 0.16ng/ul m

SJV 09/14/19

response 46901

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	33.48
125.00	15.60	42.45#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
Data File : BM022655.D
Acq On : 11 Sep 2019 13:52
Operator : HP/JU
Sample : K4706-07
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:47:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 15:06:45 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampled :
BF573

Manual Integrations
APPROVED

mohammad
9/16/2019 8:54:54 AM

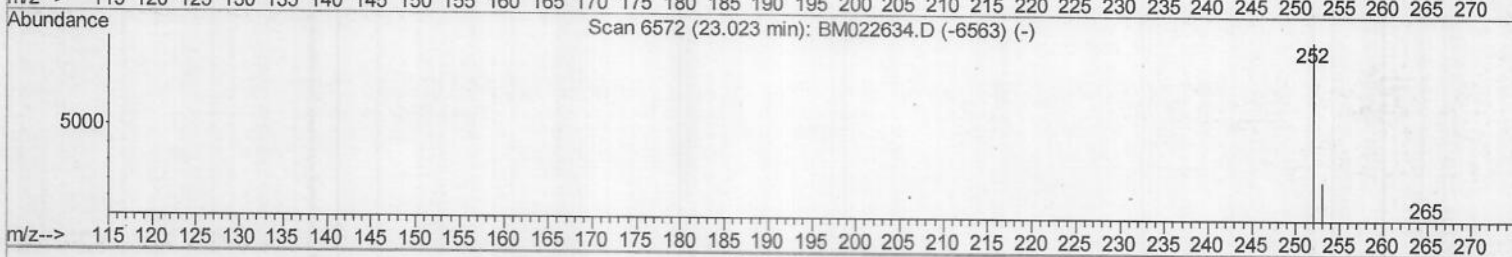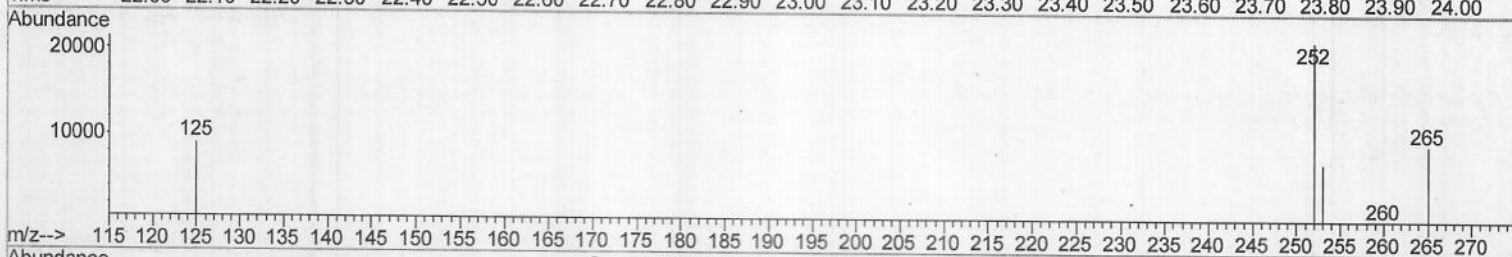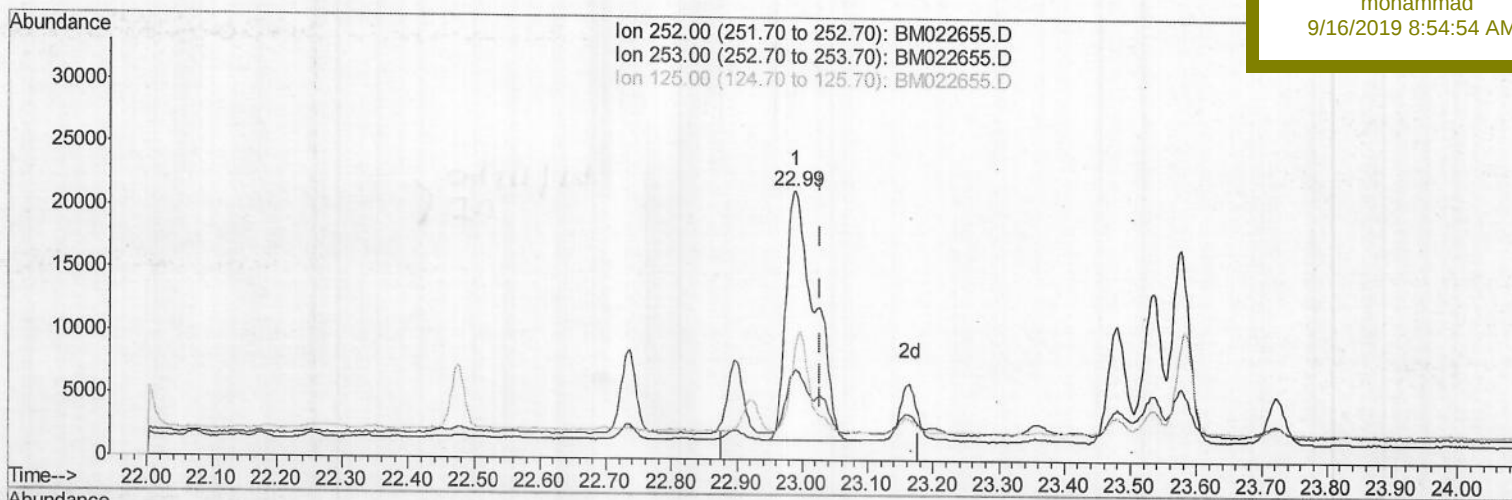

TIC: BM022655.D

(22) Benzo(k)fluoranthene
22.990min (-0.038) 0.20ng/ul
response 60581

Ion	Exp%	Act%
252.00	100	100
253.00	24.40	33.48#
125.00	14.00	42.45#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\

Data File : BM022655.D

Acq On : 11 Sep 2019 13:52

Operator : HP/JU

Sample : K4706-07

Misc :

ALS Vial : 43 Sample Multiplier: 1

Quant Time: Sep 11 15:47:20 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Sep 10 15:06:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




BF573

Manual Integrations

APPROVED

mohammad

9/16/2019 8:54:54 AM

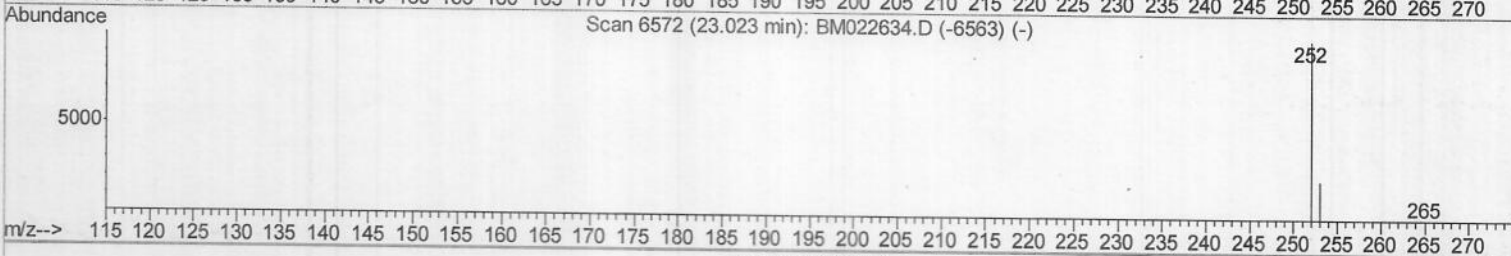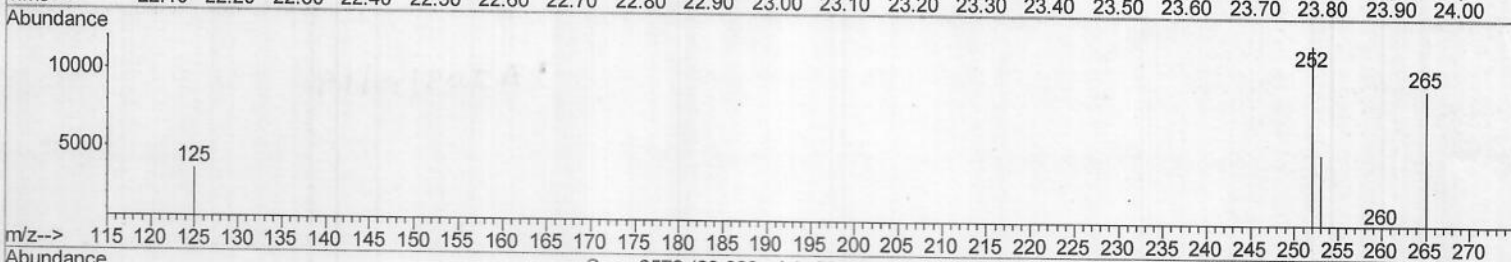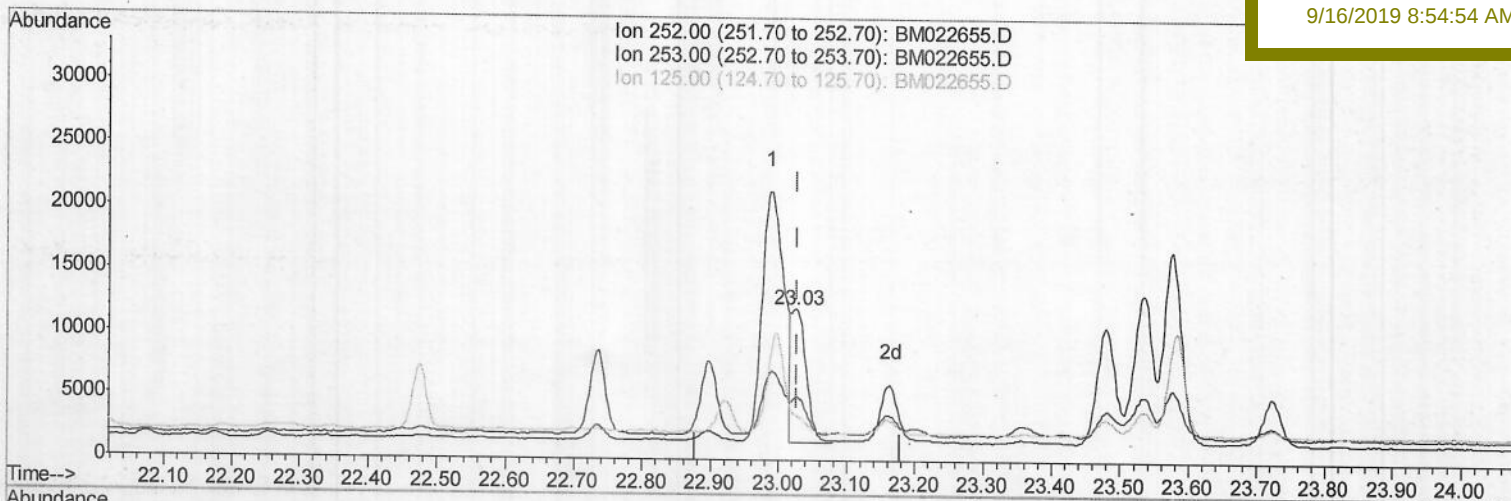

TIC: BM022655.D

(22) Benzo(k)fluoranthene

23.026min (-0.002) 0.05ng/ul m > 30 09/14/19

response 15968

Ion	Exp%	Act%
252.00	100	100
253.00	24.40	42.18#
125.00	14.00	29.71#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091019\
 Data File : BM022655.D
 Acq On : 11 Sep 2019 13:52
 Operator : HP/JU
 Sample : K4706-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 BF573

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:54 AM

Quant Time: Sep 11 15:48:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	22532	0.40	ng/ul	0.00
2) Naphthalene-d8	10.67	136	89638	0.40	ng/ul	0.02
6) Acenaphthene-d10	14.48	164	67879	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	126480m	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	84020m	0.40	ng/ul	0.00
20) Perylene-d12	23.68	264	67047m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.23	152	51080	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	111603m	0.32	ng/ul	0.00

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.68	128	54456607	213.214	ng/ul#	91
5) 2-Methylnaphthalene	12.31	142	14751923	84.249	ng/ul	99
7) Acenaphthylene	14.20	152	2923042	9.303	ng/ul	98
8) Acenaphthene	14.55	153	9899147	37.634	ng/ul	96
9) Fluorene	15.53	166	8153293	27.053	ng/ul	97
12) Phenanthrene	17.26	178	10207361m	25.331	ng/ul	
13) Anthracene	17.35	178	854415m	2.471	ng/ul	
15) Fluoranthene	19.27	202	2608788m	5.999	ng/ul	
17) Pyrene	19.63	202	1646179	4.322	ng/ul	100
18) Benzo(a)anthracene	21.37	228	128824	0.401	ng/ul	95
19) Chrysene	21.43	228	94645m	0.280	ng/ul	
21) Benzo(b)fluoranthene	22.99	252	46901m	0.161	ng/ul	
22) Benzo(k)fluoranthene	23.03	252	15968m	0.054	ng/ul	
23) Benzo(a)pyrene	23.58	252	27563	0.108	ng/ul#	57
24) Indeno(1,2,3-cd)pyrene	25.98	276	8653	0.028	ng/ul#	86
26) Benzo(g,h,i)perylene	26.70	276	6913	0.028	ng/ul#	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed