

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091019\
 Data File : BM022646.D
 Acq On : 11 Sep 2019 07:45
 Operator : HP/JU
 Sample : PB122838BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK38

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:54:32 AM

Quant Time: Sep 11 08:24:09 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 11 07:37:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	19528	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	84299	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	46979	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	101961m	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	75224m	0.40	ng/ul	0.00
20) Perylene-d12	23.67	264	66046	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	39684	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	78212m	0.28	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.69	128	10732	0.045	ng/ul#	Ovalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091019\
Data File : BM022646.D
Acq On : 11 Sep 2019 07:45
Operator : HP/JU
Sample : PB122838BL
Misc :
ALS Vial : 34 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
SBLK38

Manual Integrations
APPROVED

mohammad
9/16/2019 8:54:32 AM

Quant Time: Sep 11 08:24:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 11 07:37:53 2019
Response via : Initial Calibration

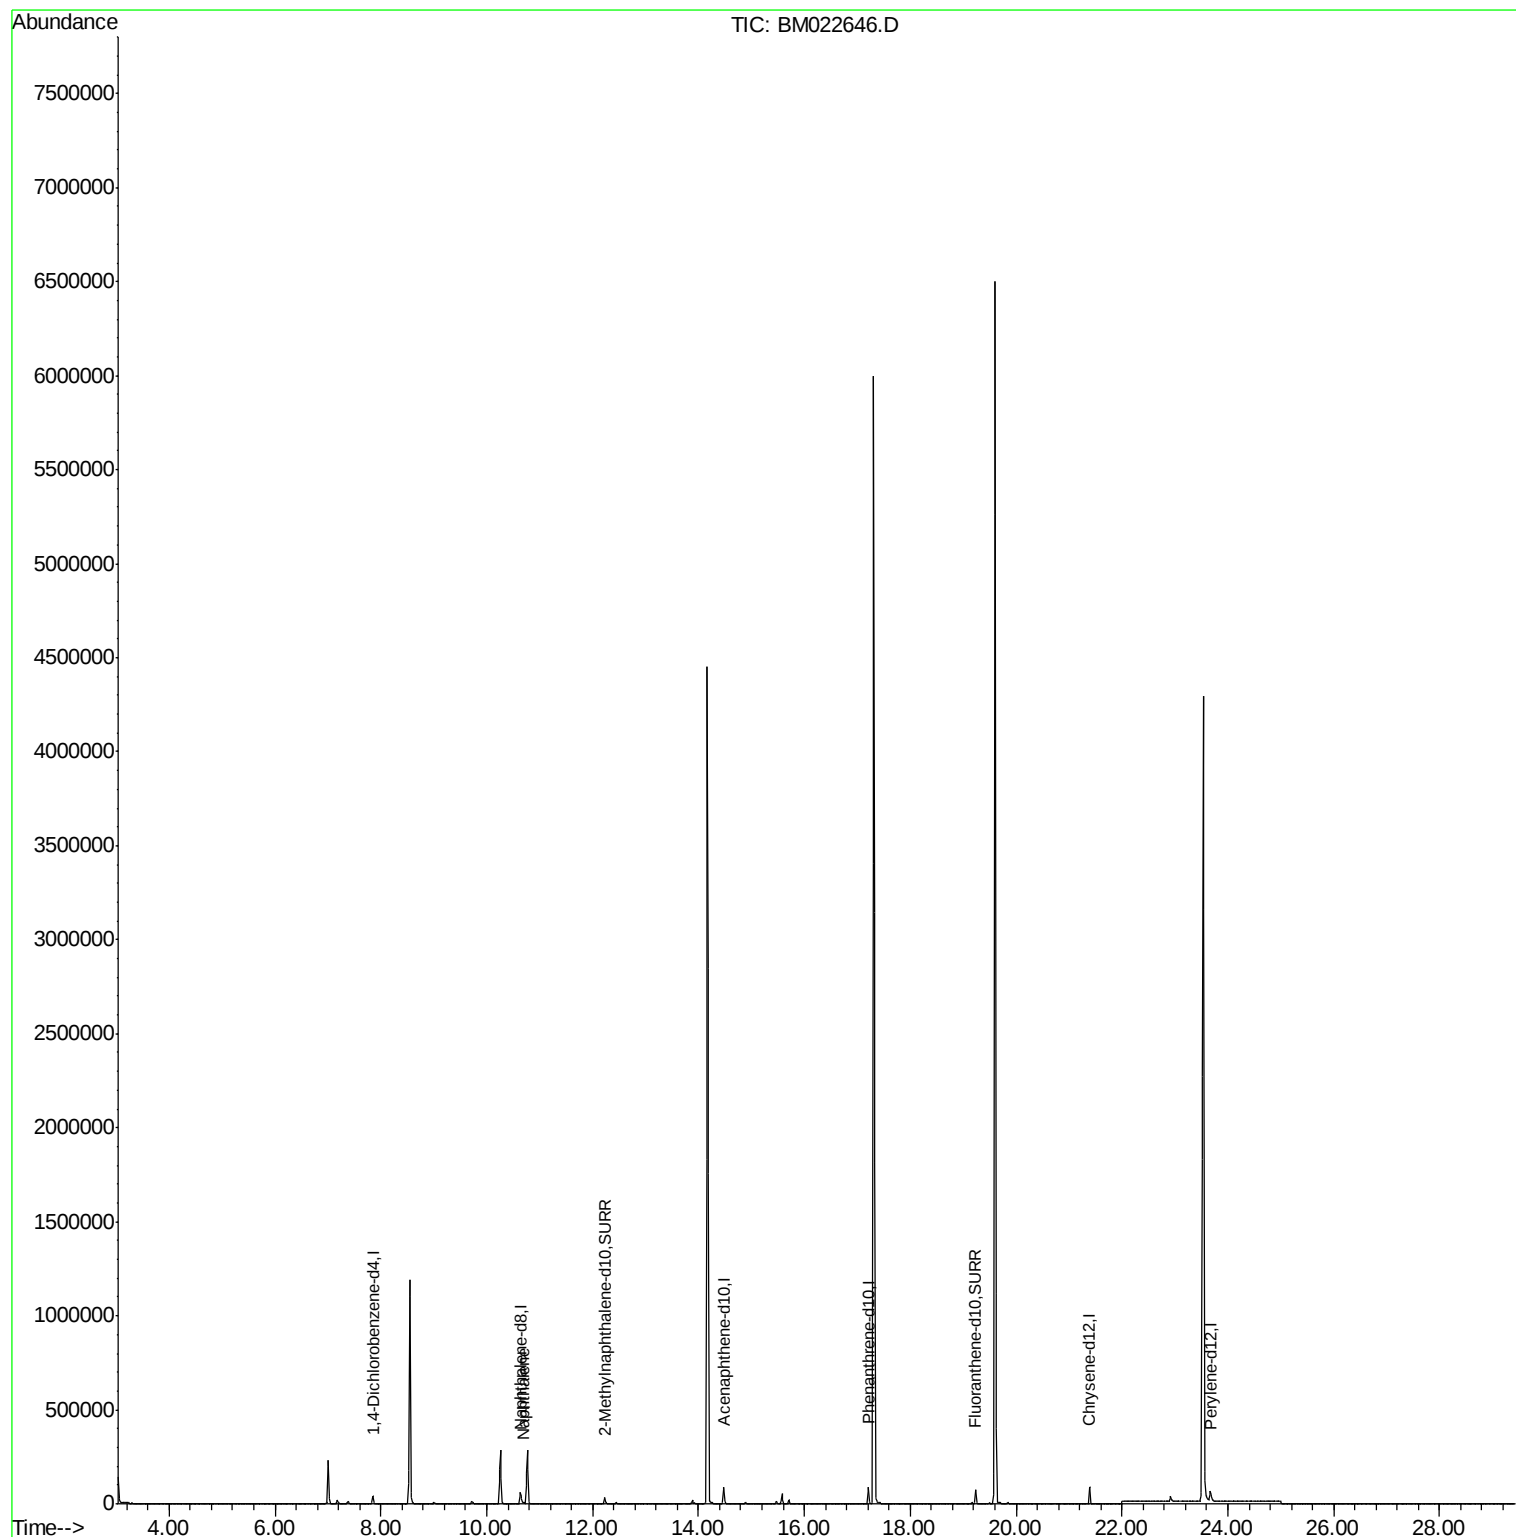

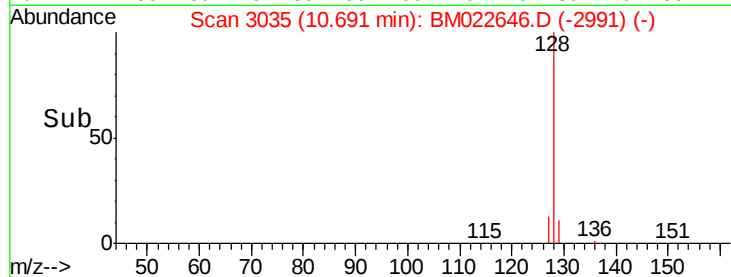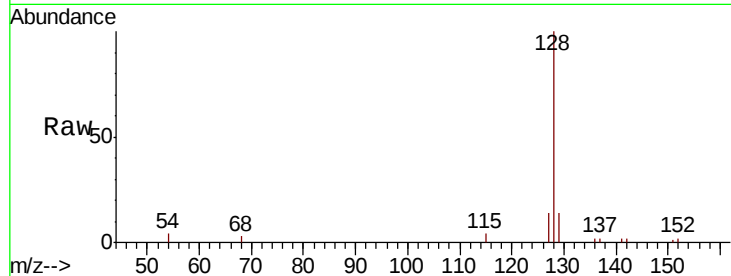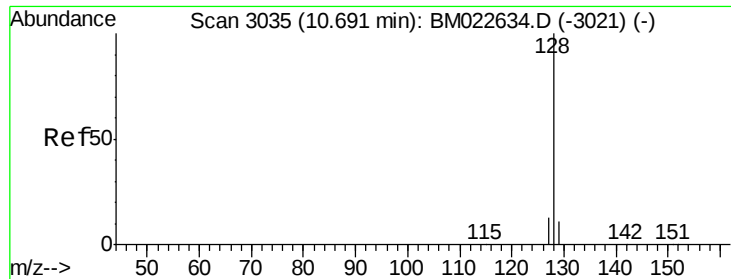

#3

Naphthalene

Concen: 0.045 ng/ul

RT: 10.69 min Scan# 3035

Delta R.T. -0.00 min

Lab File: BM022646.D

Acq: 11 Sep 2019 07:45

Tot Ion	Ratio	Lower	Upper
128	100		
129	13.6	8.8	13.2#
127	14.0	10.4	15.6

Instrument :

BNA_M

ClientSampleId :

SBLK38

Manual Integrations
APPROVED

mohammad
9/16/2019 8:54:32 AM

