

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041778.D
 Acq On : 11 Sep 2023 14:30
 Operator : MA/JU
 Sample : PB155273BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK273

Quant Time: Sep 12 04:25:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.984	152	3689	0.400	ng/ul	0.00
4) Naphthalene-d8	10.796	136	8943	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.625	164	4152	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.375	188	7678	0.400	ng/ul	0.00
17) Chrysene-d12	21.545	240	2946	0.400	ng/ul	0.00
23) Perylene-d12	23.968	264	3468	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	35528	6.302	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.379	152	3630	0.315	ng/ul	0.00
18) Fluoranthene-d10	19.394	212	4489	0.314	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.766	202	1717	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.813	252	3103	0.123	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
Data File : BM041778.D
Acq On : 11 Sep 2023 14:30
Operator : MA/JU
Sample : PB155273BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK273

Quant Time: Sep 12 04:25:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration




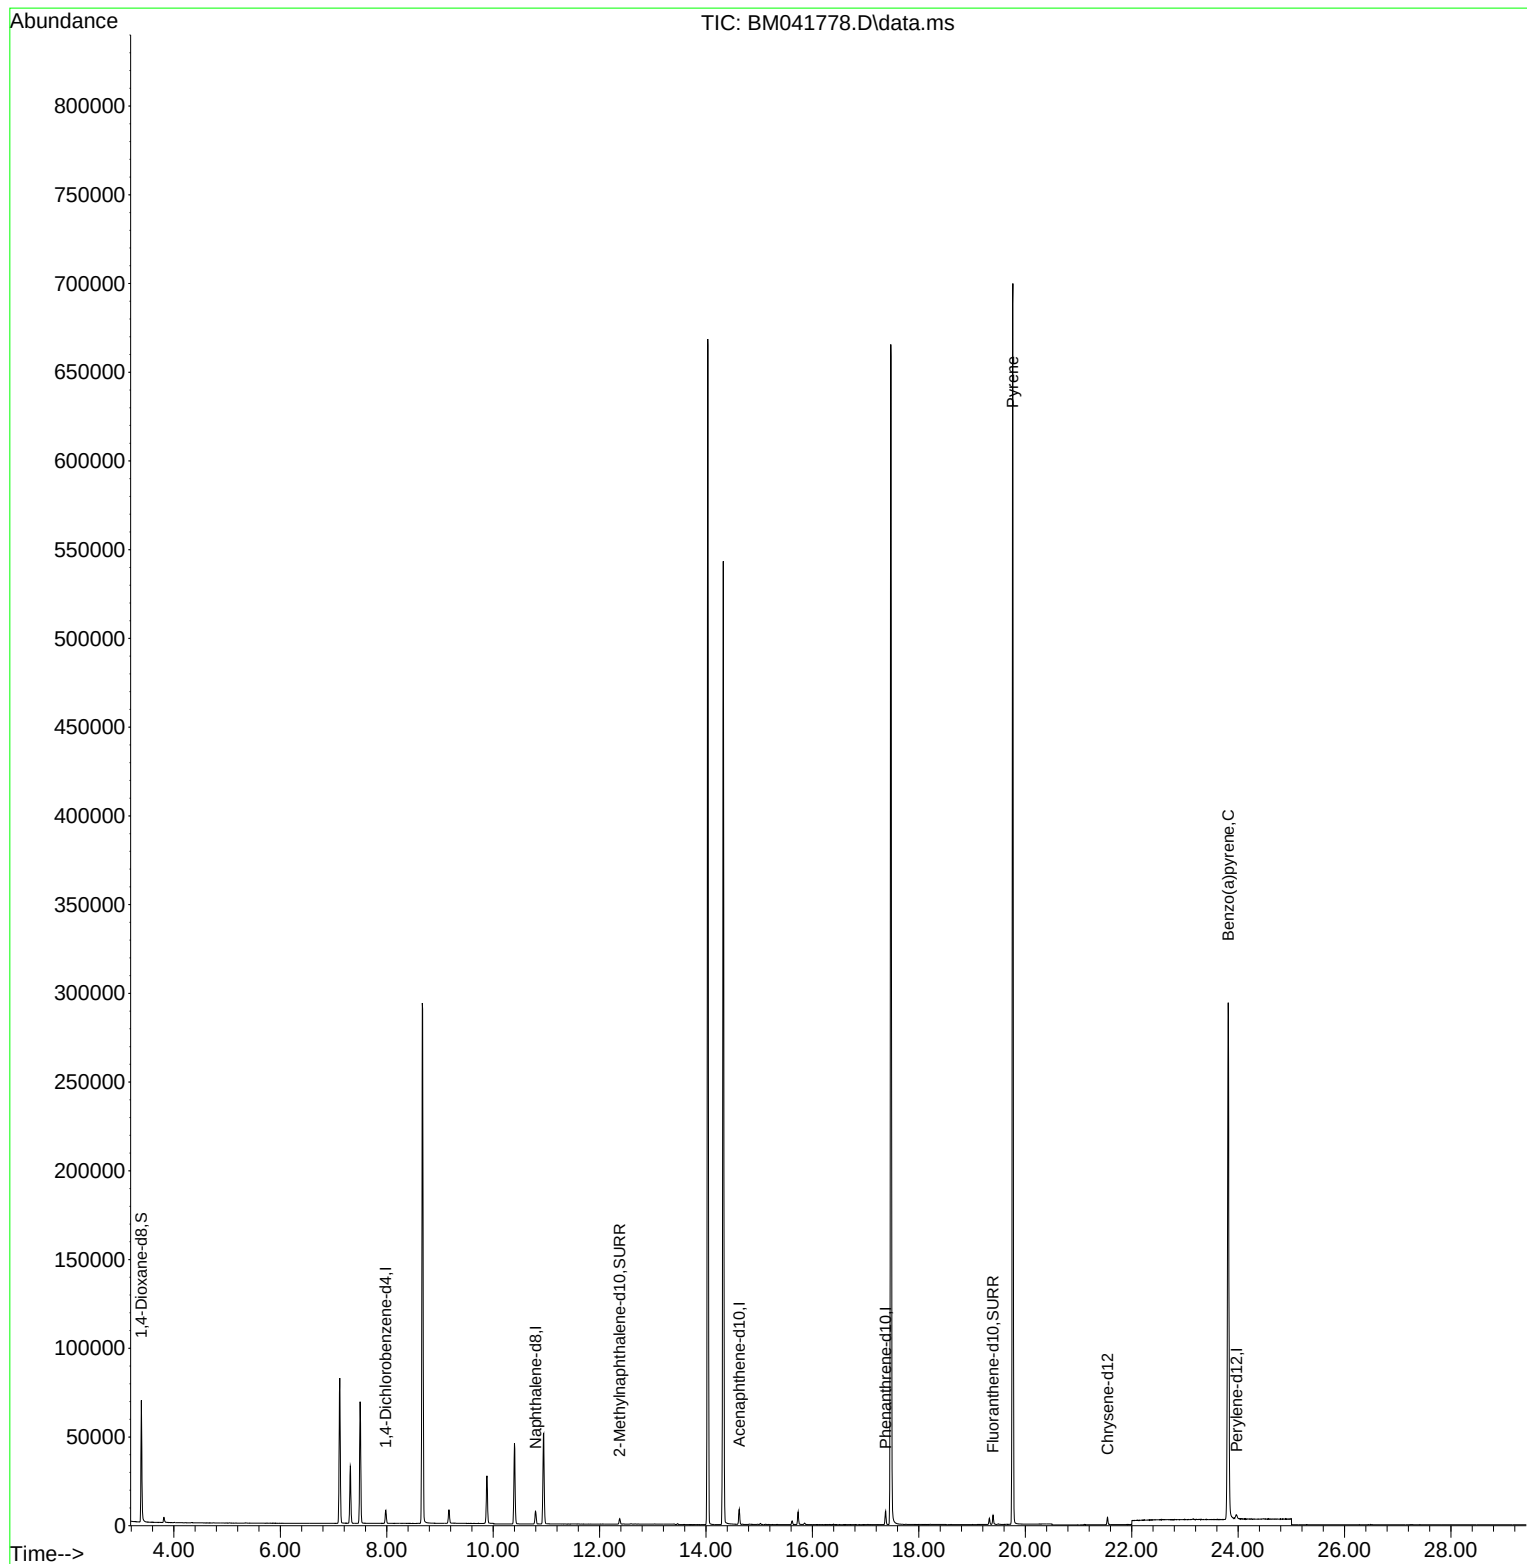


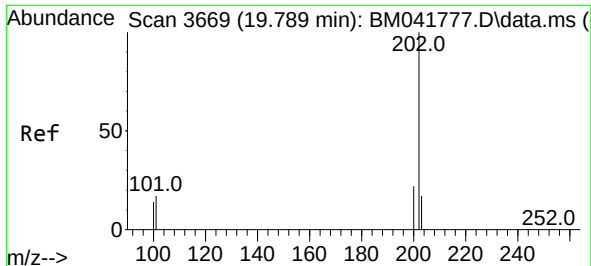

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.766 min Scan# 30
Delta R.T. -0.032 min
Lab File: BM041778.D
Acq: 11 Sep 2023 14:30

Instrument :
BNA_M
ClientSampleId :
SBLK273

Tgt Ion:202 Resp: 1717
Ion Ratio Lower Upper
202 100
101 171.6 11.8 17.8#
100 1225.6 9.8 14.6#

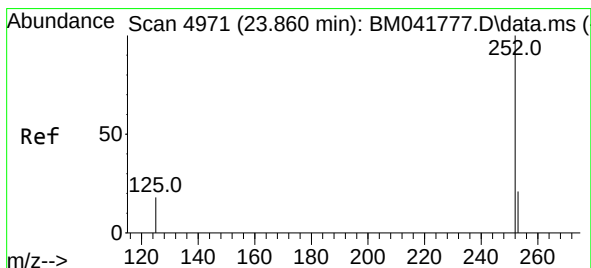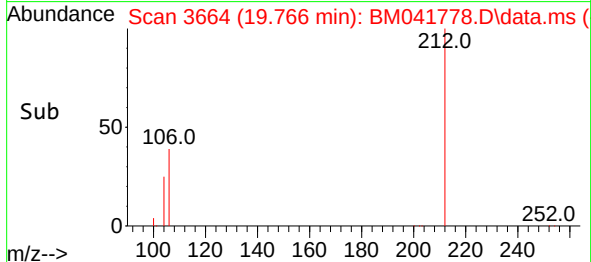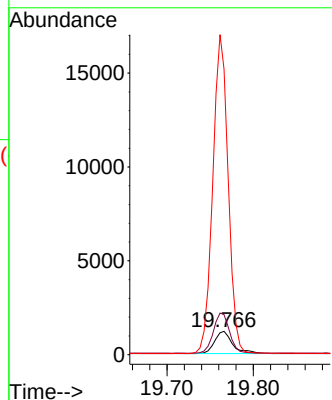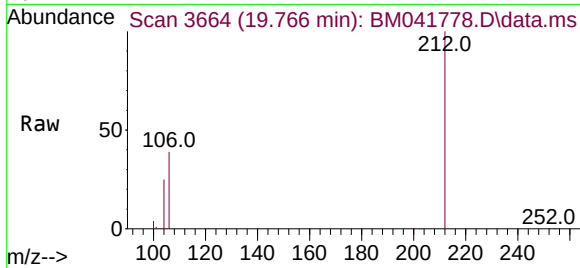

#26
Benzo(a)pyrene
Concen: 0.123 ng/ul
RT: 23.813 min Scan# 4955
Delta R.T. -0.050 min
Lab File: BM041778.D
Acq: 11 Sep 2023 14:30

Tgt Ion:252 Resp: 3103
Ion Ratio Lower Upper
252 100
253 48.8 22.4 33.6#
125 55.8 21.0 31.4#

