

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041779.D
 Acq On : 11 Sep 2023 15:07
 Operator : MA/JU
 Sample : PB155276BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK276

Quant Time: Sep 12 04:26:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.984	152	3961	0.400	ng/ul	0.00
4) Naphthalene-d8	10.796	136	9584	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.624	164	4355	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.375	188	7817	0.400	ng/ul	0.00
17) Chrysene-d12	21.545	240	2862	0.400	ng/ul	0.00
23) Perylene-d12	23.965	264	3483	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	38351	6.335	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.379	152	3888	0.315	ng/ul	0.00
18) Fluoranthene-d10	19.394	212	4413	0.318	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.761	202	1696	0.051	ng/ul#	1
26) Benzo(a)pyrene	23.810	252	3053	0.121	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
Data File : BM041779.D
Acq On : 11 Sep 2023 15:07
Operator : MA/JU
Sample : PB155276BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK276

Quant Time: Sep 12 04:26:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration




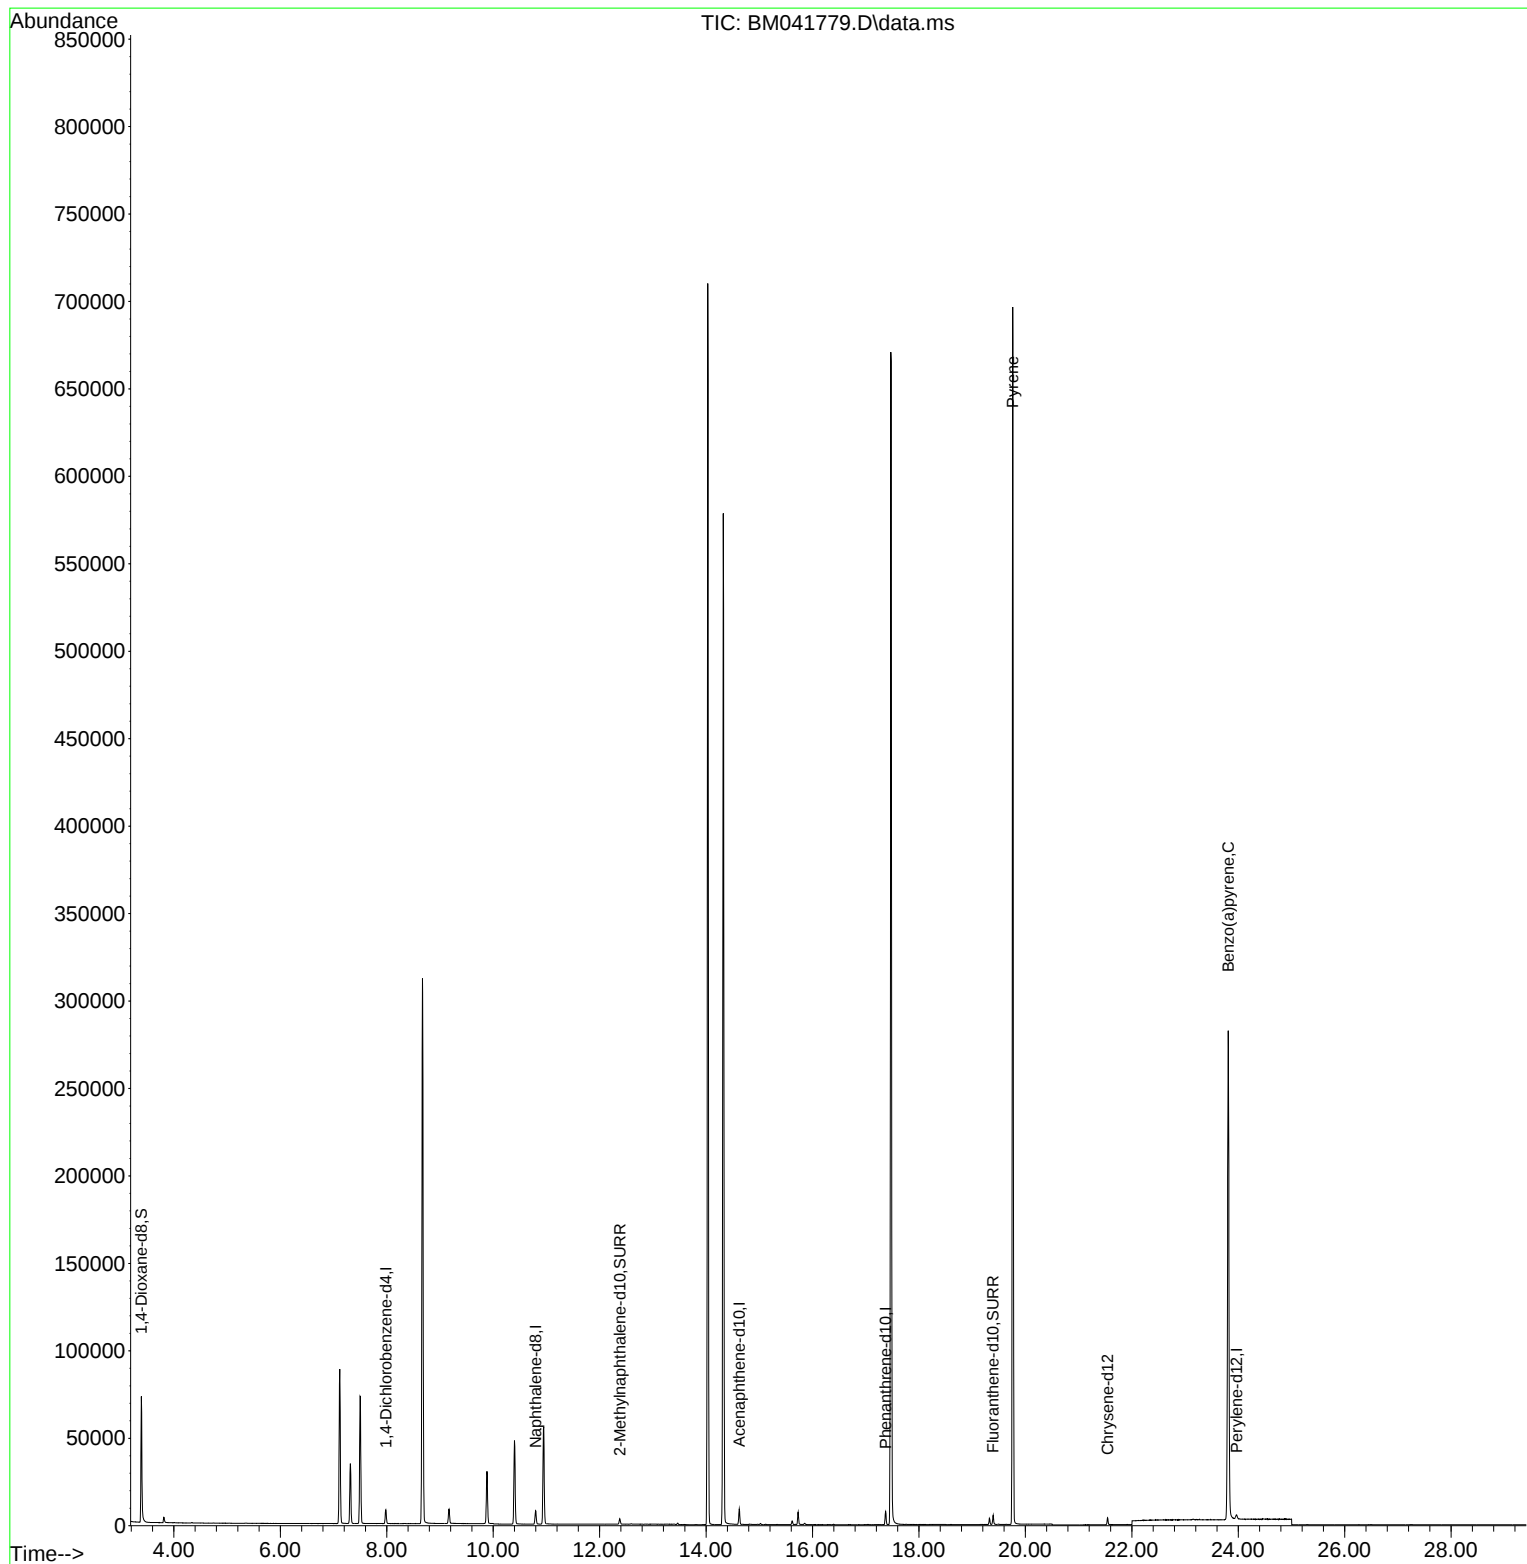


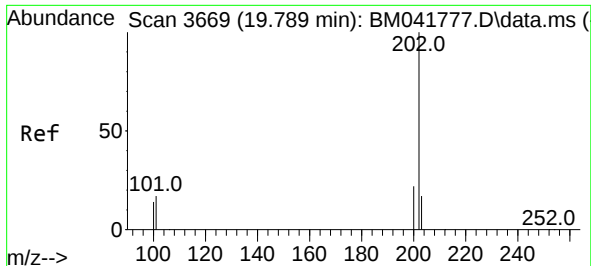

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.761 min Scan# 30
Delta R.T. -0.037 min
Lab File: BM041779.D
Acq: 11 Sep 2023 15:07

Instrument :
BNA_M
ClientSampleId :
SBLK276

Tgt Ion:202 Resp: 1696
Ion Ratio Lower Upper
202 100
101 183.6 11.8 17.8#
100 1389.9 9.8 14.6#

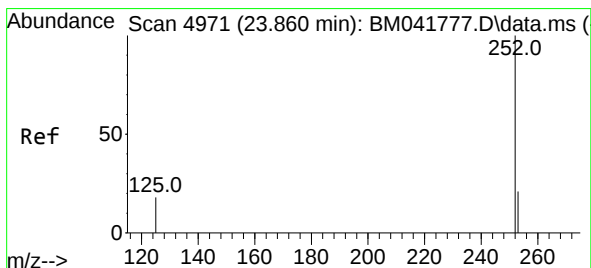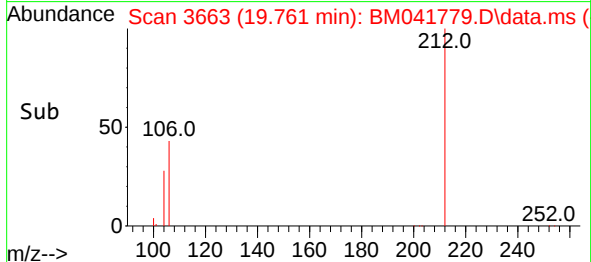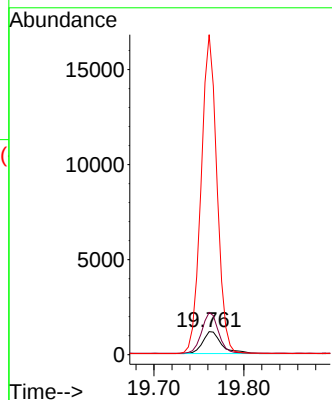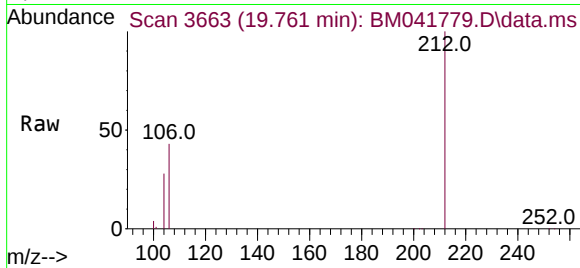

#26
Benzo(a)pyrene
Concen: 0.121 ng/ul
RT: 23.810 min Scan# 4954
Delta R.T. -0.052 min
Lab File: BM041779.D
Acq: 11 Sep 2023 15:07

Tgt Ion:252 Resp: 3053
Ion Ratio Lower Upper
252 100
253 48.2 22.4 33.6#
125 56.4 21.0 31.4#

