

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041787.D
 Acq On : 11 Sep 2023 20:10
 Operator : MA/JU
 Sample : 04247-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJA1

Quant Time: Sep 12 04:27:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.984	152	4397	0.400	ng/ul	0.00
4) Naphthalene-d8	10.797	136	10549	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.625	164	4742	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.376	188	8463	0.400	ng/ul	0.00
17) Chrysene-d12	21.543	240	3019	0.400	ng/ul	0.00
23) Perylene-d12	23.963	264	3877	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	31050	4.621	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.375	152	4400	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.395	212	6078	0.415	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.423	88	72352	10.364	ng/ul	87
20) Pyrene	19.762	202	2429	0.069	ng/ul#	1
26) Benzo(a)pyrene	23.808	252	3820	0.136	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
Data File : BM041787.D
Acq On : 11 Sep 2023 20:10
Operator : MA/JU
Sample : 04247-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJA1

Quant Time: Sep 12 04:27:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration




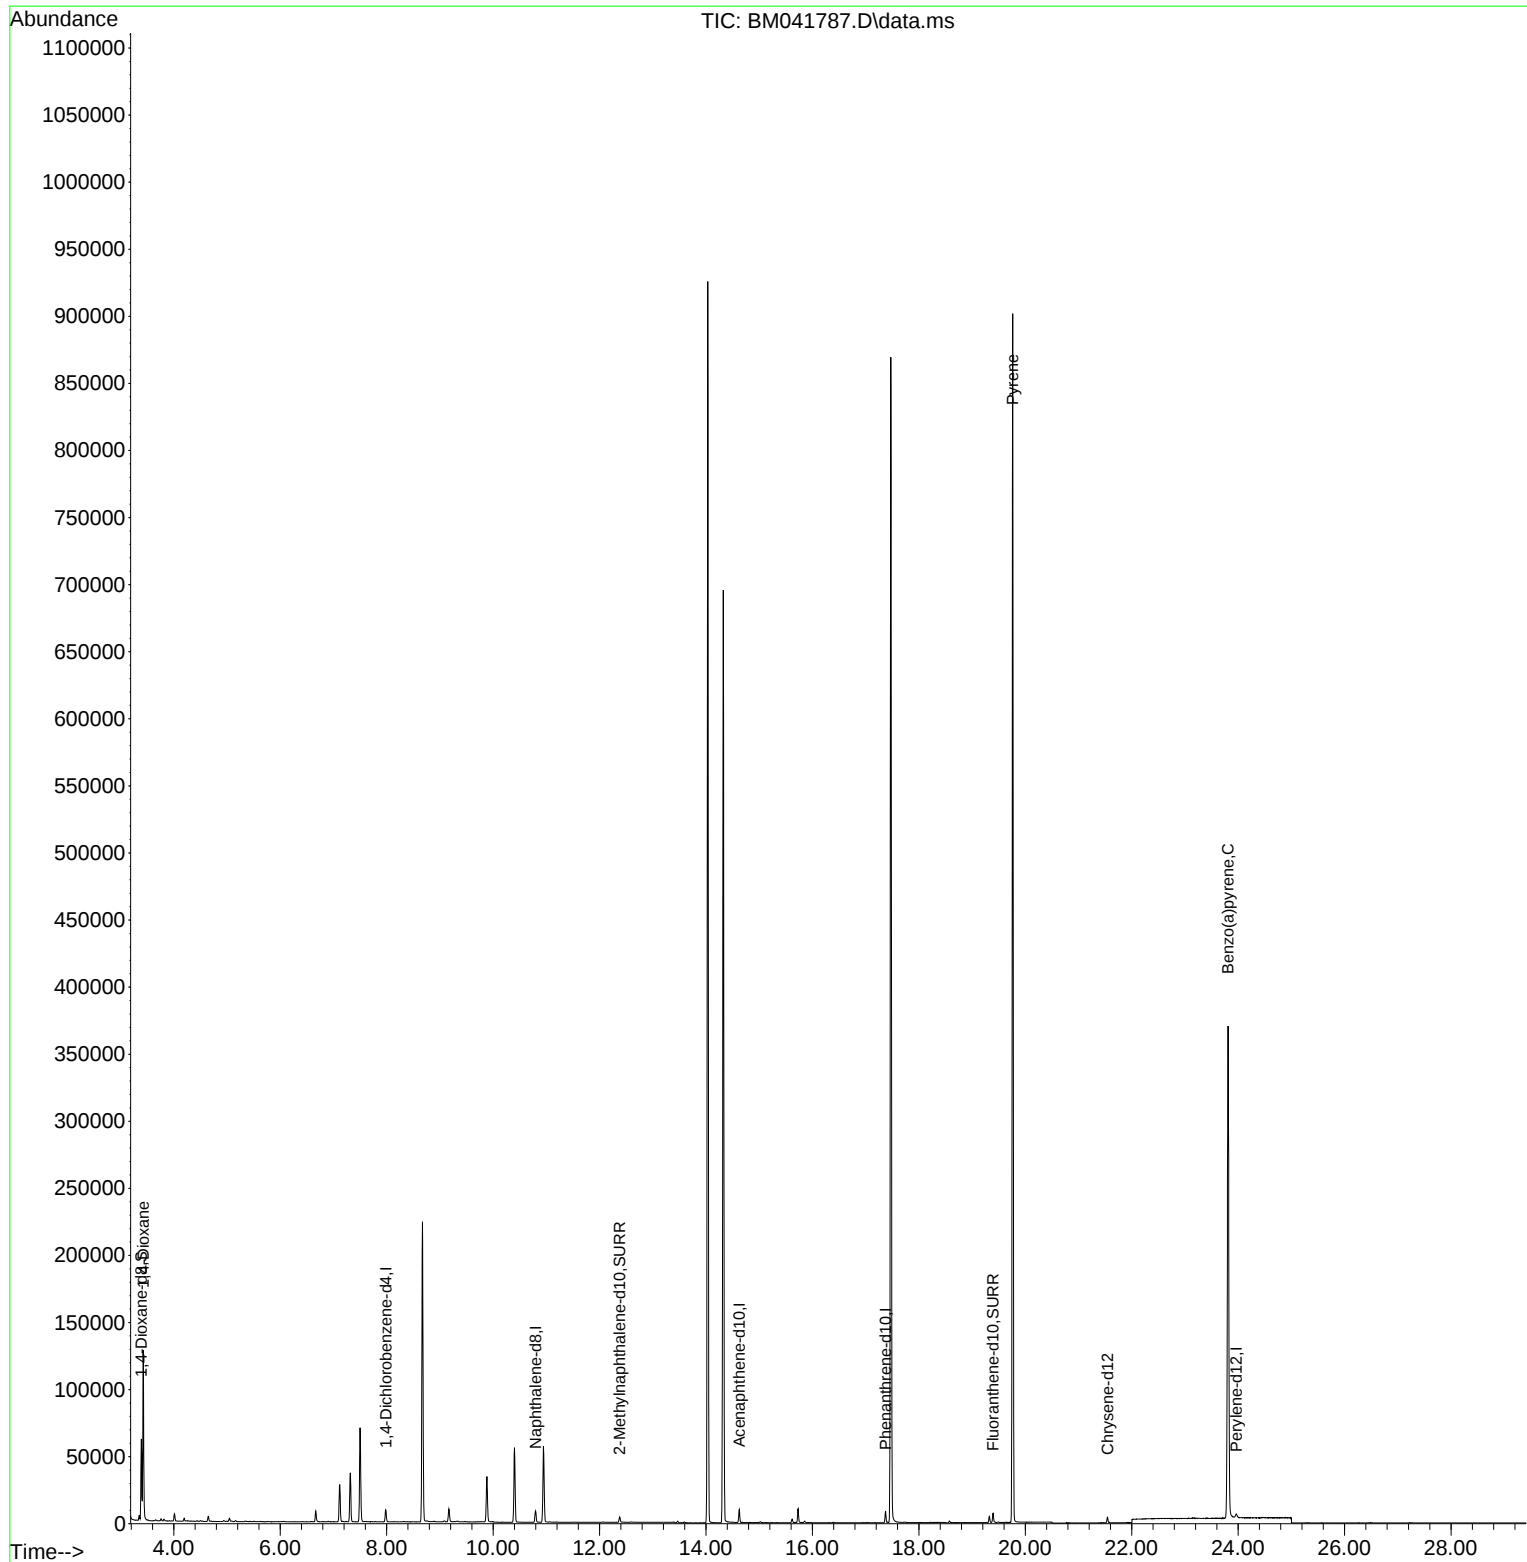


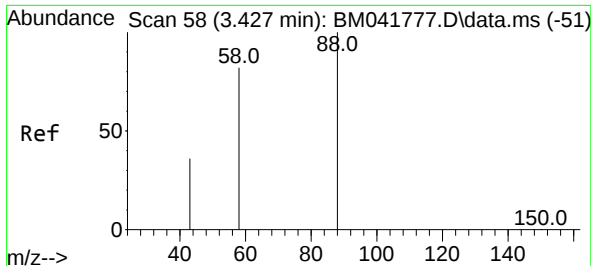

#2
 1,4-Dioxane
 Concen: 10.364 ng/ul
 RT: 3.423 min Scan# 51
 Delta R.T. -0.012 min
 Lab File: BM041787.D
 Acq: 11 Sep 2023 20:10




Instrument :
 BNA_M
 ClientSampleId :
 BBJA1


Tgt Ion: 88 Resp: 72352
 Ion Ratio Lower Upper
 88 100
 43 36.9 33.8 50.6
 58 81.0 54.2 81.2

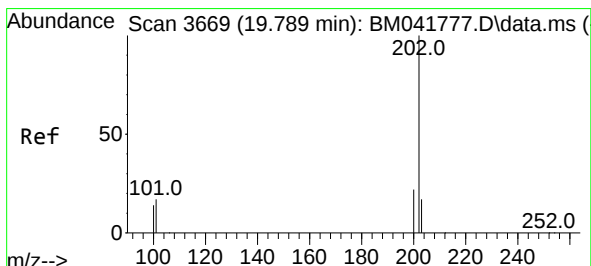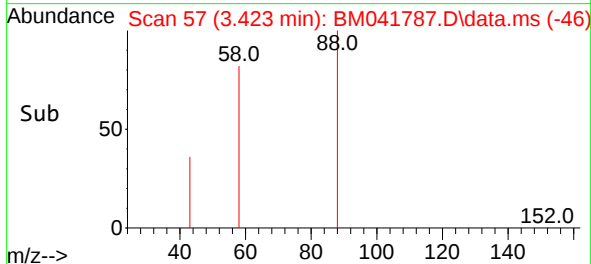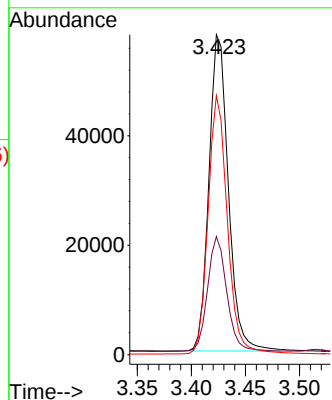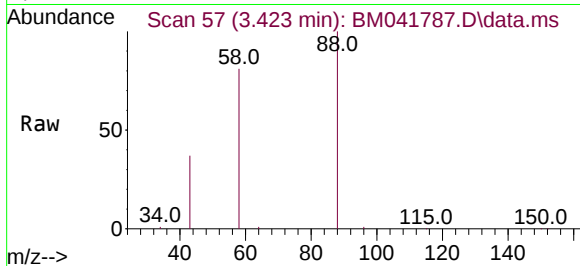

#20
 Pyrene
 Concen: 0.069 ng/ul
 RT: 19.762 min Scan# 3663
 Delta R.T. -0.036 min
 Lab File: BM041787.D
 Acq: 11 Sep 2023 20:10


Tgt Ion: 202 Resp: 2429
 Ion Ratio Lower Upper
 202 100
 101 182.0 11.8 17.8#
 100 1366.1 9.8 14.6#

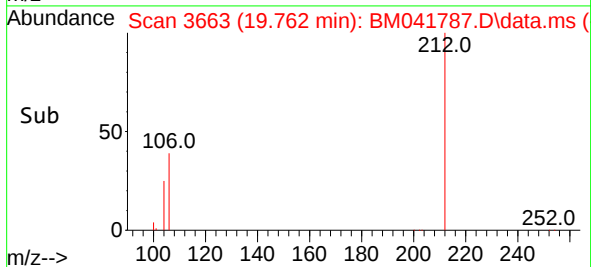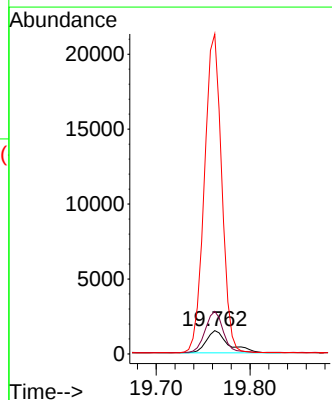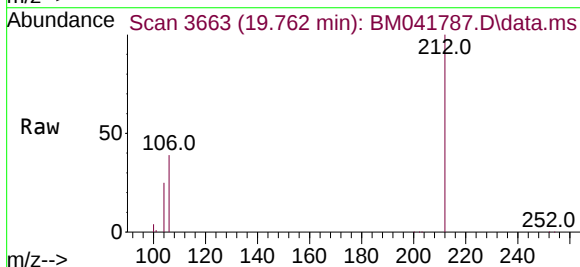

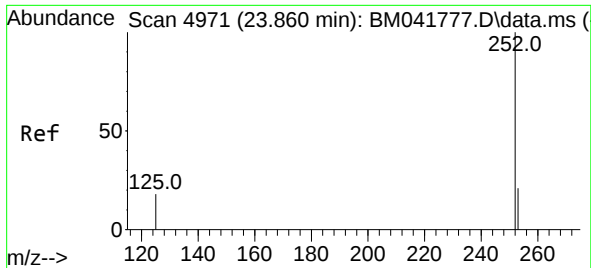

#26
 Benzo(a)pyrene
 Concen: 0.136 ng/ul
 RT: 23.808 min Scan# 4953
 Delta R.T. -0.054 min
 Lab File: BM041787.D
 Acq: 11 Sep 2023 20:10

Instrument :
 BNA_M
 ClientSampleId :
 BBJA1

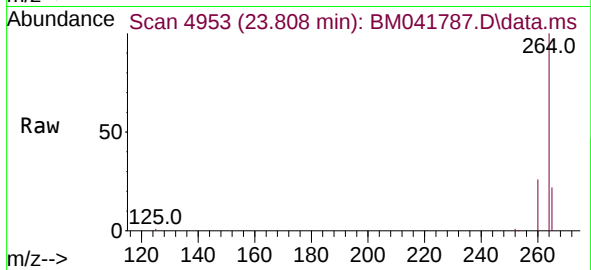

Tgt Ion:252 Resp: 3820
 Ion Ratio Lower Upper
 252 100
 253 48.9 22.4 33.6#
 125 54.0 21.0 31.4#

