

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041793.D
 Acq On : 12 Sep 2023 00:30
 Operator : MA/JU
 Sample : PB155326BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK326

Quant Time: Sep 12 04:52:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 04:50:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.979	152	5369	0.400	ng/ul	0.00
4) Naphthalene-d8	10.796	136	12680	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.624	164	5745	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.371	188	10714	0.400	ng/ul	0.00
17) Chrysene-d12	21.545	240	3726	0.400	ng/ul	0.00
23) Perylene-d12	23.965	264	4791	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	38368	4.676	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.374	152	3949	0.242	ng/ul	0.00
18) Fluoranthene-d10	19.394	212	4698	0.260	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.614	166	2049	0.066	ng/ul#	14
20) Pyrene	19.761	202	1801	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.807	252	3417	0.098	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
Data File : BM041793.D
Acq On : 12 Sep 2023 00:30
Operator : MA/JU
Sample : PB155326BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK326

Quant Time: Sep 12 04:52:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 04:50:34 2023
Response via : Initial Calibration

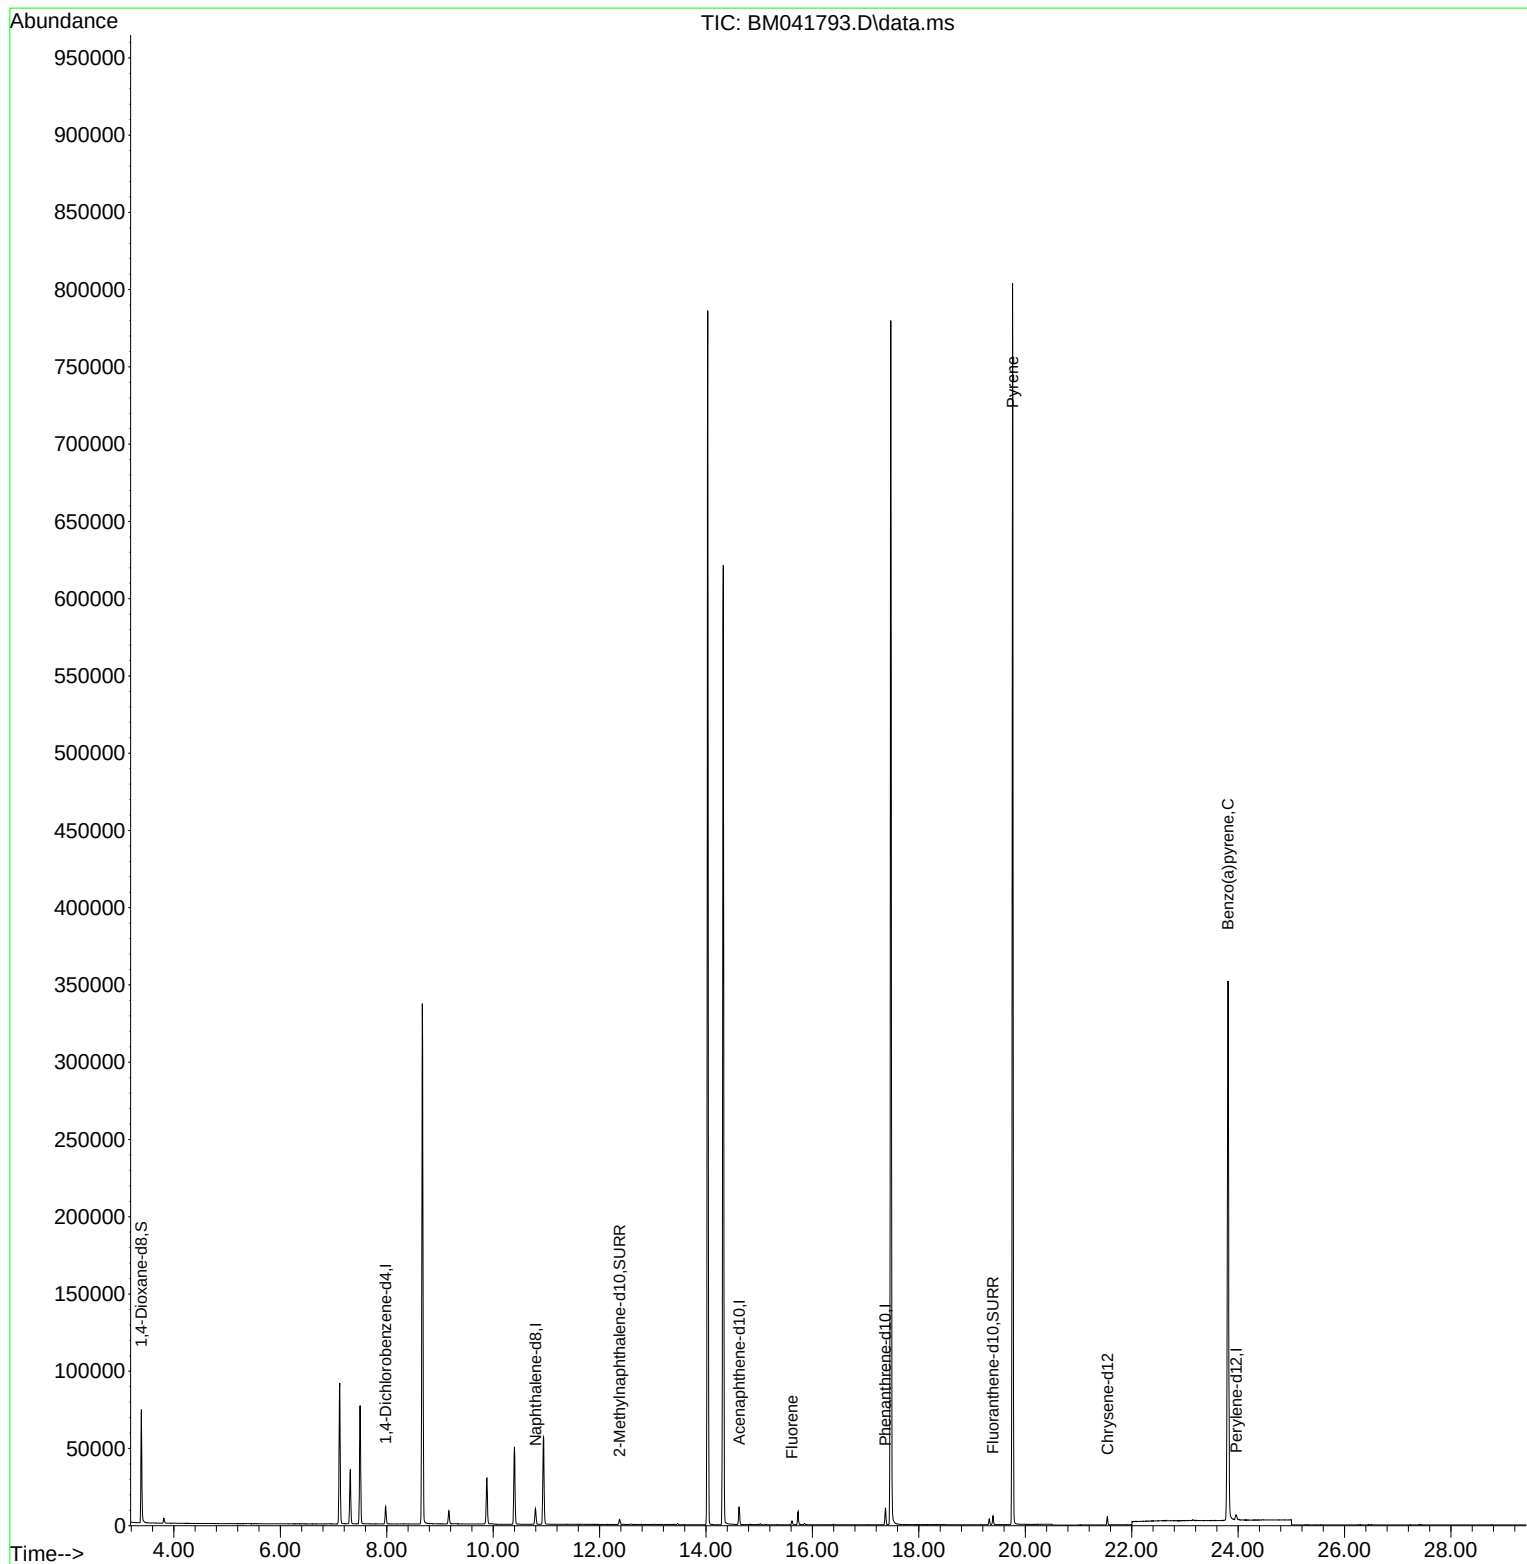

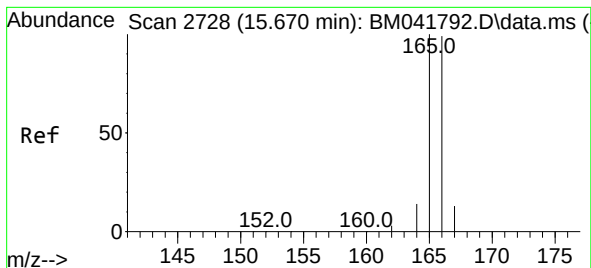

#12

Fluorene

Concen: 0.066 ng/ul

RT: 15.614 min Scan# 21

Delta R.T. -0.056 min

Lab File: BM041793.D

Acq: 12 Sep 2023 00:30

Instrument :

BNA_M

ClientSampleId :

SBLK326





Tgt Ion:166 Resp: 2049

Ion Ratio Lower Upper

166 100

165 8.3 79.4 119.2#

167 32.4 11.3 16.9#

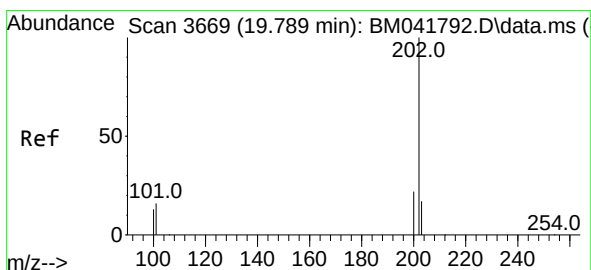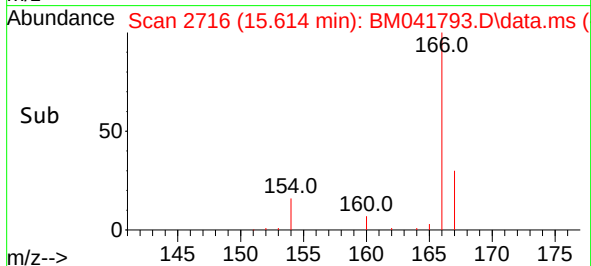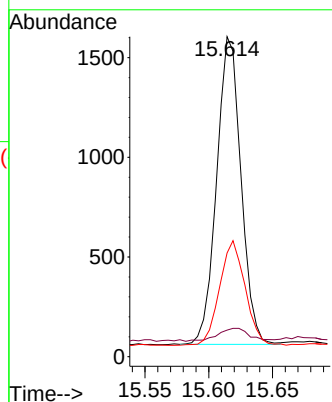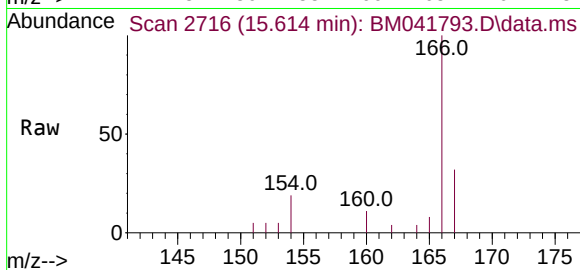

#20

Pyrene

Concen: 0.041 ng/ul

RT: 19.761 min Scan# 3663

Delta R.T. -0.028 min

Lab File: BM041793.D

Acq: 12 Sep 2023 00:30




Tgt Ion:202 Resp: 1801


Ion Ratio Lower Upper

202 100

101 180.1 11.8 17.8#


100 1344.7 9.8 14.6#

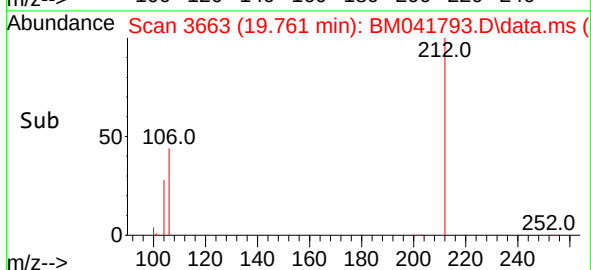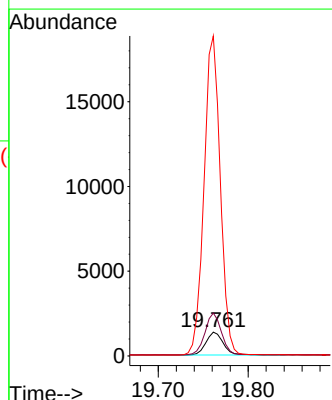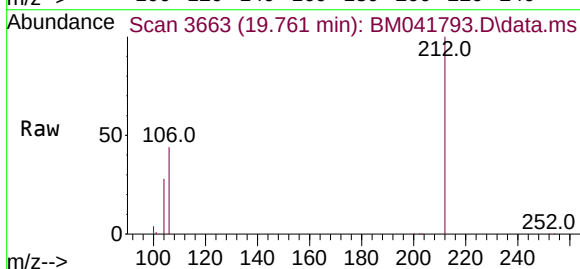

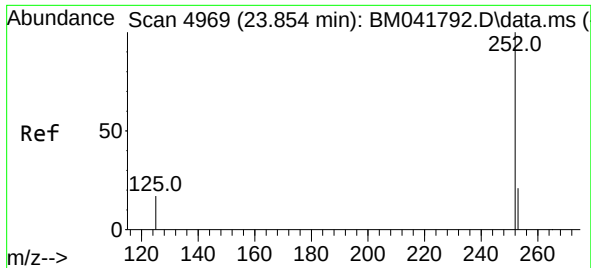

#26
Benzo(a)pyrene
Concen: 0.098 ng/ul
RT: 23.807 min Scan# 49
Delta R.T. -0.047 min
Lab File: BM041793.D
Acq: 12 Sep 2023 00:30

Instrument :
BNA_M
ClientSampleId :
SBLK326

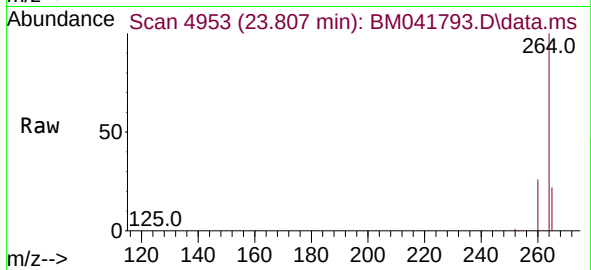

Tgt Ion:252 Resp: 3417
Ion Ratio Lower Upper
252 100
253 46.1 22.4 33.6#
125 51.5 21.0 31.4#

