

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041796.D
 Acq On : 12 Sep 2023 02:20
 Operator : MA/JU
 Sample : 04235-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EYZE0

Quant Time: Sep 12 04:52:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 04:50:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.979	152	5700	0.400	ng/ul	0.00
4) Naphthalene-d8	10.796	136	14162	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.624	164	6229	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.371	188	11330	0.400	ng/ul	0.00
17) Chrysene-d12	21.542	240	4706	0.400	ng/ul	0.00
23) Perylene-d12	23.959	264	4863	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.385	96	19599	2.250	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.374	152	2498	0.137	ng/ul	0.00
18) Fluoranthene-d10	19.394	212	3152	0.138	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.845	128	9504	0.204	ng/ul	99
7) 2-Methylnaphthalene	12.451	142	5906	0.224	ng/ul	100
8) 1-Methylnaphthalene	12.671	142	4527	0.171	ng/ul	99
10) Acenaphthylene	14.351	152	7921	0.206	ng/ul	98
11) Acenaphthene	14.685	153	3675	0.123	ng/ul	99
12) Fluorene	15.670	166	4859	0.145	ng/ul	98
15) Phenanthrene	17.417	178	117259	2.451	ng/ul	98
16) Anthracene	17.506	178	24268	0.592	ng/ul	99
19) Fluoranthene	19.422	202	252141	4.540	ng/ul	98
20) Pyrene	19.789	202	225054	4.079	ng/ul	98
21) Benzo(a)anthracene	21.524	228	86025	2.241	ng/ul	100
22) Chrysene	21.580	228	90931	2.196	ng/ul	98
24) Benzo(b)fluoranthene	23.214	252	122386	2.813	ng/ul	92
26) Benzo(a)pyrene	23.851	252	79765	2.256	ng/ul#	89
27) Indeno(1,2,3-cd)pyrene	26.461	276	59157	1.219	ng/ul#	99
28) Dibenzo(a,h)anthracene	26.475	278	13278	0.390	ng/ul#	93
29) Benzo(g,h,i)perylene	27.246	276	58289	1.356	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
Data File : BM041796.D
Acq On : 12 Sep 2023 02:20
Operator : MA/JU
Sample : 04235-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EZYEO

Quant Time: Sep 12 04:52:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 04:50:34 2023
Response via : Initial Calibration




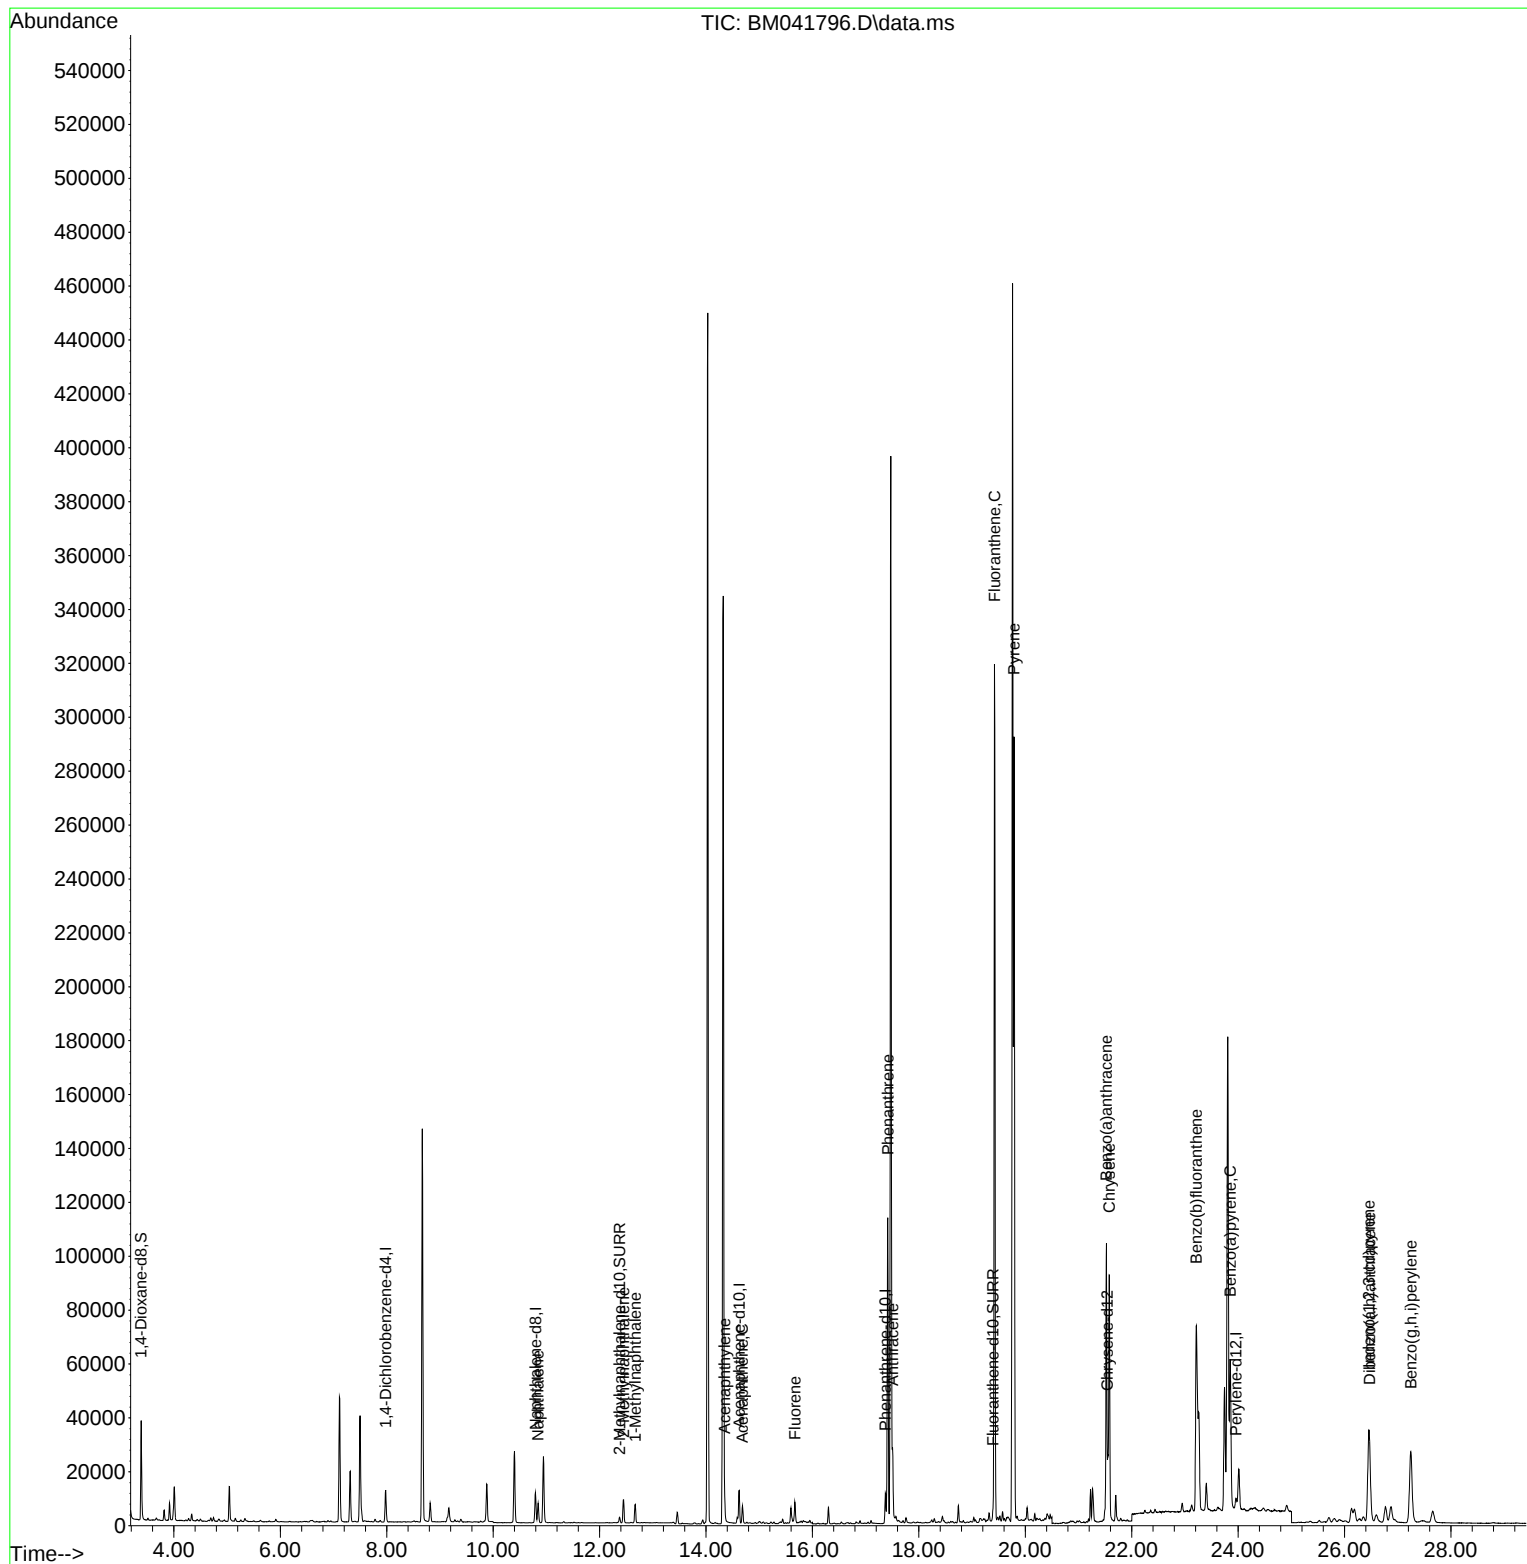


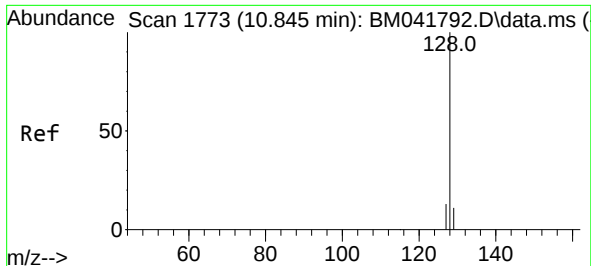

#5
Naphthalene
Concen: 0.204 ng/ul
RT: 10.845 min Scan# 1773
Delta R.T. -0.000 min
Lab File: BM041796.D
Acq: 12 Sep 2023 02:20




Instrument :
BNA_M
ClientSampleId :
EZYEO


Tgt Ion:	128	Resp:	9504
Ion Ratio	Lower	Upper	
128	100		
129	12.3	9.4	14.0
127	14.1	11.0	16.6

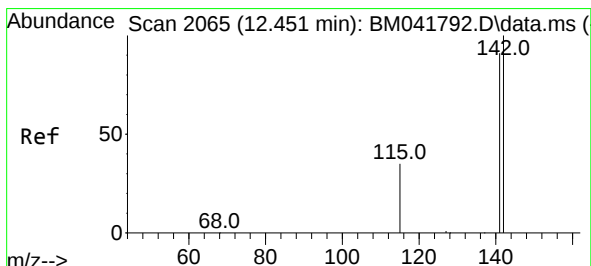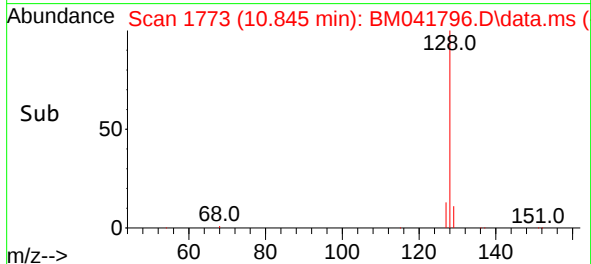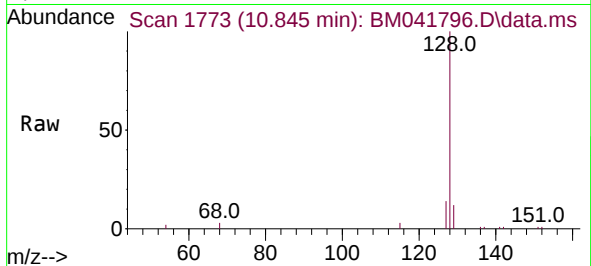

#7
2-Methylnaphthalene
Concen: 0.224 ng/ul
RT: 12.451 min Scan# 2065
Delta R.T. -0.000 min
Lab File: BM041796.D
Acq: 12 Sep 2023 02:20

Tgt Ion:	142	Resp:	5906
Ion Ratio	Lower	Upper	
142	100		
141	89.8	72.2	108.2


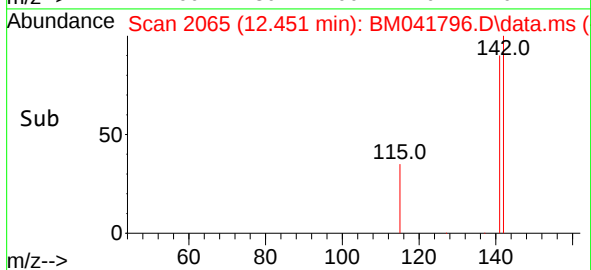

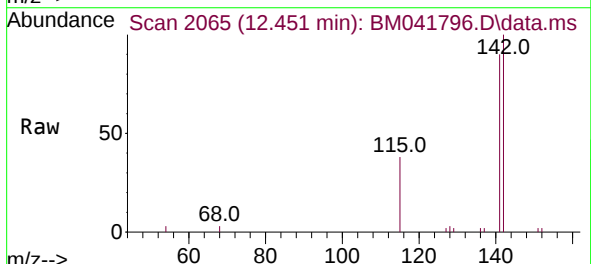


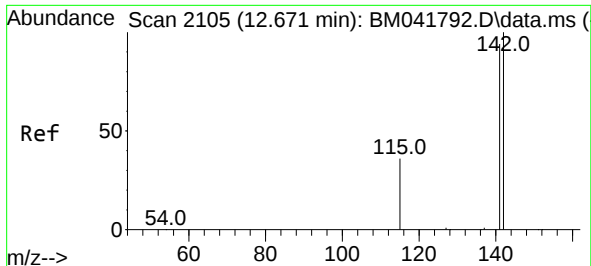

#8
1-Methylnaphthalene
Concen: 0.171 ng/ul
RT: 12.671 min Scan# 2105
Delta R.T. -0.000 min
Lab File: BM041796.D
Acq: 12 Sep 2023 02:20




Instrument :
BNA_M
ClientSampleId :
EZYEO


Tgt Ion:142 Resp: 4527
Ion Ratio Lower Upper
142 100
141 93.8 74.4 111.6

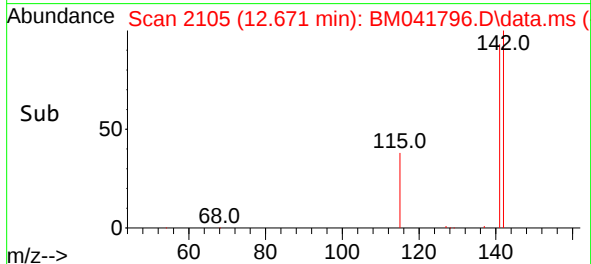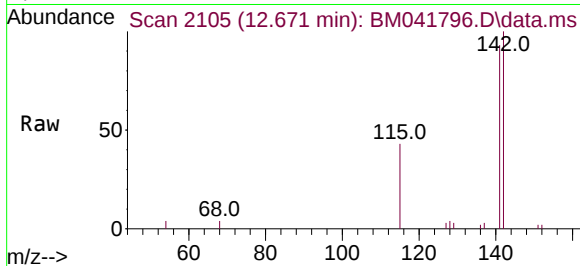

#10
Acenaphthylene
Concen: 0.206 ng/ul
RT: 14.351 min Scan# 2443
Delta R.T. -0.000 min
Lab File: BM041796.D
Acq: 12 Sep 2023 02:20

Tgt Ion:152 Resp: 7921
Ion Ratio Lower Upper
152 100
151 20.8 16.4 24.6
153 15.1 11.1 16.7

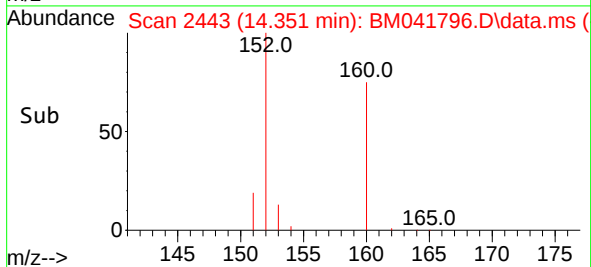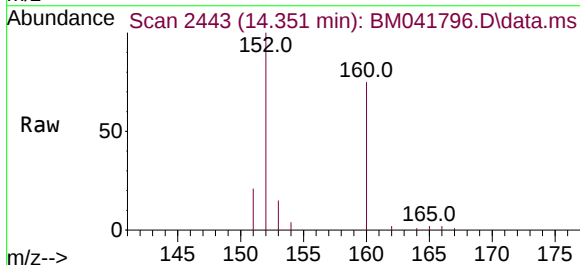



#11

Acenaphthene

Concen: 0.123 ng/ul

RT: 14.685 min Scan# 2515

Delta R.T. -0.000 min

Lab File: BM041796.D

Acq: 12 Sep 2023 02:20

Instrument :

BNA_M

ClientSampleId :

EZYE0





Tgt Ion:153 Resp: 3675

Ion Ratio Lower Upper

153 100

152 54.5 43.4 65.2

154 87.4 69.4 104.0

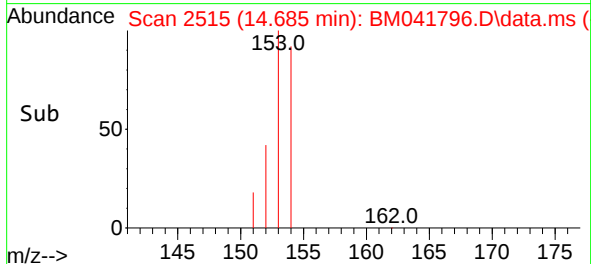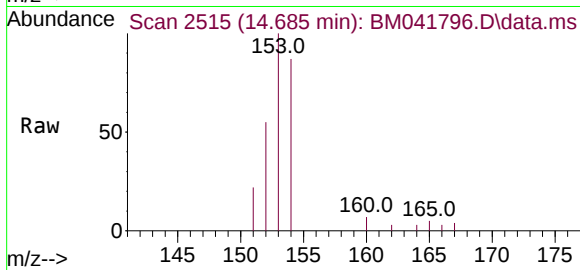

#12

Fluorene

Concen: 0.145 ng/ul

RT: 15.670 min Scan# 2728

Delta R.T. -0.000 min

Lab File: BM041796.D

Acq: 12 Sep 2023 02:20




Tgt Ion:166 Resp: 4859


Ion Ratio Lower Upper

166 100

165 100.3 79.4 119.2

167 16.7 11.3 16.9



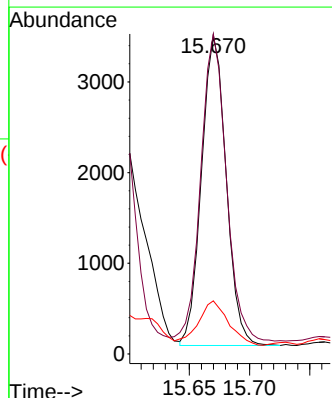
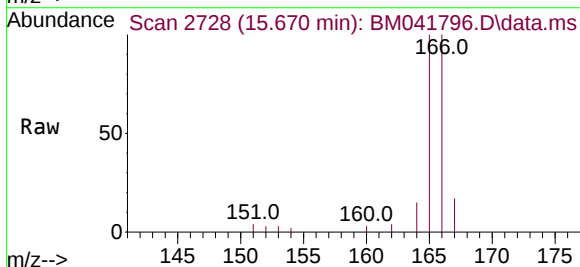


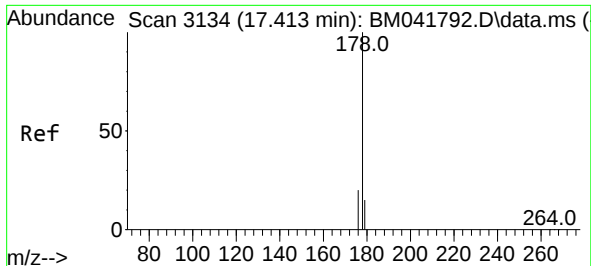

#15
Phenanthrene
Concen: 2.451 ng/ul
RT: 17.417 min Scan# 3134
Delta R.T. 0.004 min
Lab File: BM041796.D
Acq: 12 Sep 2023 02:20




Instrument :
BNA_M
ClientSampleId :
EZYEO


Tgt Ion:178 Resp: 117259
Ion Ratio Lower Upper
178 100
179 15.5 12.9 19.3
176 20.1 16.9 25.3

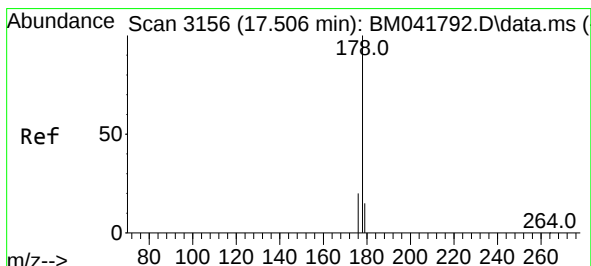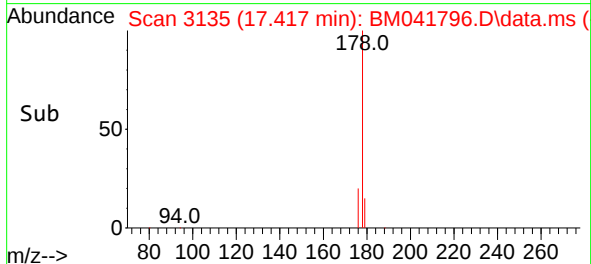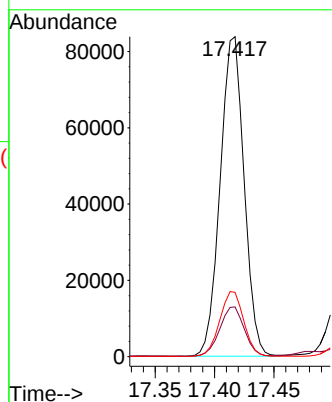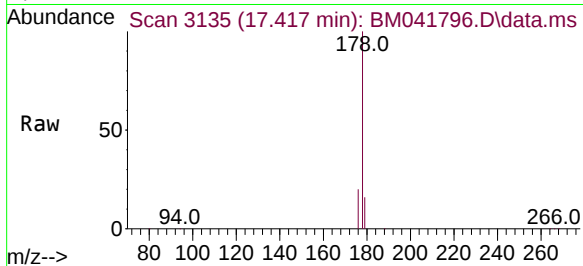

#16
Anthracene
Concen: 0.592 ng/ul
RT: 17.506 min Scan# 3156
Delta R.T. -0.000 min
Lab File: BM041796.D
Acq: 12 Sep 2023 02:20

Tgt Ion:178 Resp: 24268
Ion Ratio Lower Upper
178 100
179 16.7 12.9 19.3
176 20.3 15.8 23.8


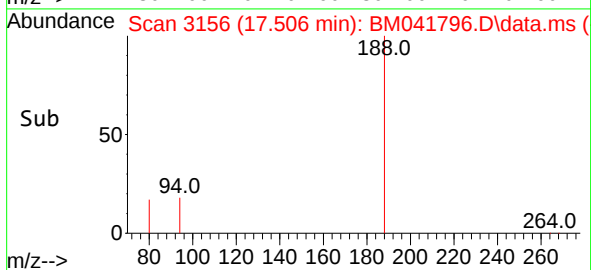

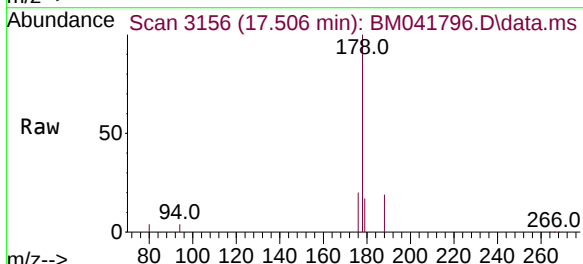




#19
Fluoranthene
Concen: 4.540 ng/u1
RT: 19.422 min Scan# 3590
Delta R.T. -0.000 min
Lab File: BM041796.D
Acq: 12 Sep 2023 02:20




Instrument :
BNA_M
ClientSampleId :
EZYEO


Tgt Ion:202 Resp: 252141
Ion Ratio Lower Upper
202 100
101 14.0 10.5 15.7
100 10.7 8.4 12.6

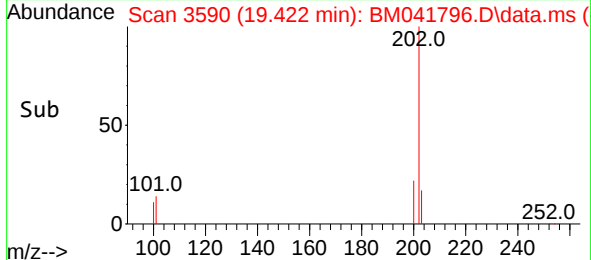

#20
Pyrene
Concen: 4.079 ng/u1
RT: 19.789 min Scan# 3669
Delta R.T. -0.000 min
Lab File: BM041796.D
Acq: 12 Sep 2023 02:20


Tgt Ion:202 Resp: 225054
Ion Ratio Lower Upper
202 100
101 15.9 11.8 17.8
100 12.9 9.8 14.6

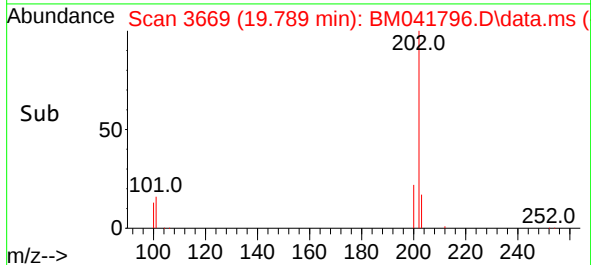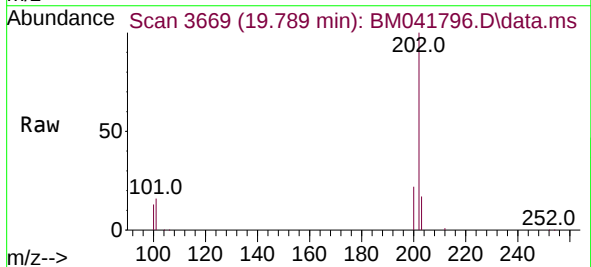



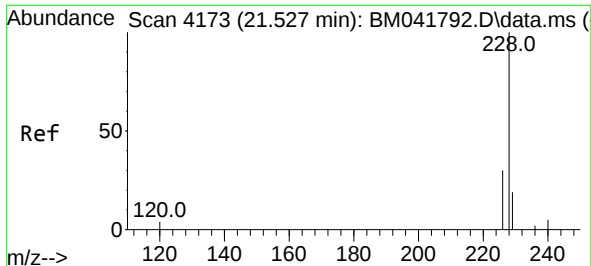


#21
Benzo(a)anthracene
Concen: 2.241 ng/ul
RT: 21.524 min Scan# 4172
Delta R.T. -0.003 min
Lab File: BM041796.D
Acq: 12 Sep 2023 02:20

Instrument :
BNA_M
ClientSampleId :
EZYEO







Tgt Ion:228 Resp: 86025
Ion Ratio Lower Upper
228 100
229 19.9 15.8 23.6
226 31.0 24.8 37.2

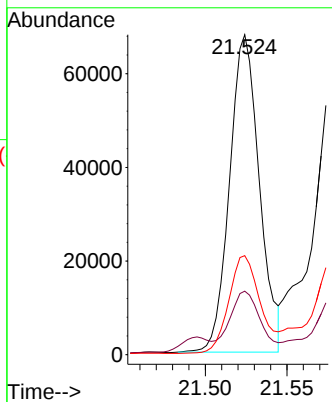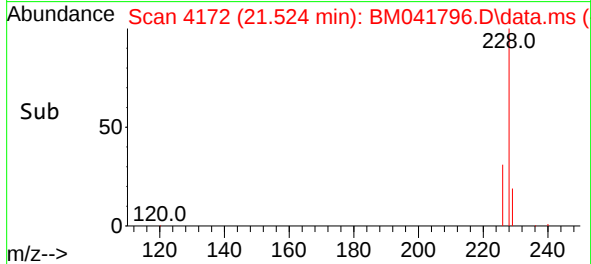

#22
Chrysene
Concen: 2.196 ng/ul
RT: 21.580 min Scan# 4191
Delta R.T. -0.000 min
Lab File: BM041796.D
Acq: 12 Sep 2023 02:20

Tgt Ion:228 Resp: 90931
Ion Ratio Lower Upper
228 100
226 34.2 27.0 40.6
229 21.6 15.4 23.2


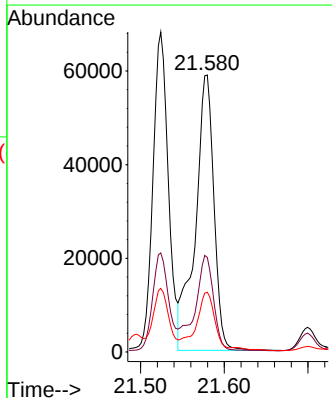
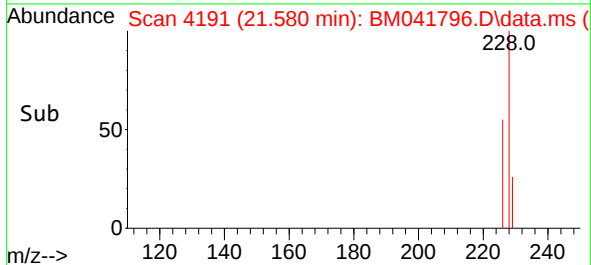
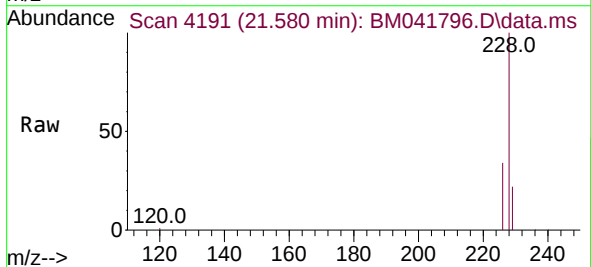


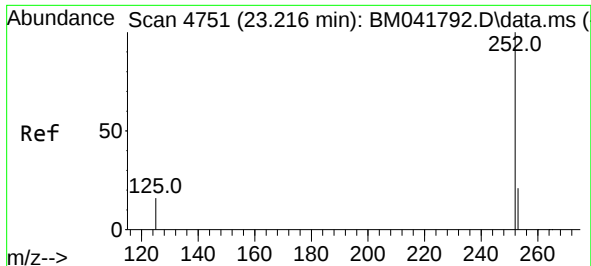

#24
Benzo(b)fluoranthene
Concen: 2.813 ng/ul
RT: 23.214 min Scan# 41
Delta R.T. -0.003 min
Lab File: BM041796.D
Acq: 12 Sep 2023 02:20




Instrument :
BNA_M
ClientSampleId :
EZYEO


Tgt Ion:252 Resp: 122386
Ion Ratio Lower Upper
252 100
253 22.8 0.0 52.4
125 17.3 0.0 42.8

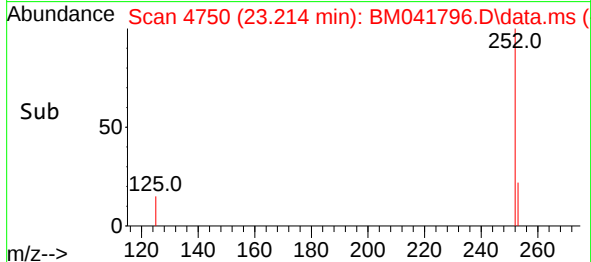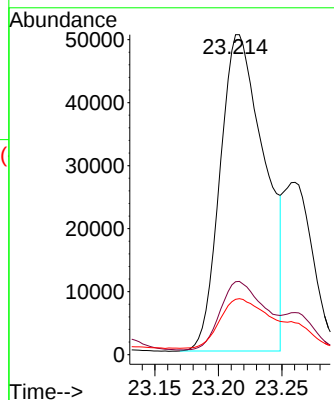

#26
Benzo(a)pyrene
Concen: 2.256 ng/ul
RT: 23.851 min Scan# 4968
Delta R.T. -0.003 min
Lab File: BM041796.D
Acq: 12 Sep 2023 02:20

Tgt Ion:252 Resp: 79765
Ion Ratio Lower Upper
252 100
253 23.4 22.4 33.6
125 19.0 21.0 31.4#

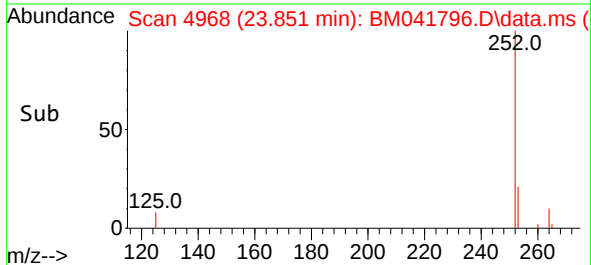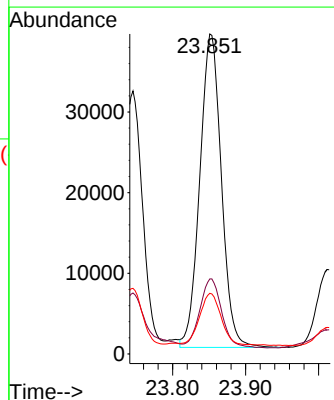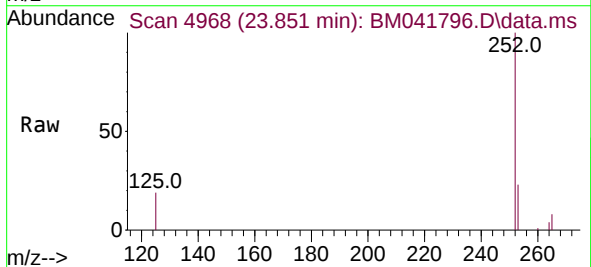

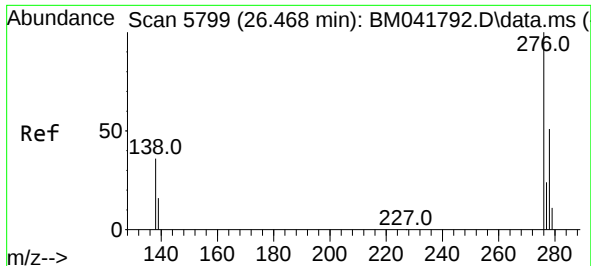

#27

Indeno(1,2,3-cd)pyrene

Concen: 1.219 ng/ul

RT: 26.461 min Scan# 5

Delta R.T. -0.007 min

Lab File: BM041796.D

Acq: 12 Sep 2023 02:20

Instrument :

BNA_M

ClientSampleId :

EZYE0





Tgt Ion:276 Resp: 59157

Ion Ratio Lower Upper

276 100

138 33.7 26.4 39.6

227 0.3 0.1 0.1#

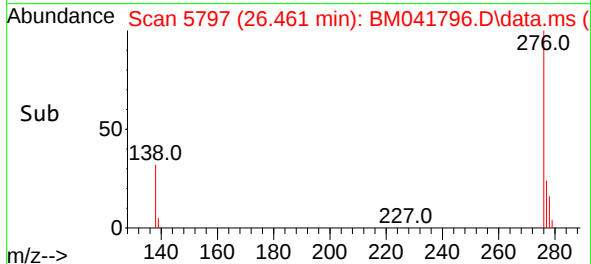

#28

Dibenzo(a,h)anthracene

Concen: 0.390 ng/ul

RT: 26.475 min Scan# 5801

Delta R.T. -0.010 min

Lab File: BM041796.D

Acq: 12 Sep 2023 02:20




Tgt Ion:278 Resp: 13278


Ion Ratio Lower Upper

278 100

139 35.4 23.0 34.6#


279 29.7 22.9 34.3

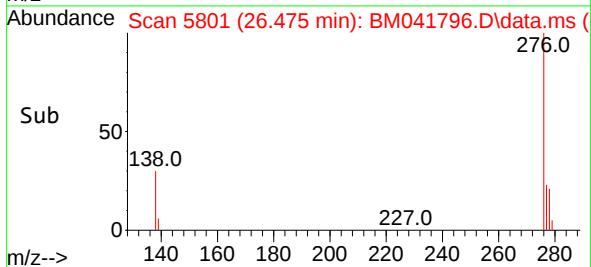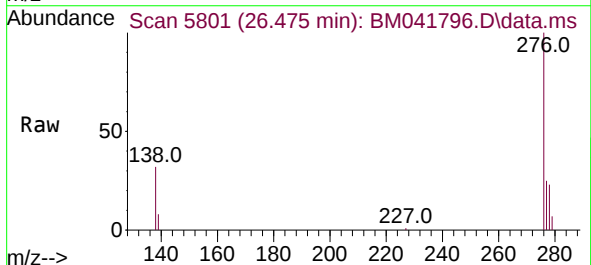



#29
 Benzo(g,h,i)perylene
 Concen: 1.356 ng/ul
 RT: 27.246 min Scan# 6031
 Delta R.T. -0.000 min
 Lab File: BM041796.D
 Acq: 12 Sep 2023 02:20

Instrument :
 BNA_M
 ClientSampleId :
 EYZE0

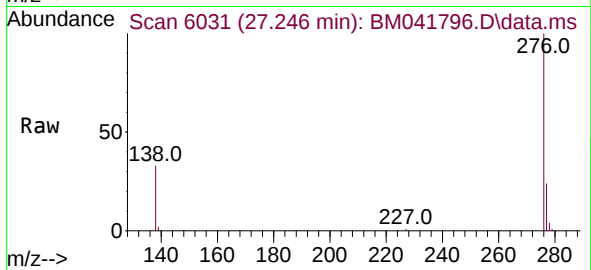

Tgt Ion:	276	Resp:	58289
Ion	Ratio	Lower	Upper
276	100		
138	33.0	25.0	37.4
277	23.8	20.2	30.2

