




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041782.D
 Acq On : 11 Sep 2023 17:04
 Operator : MA/JU
 Sample : 04247-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJ81

Manual IntegrationsAPPROVED

Quant Time: Sep 12 04:26:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/12/2023
 Supervised By :mohammad ahmed 09/13/2023

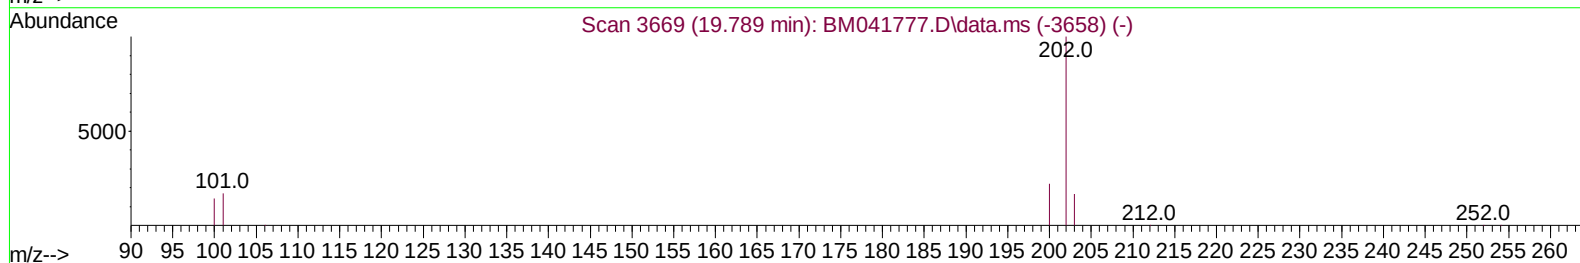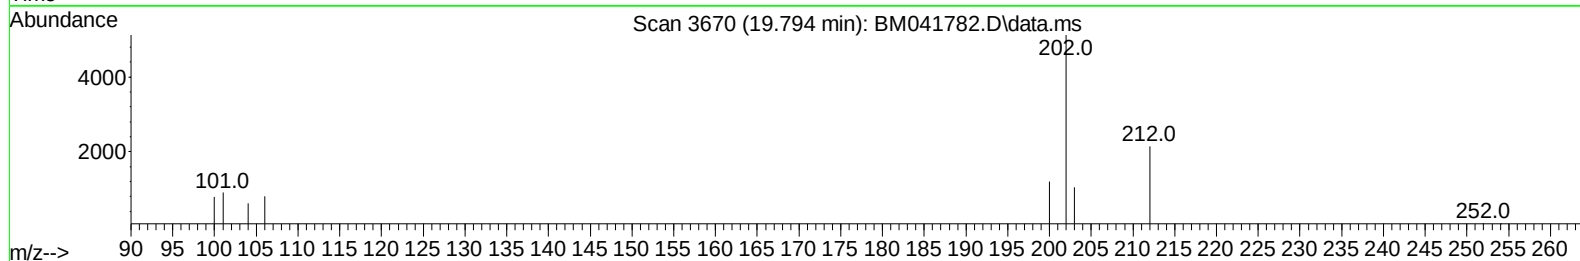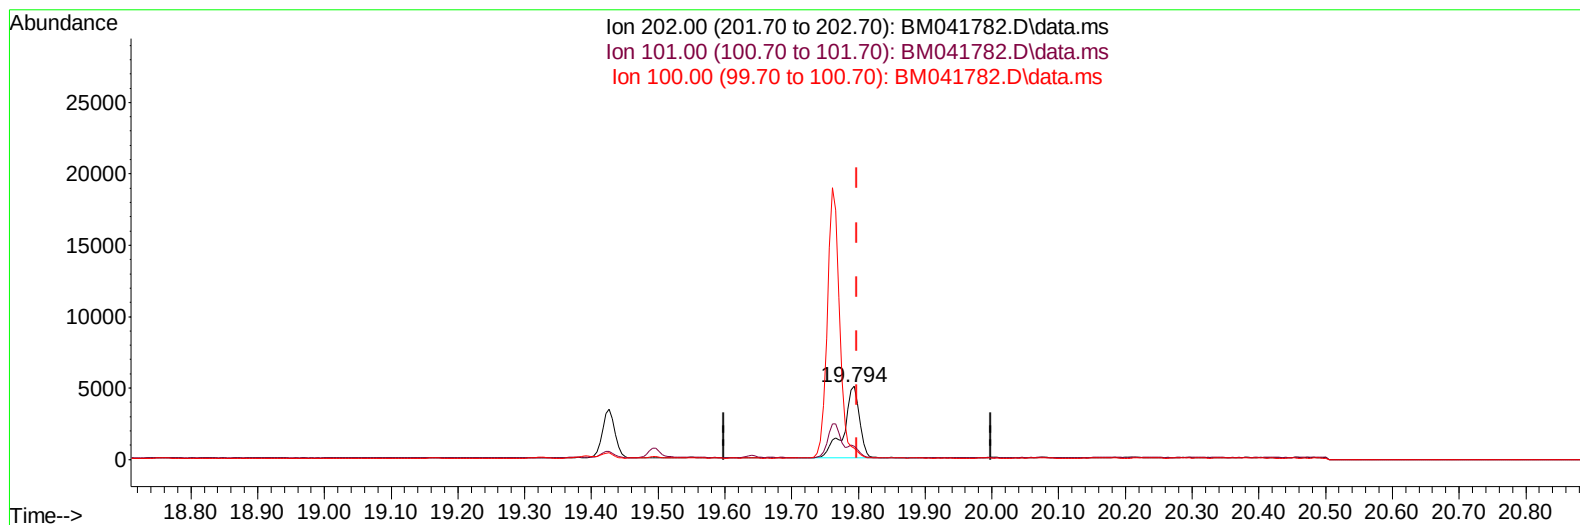

TIC: BM041782.D\data.ms

(20) Pyrene

19.794min (-0.005) 0.21 ng/u1

response 8186

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.80	17.75
100.00	12.20	15.57#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041782.D
 Acq On : 11 Sep 2023 17:04
 Operator : MA/JU
 Sample : 04247-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJ81

Manual IntegrationsAPPROVED

Quant Time: Sep 12 04:26:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/12/2023
 Supervised By :mohammad ahmed 09/13/2023

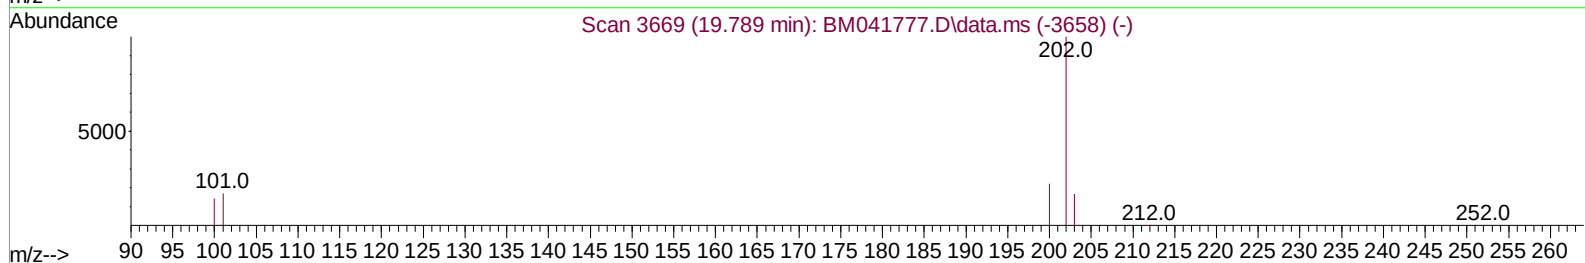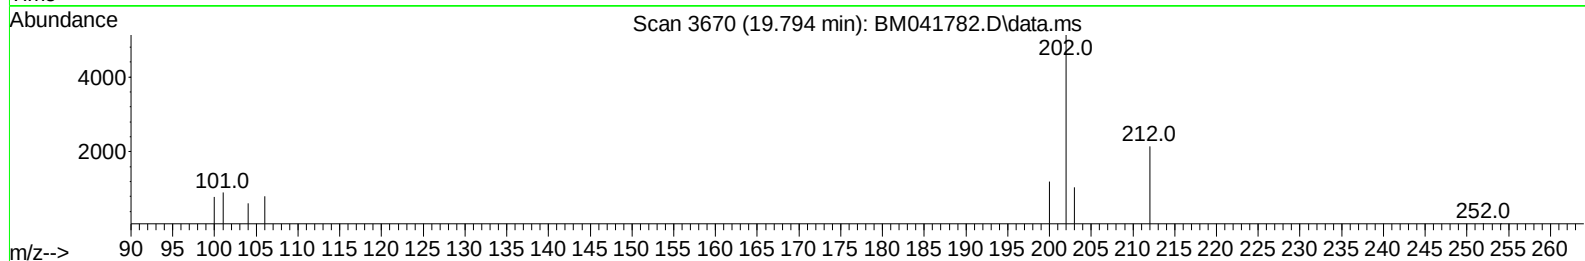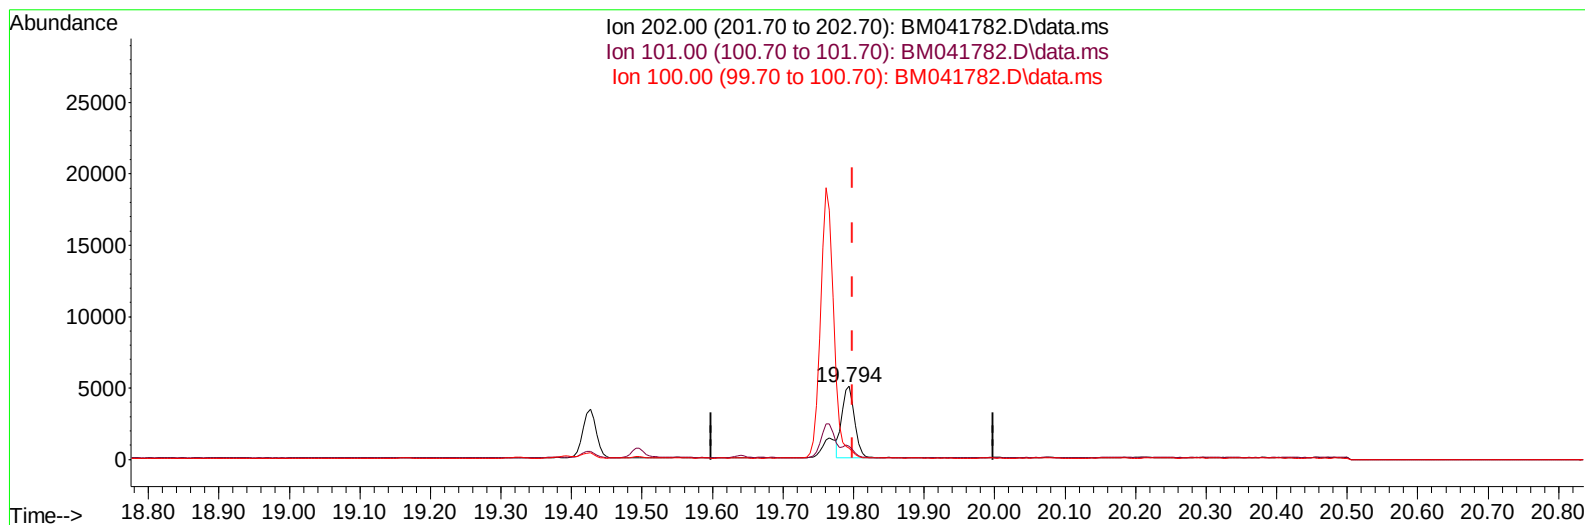

TIC: BM041782.D\data.ms

(20) Pyrene

19.794min (-0.005) 0.16 ng/ul m

response 6242

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.80	17.75
100.00	12.20	15.57#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041782.D
 Acq On : 11 Sep 2023 17:04
 Operator : MA/JU
 Sample : 04247-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJ81

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/12/2023
 Supervised By :mohammad ahmed 09/13/2023

Quant Time: Sep 12 04:26:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.984	152		4165	0.400	ng/ul	0.00
4) Naphthalene-d8	10.796	136		9755	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.624	164		4360	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.375	188		8277	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.548	240		3392	0.400	ng/ul	0.00
23) Perylene-d12	23.968	264		3990	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.389	96		28478	4.474	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.379	152		3808	0.303	ng/ul	0.00
18) Fluoranthene-d10	19.394	212		5360	0.326	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.423	88		261117	39.489	ng/ul#	85
16) Anthracene	17.510	178		2437	0.081	ng/ul#	85
19) Fluoranthene	19.427	202		4415	0.110	ng/ul#	92
20) Pyrene	19.794	202		6242m	0.157	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
Data File : BM041782.D
Acq On : 11 Sep 2023 17:04
Operator : MA/JU
Sample : 04247-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJ81

Manual IntegrationsAPPROVED

Quant Time: Sep 12 04:26:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/12/2023
Supervised By :mohammad ahmed 09/13/2023

