

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041780.D
 Acq On : 11 Sep 2023 15:45
 Operator : MA/JU
 Sample : 04247-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHAS6

Quant Time: Sep 12 04:26:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.984	152	4120	0.400	ng/ul	0.00
4) Naphthalene-d8	10.801	136	9531	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.624	164	4237	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.375	188	7546	0.400	ng/ul	0.00
17) Chrysene-d12	21.545	240	2884	0.400	ng/ul	0.00
23) Perylene-d12	23.965	264	3292	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	24420	3.878	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.379	152	3949	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.394	212	4850	0.347	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.427	88	337	0.052	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
Data File : BM041780.D
Acq On : 11 Sep 2023 15:45
Operator : MA/JU
Sample : 04247-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHAS6


Quant Time: Sep 12 04:26:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration

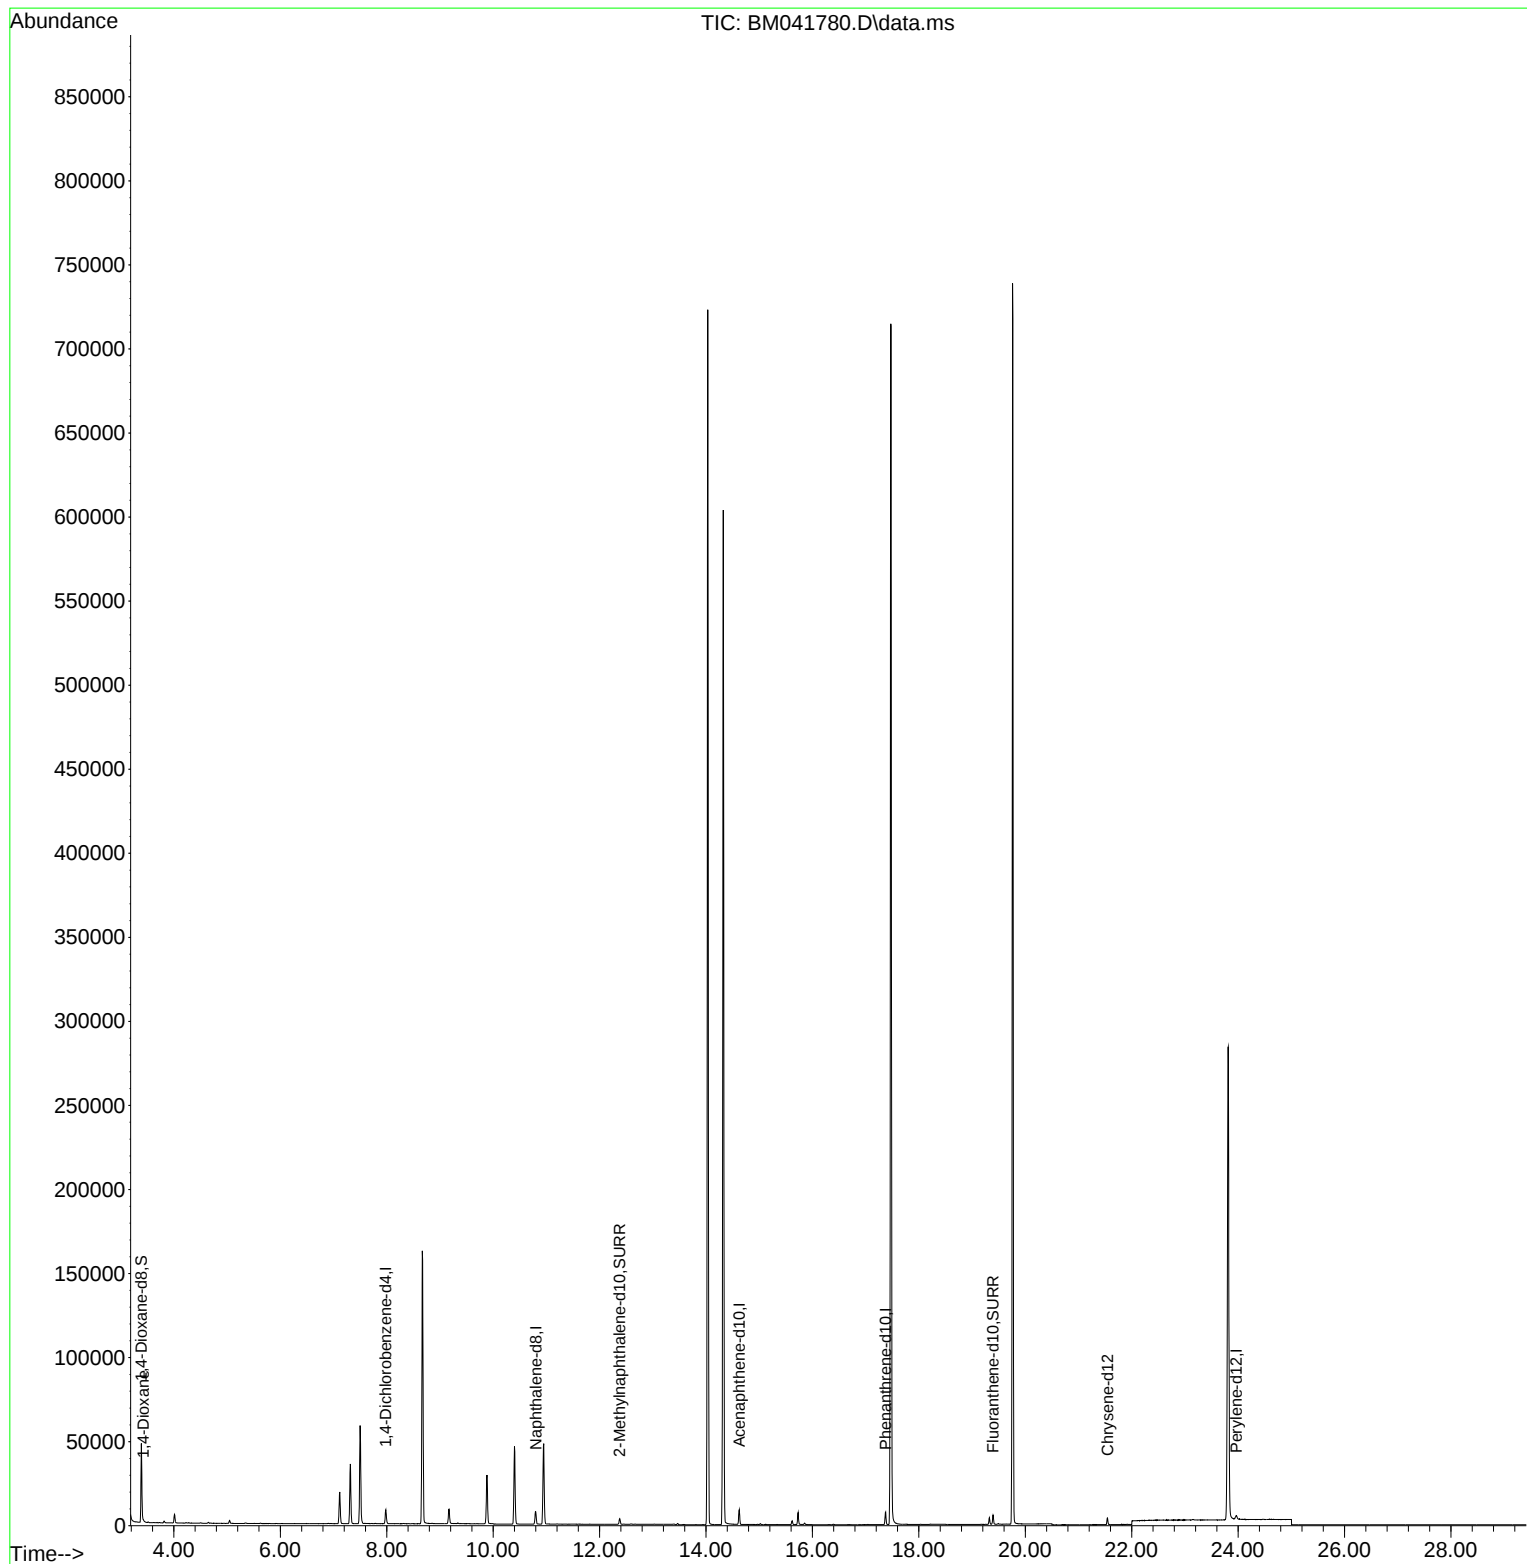

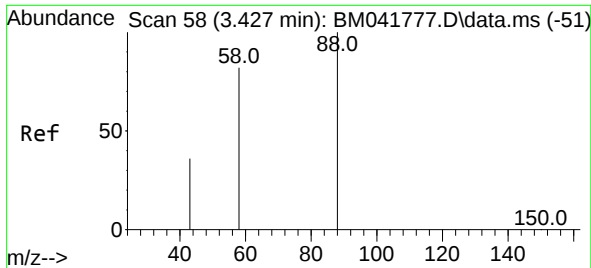

#2
 1,4-Dioxane
 Concen: 0.052 ng/ul
 RT: 3.427 min Scan# 51
 Delta R.T. -0.008 min
 Lab File: BM041780.D
 Acq: 11 Sep 2023 15:45

Instrument :
 BNA_M
 ClientSampleId :
 BHAS6

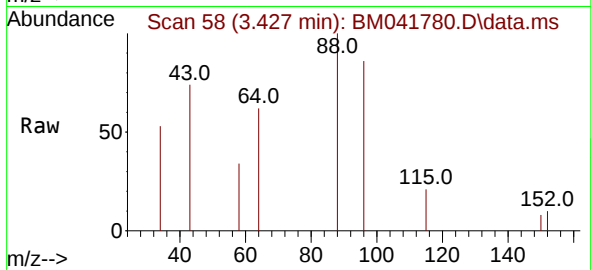

Tgt Ion:	88	Resp:	337
Ion	Ratio	Lower	Upper
88	100		
43	73.5	33.8	50.6#
58	33.8	54.2	81.2#

