

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041783.D
 Acq On : 11 Sep 2023 17:41
 Operator : MA/JU
 Sample : 04247-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBKB6

Quant Time: Sep 12 04:26:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.984	152	4181	0.400	ng/ul	0.00
4) Naphthalene-d8	10.796	136	10390	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.624	164	4573	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.375	188	7769	0.400	ng/ul	0.00
17) Chrysene-d12	21.545	240	2980	0.400	ng/ul	0.00
23) Perylene-d12	23.962	264	3523	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	27496	4.303	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.379	152	4085	0.305	ng/ul	0.00
18) Fluoranthene-d10	19.394	212	5922	0.410	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.851	128	1049	0.031	ng/ul#	Qvalue 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
Data File : BM041783.D
Acq On : 11 Sep 2023 17:41
Operator : MA/JU
Sample : 04247-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBKB6


Quant Time: Sep 12 04:26:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration

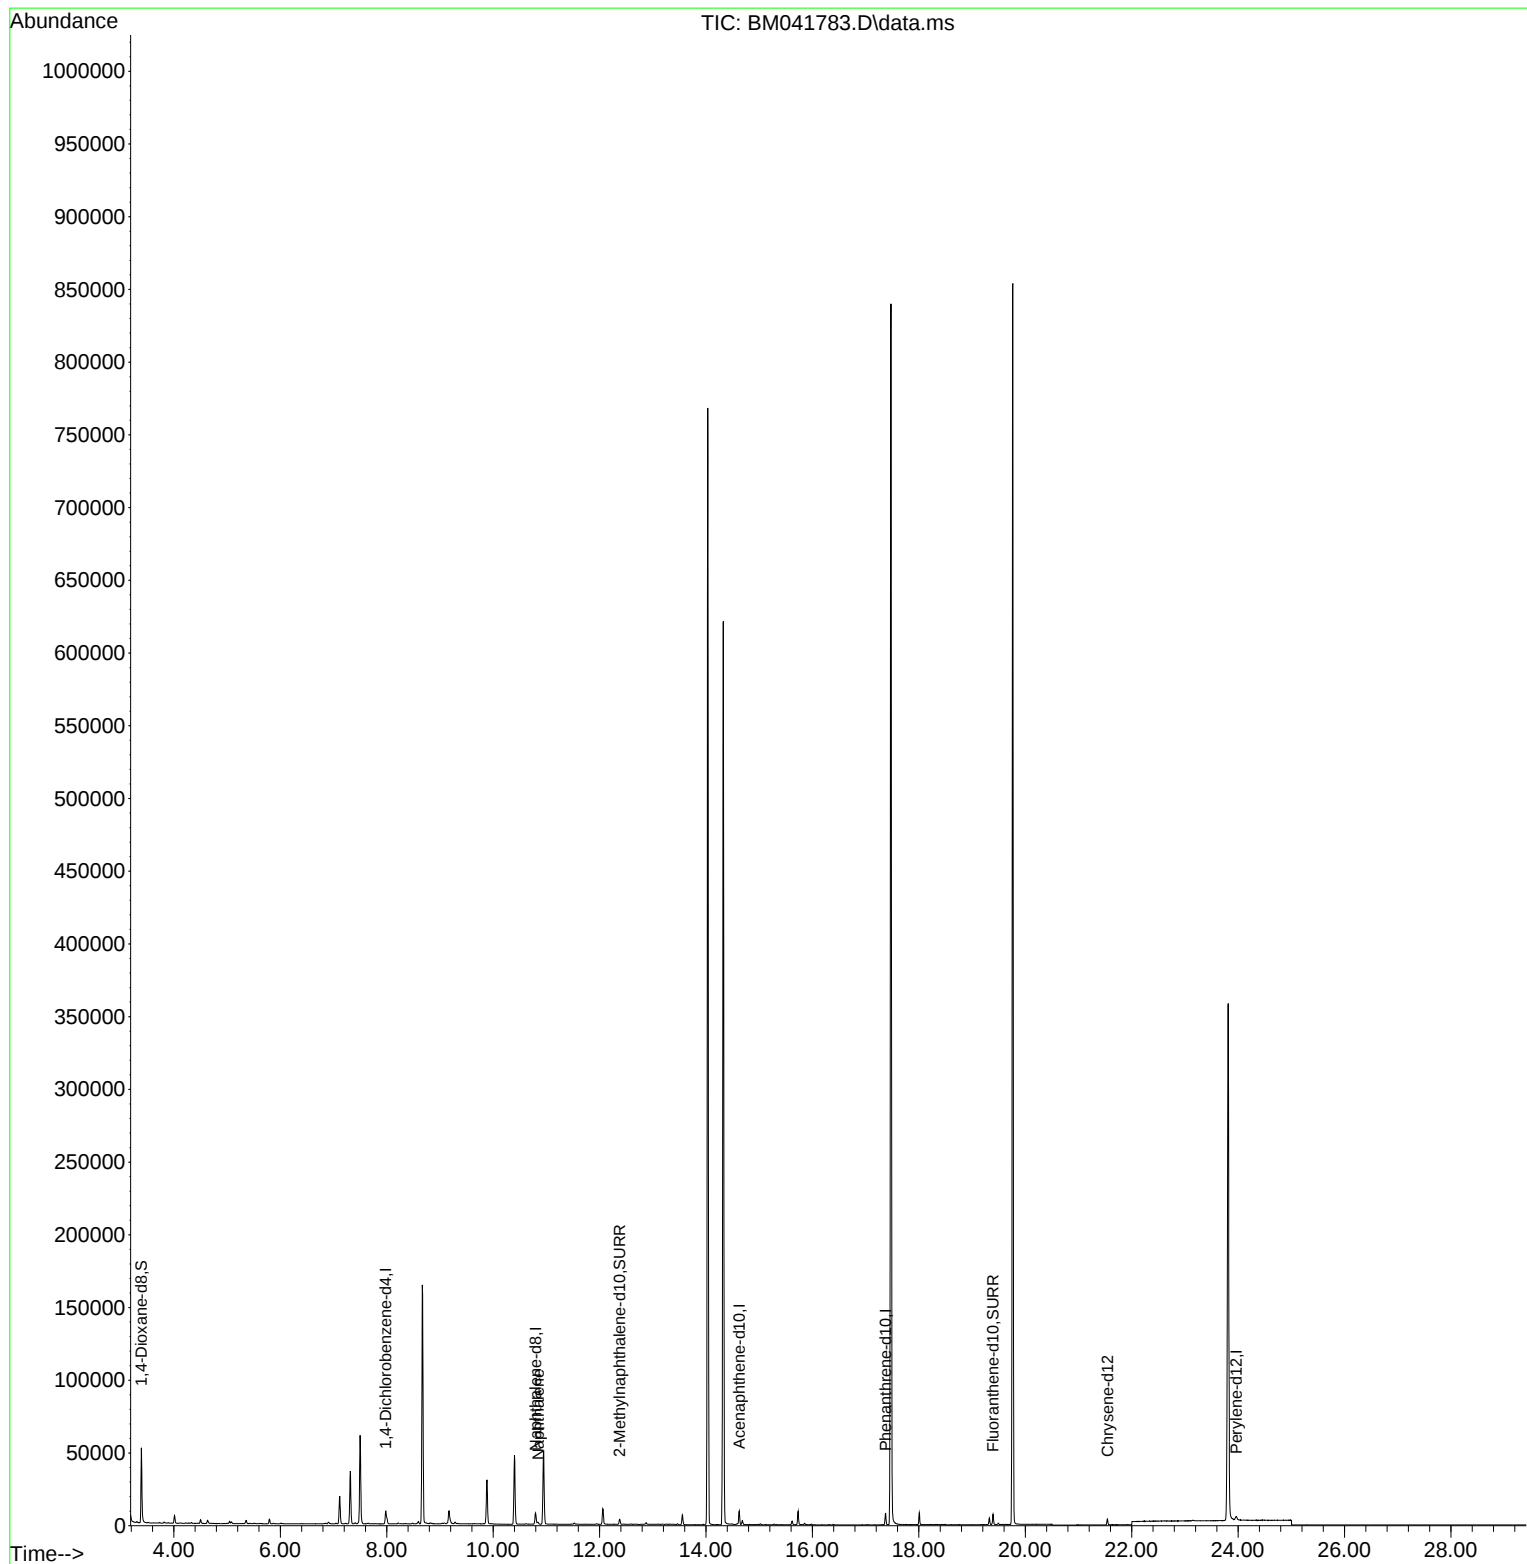

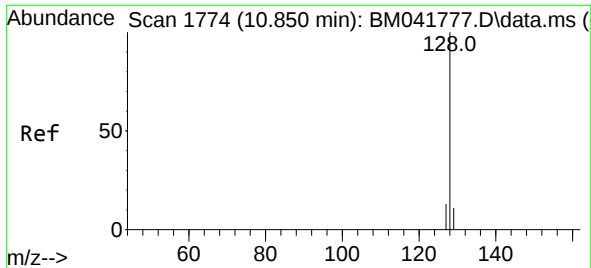

#5
Naphthalene
Concen: 0.031 ng/ul
RT: 10.851 min Scan# 11
Delta R.T. -0.005 min
Lab File: BM041783.D
Acq: 11 Sep 2023 17:41

Instrument :
BNA_M
ClientSampleId :
BBKB6

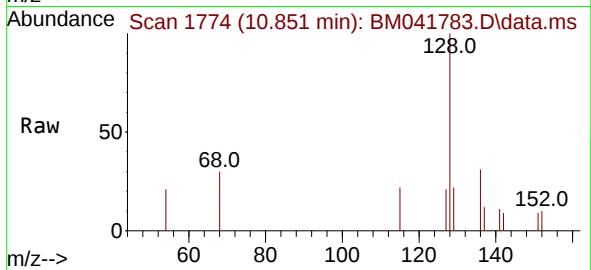

Tgt Ion	Ratio	Lower	Upper
128	100		
129	22.2	9.4	14.0#
127	20.8	11.0	16.6#

