

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041785.D
 Acq On : 11 Sep 2023 18:56
 Operator : MA/JU
 Sample : 04247-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHA05

Quant Time: Sep 12 04:27:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.984	152	3857	0.400	ng/ul	0.00
4) Naphthalene-d8	10.796	136	9630	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.624	164	5008	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.375	188	10065	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.545	240	3802	0.400	ng/ul	# 0.00
23) Perylene-d12	23.965	264	4447	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	26809	4.548	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.379	152	5085	0.410	ng/ul	0.00
18) Fluoranthene-d10	19.394	212	8161	0.443	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.427	88	70258	11.474	ng/ul	87
14) Pentachlorophenol	17.004	266	564	0.140	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
Data File : BM041785.D
Acq On : 11 Sep 2023 18:56
Operator : MA/JU
Sample : 04247-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHA05

Quant Time: Sep 12 04:27:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration




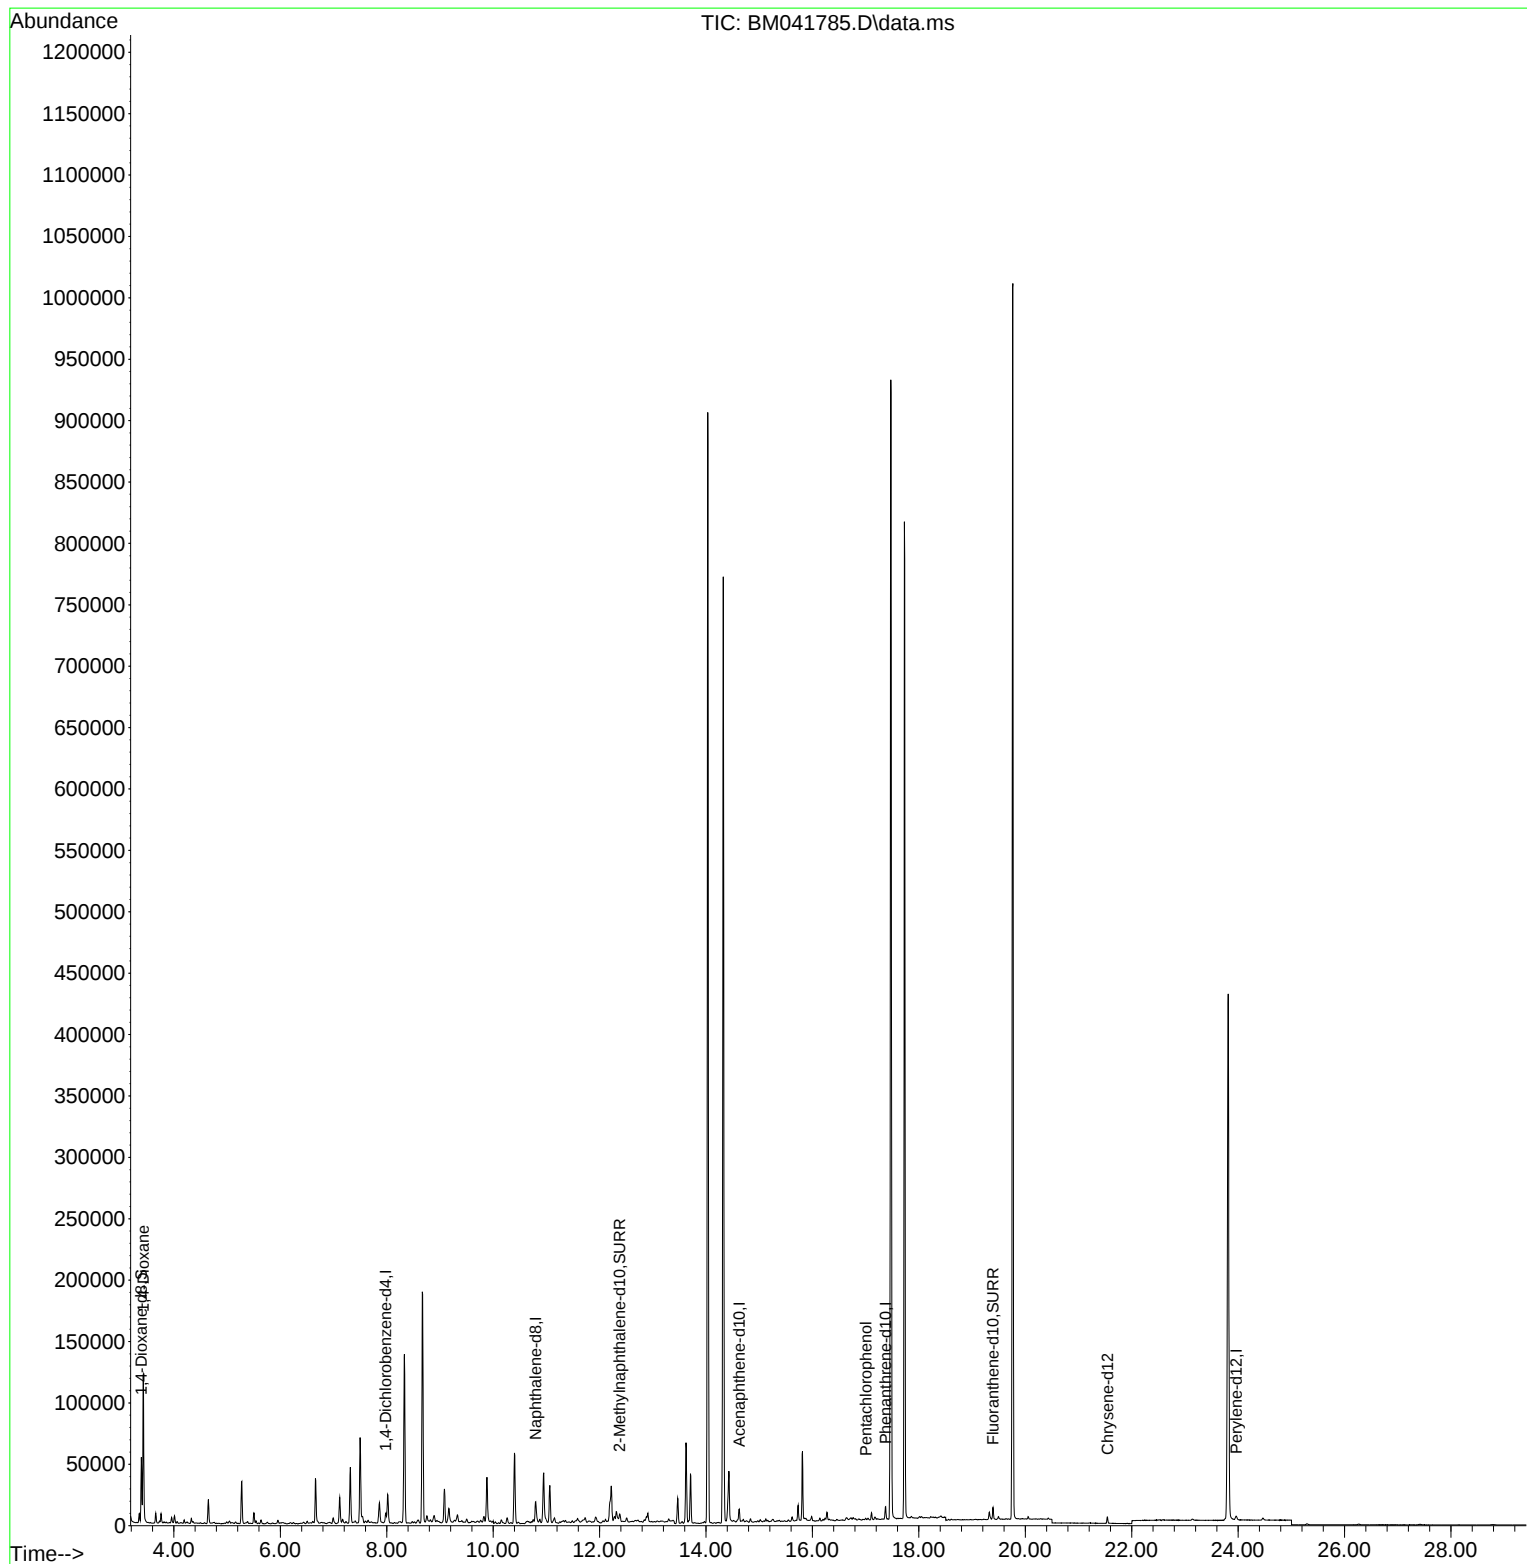


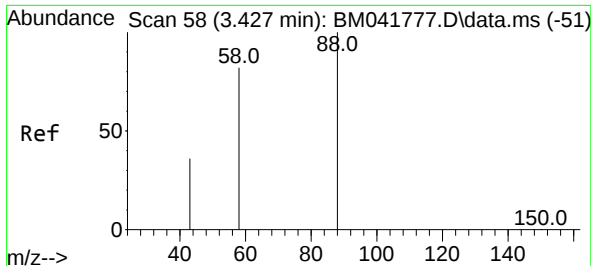

#2
 1,4-Dioxane
 Concen: 11.474 ng/ul
 RT: 3.427 min Scan# 51
 Delta R.T. -0.008 min
 Lab File: BM041785.D
 Acq: 11 Sep 2023 18:56

Instrument :
 BNA_M
 ClientSampleId :
 BHA05

Tgt Ion: 88 Resp: 70258
 Ion Ratio Lower Upper
 88 100
 43 36.8 33.8 50.6
 58 79.9 54.2 81.2

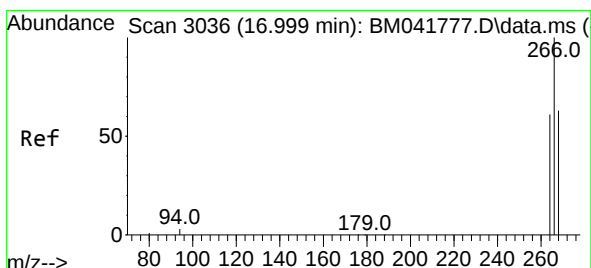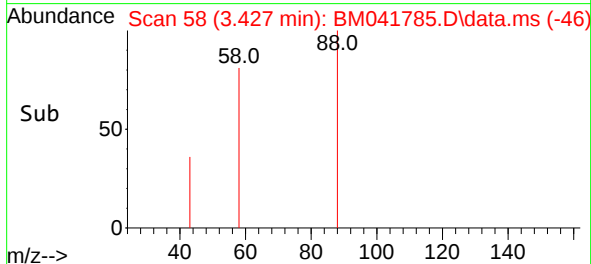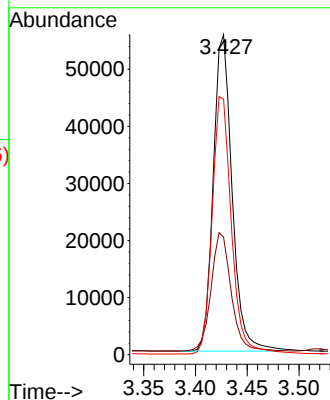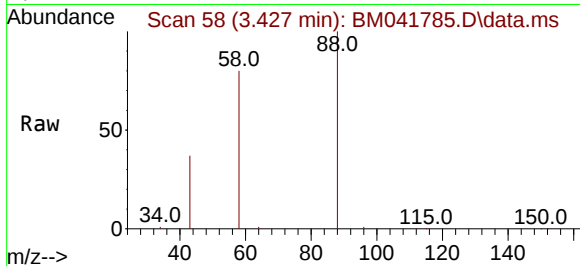

#14
 Pentachlorophenol
 Concen: 0.140 ng/ul
 RT: 17.004 min Scan# 3037
 Delta R.T. 0.000 min
 Lab File: BM041785.D
 Acq: 11 Sep 2023 18:56

Tgt Ion: 266 Resp: 564
 Ion Ratio Lower Upper
 266 100
 264 61.9 50.0 75.0
 268 62.9 50.8 76.2

